

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060419\
 Data File : P0056835.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jun 2019 16:38
 Operator : SM/SJ
 Sample : K3165-07RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 51419RE

Manual Integrations
 APPROVED

Ankita
 6/5/2019 4:48:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 16:53:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.240	3.574	2838591	158224	74.147m	4.798m#
2)	SA Decachlor...	9.826	8.507	604756	389118	12.321m	10.913

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060419\
Data File : P0056835.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2019 16:38
Operator : SM/SJ
Sample : K3165-07RE
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
51419RE


Manual Integrations
APPROVED

Ankita
6/5/2019 4:48:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 16:53:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

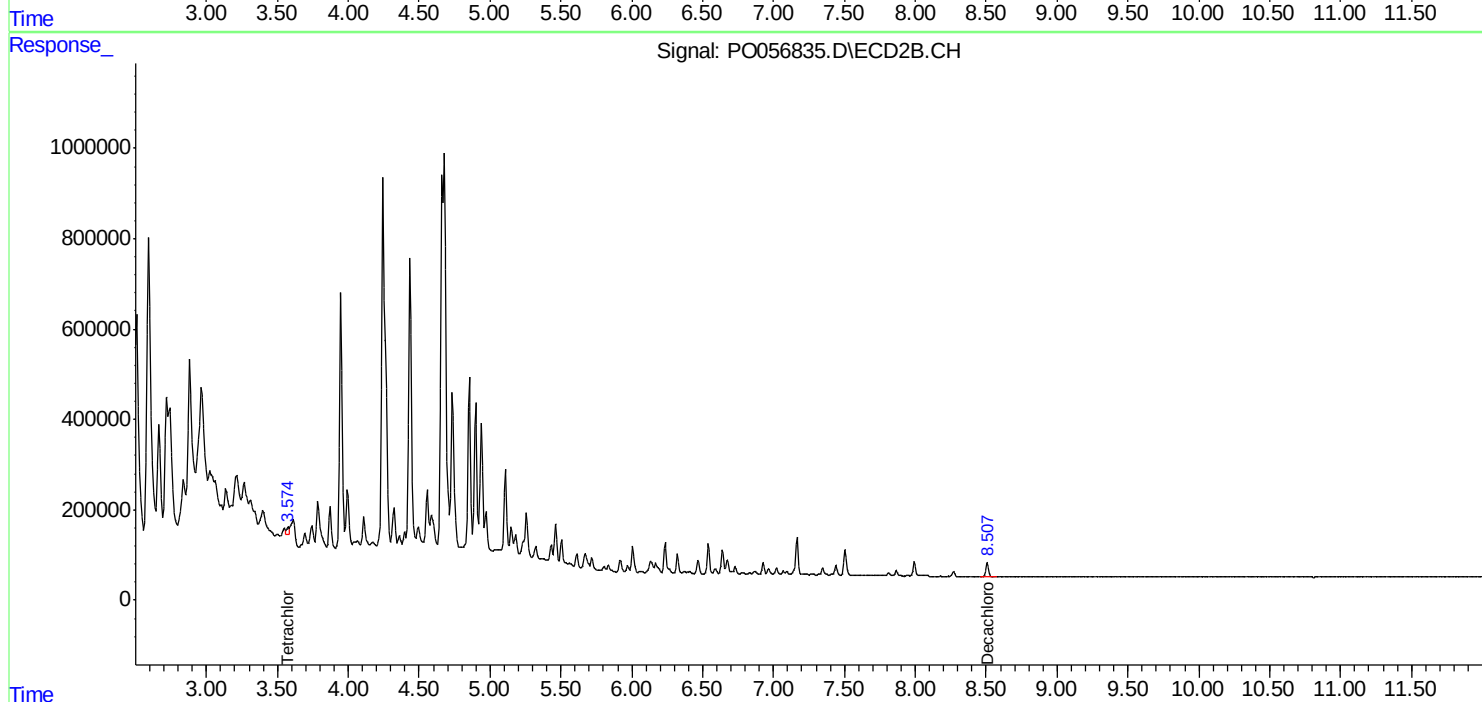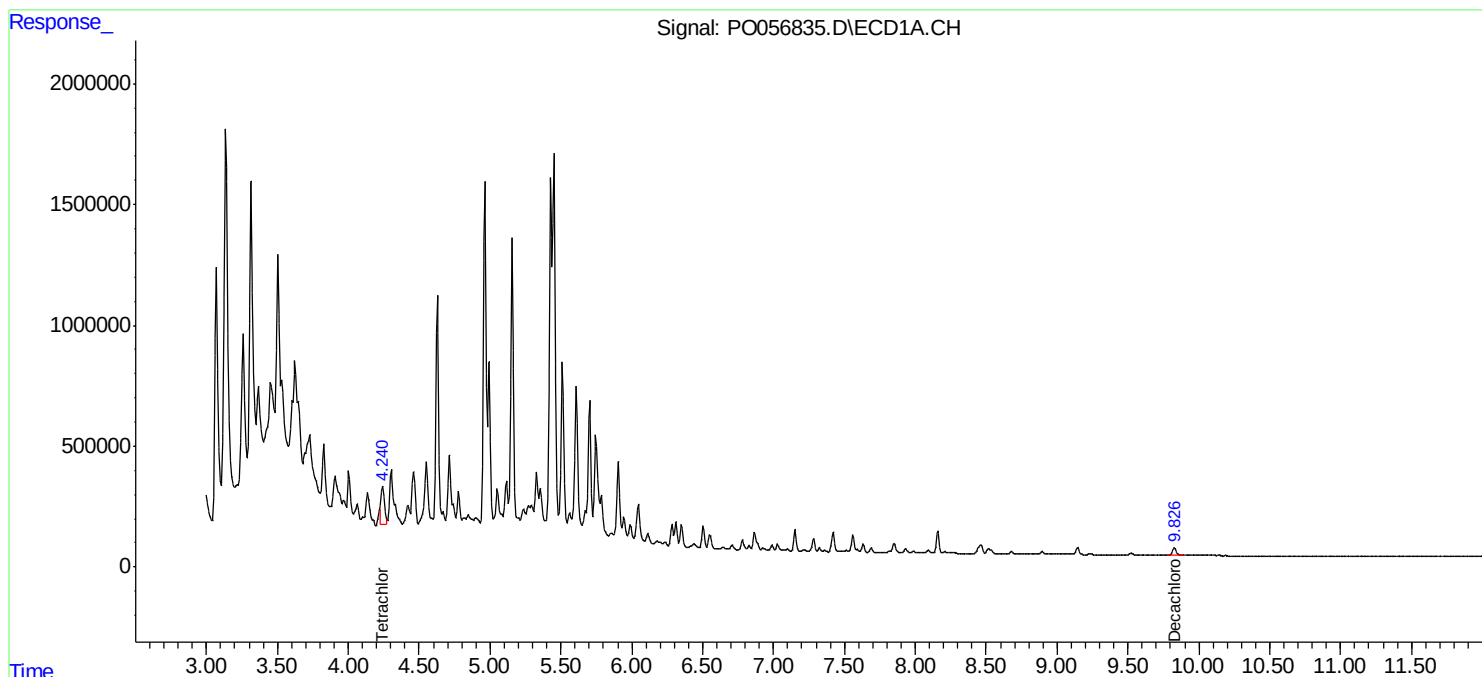

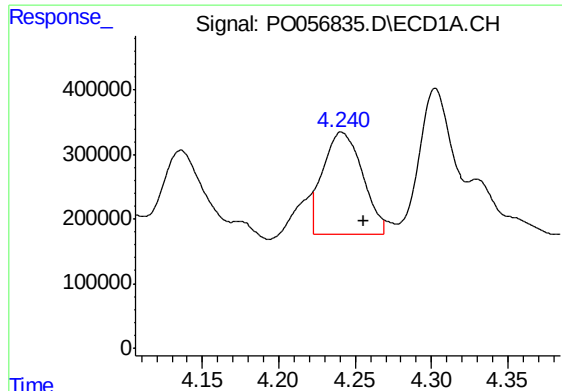


#1 Tetrachloro-m-xylene

R.T.: 4.240 min
Delta R.T.: -0.016 min
Response: 2838591
Conc: 74.15 ng/ml m

Instrument :
ECD_O
ClientSampleId :
51419RE


Manual Integrations
APPROVED

Ankita
6/5/2019 4:48:45 PM

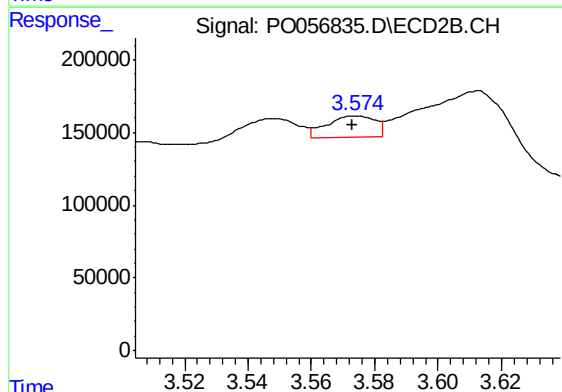


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.000 min
Response: 158224
Conc: 4.80 ng/ml m

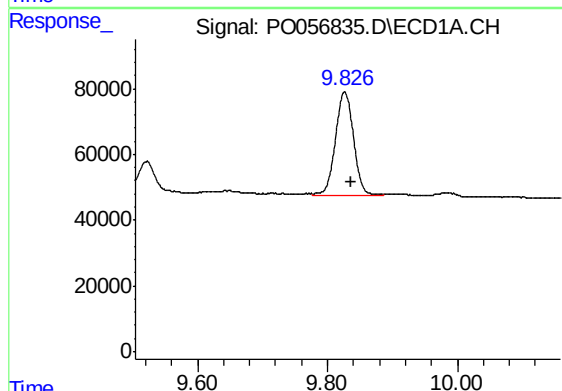

#2 Decachlorobiphenyl

R.T.: 9.826 min
Delta R.T.: -0.010 min
Response: 604756
Conc: 12.32 ng/ml m

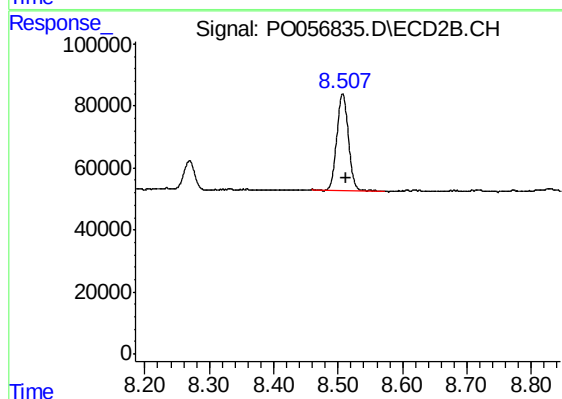

#2 Decachlorobiphenyl

R.T.: 8.507 min
Delta R.T.: -0.006 min
Response: 389118
Conc: 10.91 ng/ml