

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060419\
 Data File : P0056850.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jun 2019 20:54
 Operator : SM/SJ
 Sample : K3171-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-SF-03-008-B

Manual Integrations
 APPROVED

Ankita
 6/6/2019 11:02:45 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 02:17:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.249	3.568	983455	727585	25.689m	22.062m
2)	SA Decachlor...	9.822	8.502	969844	615376	19.759	17.258

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO060419\
Data File : PO056850.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2019 20:54
Operator : SM/SJ
Sample : K3171-03
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-SF-03-008-B


Manual Integrations
APPROVED

Ankita
6/6/2019 11:02:45 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 02:17:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

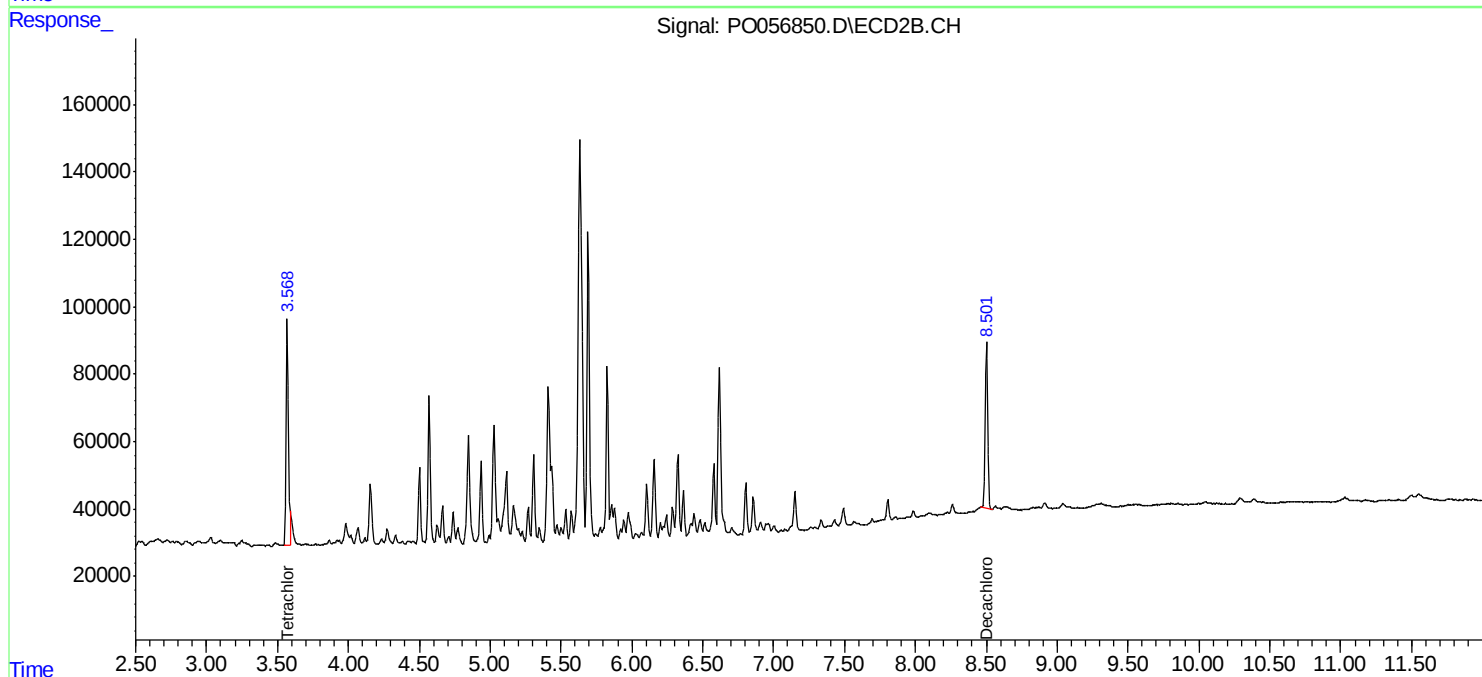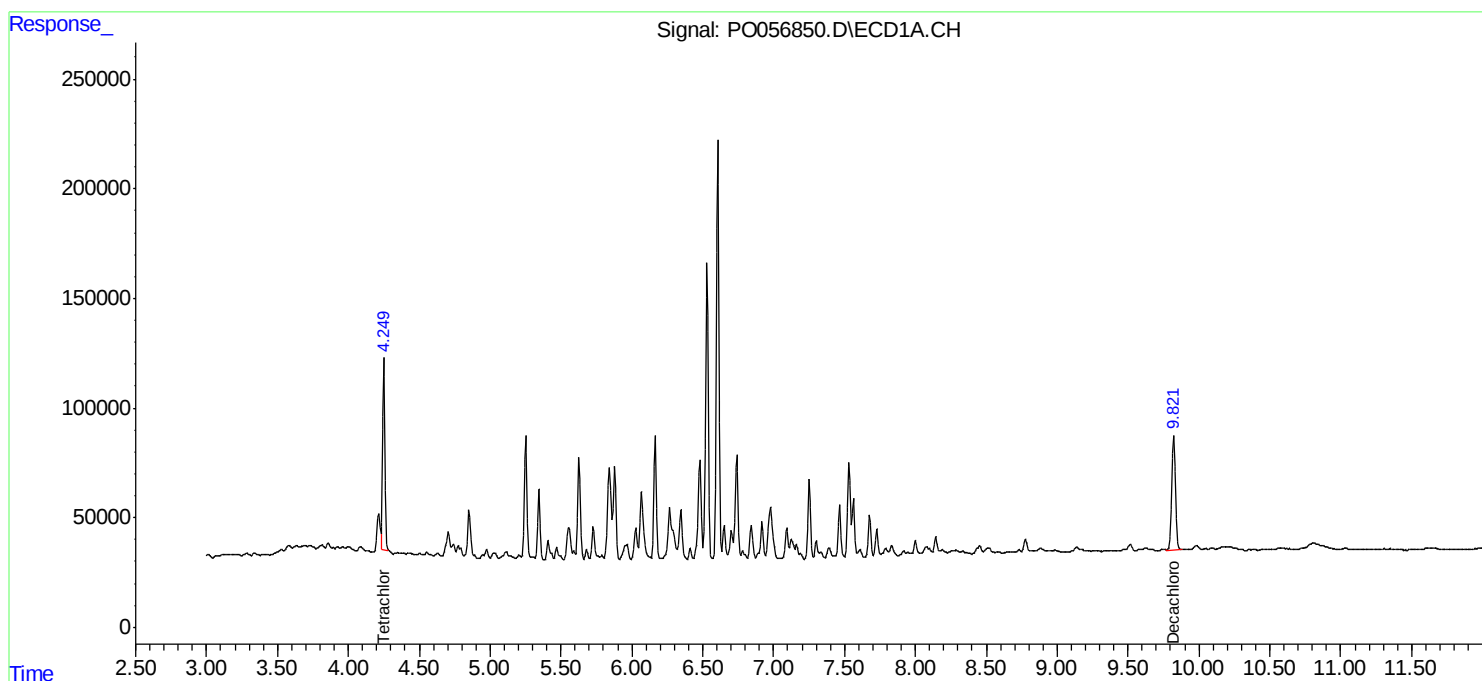

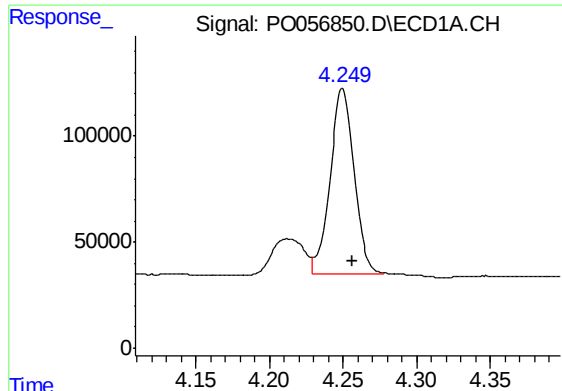


#1 Tetrachloro-m-xylene

R.T.: 4.249 min
Delta R.T.: -0.007 min
Response: 983455
Conc: 25.69 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-008-B


Manual Integrations
APPROVED

Ankita
6/6/2019 11:02:45 AM

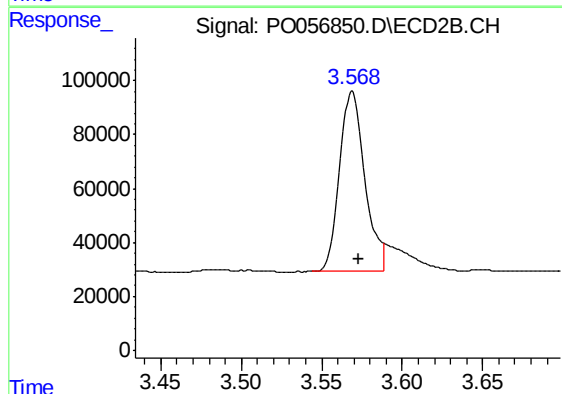


#1 Tetrachloro-m-xylene

R.T.: 3.568 min
Delta R.T.: -0.005 min
Response: 727585
Conc: 22.06 ng/ml m

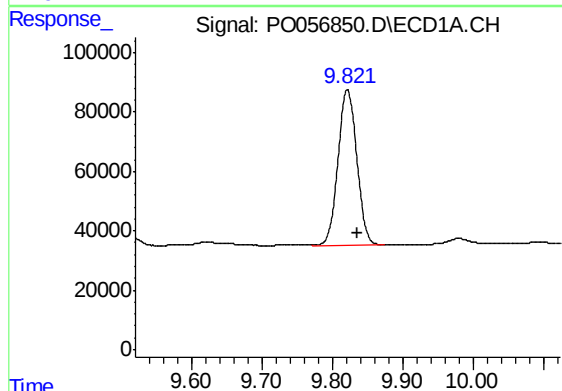

#2 Decachlorobiphenyl

R.T.: 9.822 min
Delta R.T.: -0.014 min
Response: 969844
Conc: 19.76 ng/ml

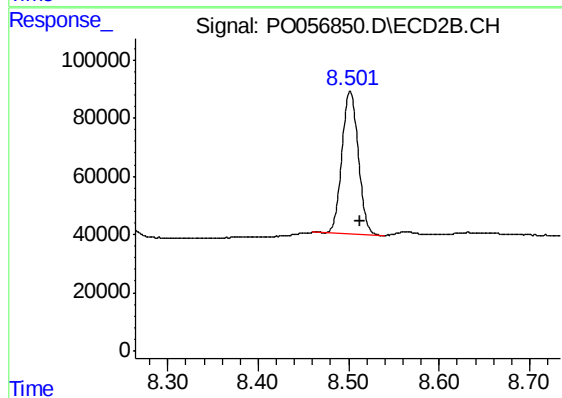

#2 Decachlorobiphenyl

R.T.: 8.502 min
Delta R.T.: -0.011 min
Response: 615376
Conc: 17.26 ng/ml