

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060419\
 Data File : P0056851.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jun 2019 21:11
 Operator : SM/SJ
 Sample : K3173-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-SF-02-004-A

Manual Integrations
 APPROVED

Ankita
 6/7/2019 4:04:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 02:17:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.248	3.568	875790	713833	22.877m	21.645m
2)	SA Decachlor...	9.820	8.501	833777	542060	16.987m	15.202

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO060419\
Data File : PO056851.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2019 21:11
Operator : SM/SJ
Sample : K3173-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-SF-02-004-A


Manual Integrations
APPROVED

Ankita
6/7/2019 4:04:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 02:17:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

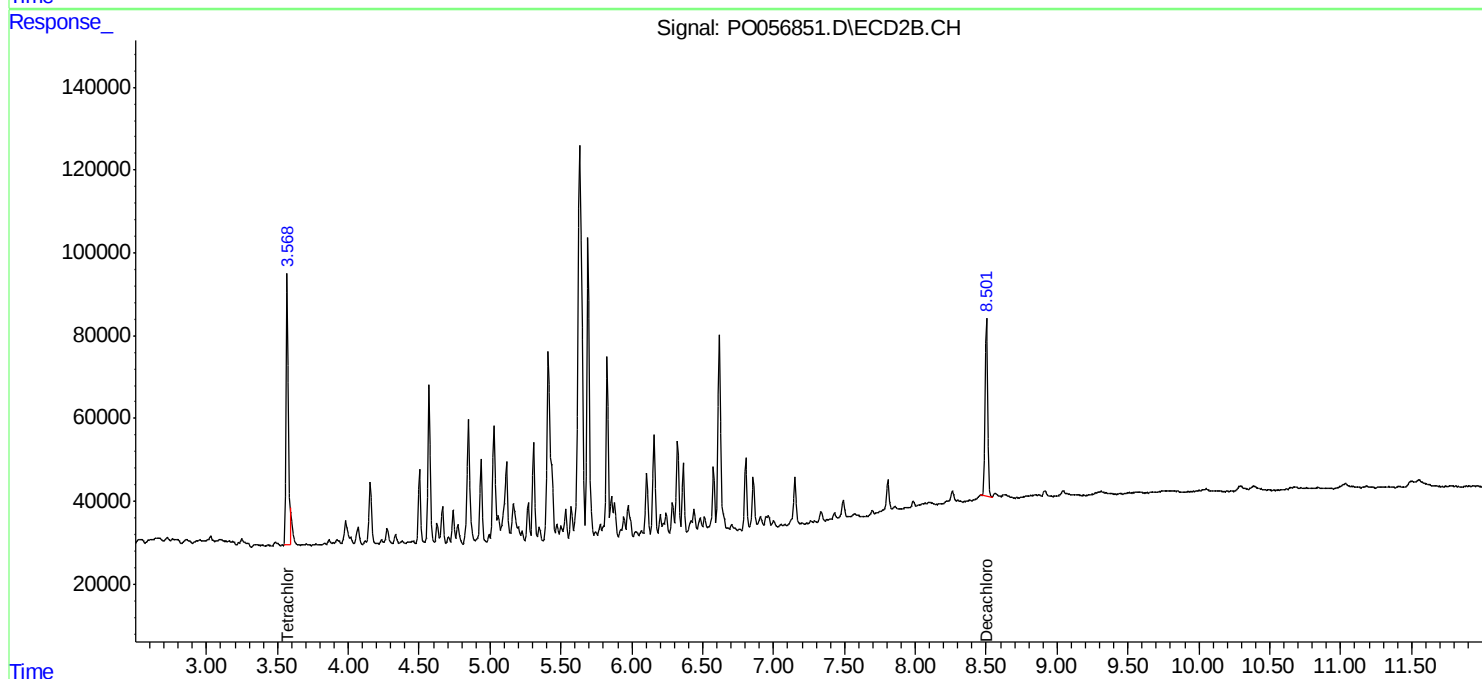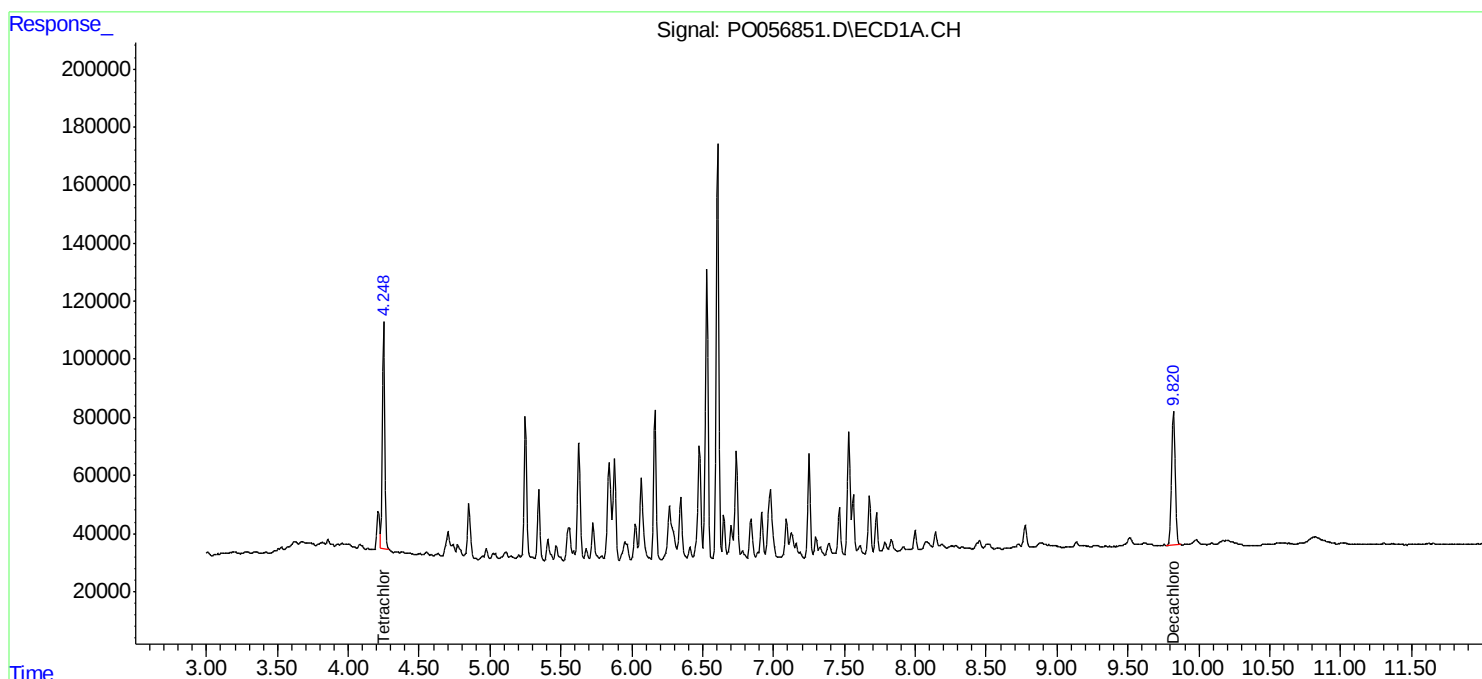

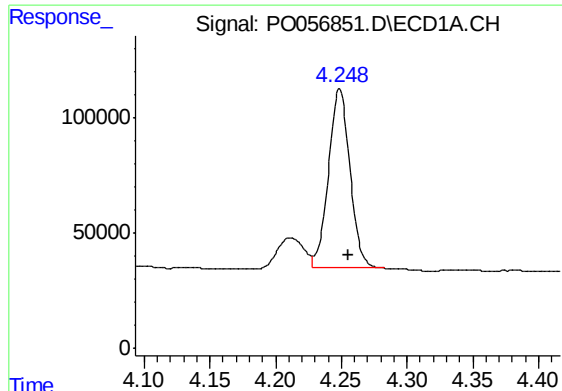


#1 Tetrachloro-m-xylene

R.T.: 4.248 min
Delta R.T.: -0.008 min
Response: 875790
Conc: 22.88 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-SF-02-004-A


Manual Integrations
APPROVED

Ankita
6/7/2019 4:04:02 PM

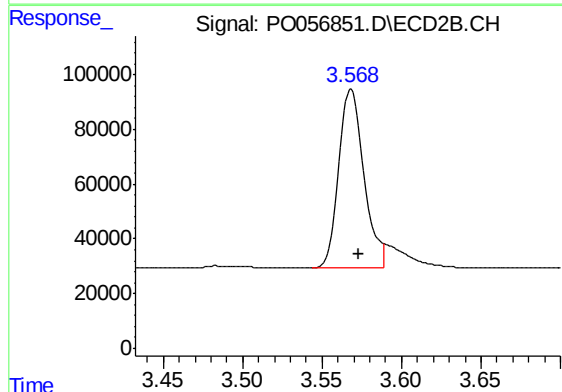


#1 Tetrachloro-m-xylene

R.T.: 3.568 min
Delta R.T.: -0.005 min
Response: 713833
Conc: 21.65 ng/ml m

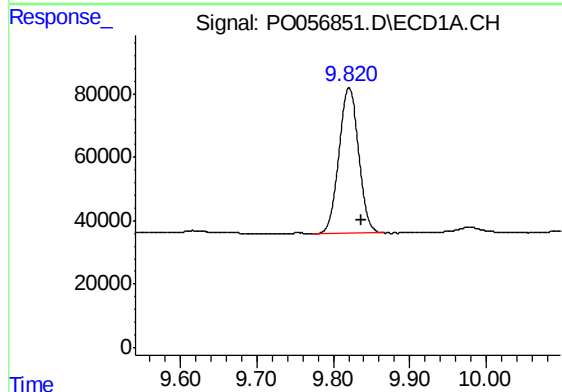

#2 Decachlorobiphenyl

R.T.: 9.820 min
Delta R.T.: -0.017 min
Response: 833777
Conc: 16.99 ng/ml m

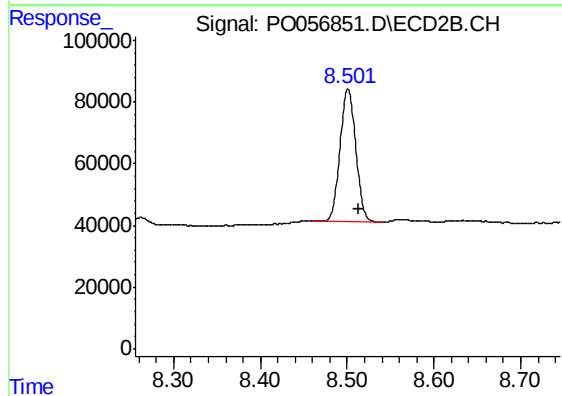

#2 Decachlorobiphenyl

R.T.: 8.501 min
Delta R.T.: -0.012 min
Response: 542060
Conc: 15.20 ng/ml