

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060419\
 Data File : P0056856.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jun 2019 22:35
 Operator : SM/SJ
 Sample : K3175-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-03-007-ABCD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 02:19:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.249	3.569	961124	866444	25.106	26.273
2) SA Decachlor...	9.823	8.502	756089	506471	15.404	14.204

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060419\
Data File : P0056856.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2019 22:35
Operator : SM/SJ
Sample : K3175-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 02:19:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

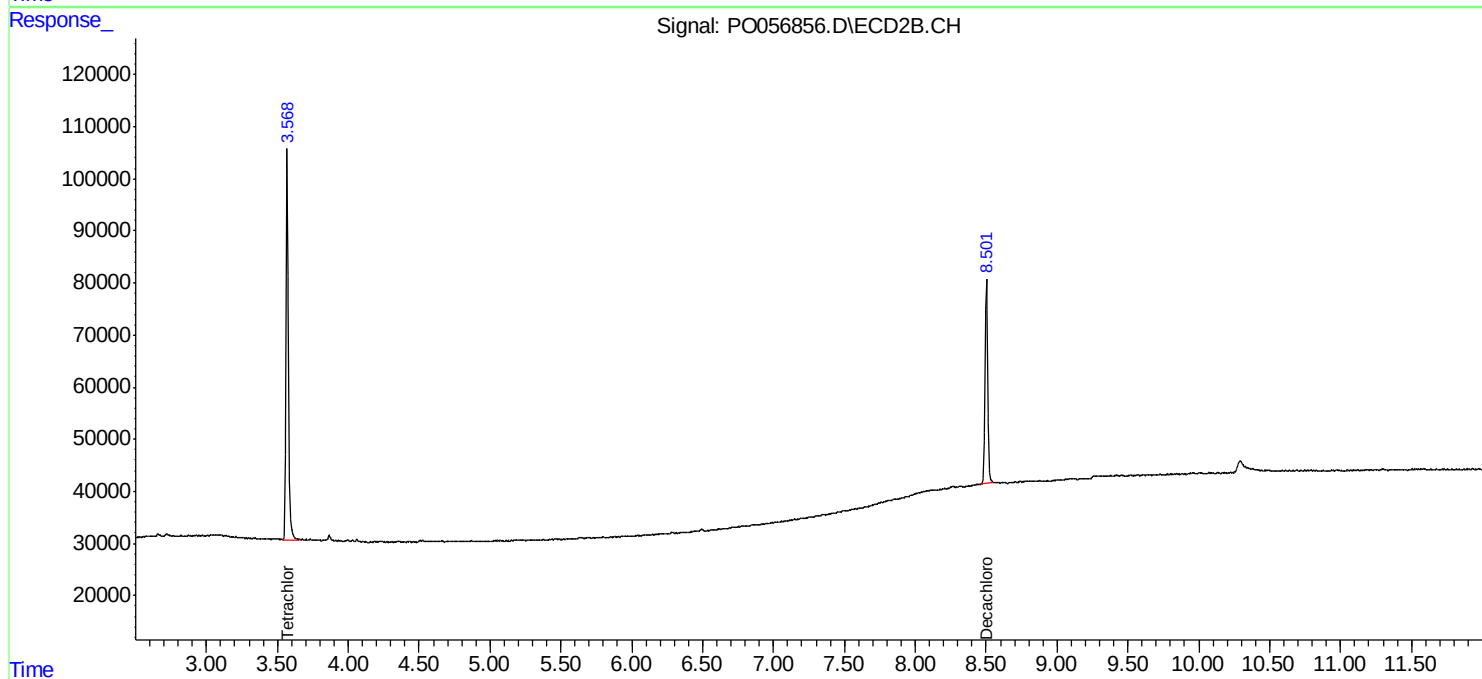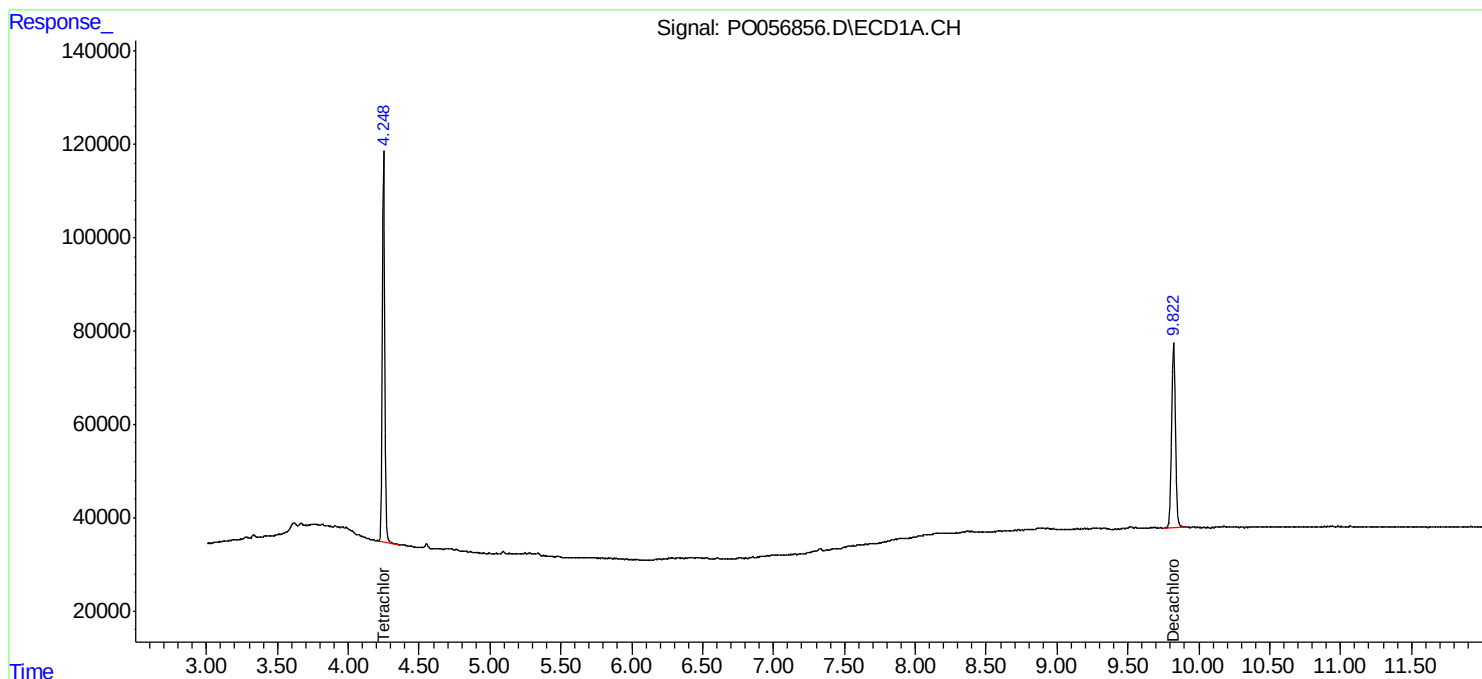


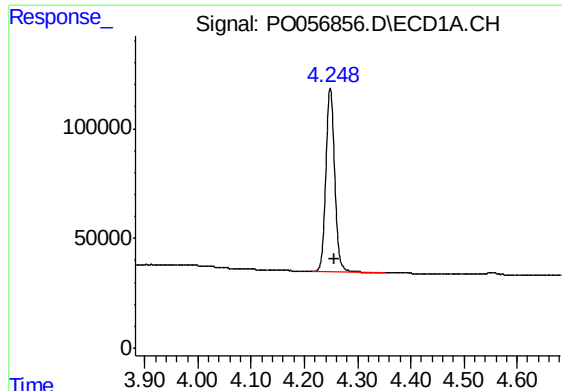

#1 Tetrachloro-m-xylene


R.T.: 4.249 min
Delta R.T.: -0.007 min
Response: 961124
Conc: 25.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCD

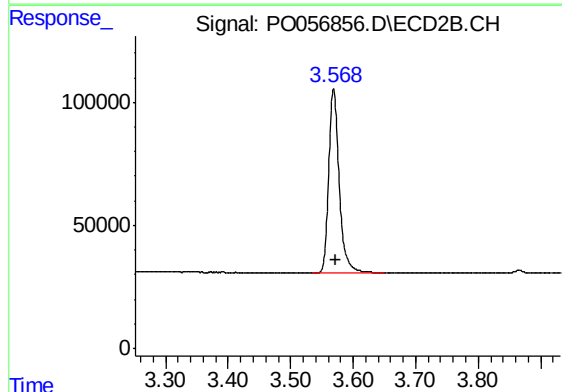


#1 Tetrachloro-m-xylene

R.T.: 3.569 min
Delta R.T.: -0.004 min
Response: 866444
Conc: 26.27 ng/ml

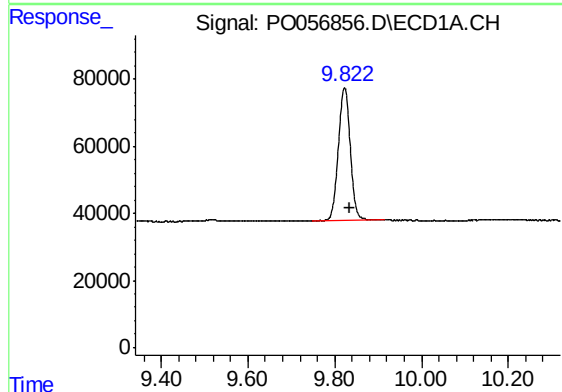

#2 Decachlorobiphenyl

R.T.: 9.823 min
Delta R.T.: -0.014 min
Response: 756089
Conc: 15.40 ng/ml

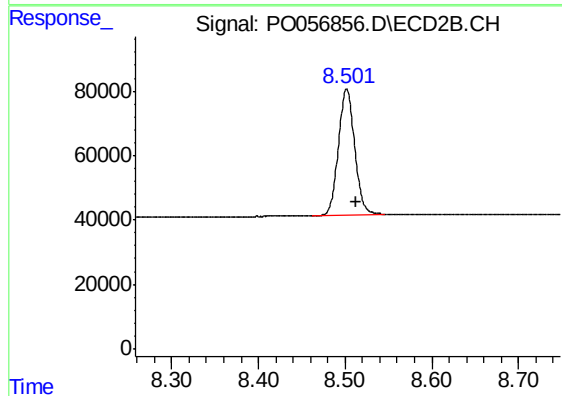

#2 Decachlorobiphenyl

R.T.: 8.502 min
Delta R.T.: -0.011 min
Response: 506471
Conc: 14.20 ng/ml