

Data Path : P:\HPCHEM1\ECD_0\Data\P0060518\
 Data File : P0045489.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jun 2018 22:21
 Operator : SM/UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:29:31 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0053018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 31 04:53:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.996	3.272	6126160	8748139	29.329	31.549
2) SA Decachlor...	9.273	7.991	8879049	9335930	38.660	33.125
Target Compounds						
7) L1 AR-1016-5	5.932	5.066	828526	307899	164.882	41.066 #
23) L5 AR-1248-3	5.932	5.066	828526	307899	95.560	19.148 #
24) L5 AR-1248-4	5.932	5.066	828526	307899	93.592	22.980 #
26) L6 AR-1254-1	0.000	5.066	0	307899	N.D.	16.615 #
32) L7 AR-1260-2	6.900	5.879	-119204	330161	N.D.	15.627 #
36) L8 AR-1262-1	0.000	5.879	0	330161	N.D.	17.442 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_0\Data\PO060518\
Data File : PO045489.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2018 22:21
Operator : SM/UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:29:31 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\PO053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

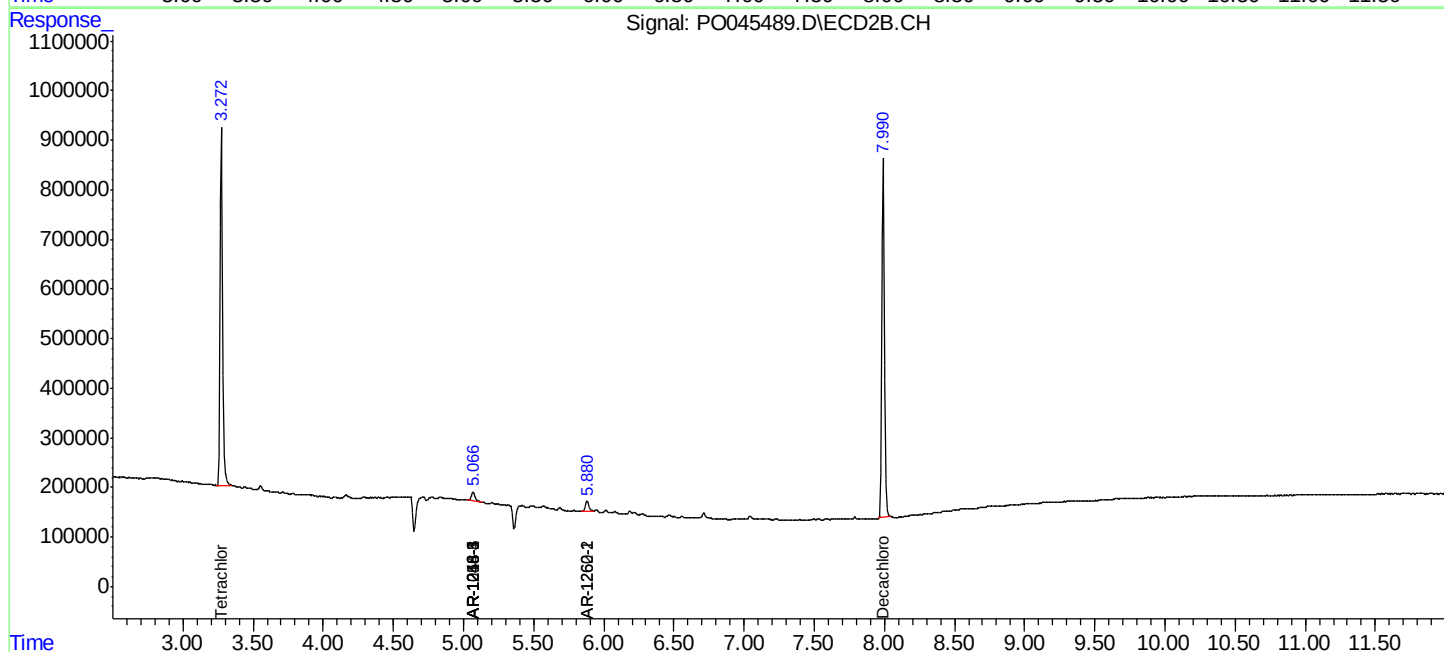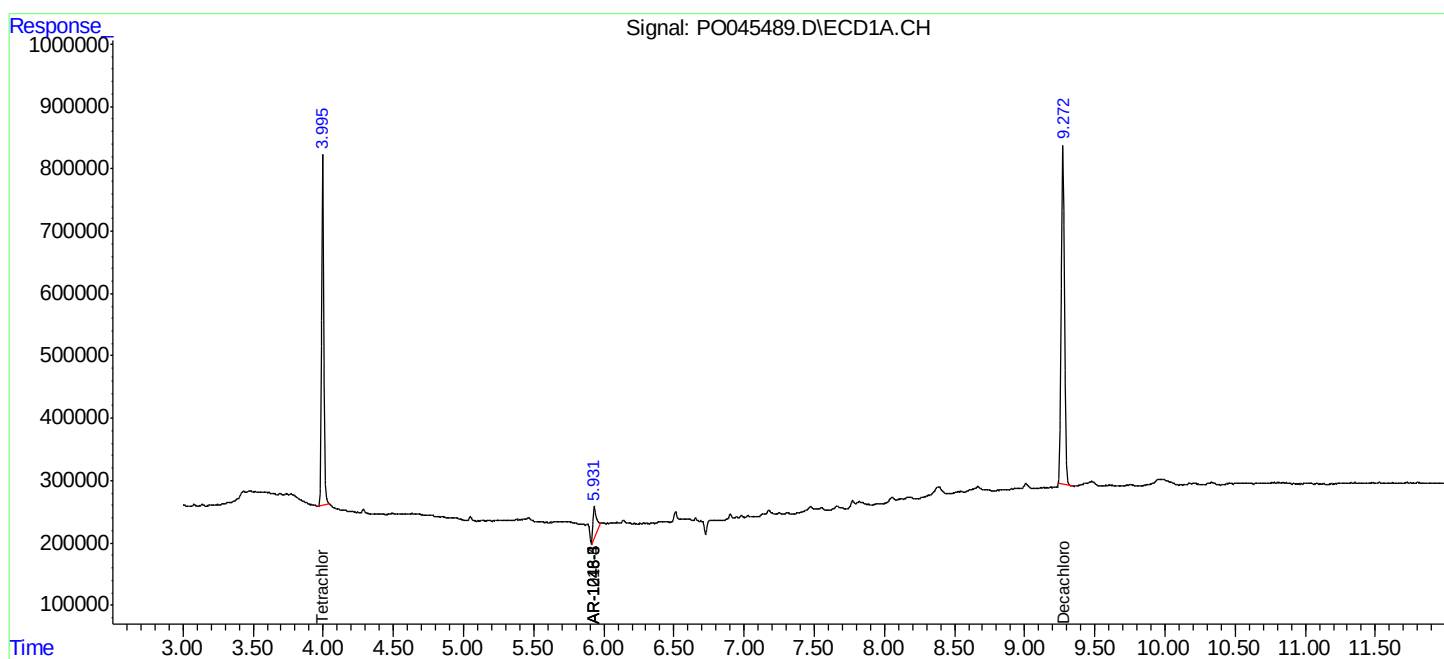


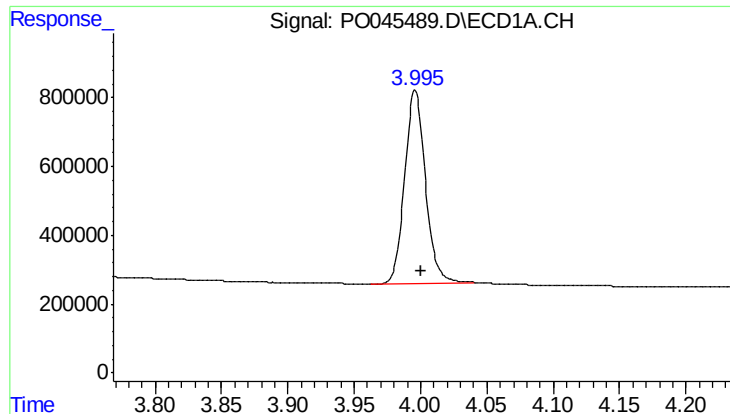

#1 Tetrachloro-m-xylene


R.T.: 3.996 min
Delta R.T.: -0.004 min
Response: 6126160
Conc: 29.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

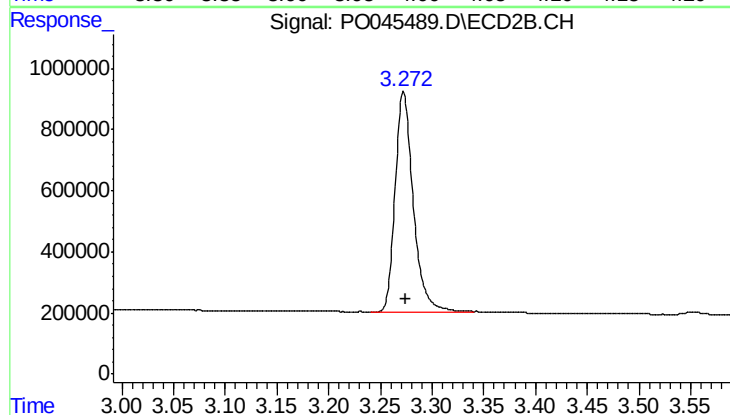


#1 Tetrachloro-m-xylene

R.T.: 3.272 min
Delta R.T.: -0.003 min
Response: 8748139
Conc: 31.55 ng/ml

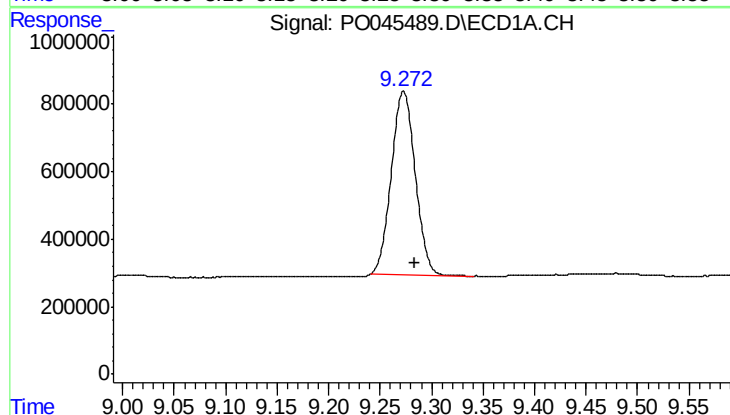


#2 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: -0.011 min
Response: 8879049
Conc: 38.66 ng/ml

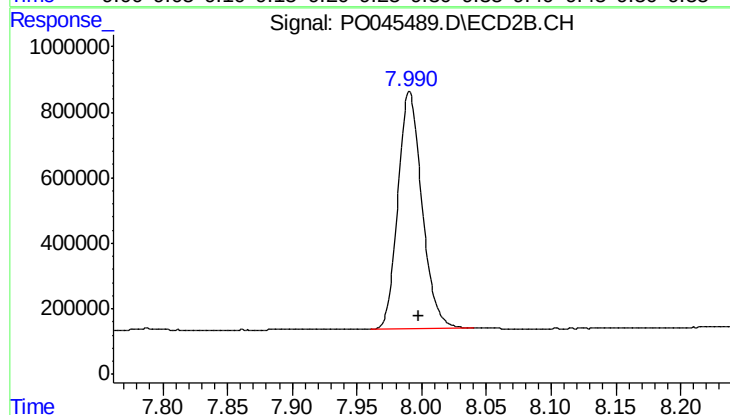

#2 Decachlorobiphenyl


R.T.: 7.991 min
Delta R.T.: -0.007 min
Response: 9335930
Conc: 33.12 ng/ml

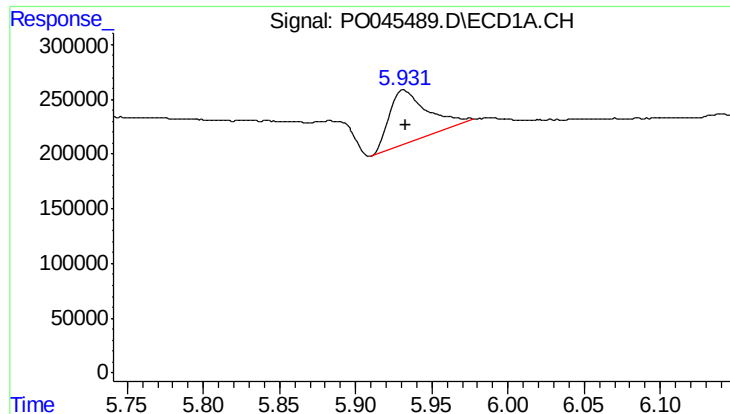

#7 AR-1016-5


R.T.: 5.932 min
Delta R.T.: -0.001 min
Response: 828526
Conc: 164.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

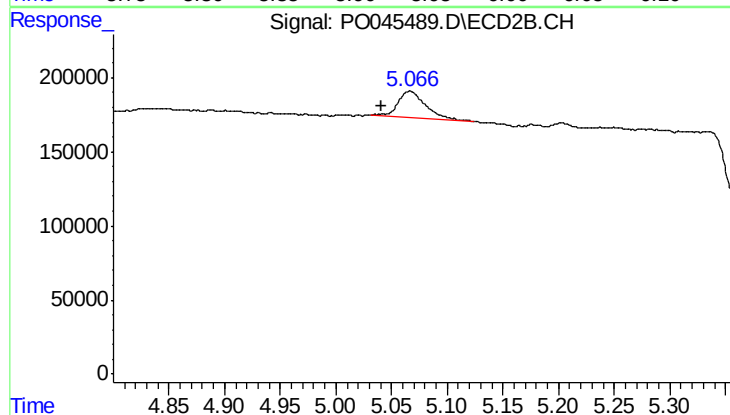


#7 AR-1016-5

R.T.: 5.066 min
Delta R.T.: 0.025 min
Response: 307899
Conc: 41.07 ng/ml

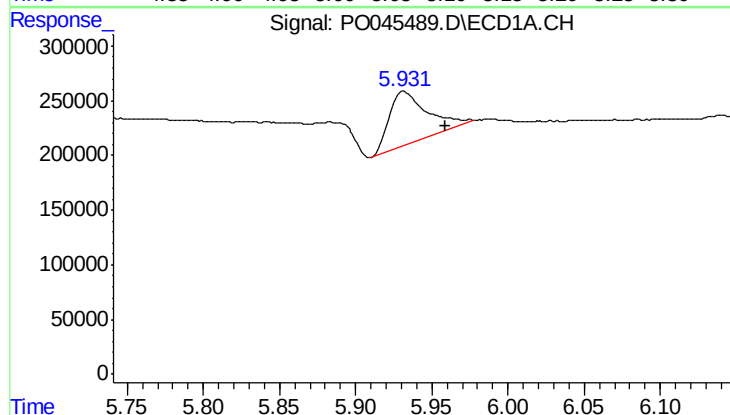


#23 AR-1248-3

R.T.: 5.932 min
Delta R.T.: -0.028 min
Response: 828526
Conc: 95.56 ng/ml

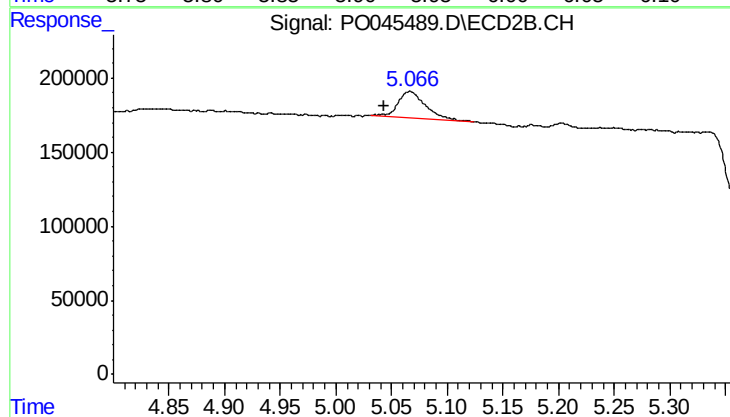

#23 AR-1248-3


R.T.: 5.066 min
Delta R.T.: 0.023 min
Response: 307899
Conc: 19.15 ng/ml

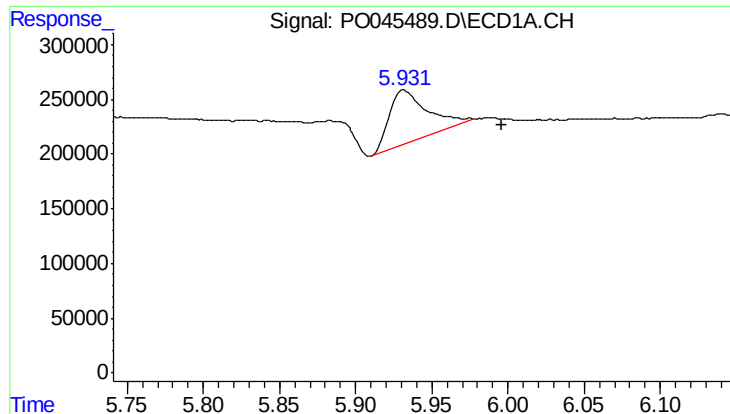

#24 AR-1248-4


R.T.: 5.932 min
Delta R.T.: -0.065 min
Response: 828526
Conc: 93.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

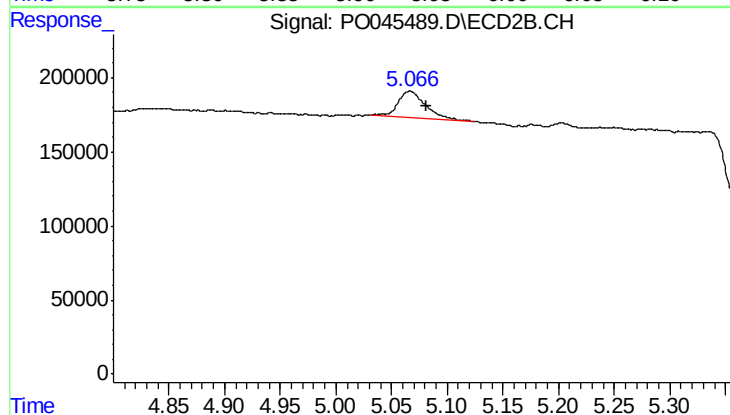


#24 AR-1248-4

R.T.: 5.066 min
Delta R.T.: -0.015 min
Response: 307899
Conc: 22.98 ng/ml

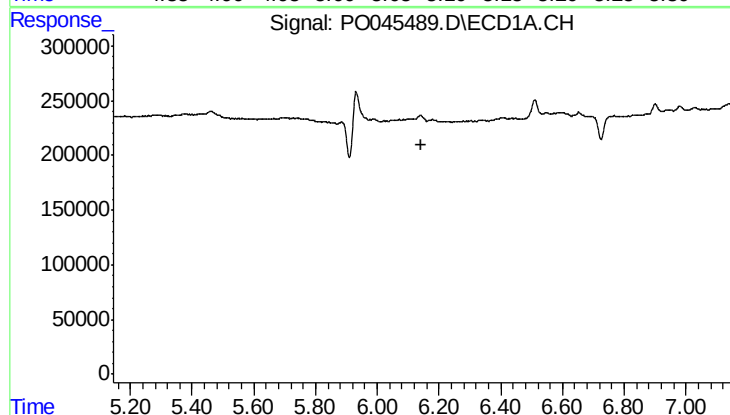


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.145 min
Response: 0
Conc: N.D.

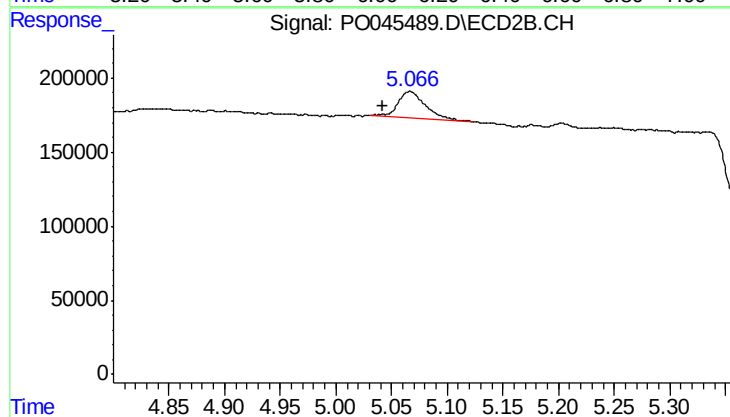

#26 AR-1254-1


R.T.: 5.066 min
Delta R.T.: 0.025 min
Response: 307899
Conc: 16.62 ng/ml

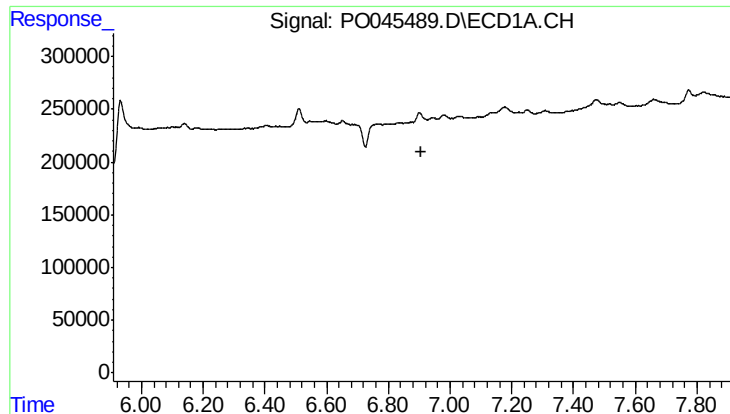

#32 AR-1260-2


R.T.: 6.900 min
Delta R.T.: -0.009 min
Response: -119204
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

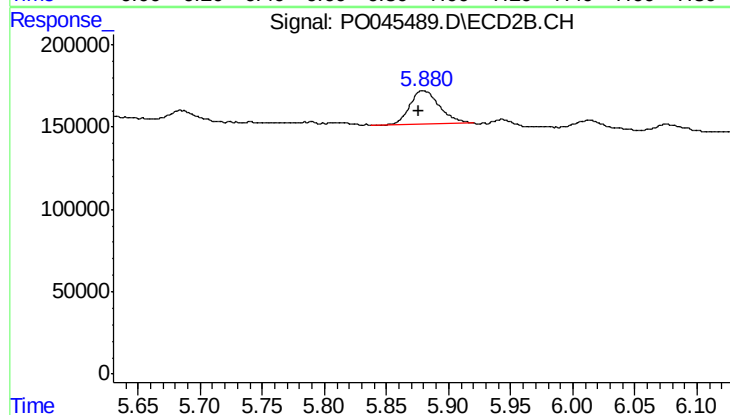


#32 AR-1260-2

R.T.: 5.879 min
Delta R.T.: 0.003 min
Response: 330161
Conc: 15.63 ng/ml

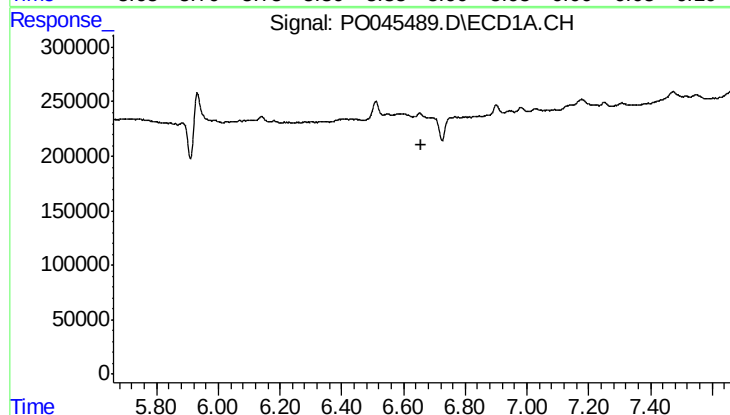

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 6.660 min
Response: 0
Conc: N.D.

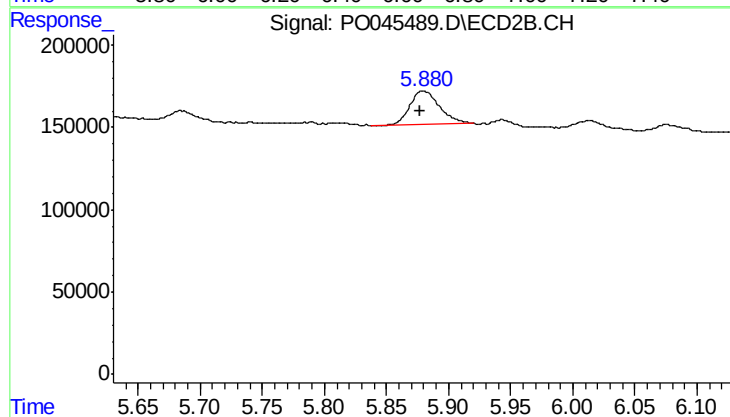

#36 AR-1262-1

R.T.: 5.879 min
Delta R.T.: 0.002 min
Response: 330161
Conc: 17.44 ng/ml