

Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060518\
 Data File : P0045467.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jun 2018 16:32
 Operator : SM/UA
 Sample : J3237-03RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AG-BASELINEWATERRE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 03:21:02 2018
 Quant Method : Y:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 31 04:53:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.999	3.278	2052360	2301868	9.826m	8.301m
2) SA Decachlor...	9.295	8.012	747943	453784	3.257	1.610m#

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060518\
Data File : P0045467.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2018 16:32
Operator : SM/UA
Sample : J3237-03RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AG-BASELINEWATERRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 03:21:02 2018
Quant Method : Y:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

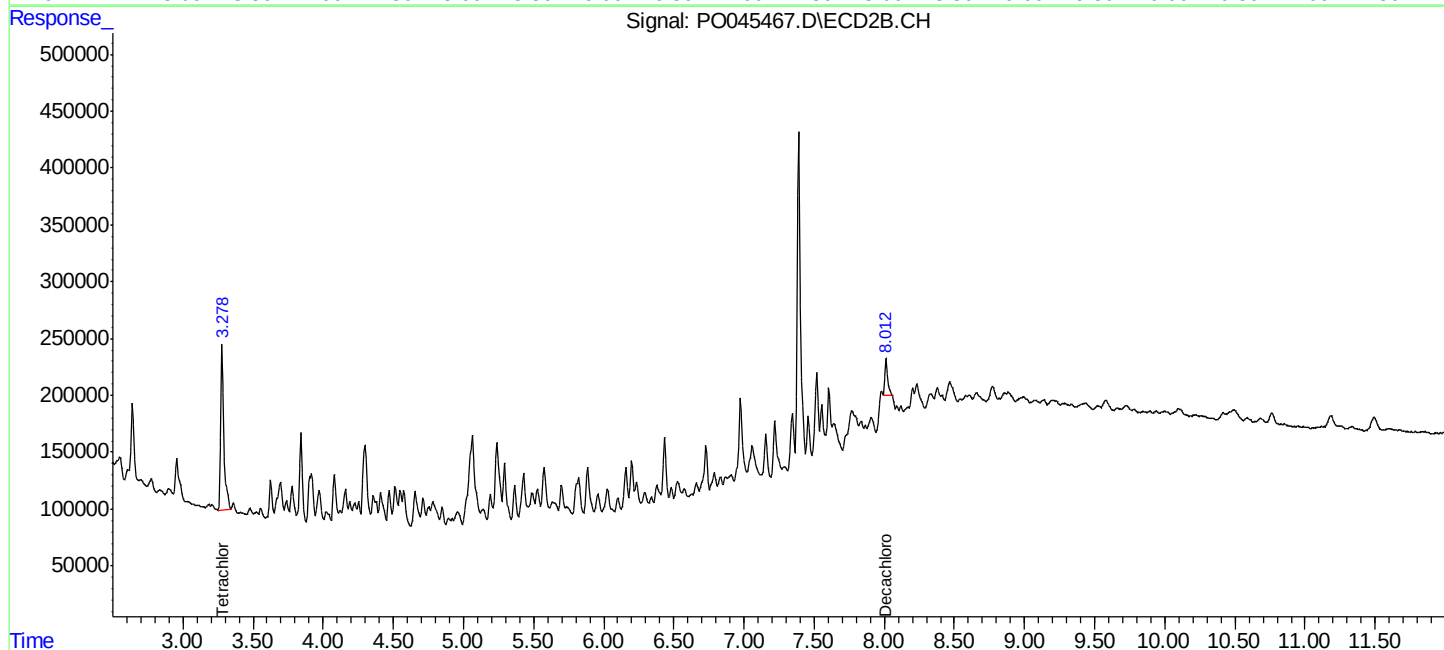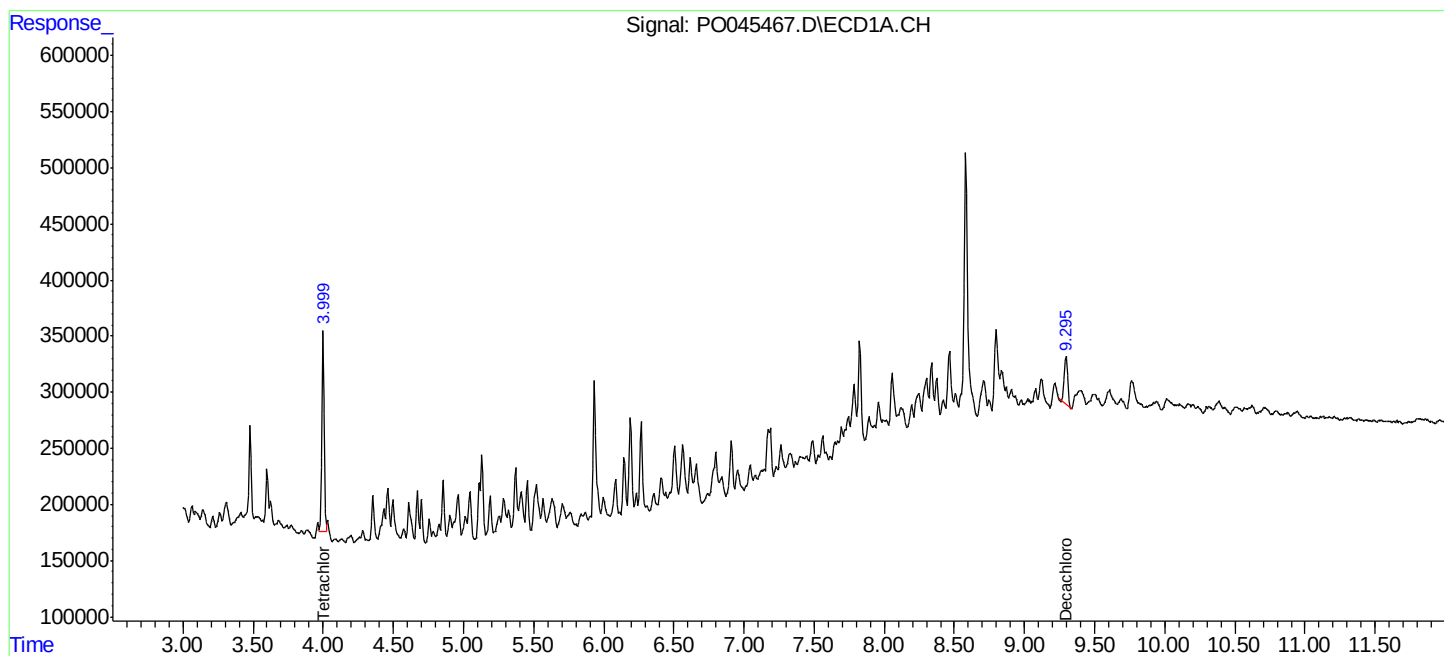


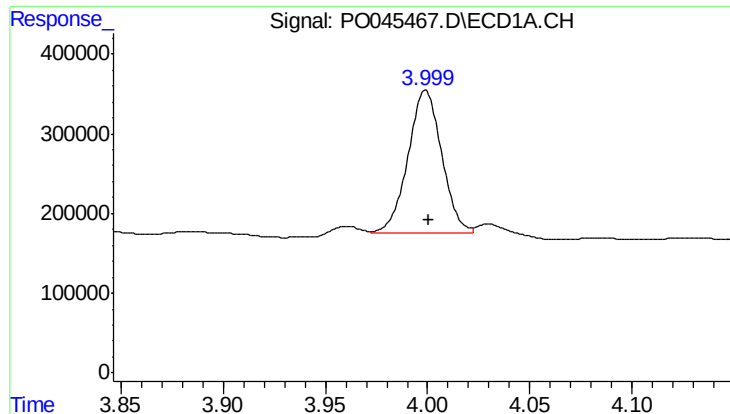

#1 Tetrachloro-m-xylene


R.T.: 3.999 min
Delta R.T.: -0.002 min
Response: 2052360
Conc: 9.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
AG-BASELINEWATERRE

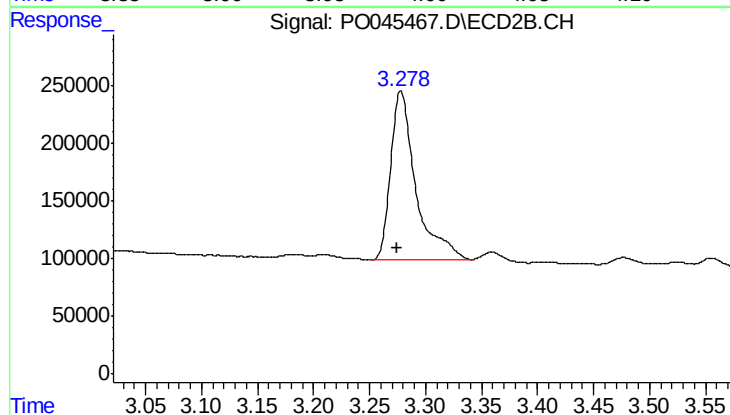


#1 Tetrachloro-m-xylene

R.T.: 3.278 min
Delta R.T.: 0.003 min
Response: 2301868
Conc: 8.30 ng/ml m

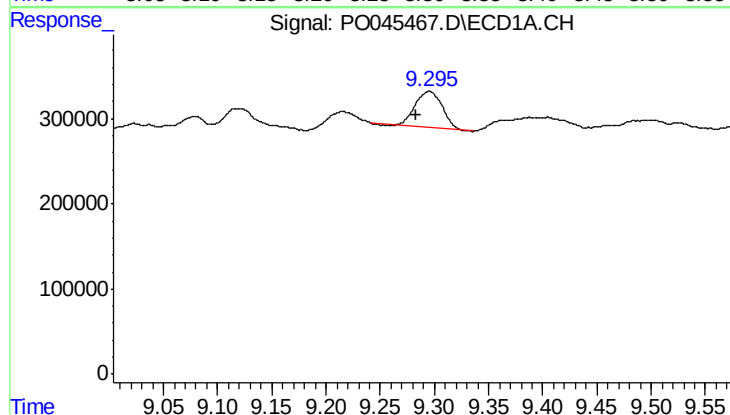

#2 Decachlorobiphenyl

R.T.: 9.295 min
Delta R.T.: 0.012 min
Response: 747943
Conc: 3.26 ng/ml

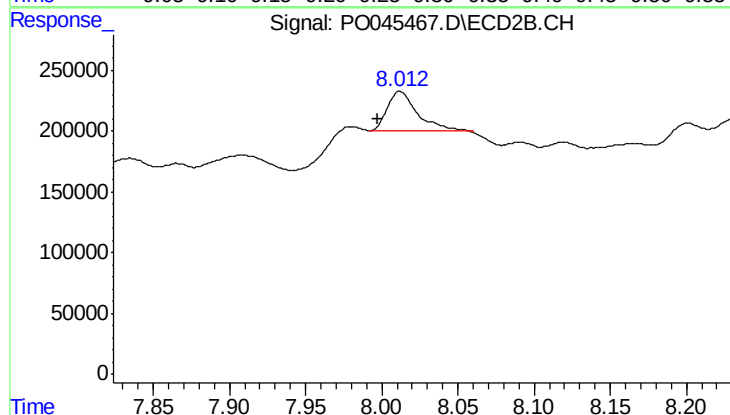

#2 Decachlorobiphenyl

R.T.: 8.012 min
Delta R.T.: 0.014 min
Response: 453784
Conc: 1.61 ng/ml m