

Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060518\
 Data File : P0045484.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jun 2018 21:03
 Operator : SM/UA
 Sample : J2677-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-03-053118

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 07:32:28 2018
 Quant Method : Y:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 31 04:53:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

	System Monitoring Compounds						
1)	SA Tetrachlo...	3.996	3.272	5153304	6781819	24.672	24.457
2)	SA Decachlor...	9.274	7.991	3417479	3227658	14.880	11.452m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060518\
Data File : P0045484.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2018 21:03
Operator : SM/UA
Sample : J2677-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OK-03-053118

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 07:32:28 2018
Quant Method : Y:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

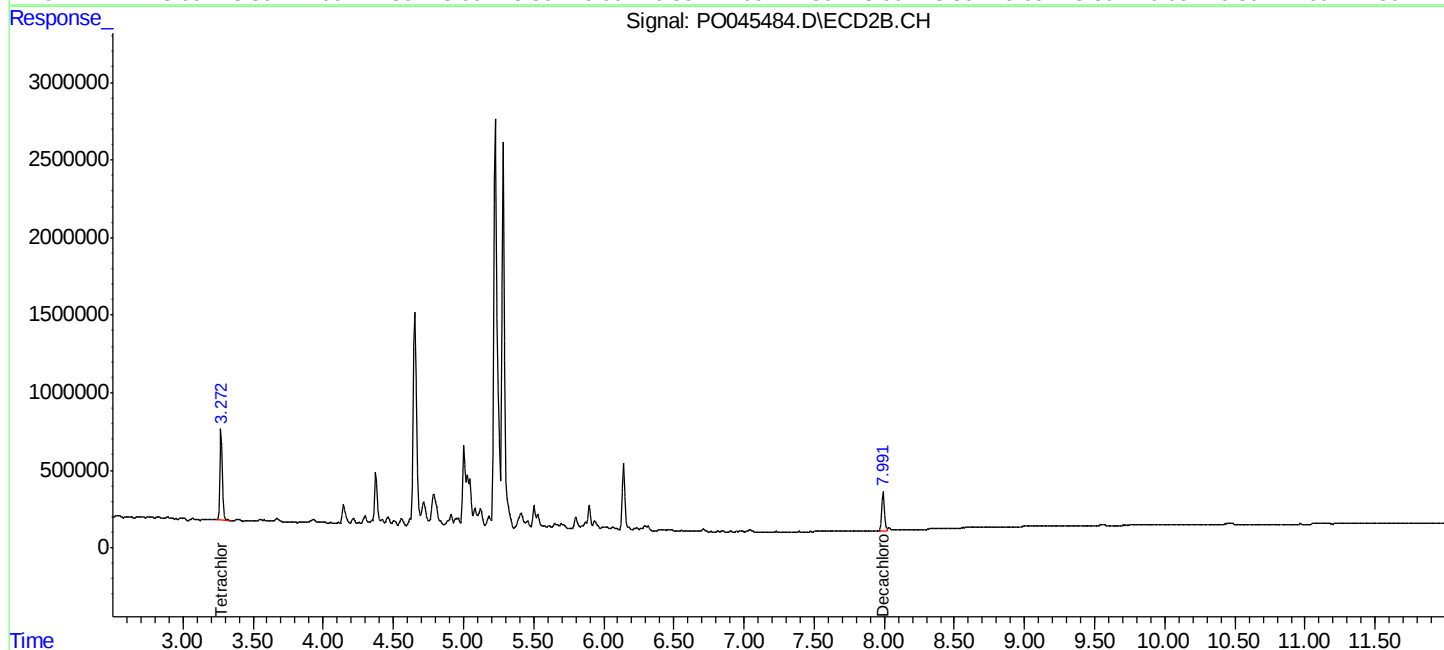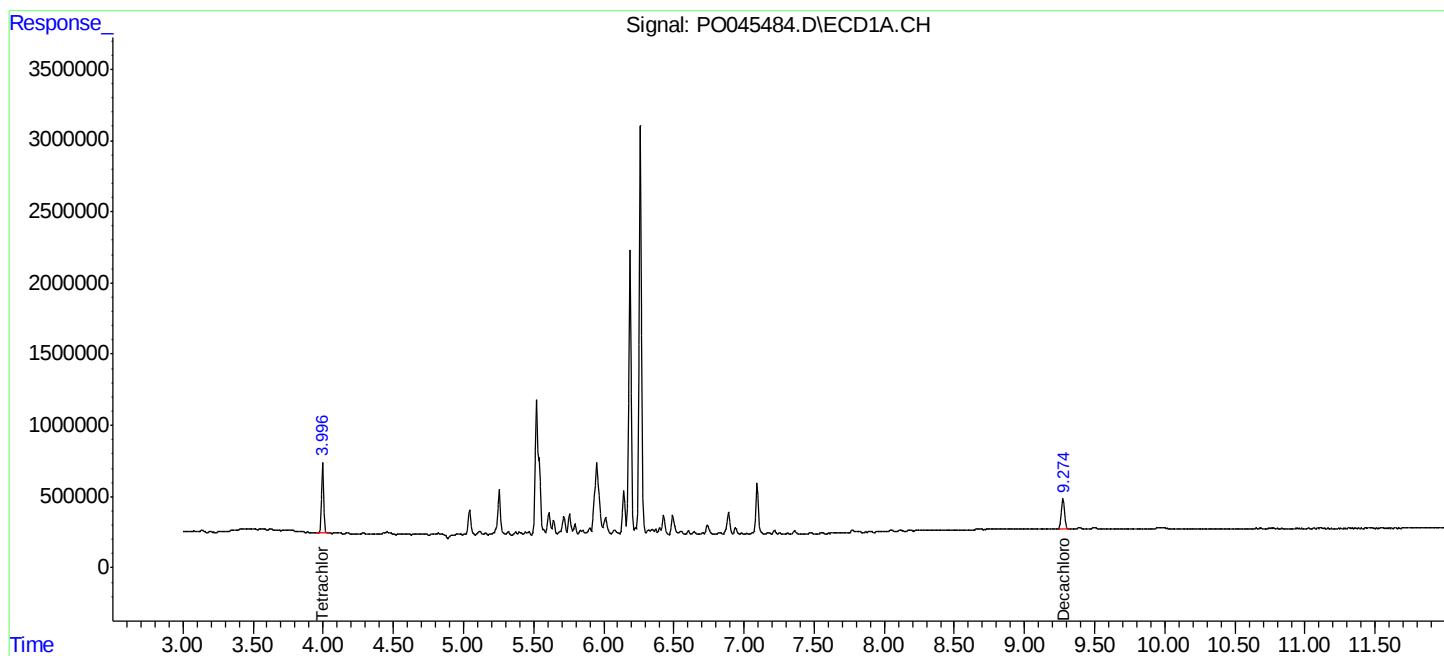


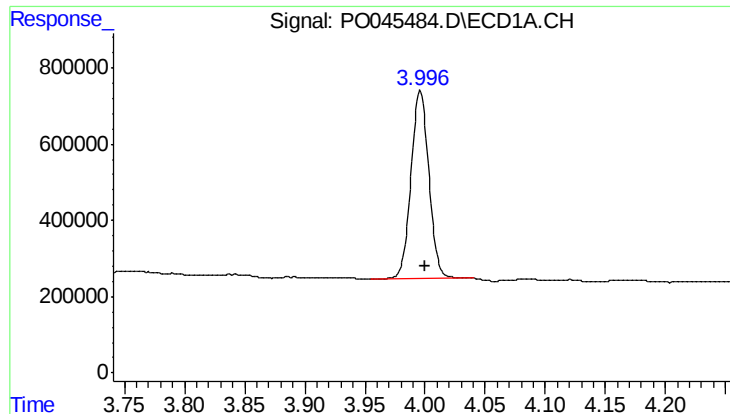

#1 Tetrachloro-m-xylene


R.T.: 3.996 min
Delta R.T.: -0.004 min
Response: 5153304
Conc: 24.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-03-053118

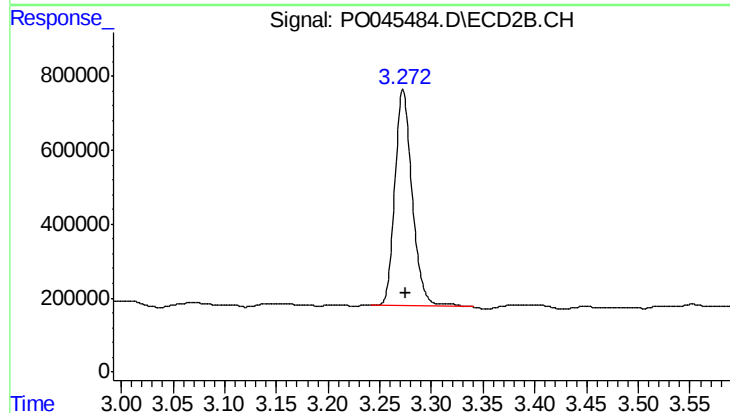


#1 Tetrachloro-m-xylene

R.T.: 3.272 min
Delta R.T.: -0.003 min
Response: 6781819
Conc: 24.46 ng/ml

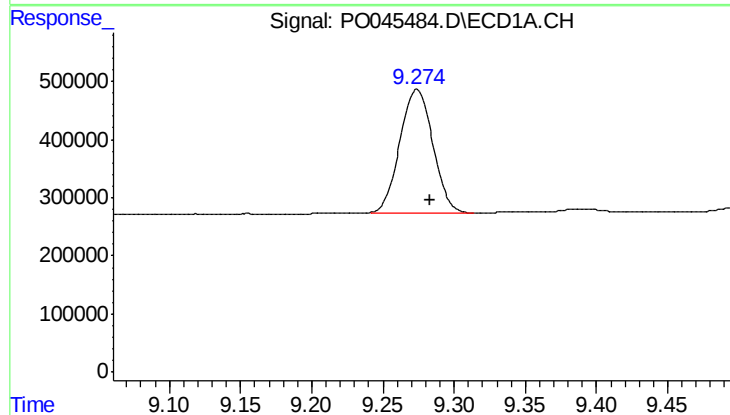

#2 Decachlorobiphenyl

R.T.: 9.274 min
Delta R.T.: -0.009 min
Response: 3417479
Conc: 14.88 ng/ml

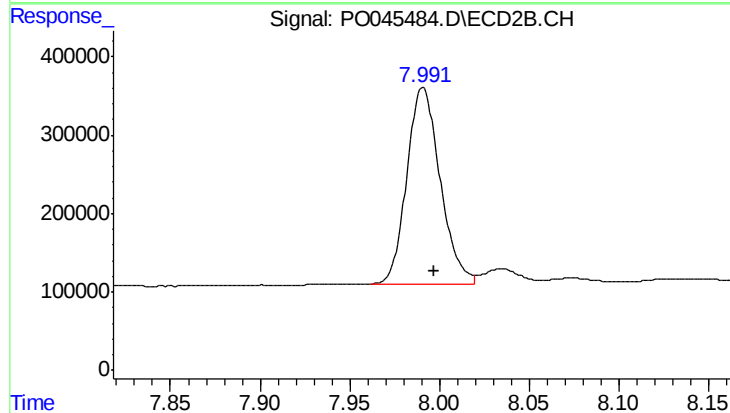

#2 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: -0.007 min
Response: 3227658
Conc: 11.45 ng/ml m