

Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060518\
Data File : P0045495.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2018 23:54
Operator : SM/UA
Sample : J3228-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-028

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 07:51:27 2018
Quant Method : Y:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.996	3.272	5329855	7354908	25.517	26.524
2) SA Decachlor...	9.273	7.991	3814568	4226519	16.609m	14.996

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060518\
Data File : P0045495.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2018 23:54
Operator : SM/UA
Sample : J3228-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-028

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 07:51:27 2018
Quant Method : Y:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

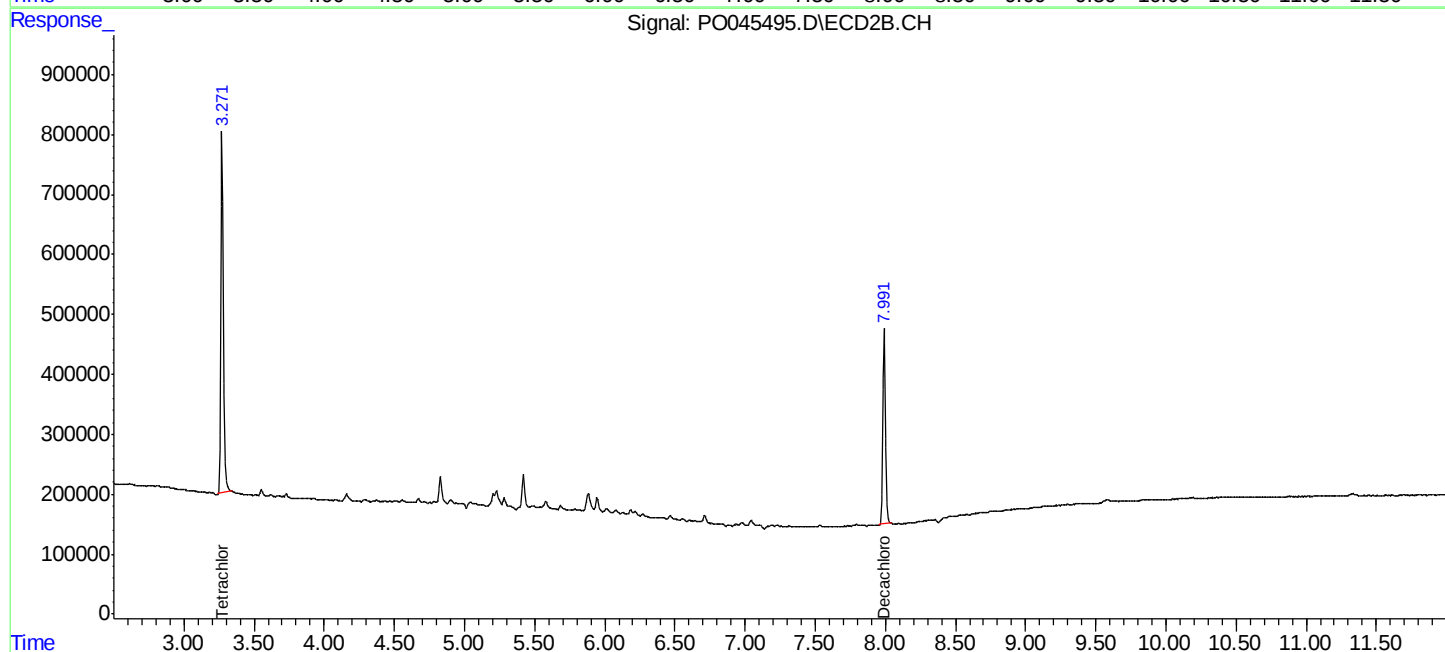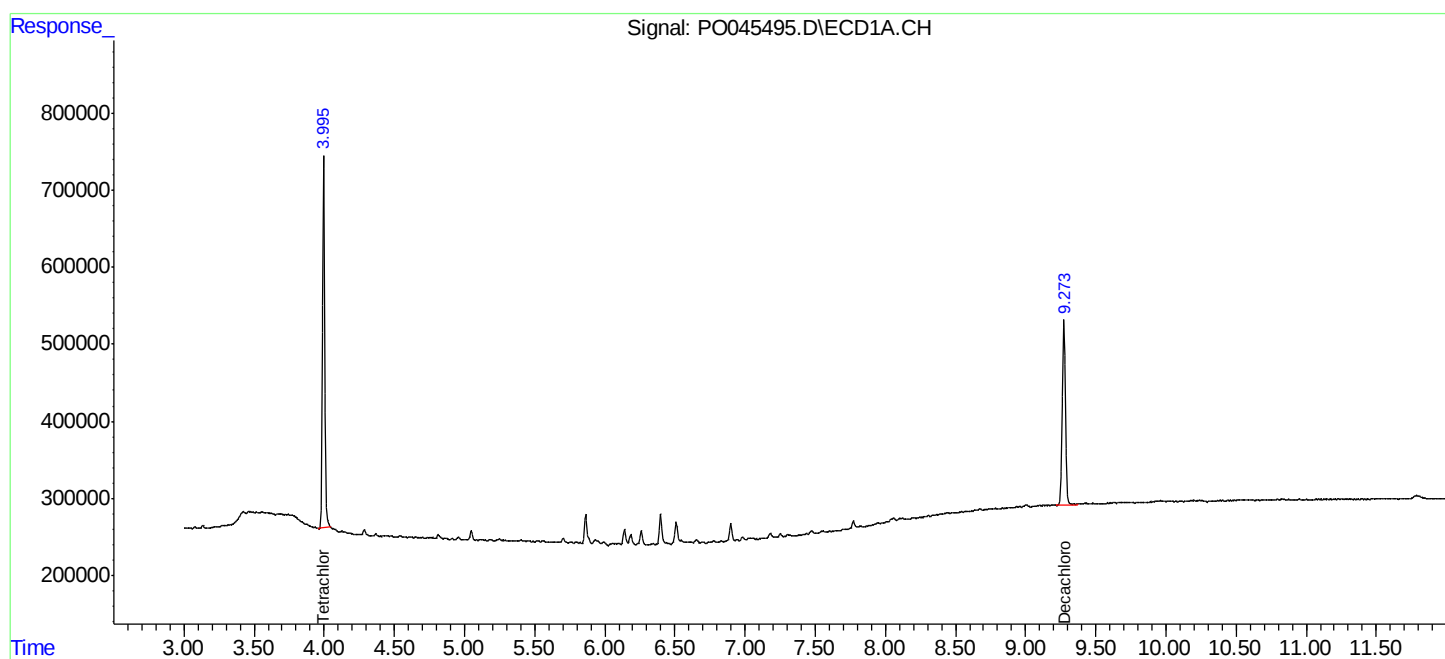


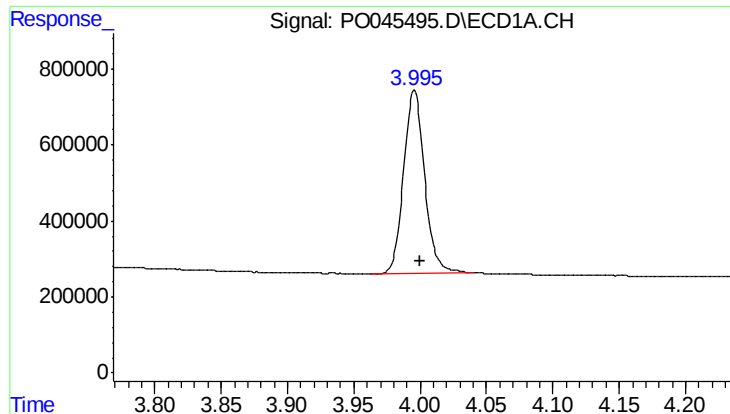

#1 Tetrachloro-m-xylene


R.T.: 3.996 min
Delta R.T.: -0.005 min
Response: 5329855
Conc: 25.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-028

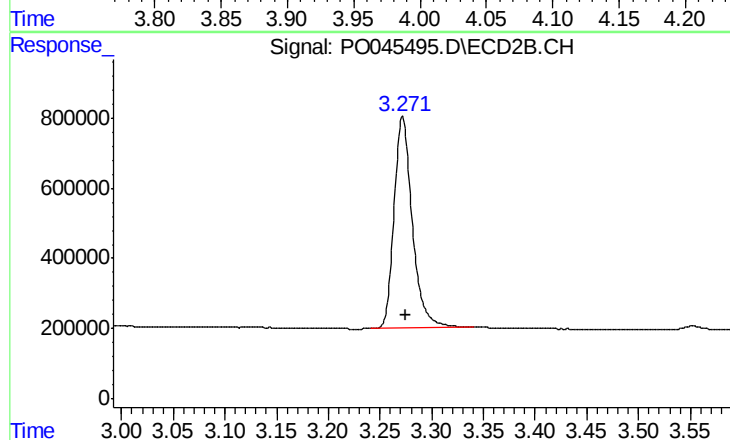


#1 Tetrachloro-m-xylene

R.T.: 3.272 min
Delta R.T.: -0.003 min
Response: 7354908
Conc: 26.52 ng/ml

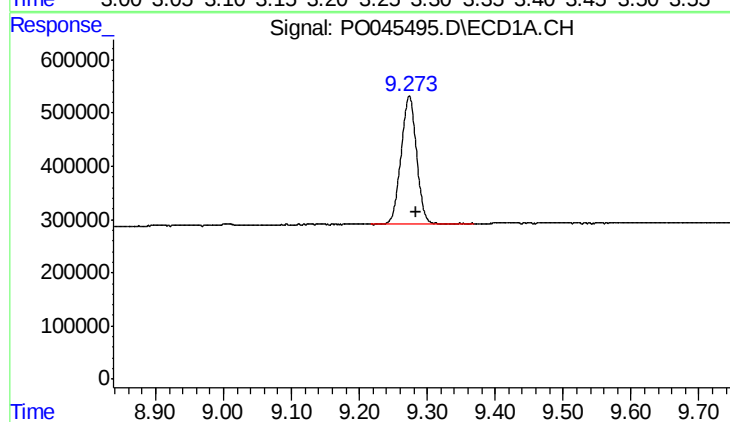

#2 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: -0.010 min
Response: 3814568
Conc: 16.61 ng/ml m

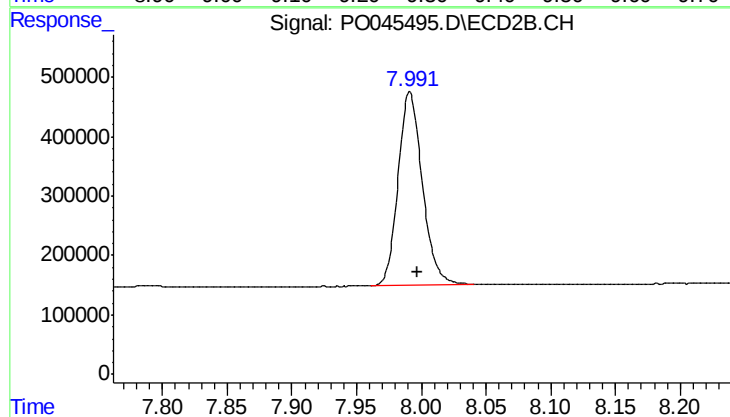

#2 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: -0.006 min
Response: 4226519
Conc: 15.00 ng/ml