

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060519\
 Data File : P0056894.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jun 2019 22:56
 Operator : SM/SJ
 Sample : K2640-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB120325BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 04:19:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.247	3.566	828224	634996	21.634	19.255
2)	SA Decachlor...	9.820	8.499	1001322	473331	20.400	13.275 #
Target Compounds							
4)	L1 AR-1016-2	0.000	4.729	0	20730	N.D.	11.506 #
12)	L3 AR-1232-2	0.000	4.729	0	20730	N.D.	21.330 #
17)	L4 AR-1242-2	0.000	4.729	0	20730	N.D.	11.527 #
28)	L6 AR-1254-3	0.000	6.013	0	32022	N.D.	8.747 #
34)	L7 AR-1260-4	0.000	6.960	0	115435	N.D.	62.028 #
39)	L8 AR-1262-4	0.000	7.542	0	71630	N.D.	13.747 #
42)	L9 AR-1268-2	0.000	7.542	0	71630	N.D.	10.258 #
45)	L9 AR-1268-5	0.000	8.246	0	125546	N.D.	7.254 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO060519\
Data File : PO056894.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jun 2019 22:56
Operator : SM/SJ
Sample : K2640-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB120325BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 04:19:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

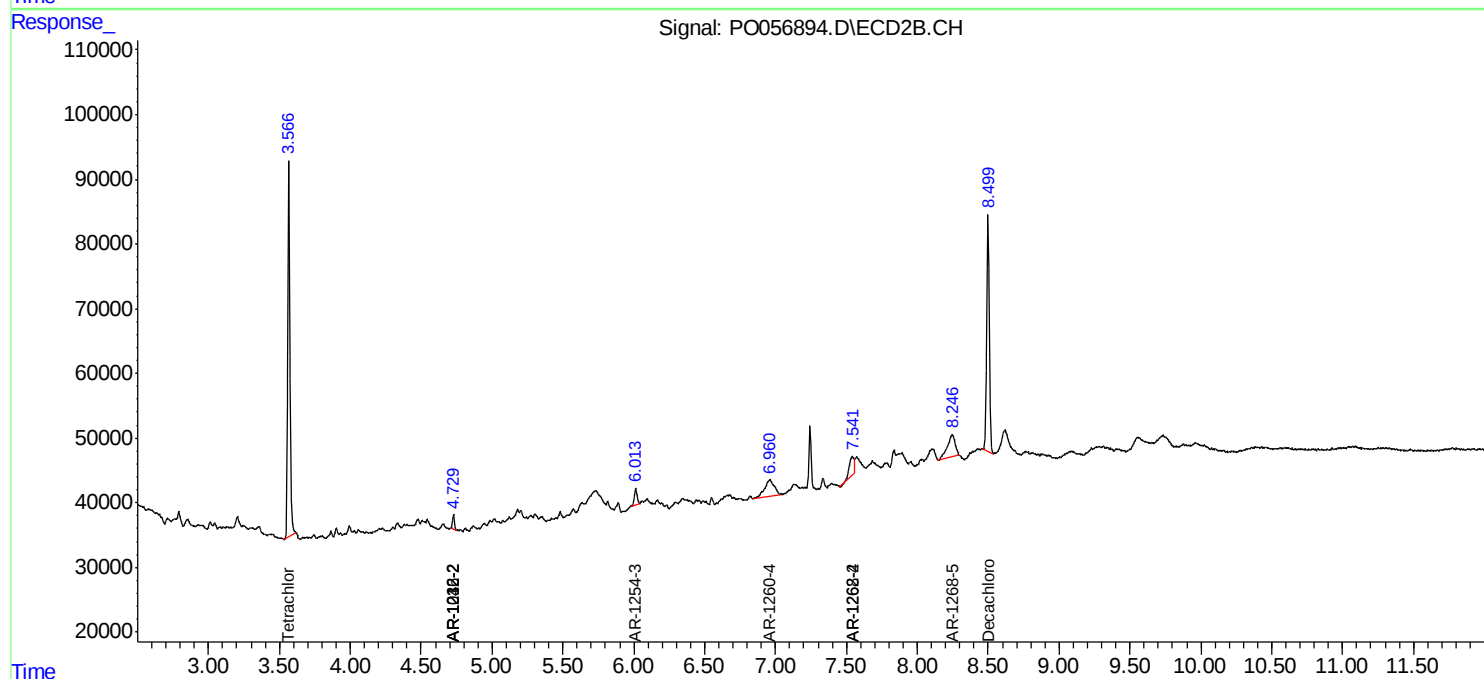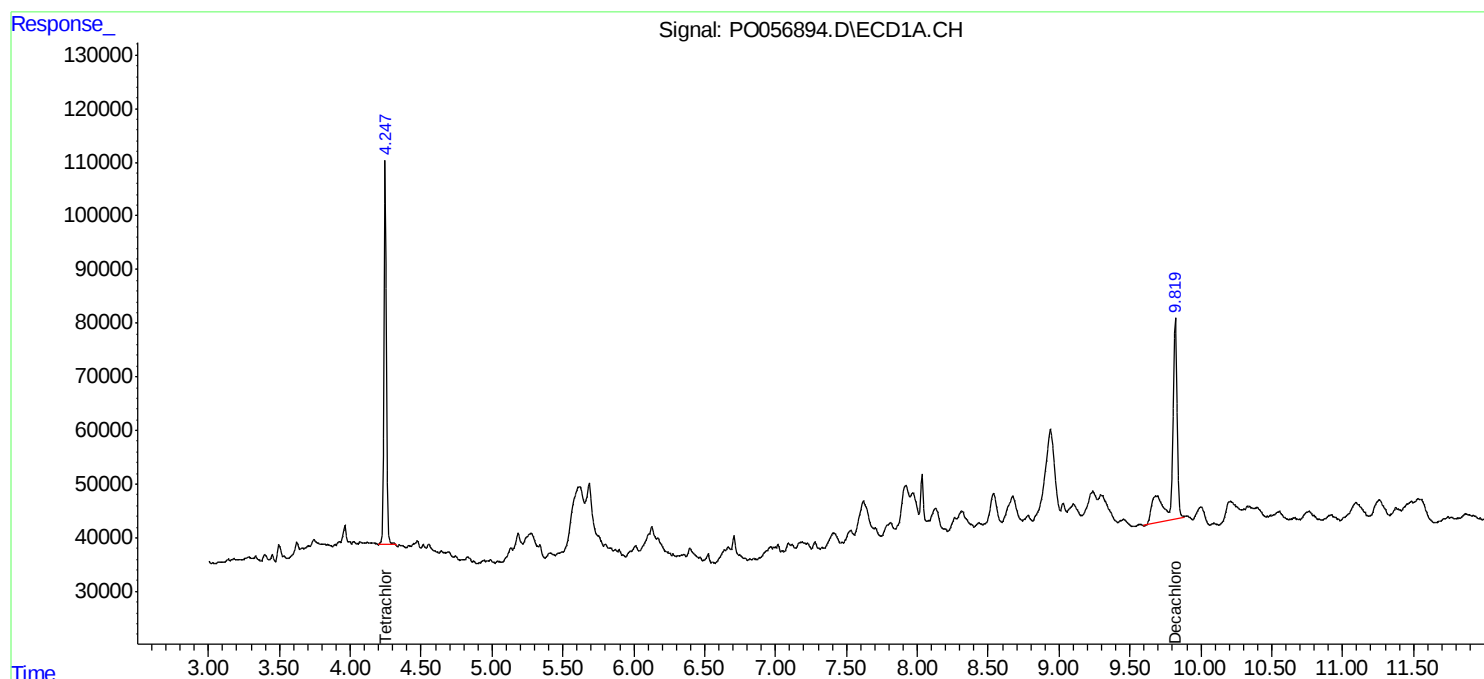


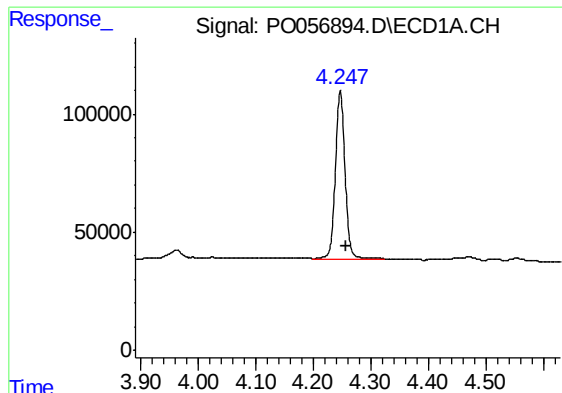

#1 Tetrachloro-m-xylene


R.T.: 4.247 min
Delta R.T.: -0.009 min
Response: 828224
Conc: 21.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB120325BL

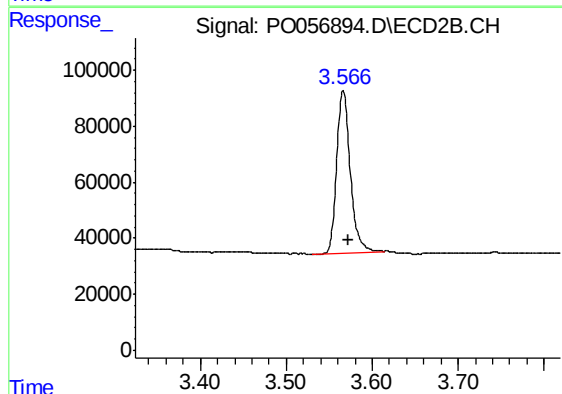


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: -0.007 min
Response: 634996
Conc: 19.25 ng/ml

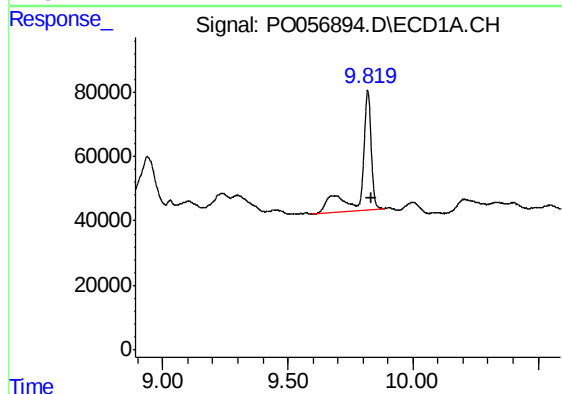


#2 Decachlorobiphenyl

R.T.: 9.820 min
Delta R.T.: -0.017 min
Response: 1001322
Conc: 20.40 ng/ml

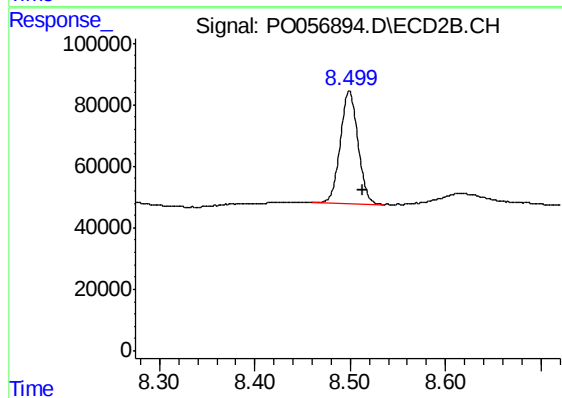

#2 Decachlorobiphenyl


R.T.: 8.499 min
Delta R.T.: -0.014 min
Response: 473331
Conc: 13.27 ng/ml

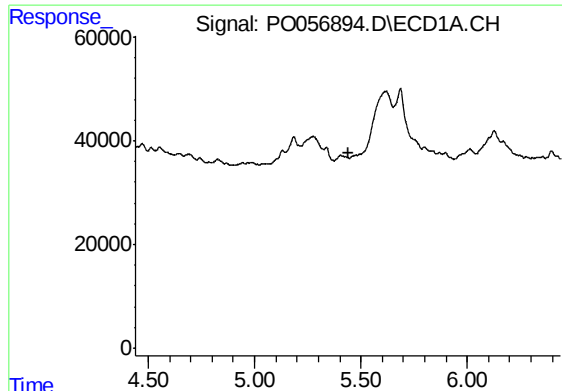

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T.: 5.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
PB120325BL

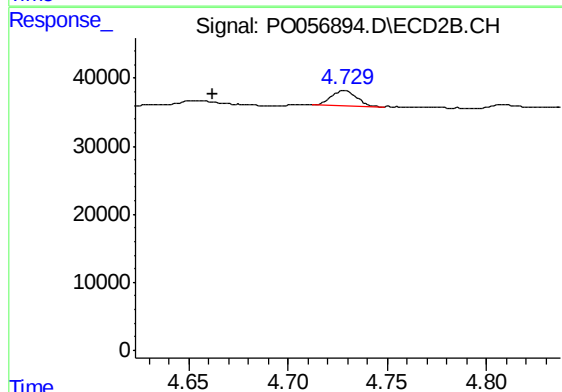


#4 AR-1016-2

R.T.: 4.729 min
Delta R.T.: 0.067 min
Response: 20730
Conc: 11.51 ng/ml

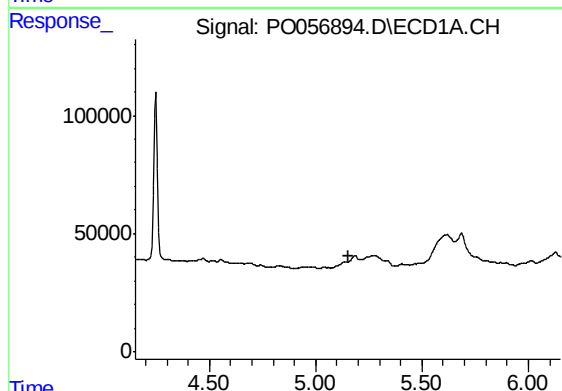


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T.: 5.152 min
Response: 0
Conc: N.D.

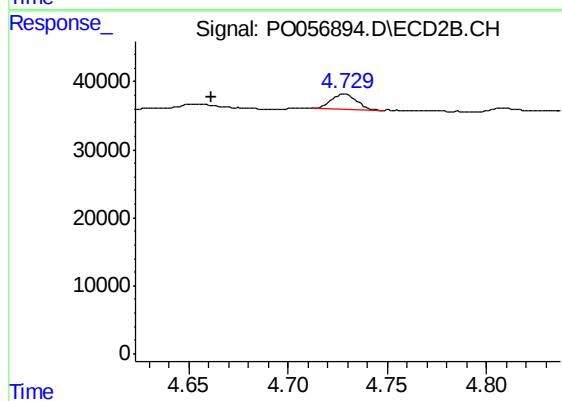

#12 AR-1232-2


R.T.: 4.729 min
Delta R.T.: 0.067 min
Response: 20730
Conc: 21.33 ng/ml

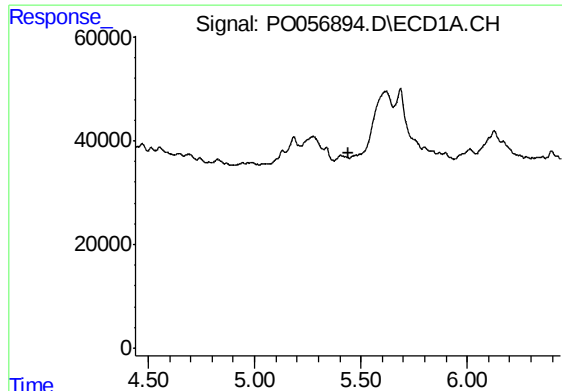

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T. : 5.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
PB120325BL

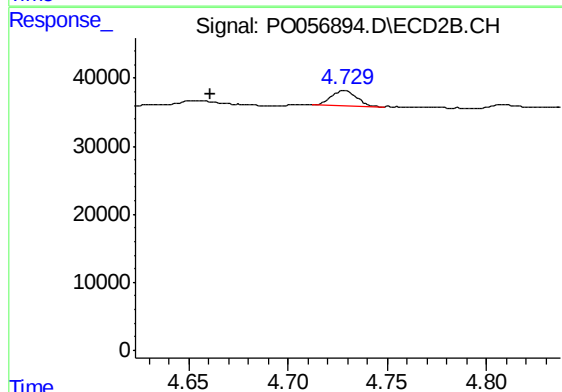


#17 AR-1242-2

R.T.: 4.729 min
Delta R.T.: 0.068 min
Response: 20730
Conc: 11.53 ng/ml

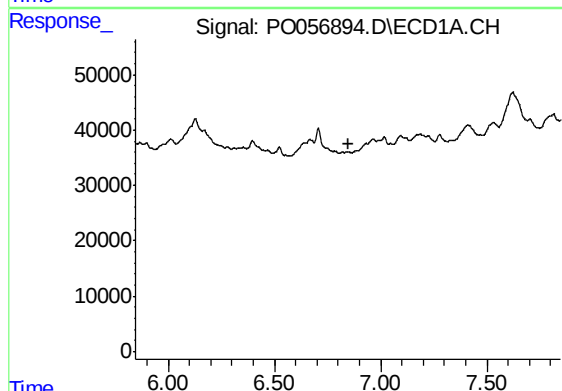


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.846 min
Response: 0
Conc: N.D.

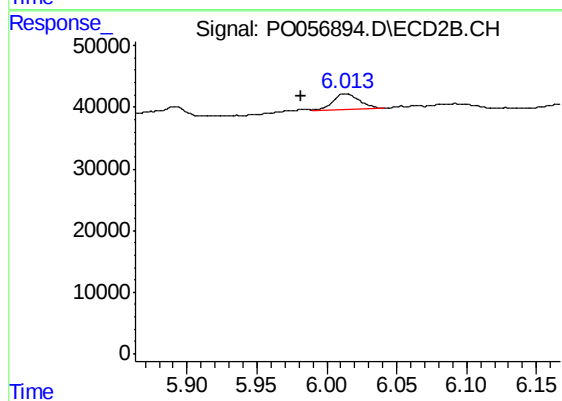

#28 AR-1254-3


R.T.: 6.013 min
Delta R.T.: 0.031 min
Response: 32022
Conc: 8.75 ng/ml

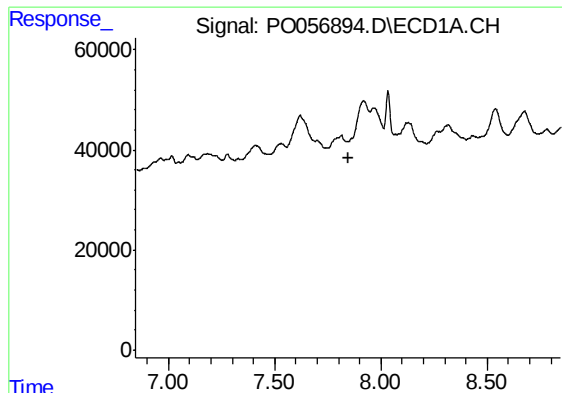

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 7.845 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
PB120325BL

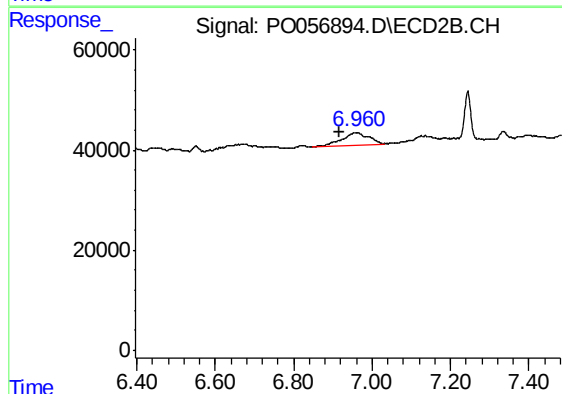


#34 AR-1260-4

R.T.: 6.960 min
Delta R.T.: 0.043 min
Response: 115435
Conc: 62.03 ng/ml

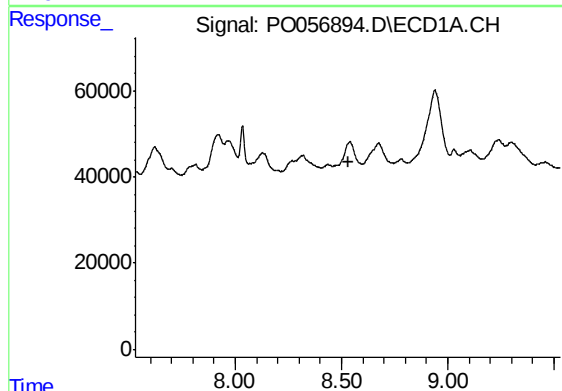


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.530 min
Response: 0
Conc: N.D.

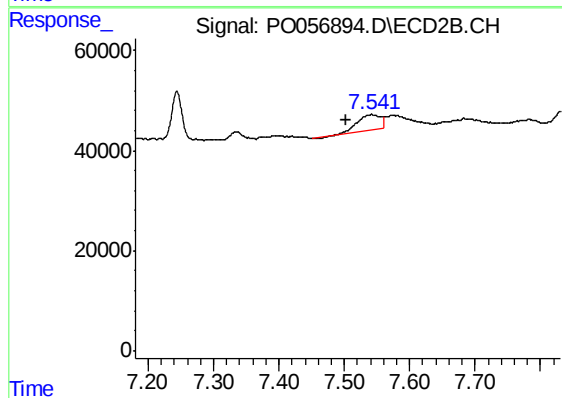

#39 AR-1262-4


R.T.: 7.542 min
Delta R.T.: 0.039 min
Response: 71630
Conc: 13.75 ng/ml

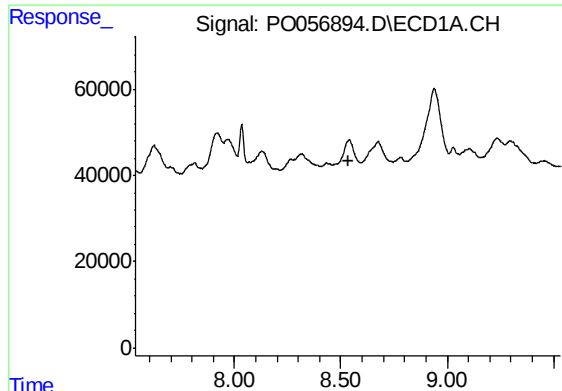

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 8.534 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
PB120325BL

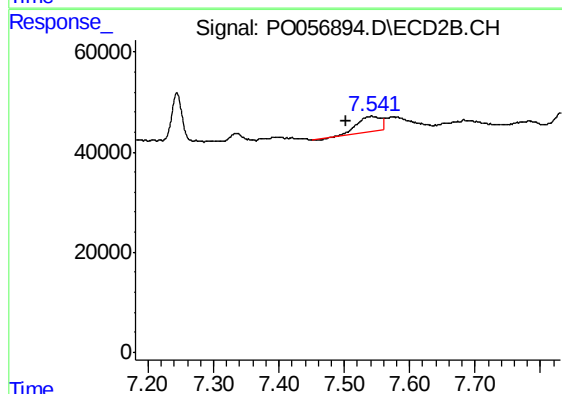


#42 AR-1268-2

R.T.: 7.542 min
Delta R.T.: 0.039 min
Response: 71630
Conc: 10.26 ng/ml

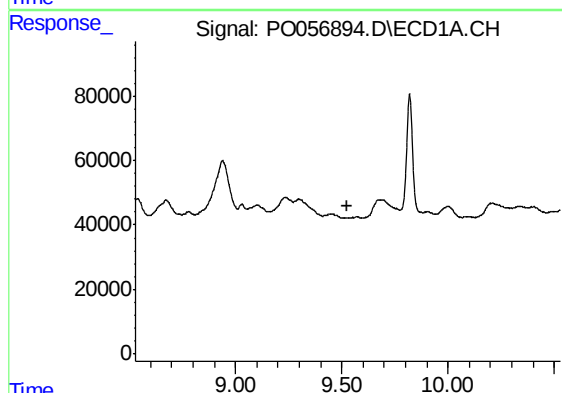

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.529 min
Response: 0
Conc: N.D.

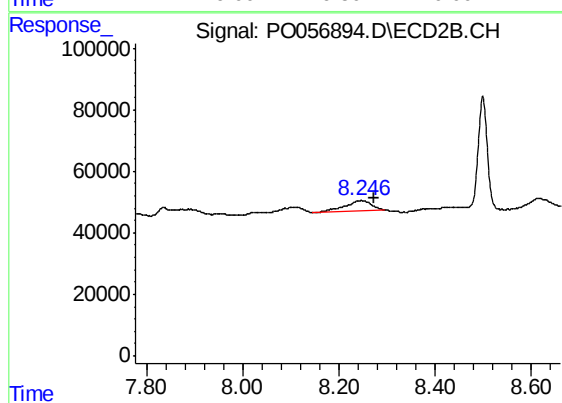

#45 AR-1268-5

R.T.: 8.246 min
Delta R.T.: -0.026 min
Response: 125546
Conc: 7.25 ng/ml