

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060519\
 Data File : P0056903.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jun 2019 2:03
 Operator : SM/SJ
 Sample : K3163-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SU-02-060419-A

Manual Integrations
 APPROVED

Ankita
 6/7/2019 4:23:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 04:24:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.246	3.566	1212810	920578	31.680m	27.915
2) SA Decachlor...	9.820	8.499	1027752	682006	20.939	19.127

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060519\
Data File : P0056903.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2019 2:03
Operator : SM/SJ
Sample : K3163-01
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SU-02-060419-A


Manual Integrations
APPROVED

Ankita
6/7/2019 4:23:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 04:24:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

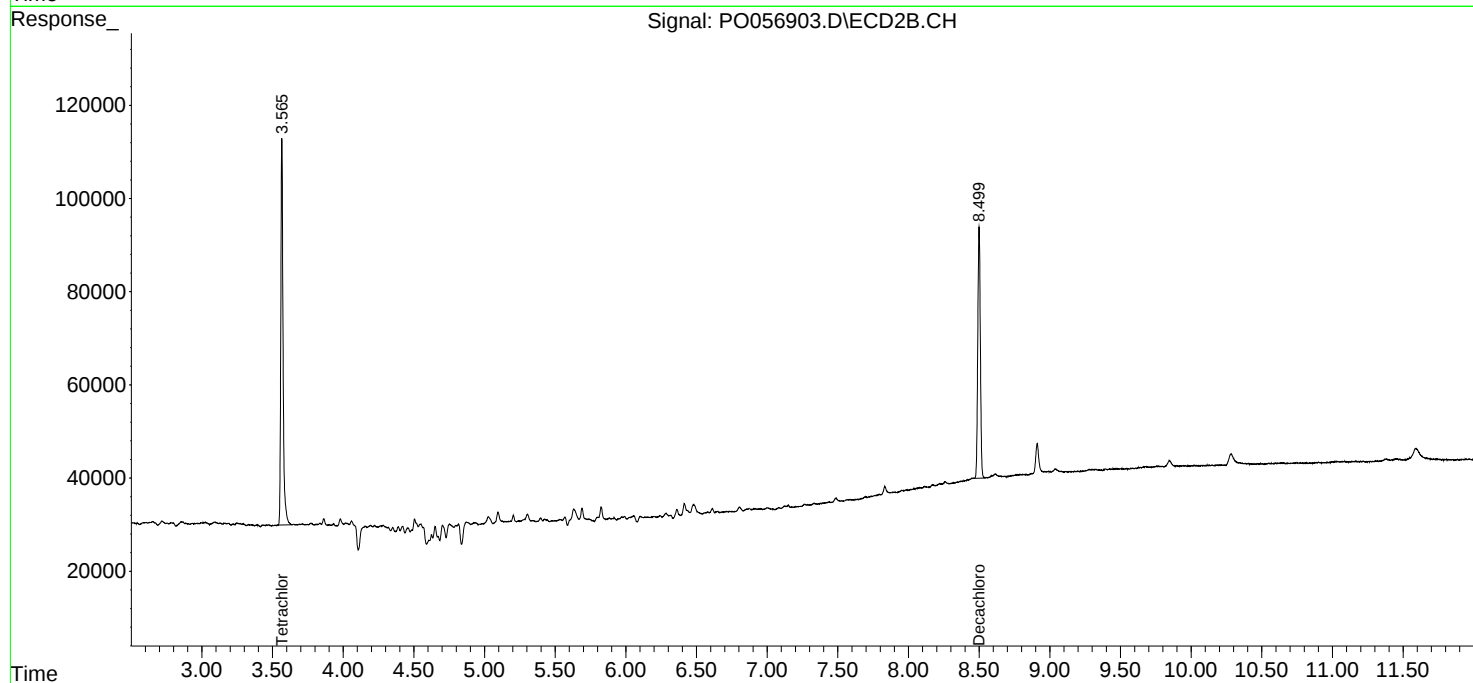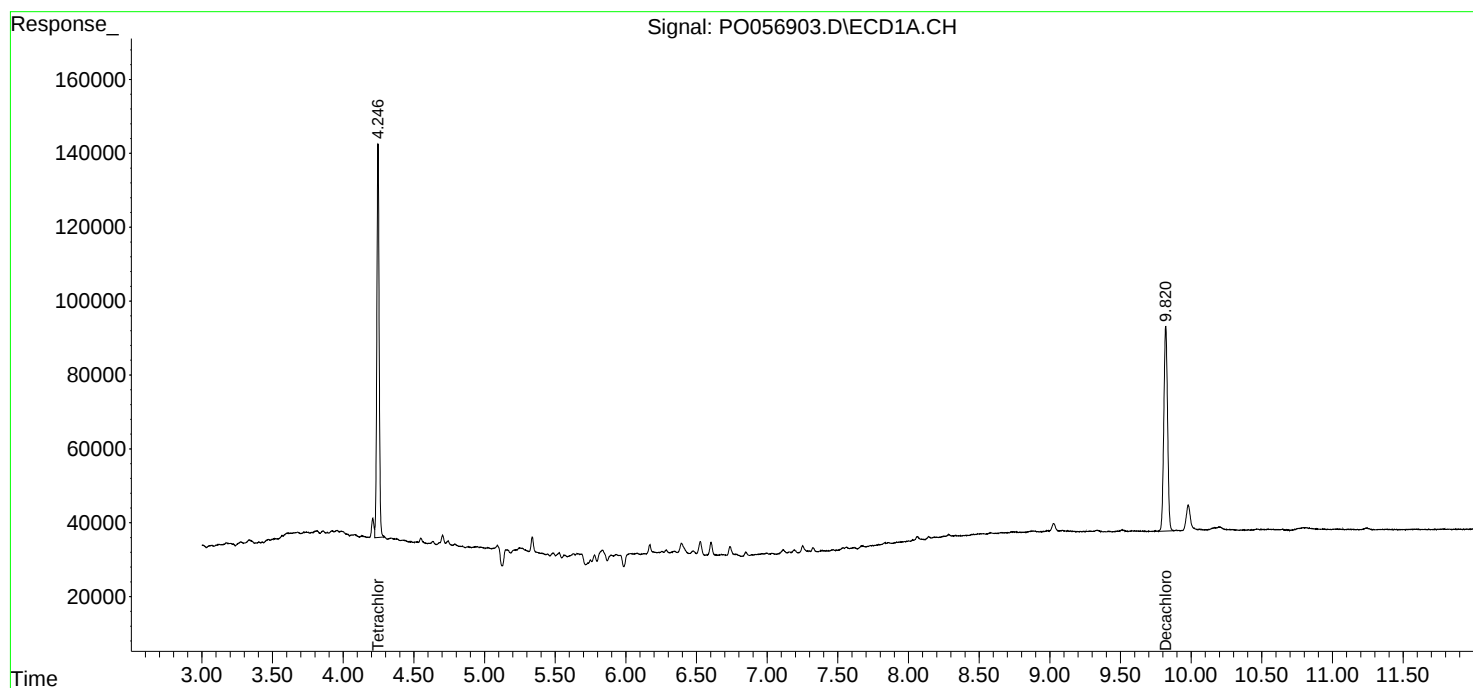

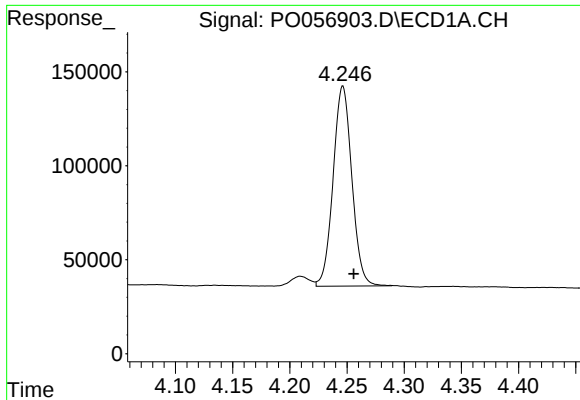


#1 Tetrachloro-m-xylene

R.T.: 4.246 min
Delta R.T.: -0.010 min
Response: 1212810
Conc: 31.68 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SU-02-060419-A


Manual Integrations
APPROVED

Ankita
6/7/2019 4:23:46 PM

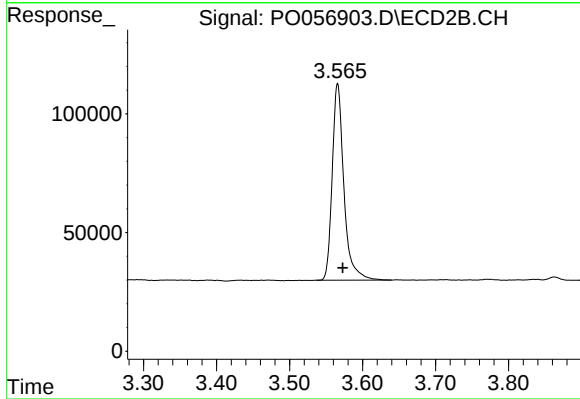


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: -0.007 min
Response: 920578
Conc: 27.91 ng/ml

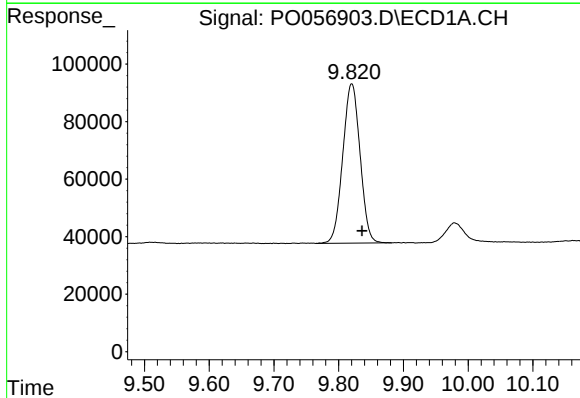

#2 Decachlorobiphenyl

R.T.: 9.820 min
Delta R.T.: -0.016 min
Response: 1027752
Conc: 20.94 ng/ml

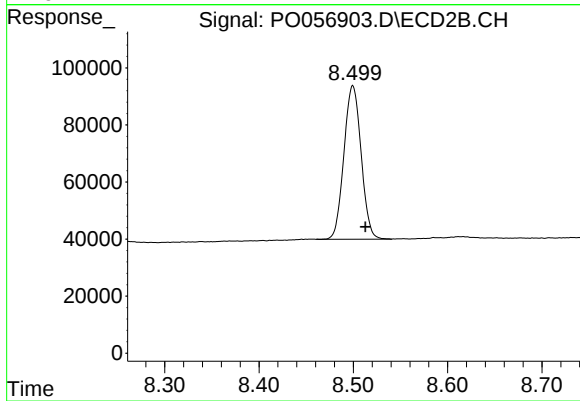

#2 Decachlorobiphenyl

R.T.: 8.499 min
Delta R.T.: -0.014 min
Response: 682006
Conc: 19.13 ng/ml