

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060520\
 Data File : P0068774.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jun 2020 00:08
 Operator : DD\AJ
 Sample : PB129328BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 05:15:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060520.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 06 05:06:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.782	3.851	627734	780873	20.288	20.627
2)	SA Decachlor...	10.661	9.101	867028	986516	20.253	20.256
Target Compounds							
9)	L2 AR-1221-2	5.135	0.000	4355	0	18.332	N.D. #
21)	L5 AR-1248-1	6.029	0.000	13904	0	19.635	N.D. #
28)	L6 AR-1254-3	7.633	0.000	8782	0	4.131	N.D. #
38)	L8 AR-1262-3	9.269	0.000	2490	0	0.799	N.D. #
39)	L8 AR-1262-4	9.269	0.000	2490	0	1.046	N.D. #
41)	L9 AR-1268-1	9.269	0.000	2490	0	0.398	N.D. #
42)	L9 AR-1268-2	9.269	0.000	2490	0	0.451	N.D. #
45)	L9 AR-1268-5	10.349	0.000	2063	0	0.137	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060520\
Data File : P0068774.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2020 00:08
Operator : DD\AJ
Sample : PB129328BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 05:15:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060520.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 06 05:06:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

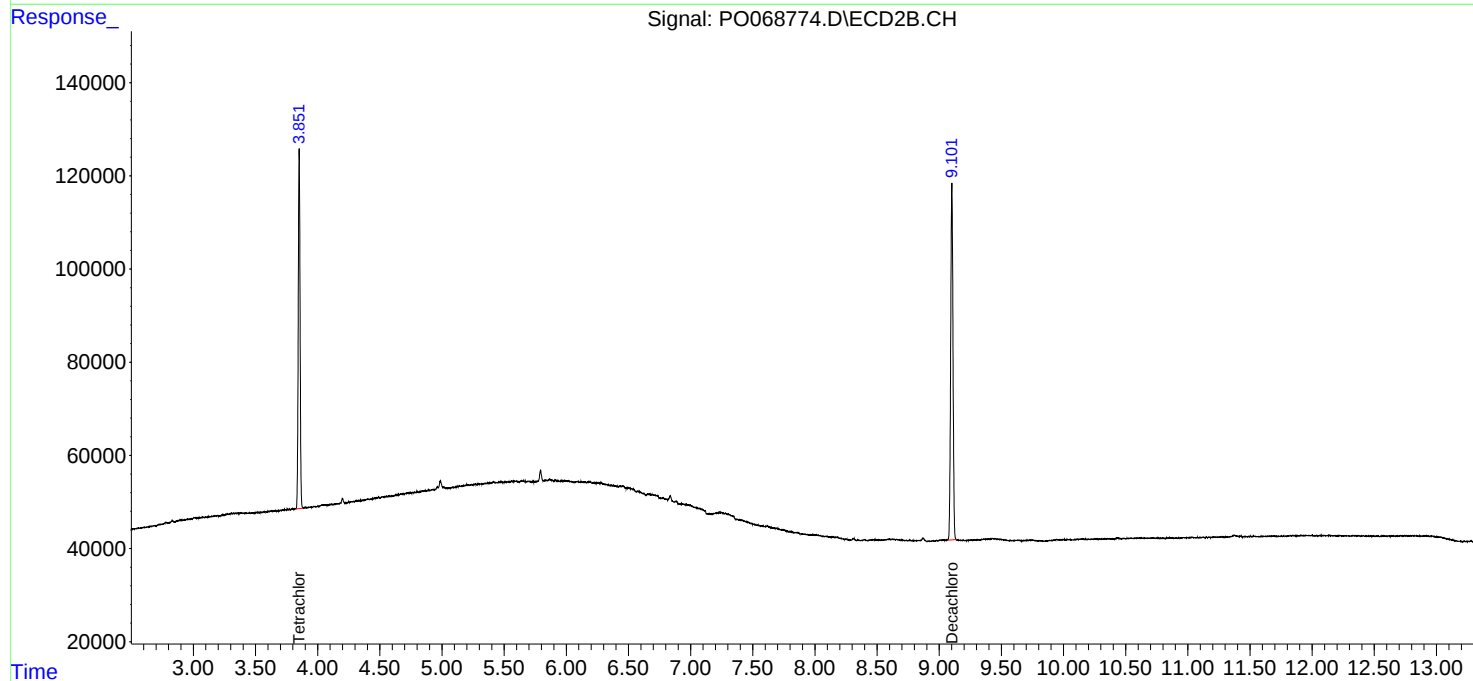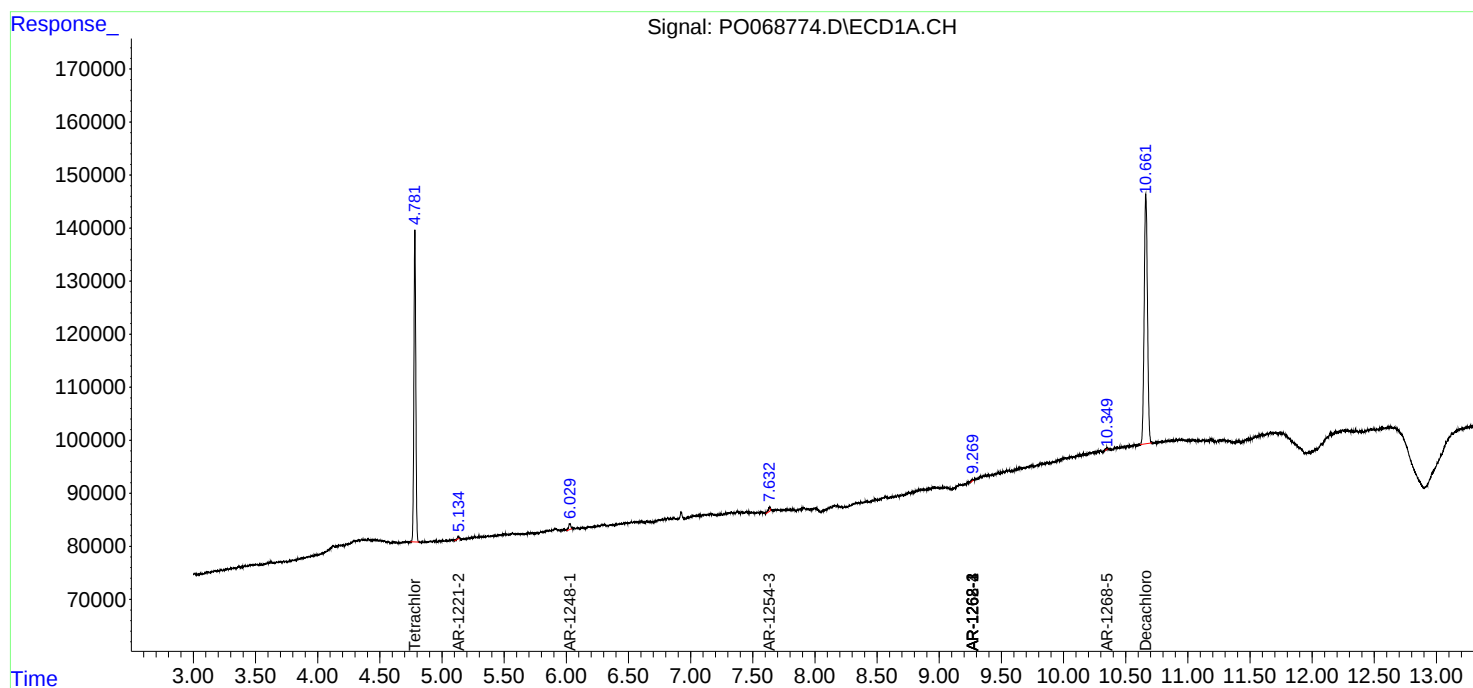


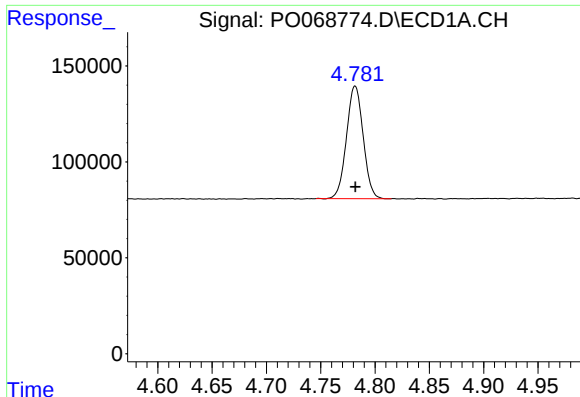

#1 Tetrachloro-m-xylene


R.T.: 4.782 min
Delta R.T.: 0.000 min
Response: 627734
Conc: 20.29 ng/ml

Instrument :
ECD_O
ClientSampleId :

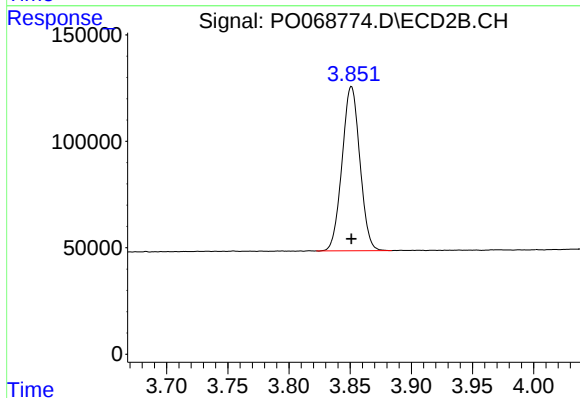


#1 Tetrachloro-m-xylene

R.T.: 3.851 min
Delta R.T.: 0.000 min
Response: 780873
Conc: 20.63 ng/ml

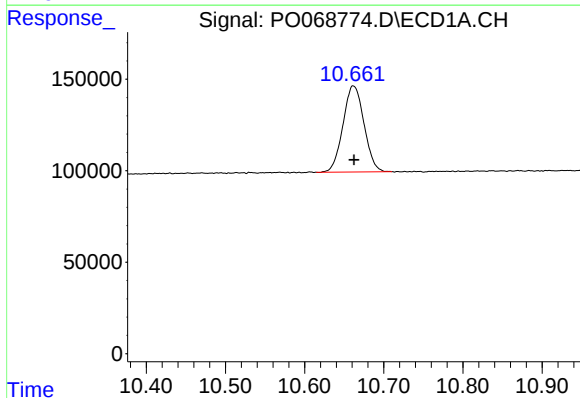


#2 Decachlorobiphenyl

R.T.: 10.661 min
Delta R.T.: -0.001 min
Response: 867028
Conc: 20.25 ng/ml

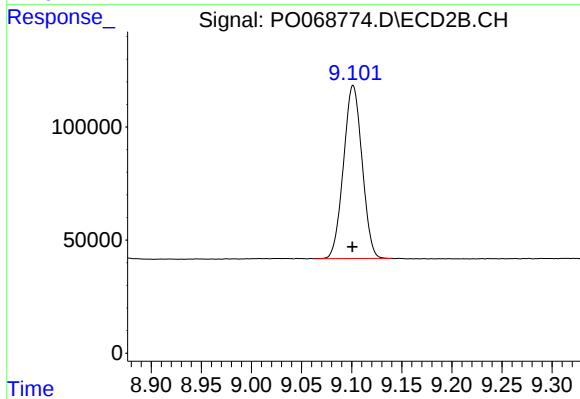

#2 Decachlorobiphenyl


R.T.: 9.101 min
Delta R.T.: 0.000 min
Response: 986516
Conc: 20.26 ng/ml

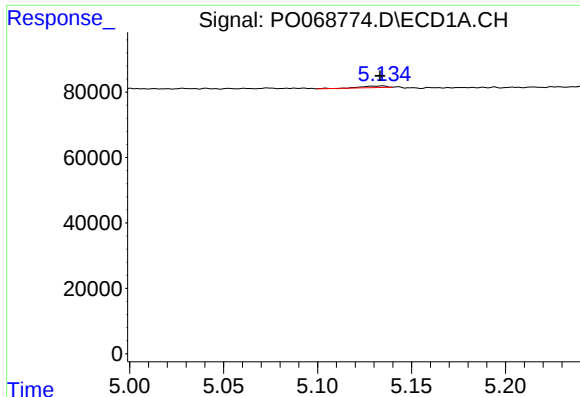

#9 AR-1221-2


R.T.: 5.135 min
Delta R.T.: 0.002 min
Response: 4355
Conc: 18.33 ng/ml

Instrument :
ECD_O
ClientSampleId :

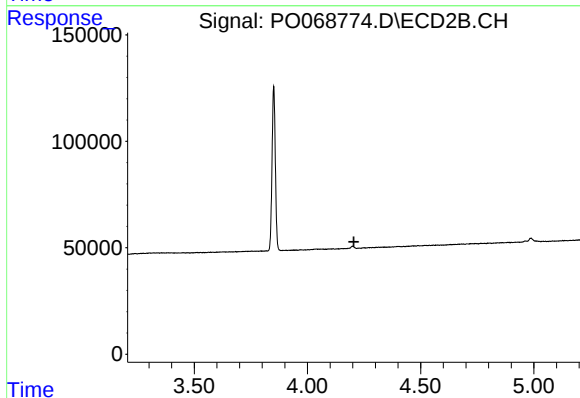


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.205 min
Response: 0
Conc: N.D.

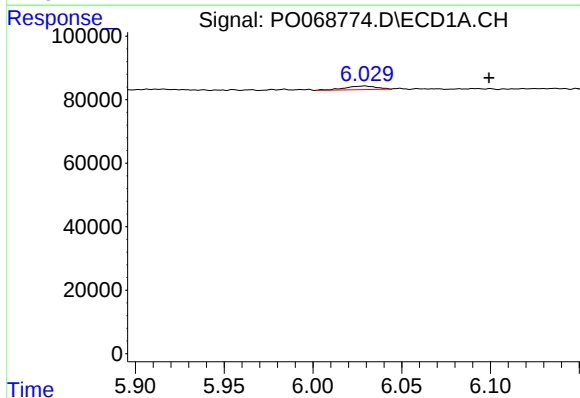


#21 AR-1248-1

R.T.: 6.029 min
Delta R.T.: -0.070 min
Response: 13904
Conc: 19.63 ng/ml

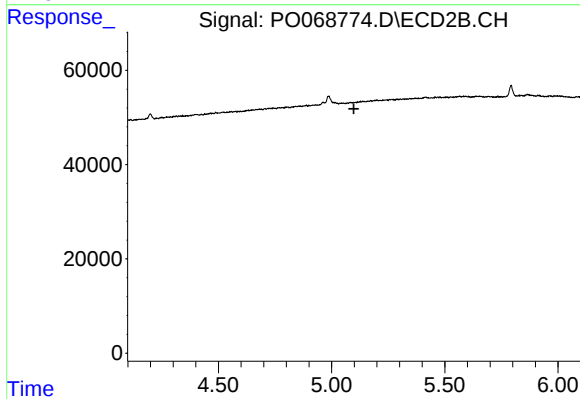

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T. : 5.098 min
Response: 0
Conc: N.D.

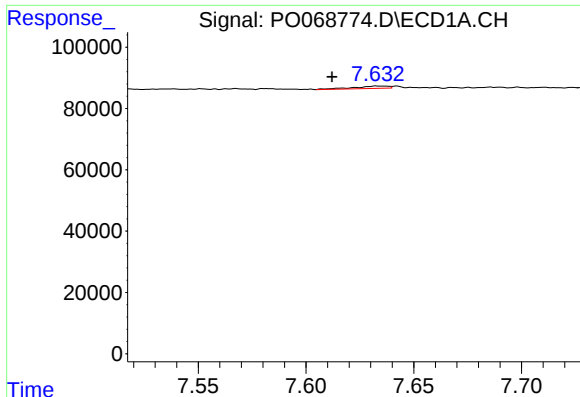

#28 AR-1254-3


R.T.: 7.633 min
Delta R.T.: 0.020 min
Response: 8782
Conc: 4.13 ng/ml

Instrument :
ECD_O
ClientSampleId :

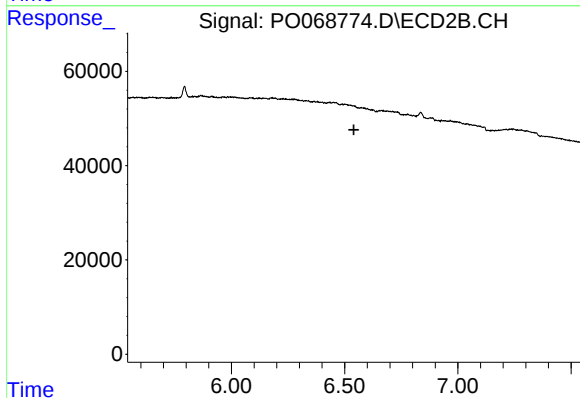


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.541 min
Response: 0
Conc: N.D.

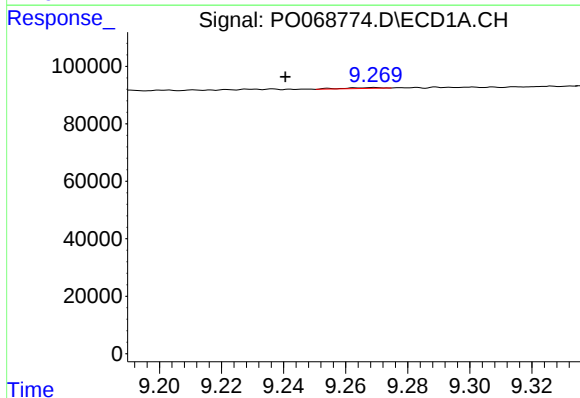


#38 AR-1262-3

R.T.: 9.269 min
Delta R.T.: 0.029 min
Response: 2490
Conc: 0.80 ng/ml

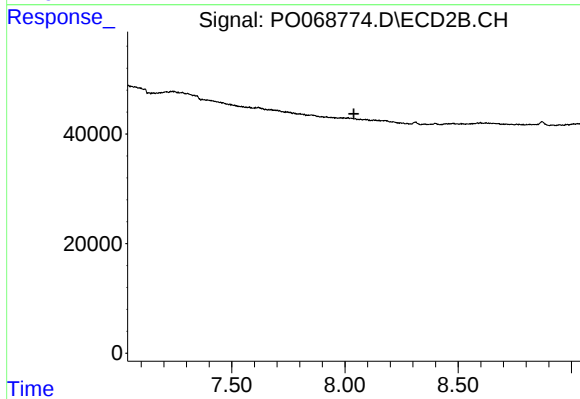

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 8.040 min
Response: 0
Conc: N.D.

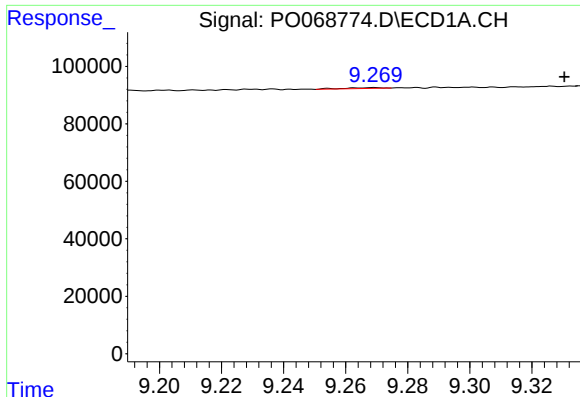

#39 AR-1262-4


R.T.: 9.269 min
Delta R.T.: -0.061 min
Response: 2490
Conc: 1.05 ng/ml

Instrument :
ECD_O
ClientSampleId :

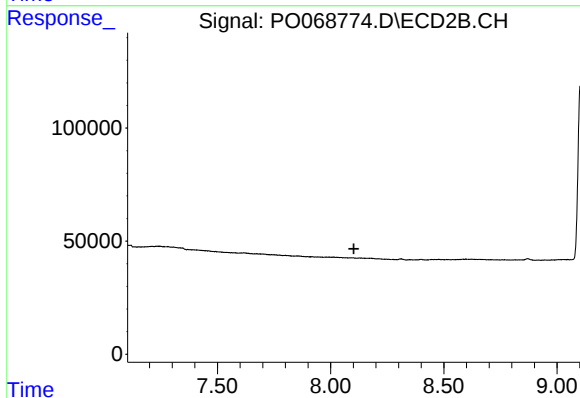


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

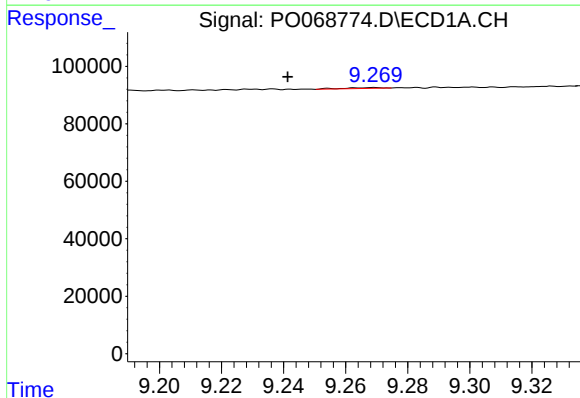


#41 AR-1268-1

R.T.: 9.269 min
Delta R.T.: 0.028 min
Response: 2490
Conc: 0.40 ng/ml

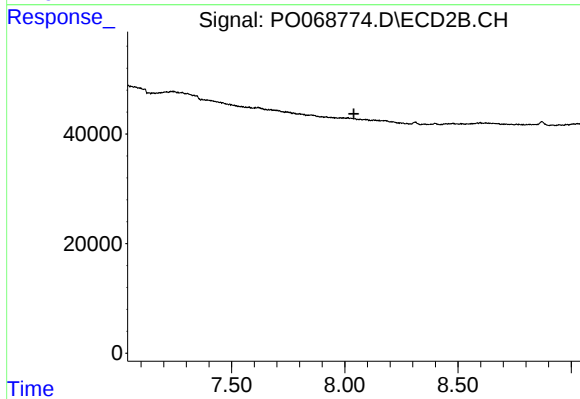

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.040 min
Response: 0
Conc: N.D.

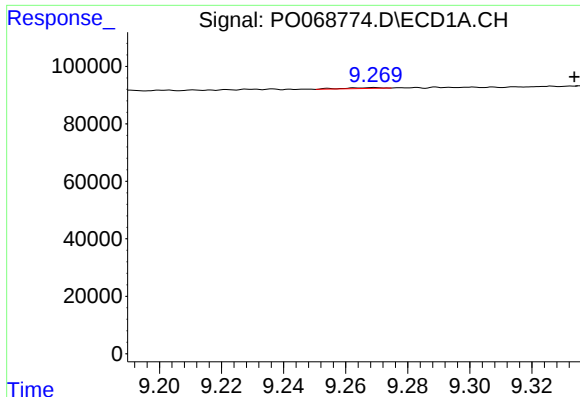

#42 AR-1268-2


R.T.: 9.269 min
Delta R.T.: -0.065 min
Response: 2490
Conc: 0.45 ng/ml

Instrument :
ECD_O
ClientSampleId :

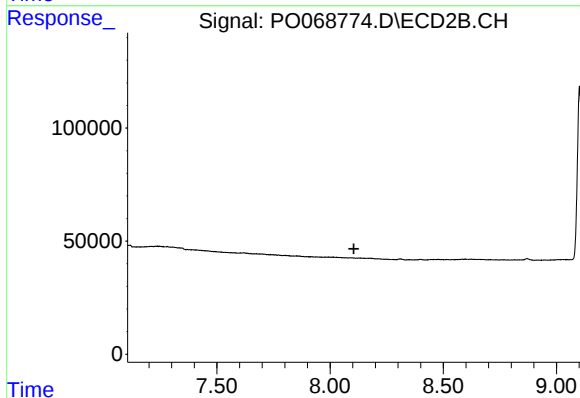


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.105 min
Response: 0
Conc: N.D.

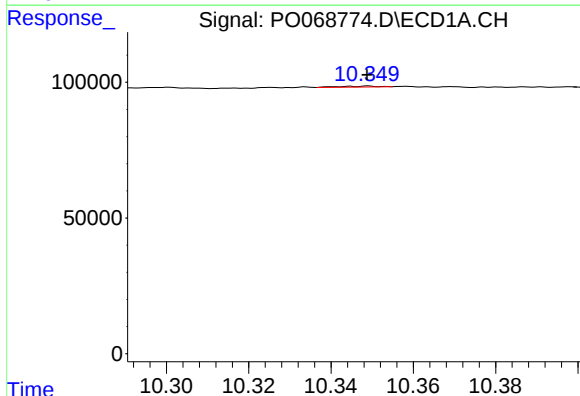

#45 AR-1268-5

R.T.: 10.349 min
Delta R.T.: 0.000 min
Response: 2063
Conc: 0.14 ng/ml

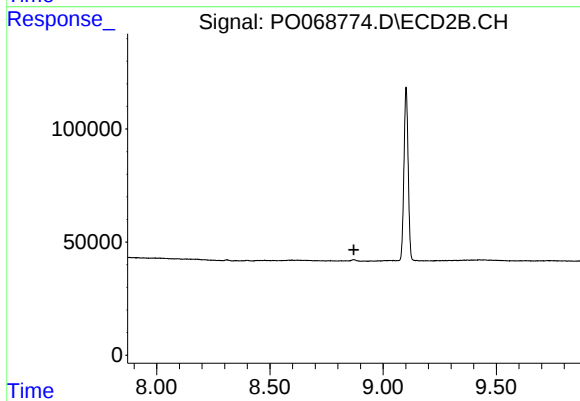

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.871 min
Response: 0
Conc: N.D.