

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060520\
 Data File : P0068771.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jun 2020 23:16
 Operator : DD\AJ
 Sample : L2858-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 N28427

Manual Integrations
 APPROVED

Sohil
 6/8/2020 10:44:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 05:13:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060520.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 06 05:06:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.781	3.851	522534	672845	16.888m	17.773
2) SA Decachlor...	10.662	9.101	460663	546007	10.761	11.211

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060520\
Data File : P0068771.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jun 2020 23:16
Operator : DD\AJ
Sample : L2858-02
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
N28427


Manual Integrations
APPROVED

Sohil
6/8/2020 10:44:50 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 05:13:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060520.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 06 05:06:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

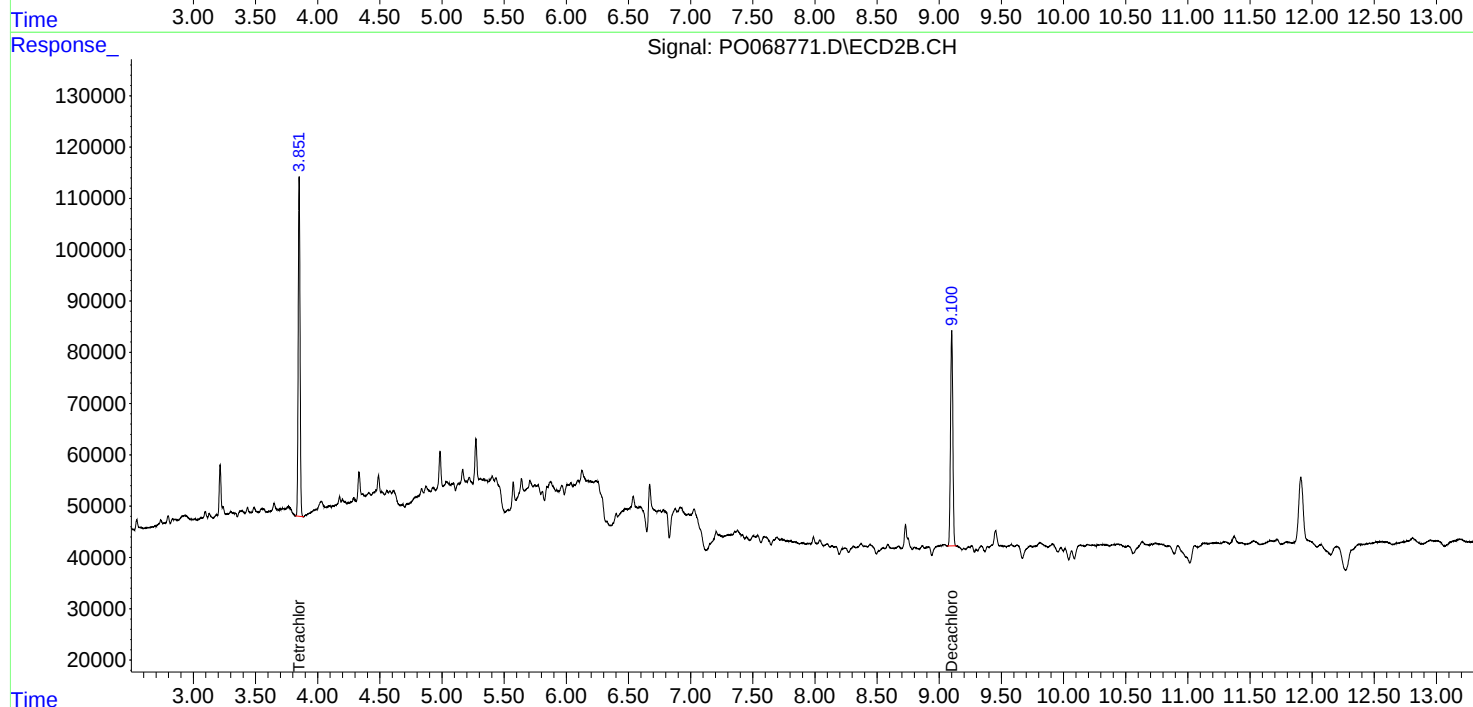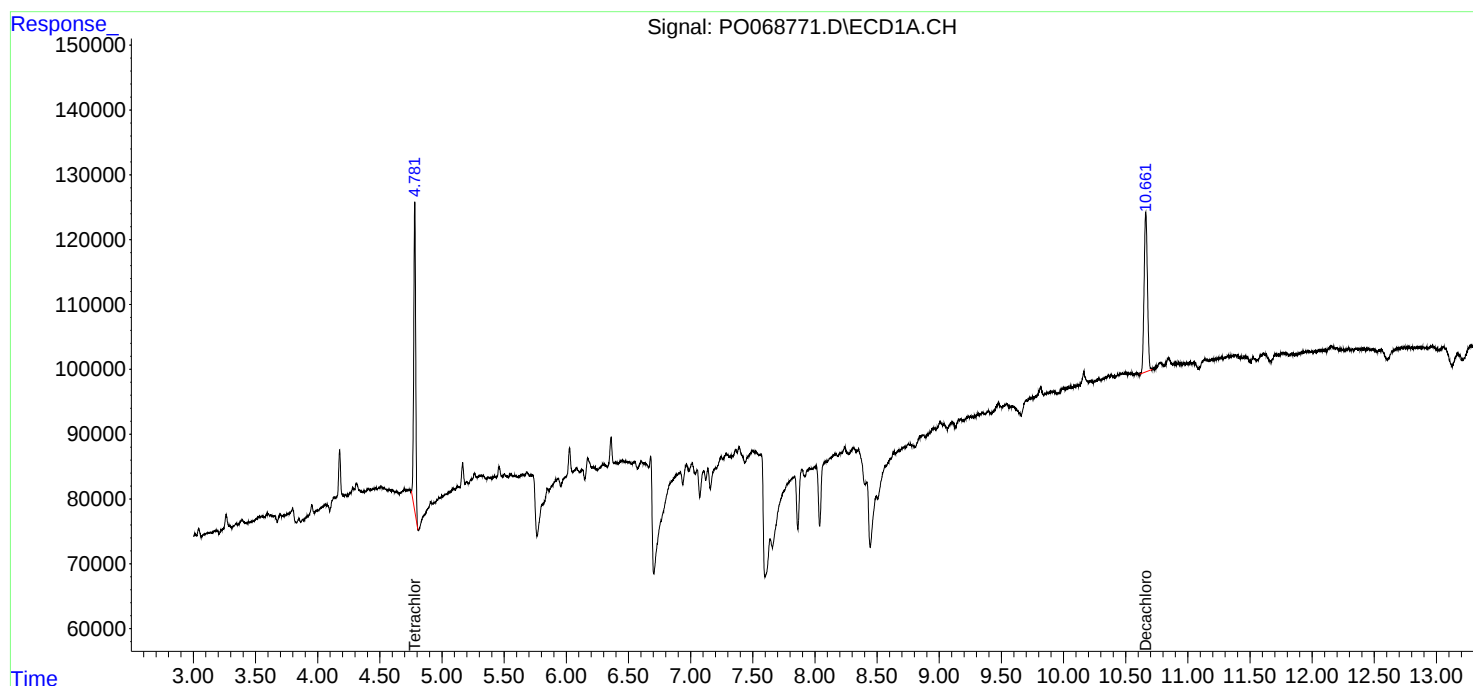

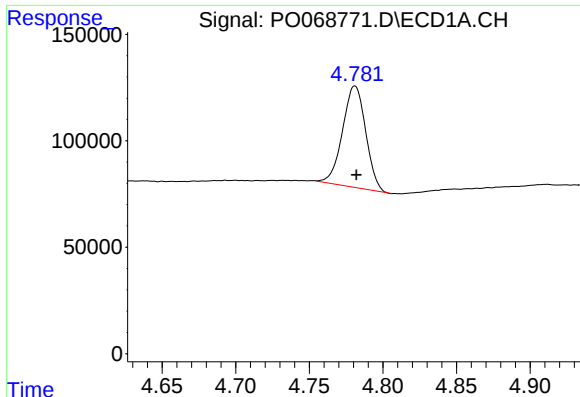


#1 Tetrachloro-m-xylene

R.T.: 4.781 min
Delta R.T.: -0.001 min
Response: 522534
Conc: 16.89 ng/ml m

Instrument :
ECD_O
ClientSampleId :
N28427


Manual Integrations
APPROVED

Sohil
6/8/2020 10:44:50 AM

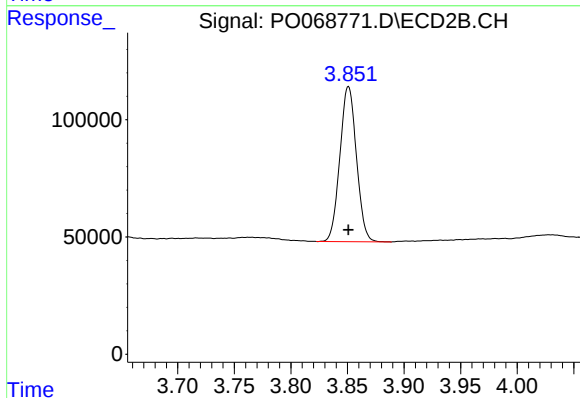


#1 Tetrachloro-m-xylene

R.T.: 3.851 min
Delta R.T.: 0.000 min
Response: 672845
Conc: 17.77 ng/ml

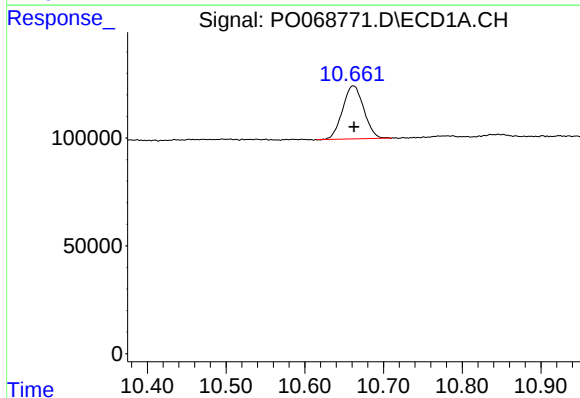

#2 Decachlorobiphenyl

R.T.: 10.662 min
Delta R.T.: 0.000 min
Response: 460663
Conc: 10.76 ng/ml

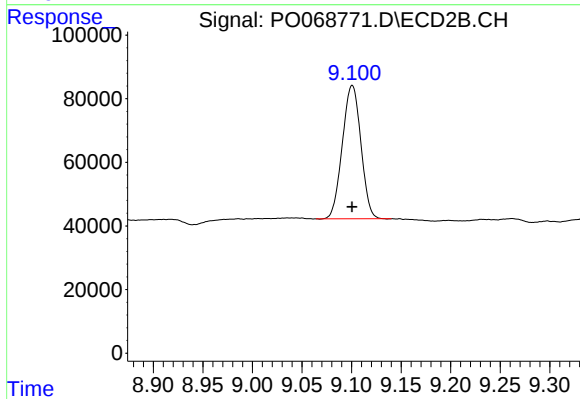

#2 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: 0.000 min
Response: 546007
Conc: 11.21 ng/ml