

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060520\
 Data File : P0068807.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jun 2020 12:09
 Operator : DD\AJ
 Sample : L2904-06
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 VE-1-2

Manual Integrations
 APPROVED

Sohil
 6/8/2020 10:45:02 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 01:16:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060520.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 06 05:06:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.779	3.850	577029	636484	18.650	16.813m
2) SA Decachlor...	10.658	9.100	454703	512701	10.622	10.527

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060520\
Data File : P0068807.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2020 12:09
Operator : DD\AJ
Sample : L2904-06
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
VE-1-2


Manual Integrations
APPROVED

Sohil
6/8/2020 10:45:02 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 01:16:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060520.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 06 05:06:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

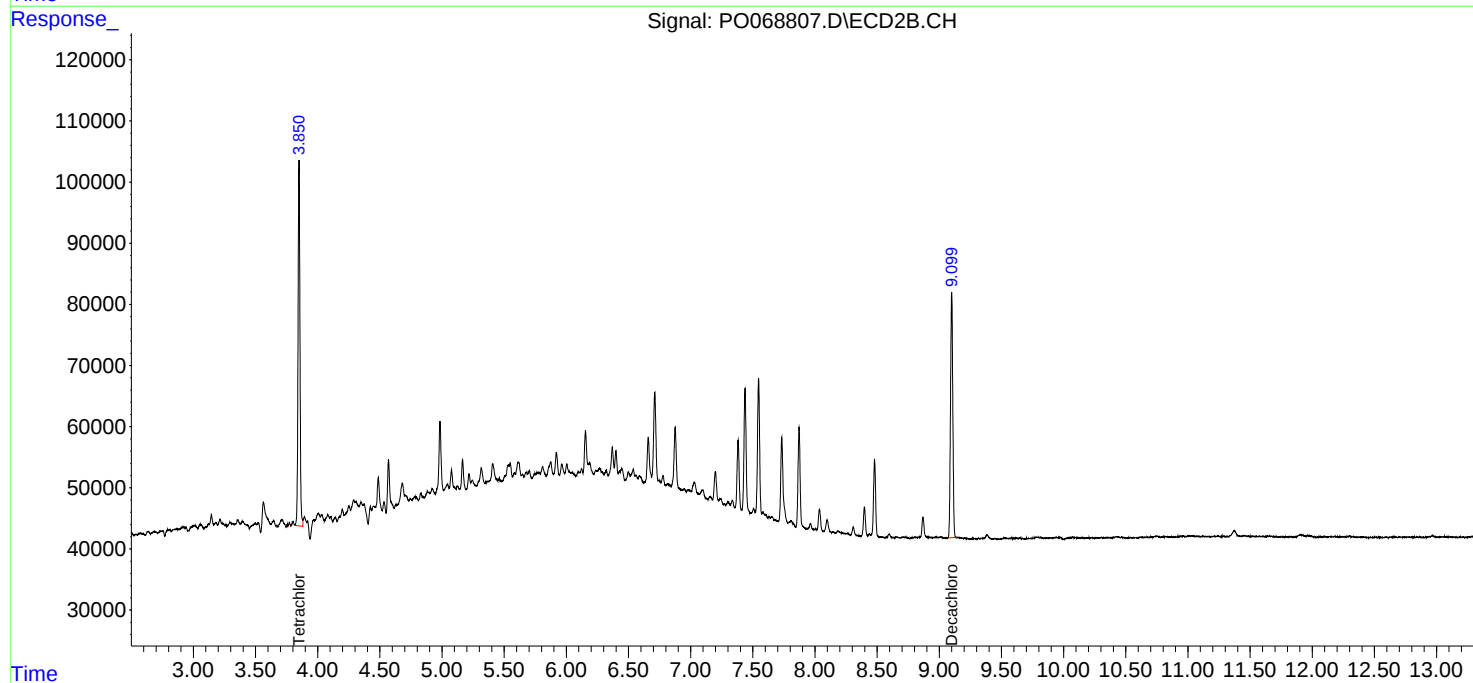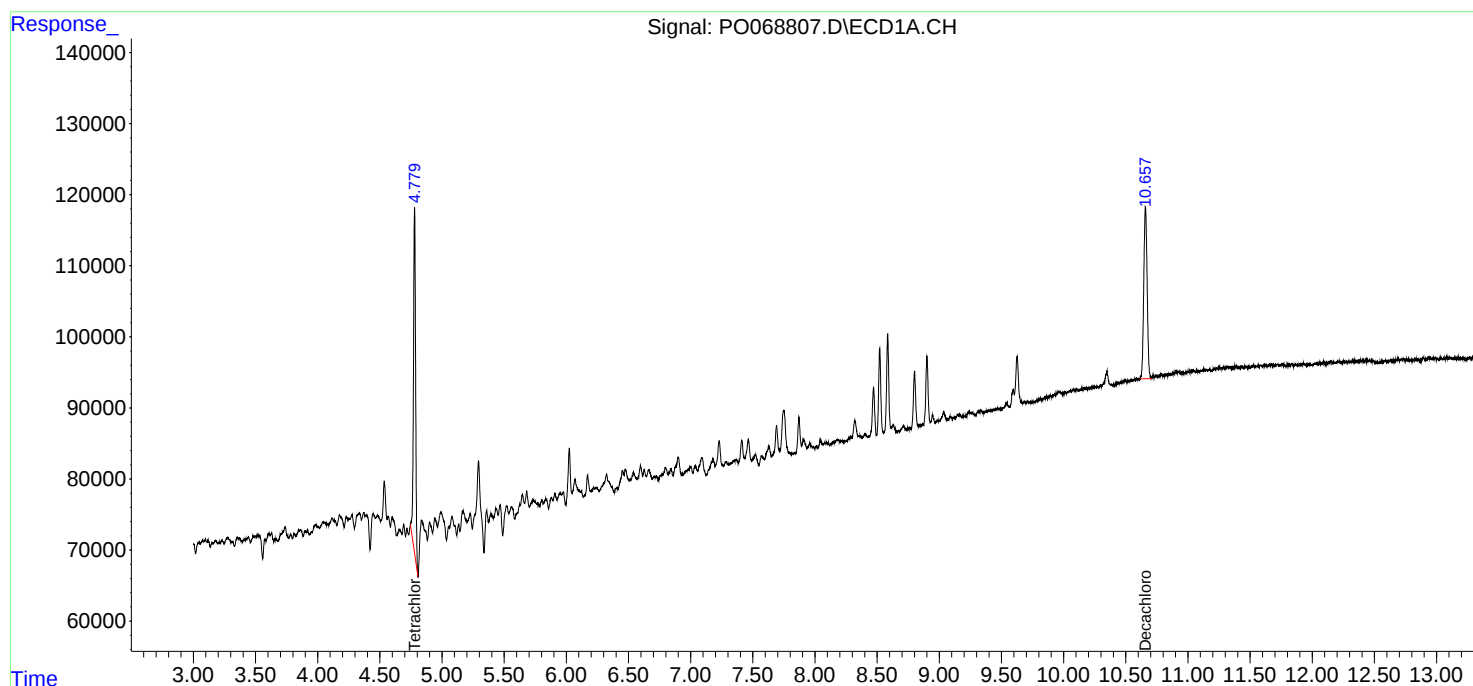

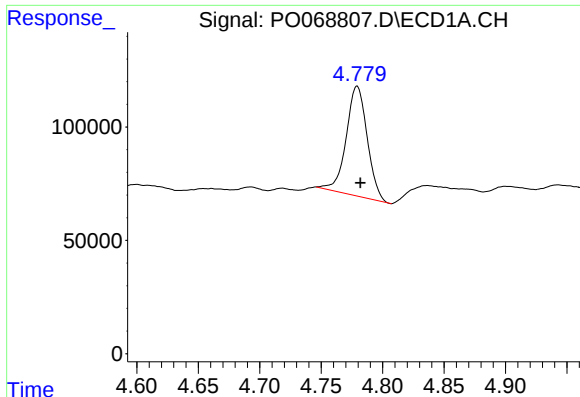


#1 Tetrachloro-m-xylene

R.T.: 4.779 min
Delta R.T.: -0.003 min
Response: 577029
Conc: 18.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
VE-1-2


Manual Integrations
APPROVED

Sohil
6/8/2020 10:45:02 AM

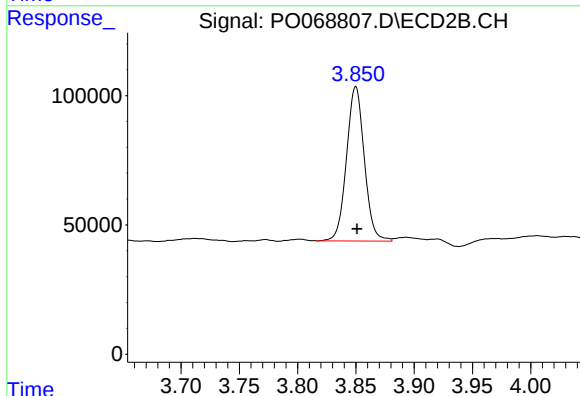


#1 Tetrachloro-m-xylene

R.T.: 3.850 min
Delta R.T.: -0.001 min
Response: 636484
Conc: 16.81 ng/ml m

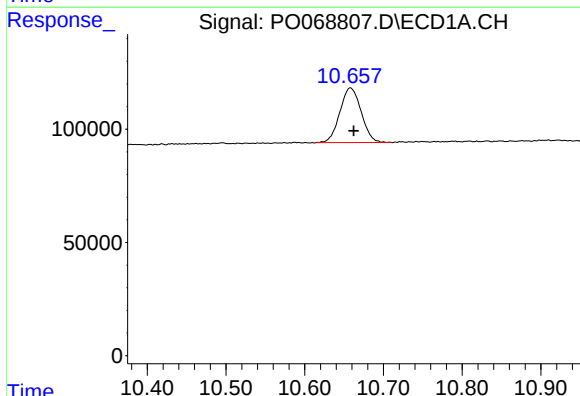

#2 Decachlorobiphenyl

R.T.: 10.658 min
Delta R.T.: -0.004 min
Response: 454703
Conc: 10.62 ng/ml

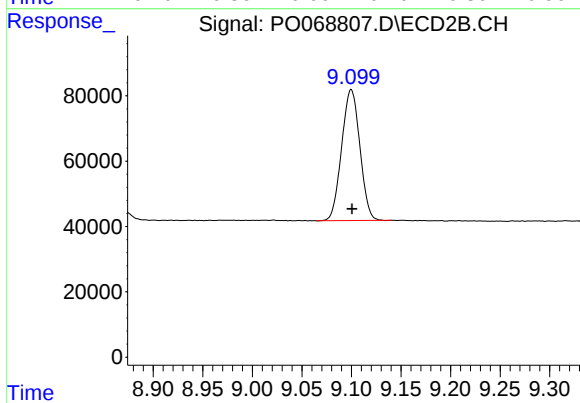

#2 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: 0.000 min
Response: 512701
Conc: 10.53 ng/ml