

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060520\
 Data File : P0068808.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jun 2020 12:27
 Operator : DD\AJ
 Sample : L2904-07
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 VE-3-1

Manual Integrations
 APPROVED

Sohil
 6/8/2020 10:45:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 01:17:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060520.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 06 05:06:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.780	3.850	303611	387220	9.813m	10.228m
2) SA Decachlor...	10.658	9.100	249531	288691	5.829	5.928

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060520\
Data File : P0068808.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2020 12:27
Operator : DD\AJ
Sample : L2904-07
Misc :
ALS Vial : 52 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
VE-3-1


Manual Integrations
APPROVED

Sohil
6/8/2020 10:45:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 01:17:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060520.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 06 05:06:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

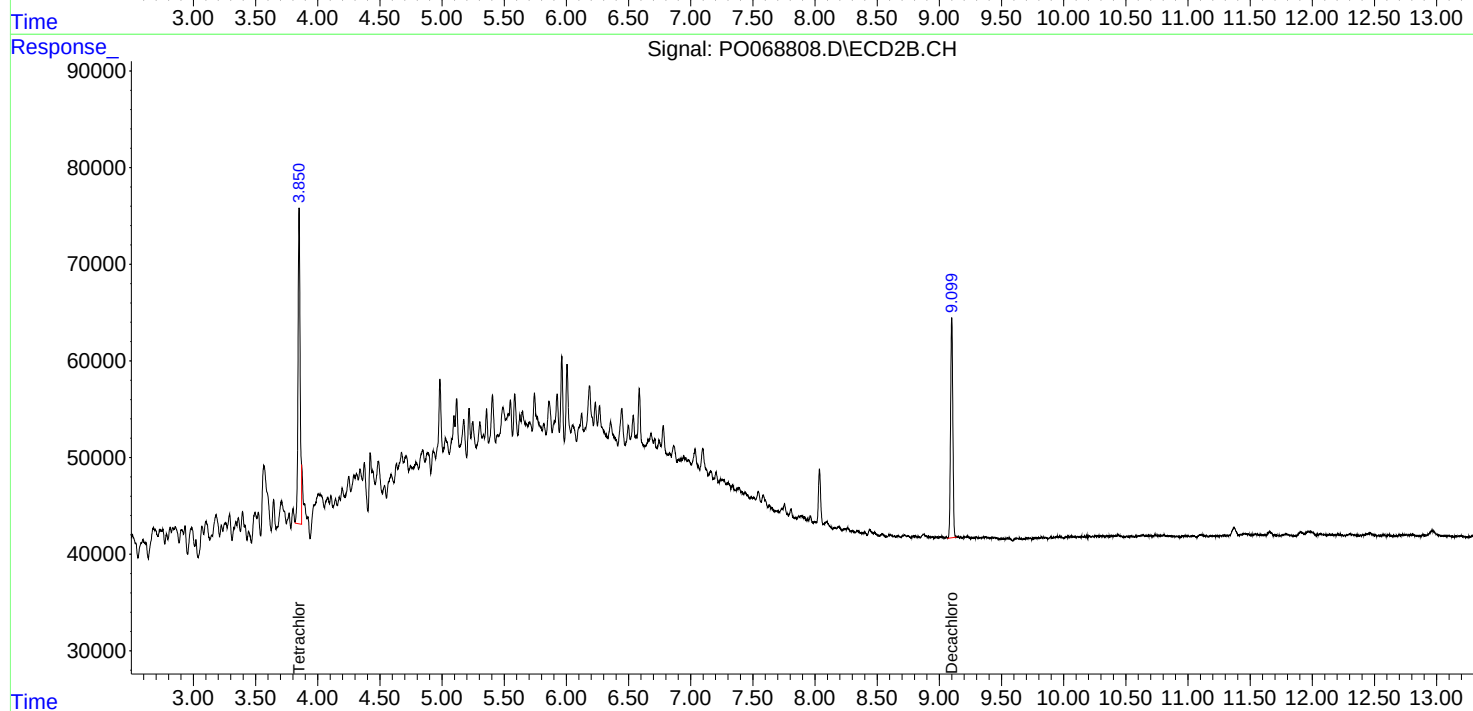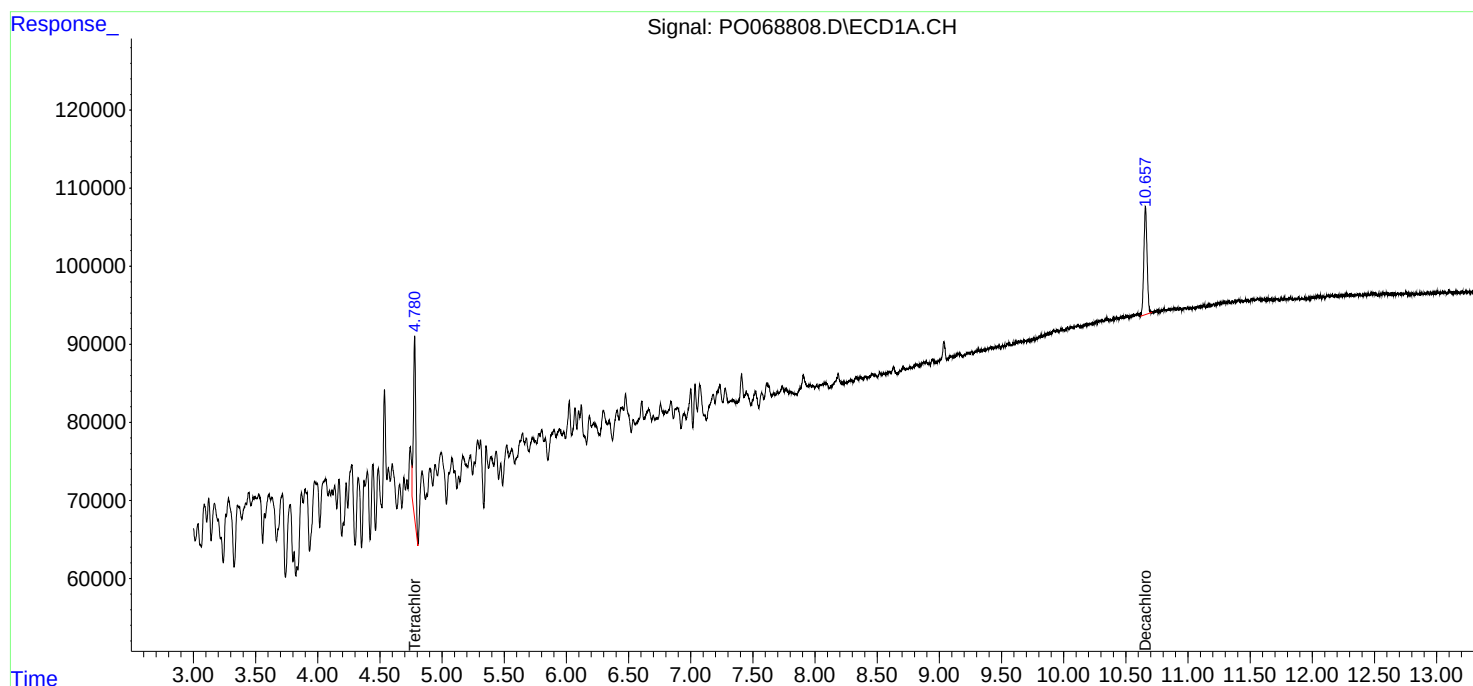

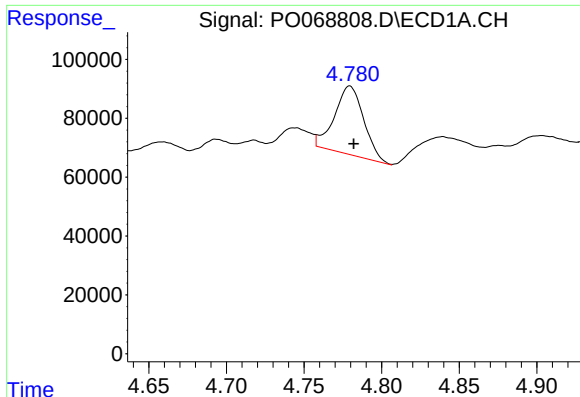


#1 Tetrachloro-m-xylene

R.T.: 4.780 min
Delta R.T.: -0.002 min
Response: 303611
Conc: 9.81 ng/ml m

Instrument :
ECD_O
ClientSampleId :
VE-3-1


Manual Integrations
APPROVED

Sohil
6/8/2020 10:45:03 AM

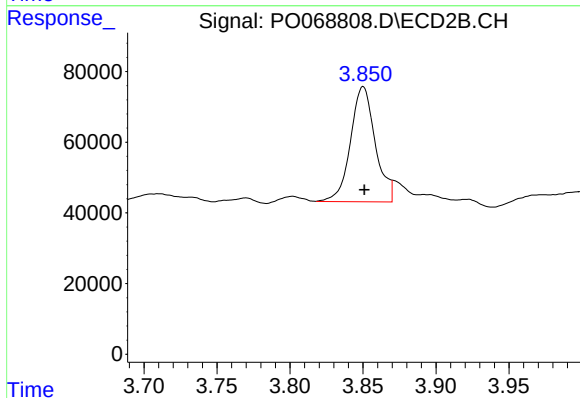


#1 Tetrachloro-m-xylene

R.T.: 3.850 min
Delta R.T.: -0.001 min
Response: 387220
Conc: 10.23 ng/ml m

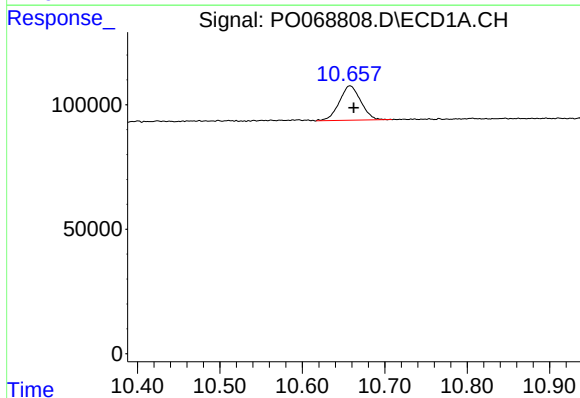

#2 Decachlorobiphenyl

R.T.: 10.658 min
Delta R.T.: -0.005 min
Response: 249531
Conc: 5.83 ng/ml

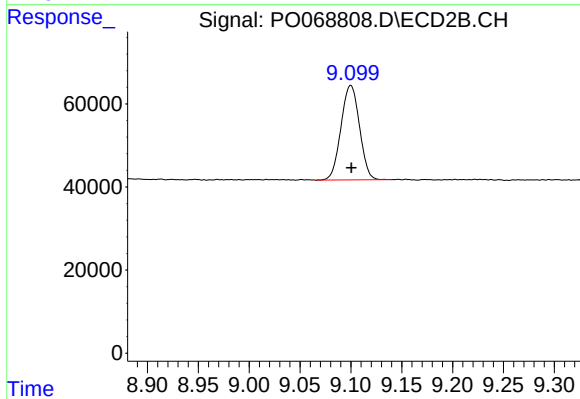

#2 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: 0.000 min
Response: 288691
Conc: 5.93 ng/ml