

Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060618\
 Data File : P0045529.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jun 2018 14:02
 Operator : SM/UA
 Sample : J3228-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-028

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 14:39:09 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 31 04:53:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.996	3.273	5016860	6698185	24.019	24.156
2) SA Decachlor...	9.273	7.991	3416558	3450323	14.876	12.242

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060618\
Data File : P0045529.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jun 2018 14:02
Operator : SM/UA
Sample : J3228-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-028

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 14:39:09 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

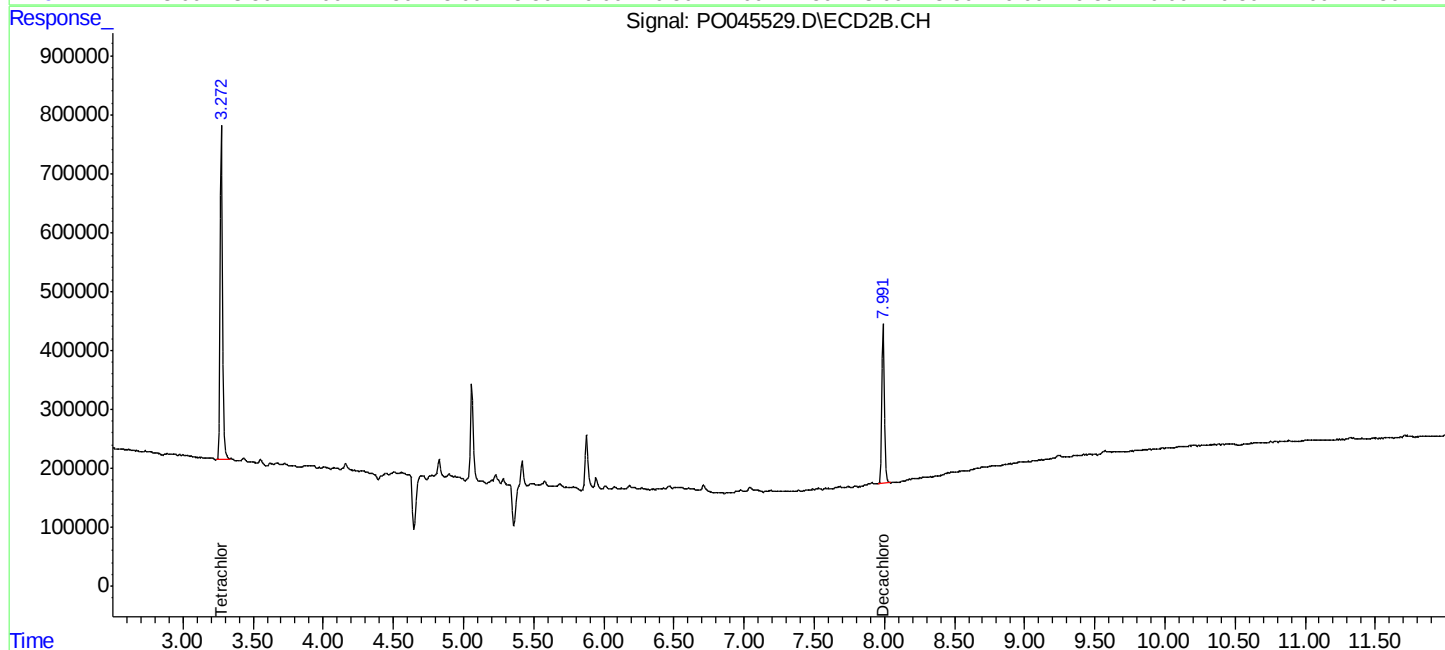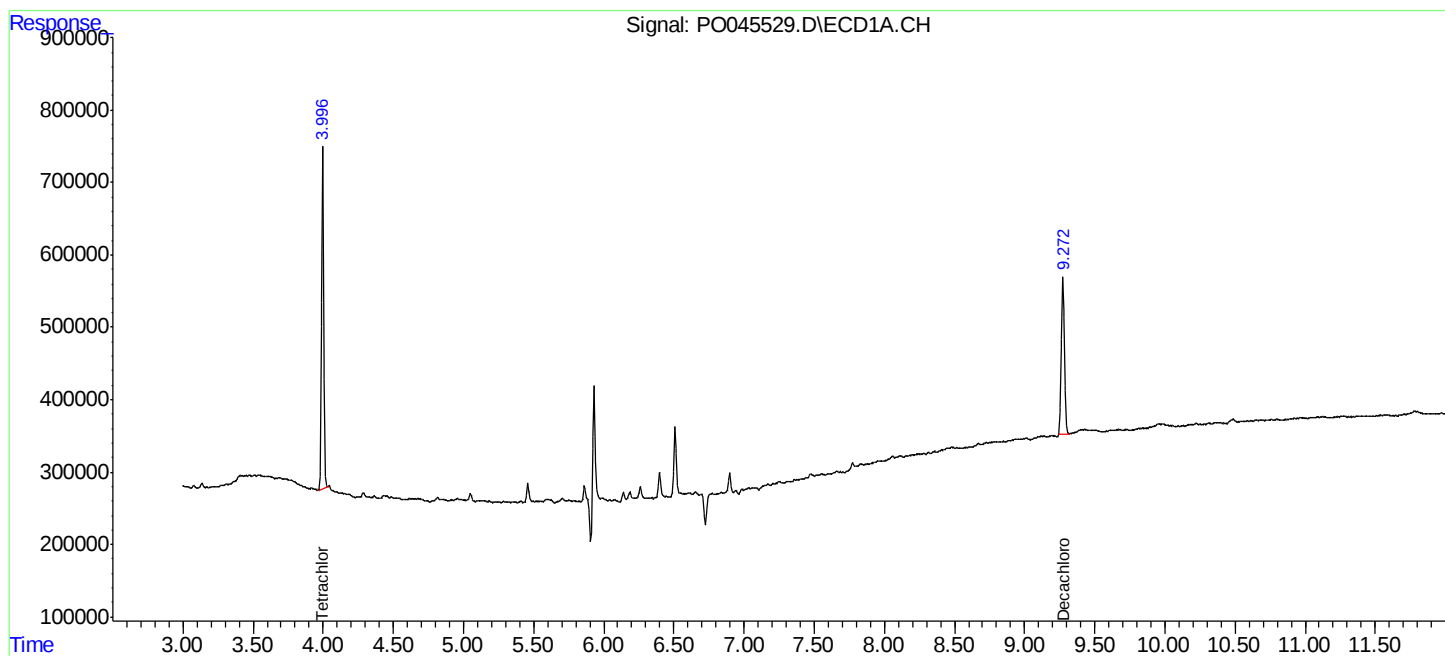


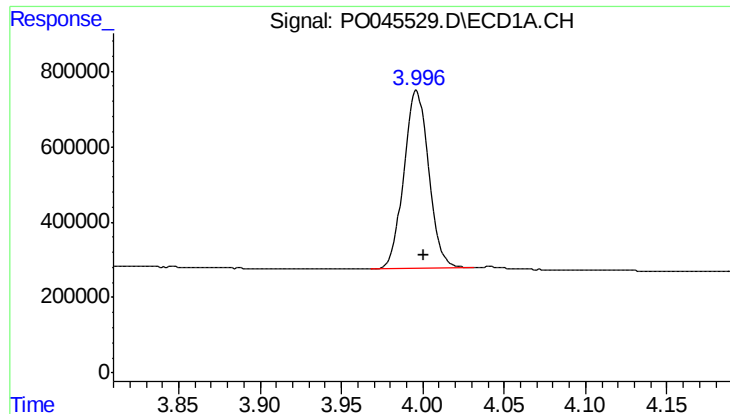

#1 Tetrachloro-m-xylene


R.T.: 3.996 min
Delta R.T.: -0.004 min
Response: 5016860
Conc: 24.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-028

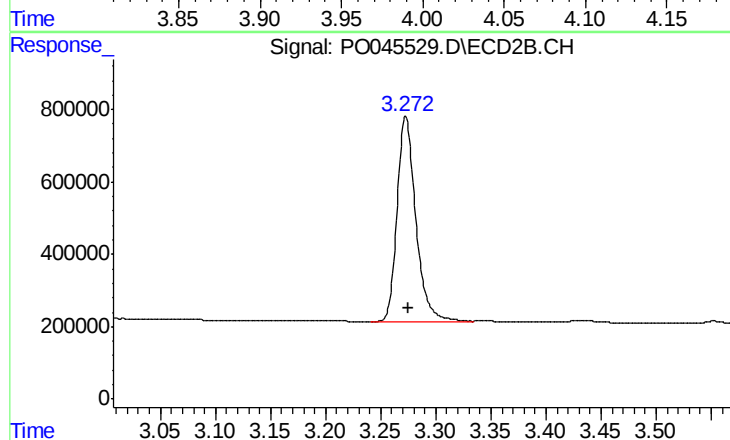


#1 Tetrachloro-m-xylene

R.T.: 3.273 min
Delta R.T.: -0.002 min
Response: 6698185
Conc: 24.16 ng/ml

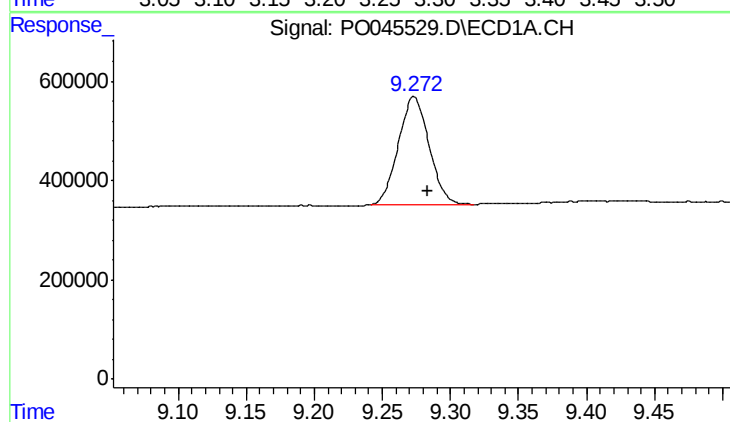

#2 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: -0.010 min
Response: 3416558
Conc: 14.88 ng/ml

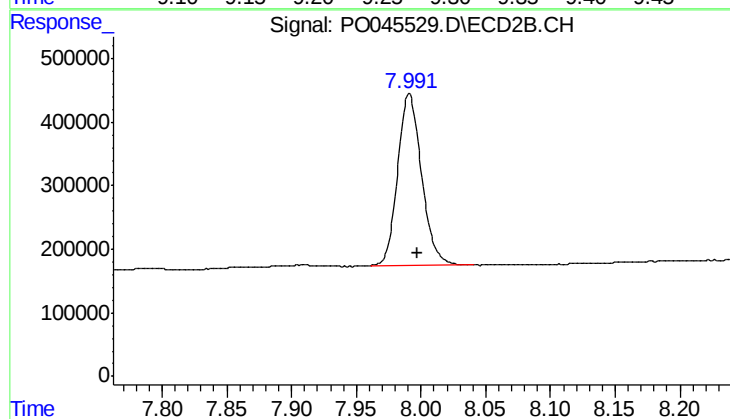

#2 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: -0.006 min
Response: 3450323
Conc: 12.24 ng/ml