

Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060618\
Data File : P0045530.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jun 2018 14:18
Operator : SM/UA
Sample : J3227-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
RO-37426-30-CHERI-LANE

Manual Integrations
APPROVED

UGO
6/6/2018 1:45:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 14:43:26 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.990	3.270	91659	2337	0.439m	0.008m#
2)	SA Decachlor...	9.274	7.971	66261	94928	0.289m	0.337m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060618\
Data File : P0045530.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jun 2018 14:18
Operator : SM/UA
Sample : J3227-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RO-37426-30-CHERI-LANE


Manual Integrations
APPROVED

UGO
6/6/2018 1:45:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 14:43:26 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

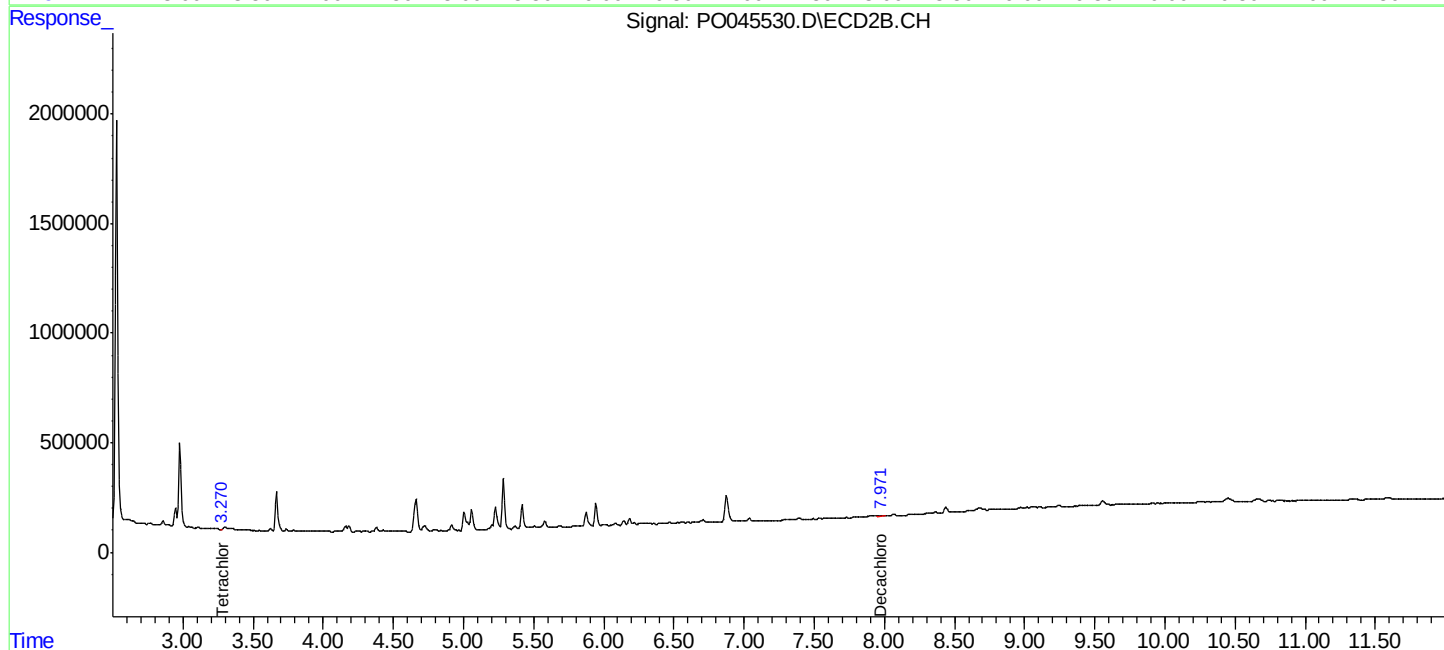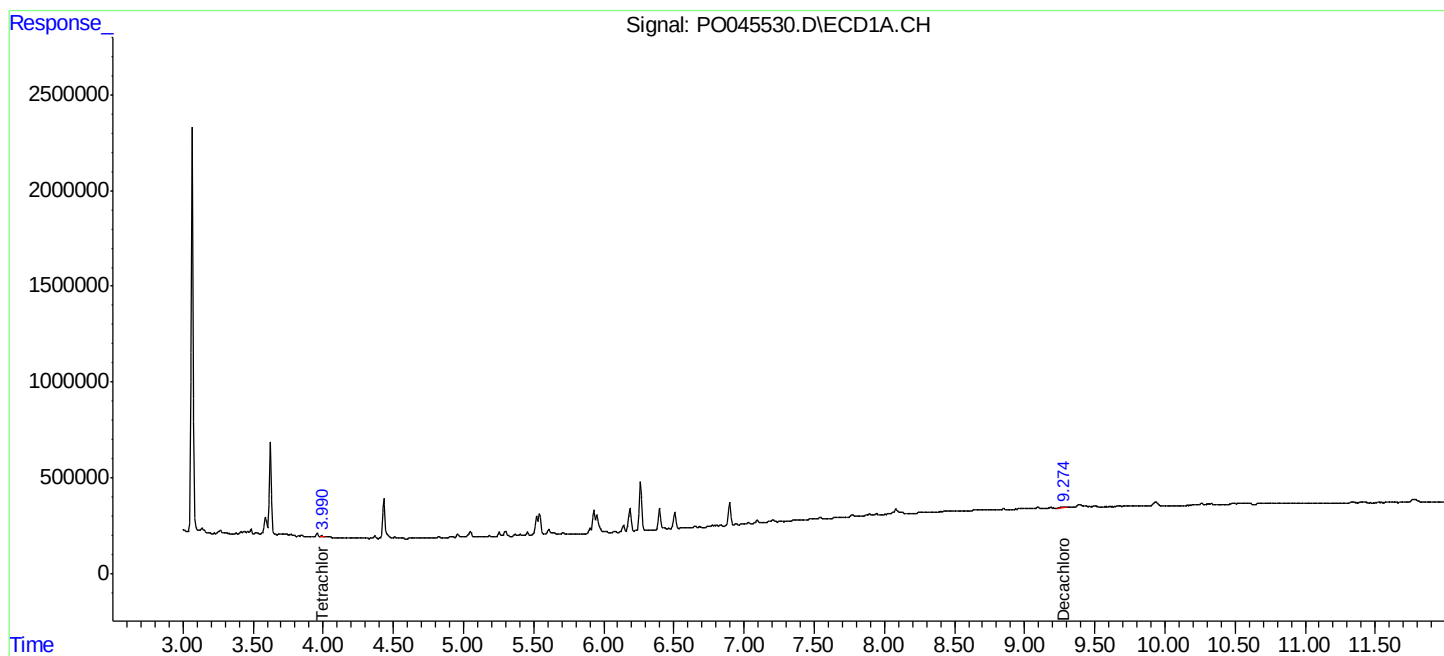

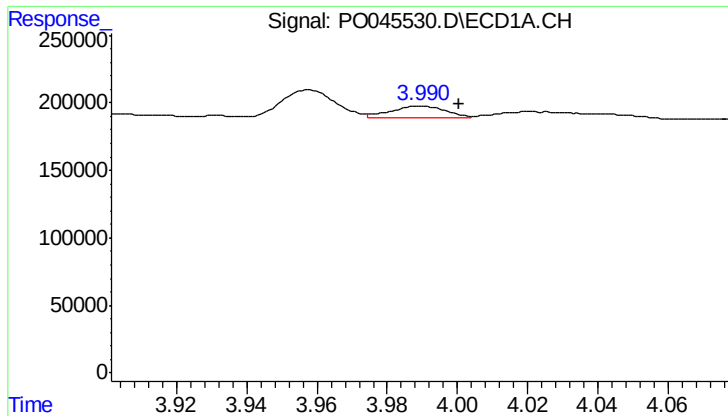


#1 Tetrachloro-m-xylene

R.T.: 3.990 min
Delta R.T.: -0.011 min
Response: 91659
Conc: 0.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-37426-30-CHERI-LANE


Manual Integrations
APPROVED

UGO
6/6/2018 1:45:25 PM

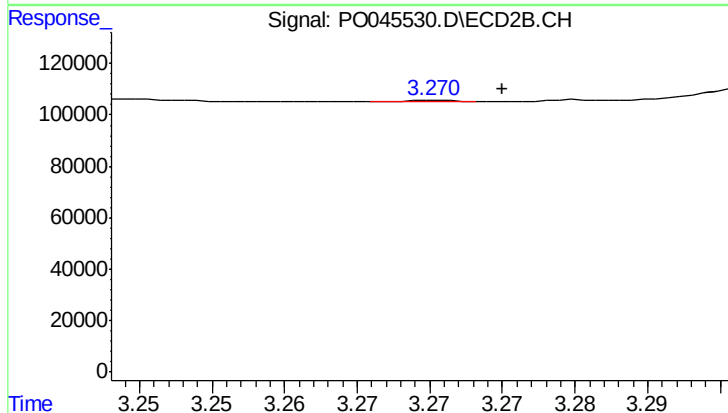


#1 Tetrachloro-m-xylene

R.T.: 3.270 min
Delta R.T.: -0.005 min
Response: 2337
Conc: 0.01 ng/ml m

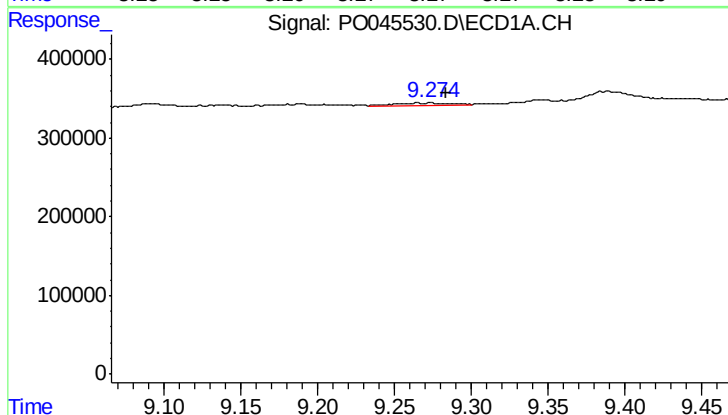

#2 Decachlorobiphenyl

R.T.: 9.274 min
Delta R.T.: -0.010 min
Response: 66261
Conc: 0.29 ng/ml m

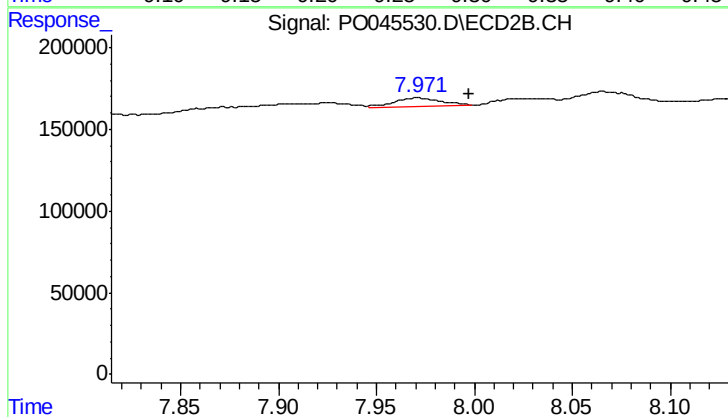

#2 Decachlorobiphenyl

R.T.: 7.971 min
Delta R.T.: -0.026 min
Response: 94928
Conc: 0.34 ng/ml m