

Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060618\
 Data File : P0045533.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jun 2018 15:22
 Operator : SM/UA
 Sample : J3226-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RS-RO-97-20

Manual Integrations
 APPROVED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 17:41:42 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 31 04:53:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	UGO

System Monitoring Compounds							
1) SA Tetrachlo...	4.001	3.278	41269	179185	0.198m	0.646m#	
2) SA Decachlor...	9.290	7.992	93663	52792	0.408m	0.187m#	6/6/2018 1:45:32 PM

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060618\
Data File : P0045533.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jun 2018 15:22
Operator : SM/UA
Sample : J3226-01
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
RS-RO-97-20

Manual Integrations
APPROVED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 17:41:42 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

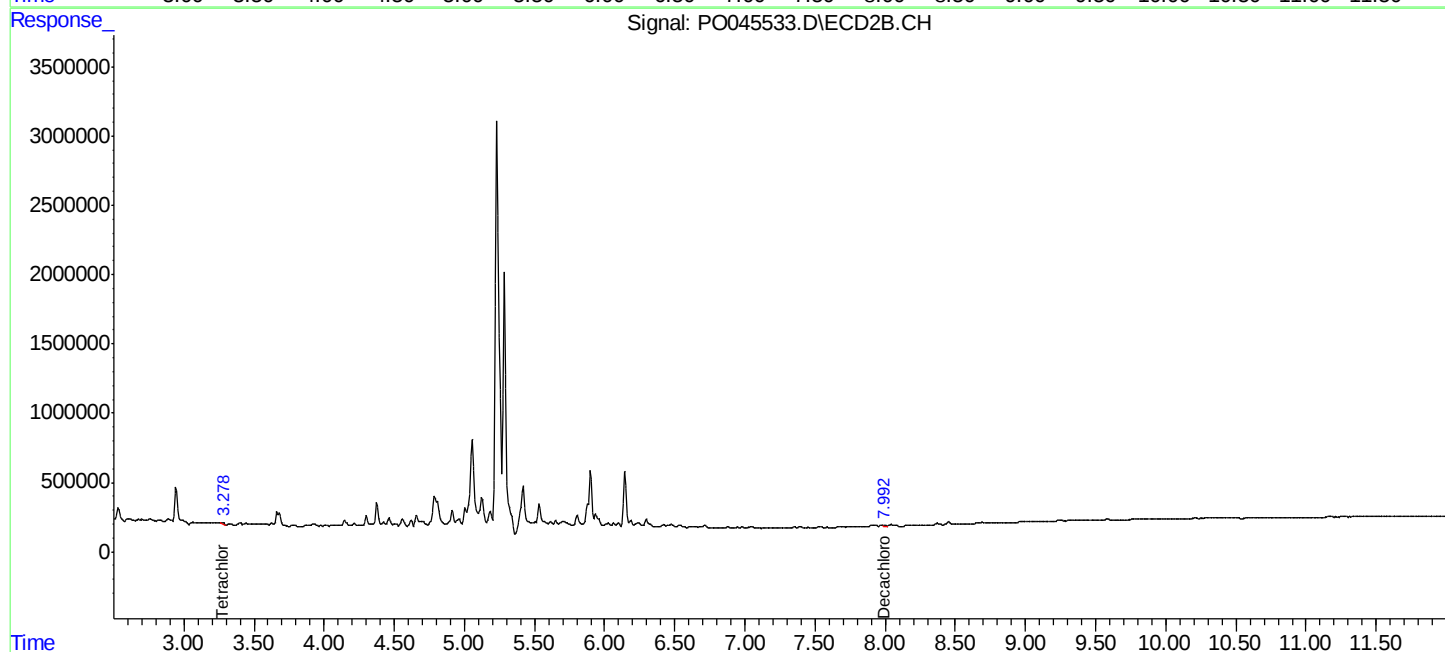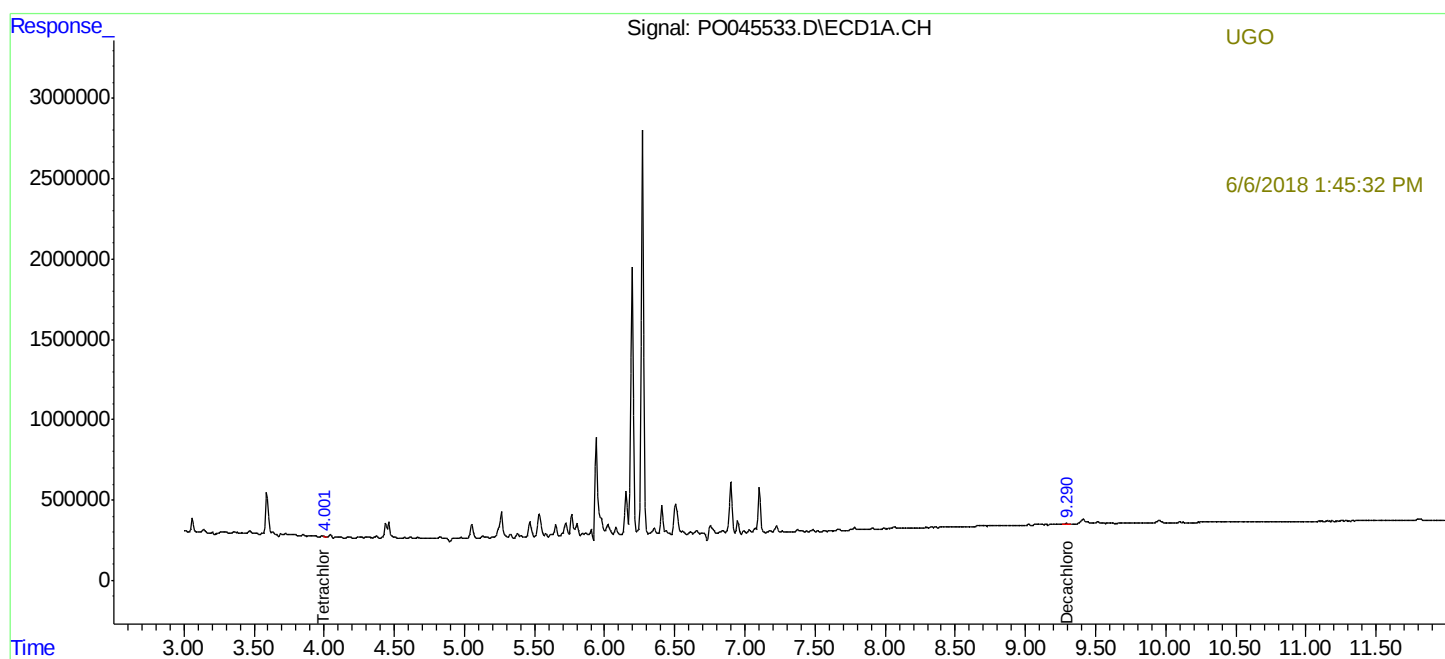

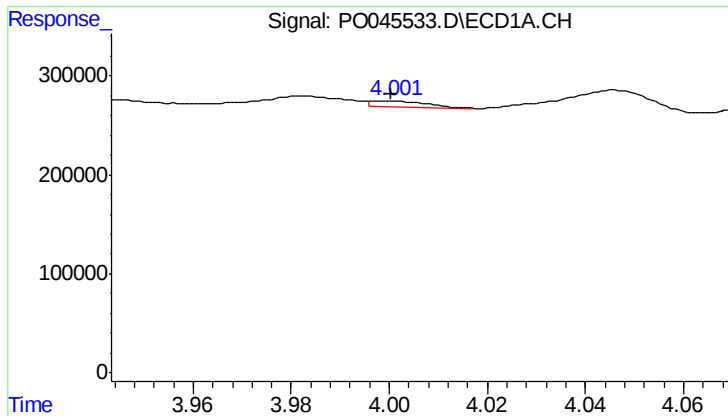


#1 Tetrachloro-m-xylene

R.T.: 4.001 min
Delta R.T.: 0.000 min
Response: 41269
Conc: 0.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
RS-RO-97-20


Manual Integrations
APPROVED

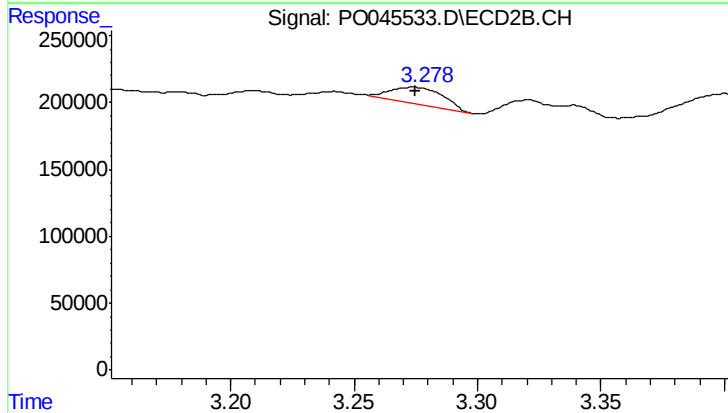

#1 Tetrachloro-m-xylene

R.T.: 3.278 min
Delta R.T.: 0.003 min
Response: 179185
Conc: 0.65 ng/ml m


UGO

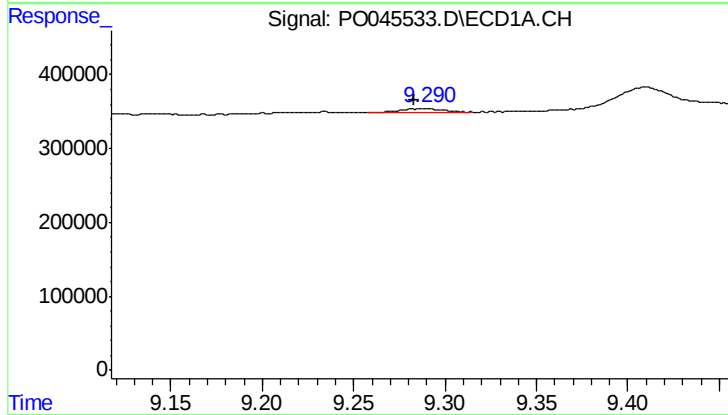

#2 Decachlorobiphenyl

6/6/2018 1:45:32 PM

R.T.: 9.290 min
Delta R.T.: 0.007 min
Response: 93663
Conc: 0.41 ng/ml m

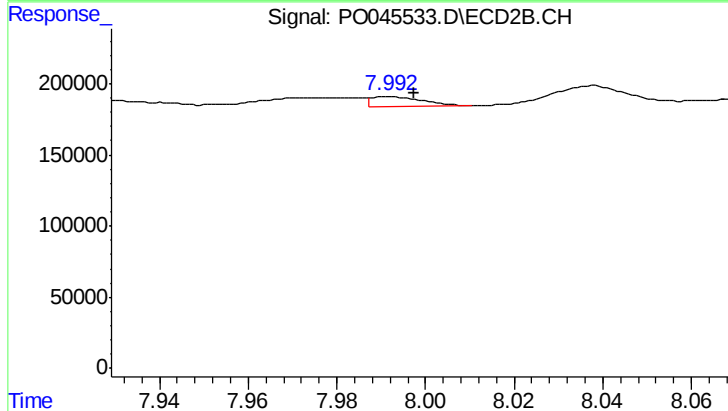

#2 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.006 min
Response: 52792
Conc: 0.19 ng/ml m