

Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060618\
Data File : P0045534.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jun 2018 15:37
Operator : SM/UA
Sample : J3226-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
RS-RB47199RT

Manual Integrations
APPROVED

UGO
6/6/2018 1:45:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 17:44:27 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.998	3.274	9694	24655	0.046m	0.089m#
2)	SA Decachlor...	9.282	7.982	12564	118474	0.055m	0.420m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060618\
Data File : P0045534.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jun 2018 15:37
Operator : SM/UA
Sample : J3226-04
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
RS-RB47199RT


Manual Integrations
APPROVED

UGO
6/6/2018 1:45:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 17:44:27 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

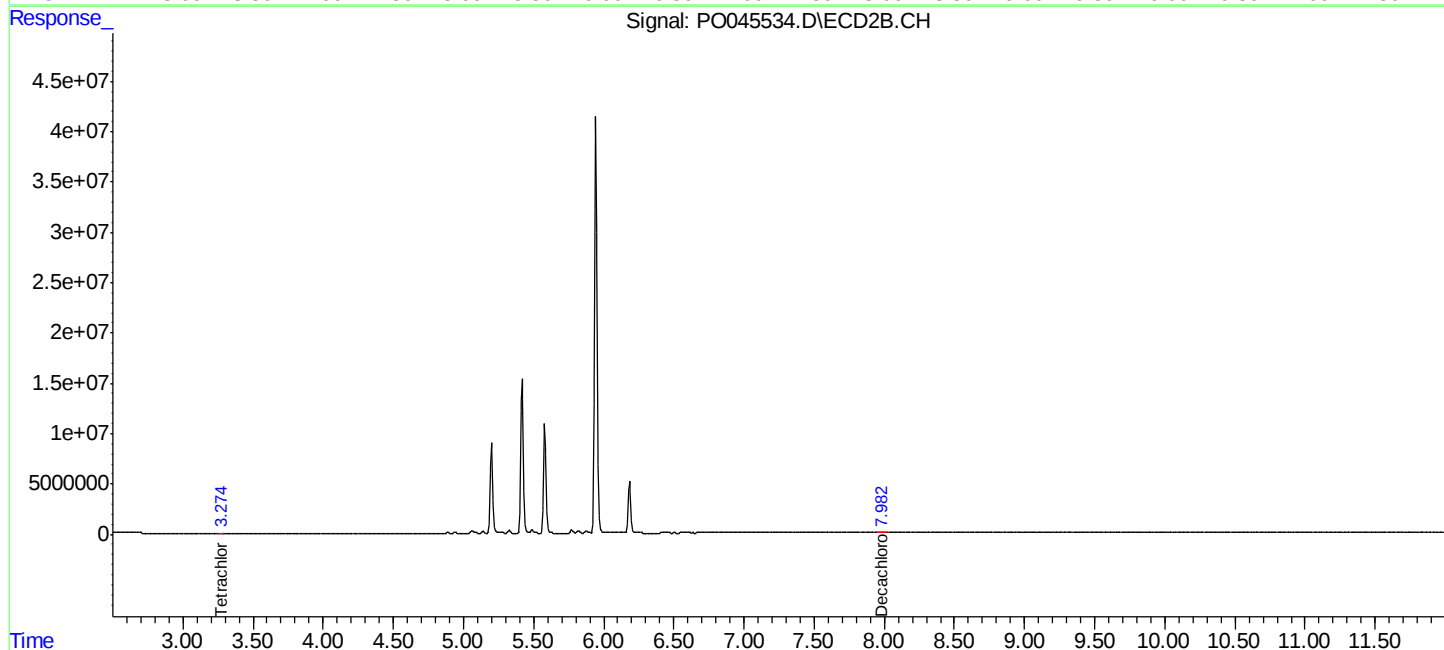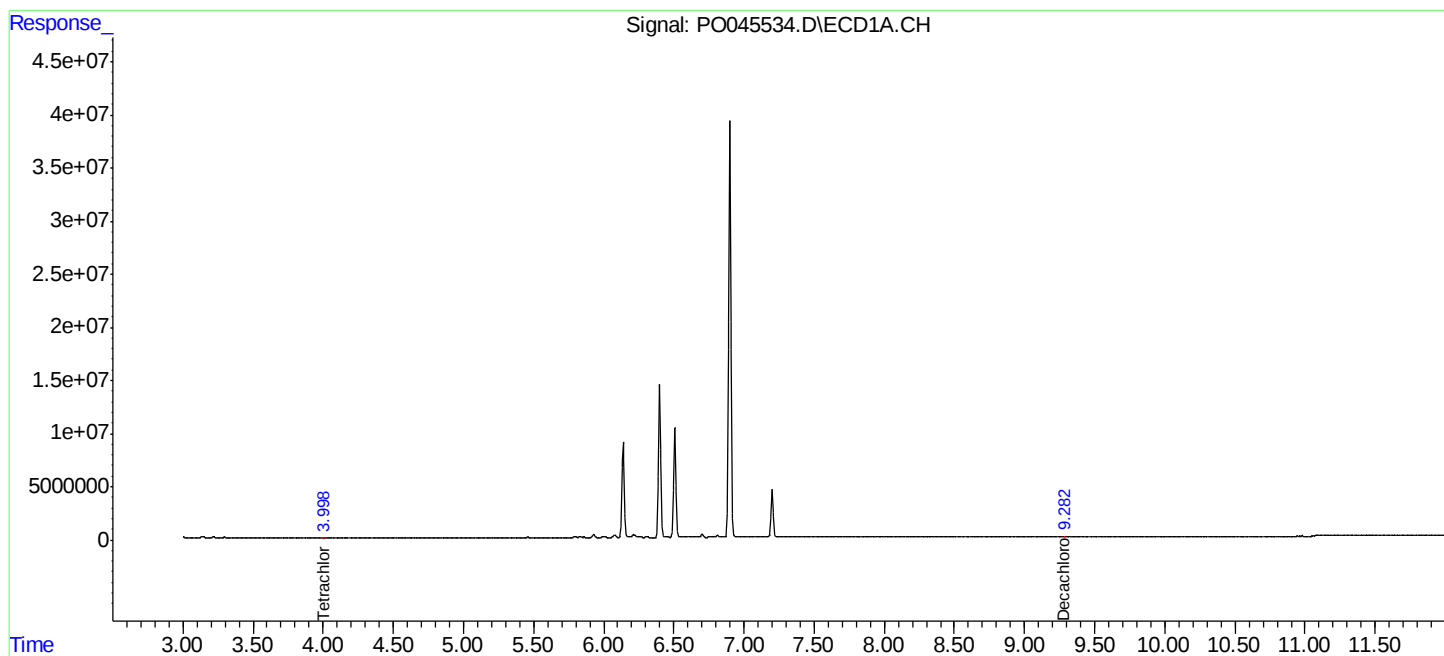

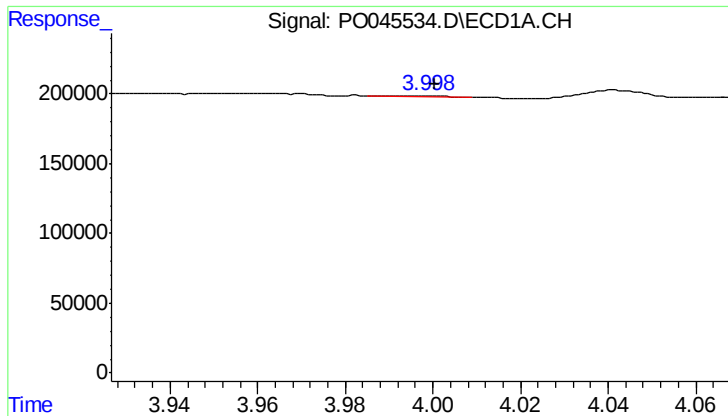


#1 Tetrachloro-m-xylene

R.T.: 3.998 min
Delta R.T.: -0.002 min
Response: 9694
Conc: 0.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
RS-RB47199RT


Manual Integrations
APPROVED

UGO
6/6/2018 1:45:37 PM

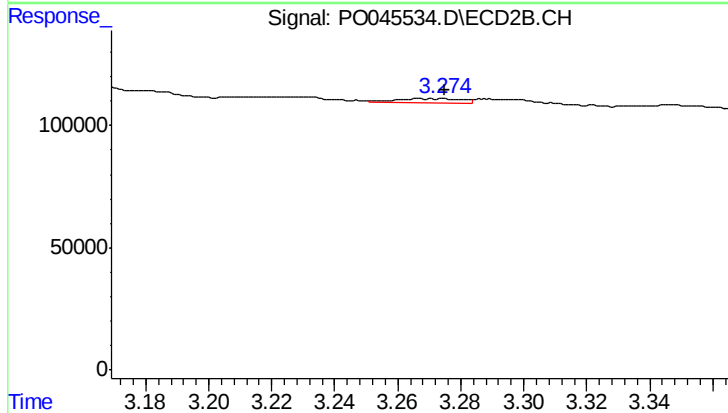


#1 Tetrachloro-m-xylene

R.T.: 3.274 min
Delta R.T.: 0.000 min
Response: 24655
Conc: 0.09 ng/ml m

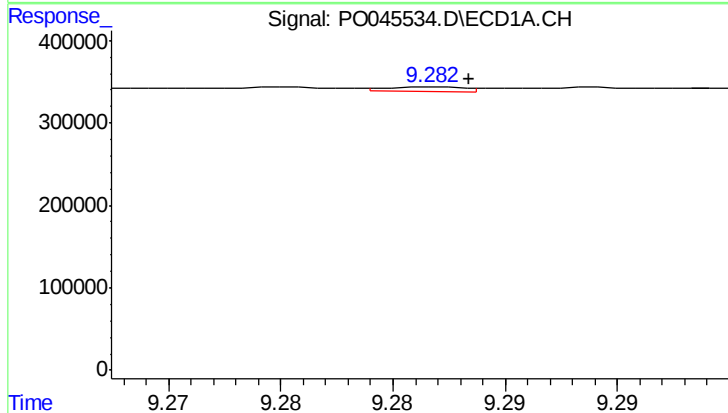

#2 Decachlorobiphenyl

R.T.: 9.282 min
Delta R.T.: -0.002 min
Response: 12564
Conc: 0.05 ng/ml m

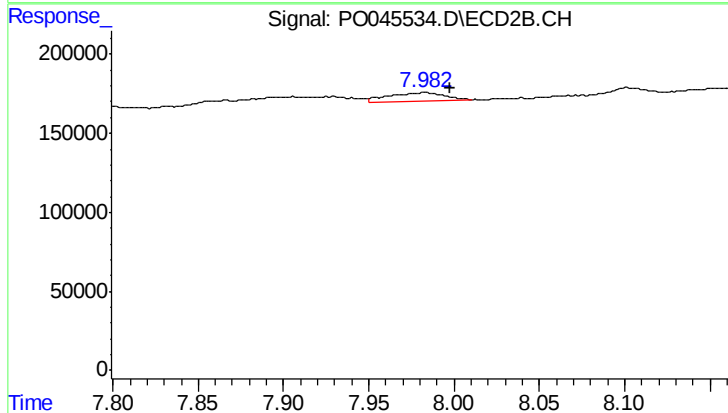

#2 Decachlorobiphenyl

R.T.: 7.982 min
Delta R.T.: -0.015 min
Response: 118474
Conc: 0.42 ng/ml m