

Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060618\
 Data File : P0045549.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jun 2018 20:00
 Operator : SM/UA
 Sample : J3218-05
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 INSIDE-WELL-SP

Manual Integrations
 APPROVED

UGO
 6/6/2018 1:45:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 00:42:45 2018
 Quant Method : Y:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 31 04:53:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.994	3.271	5218696	7198546	24.985	25.960
2) SA Decachlor...	9.270	7.989	3187126	3658143	13.877m	12.979m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060618\
Data File : P0045549.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jun 2018 20:00
Operator : SM/UA
Sample : J3218-05
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
INSIDE-WELL-SP


Manual Integrations
APPROVED

UGO
6/6/2018 1:45:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 00:42:45 2018
Quant Method : Y:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

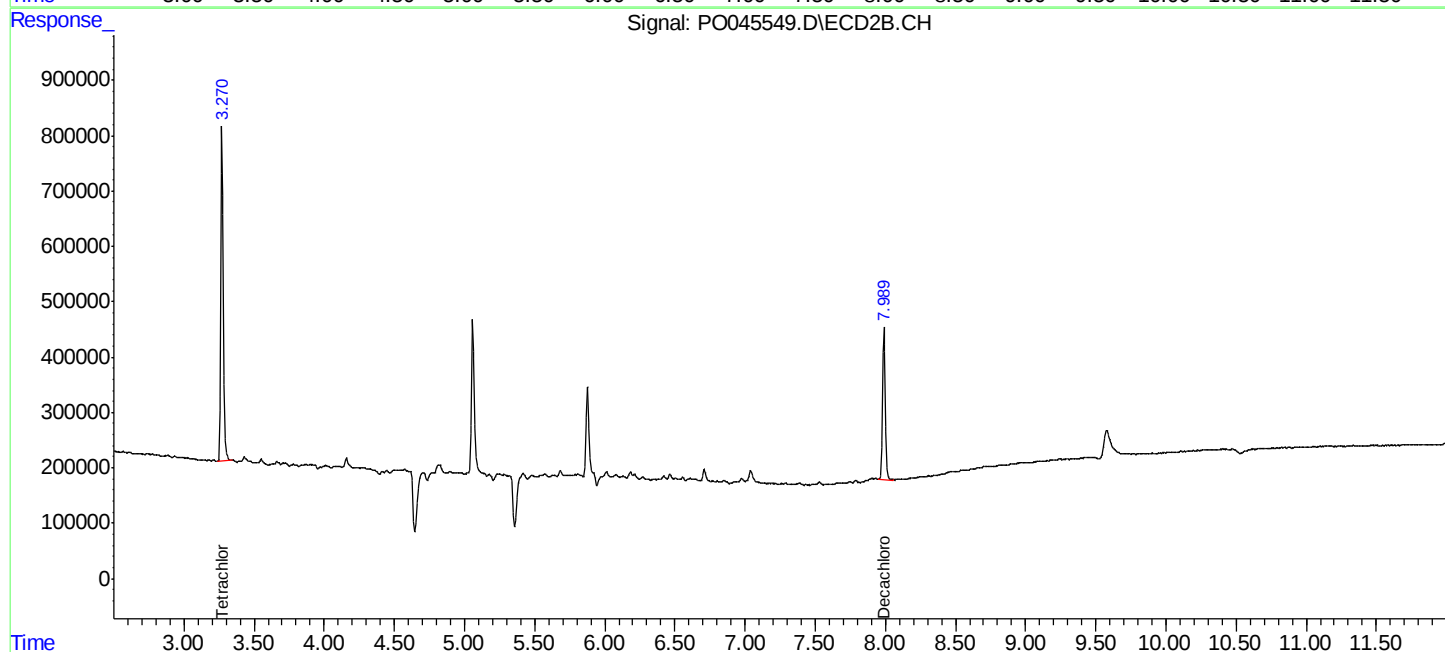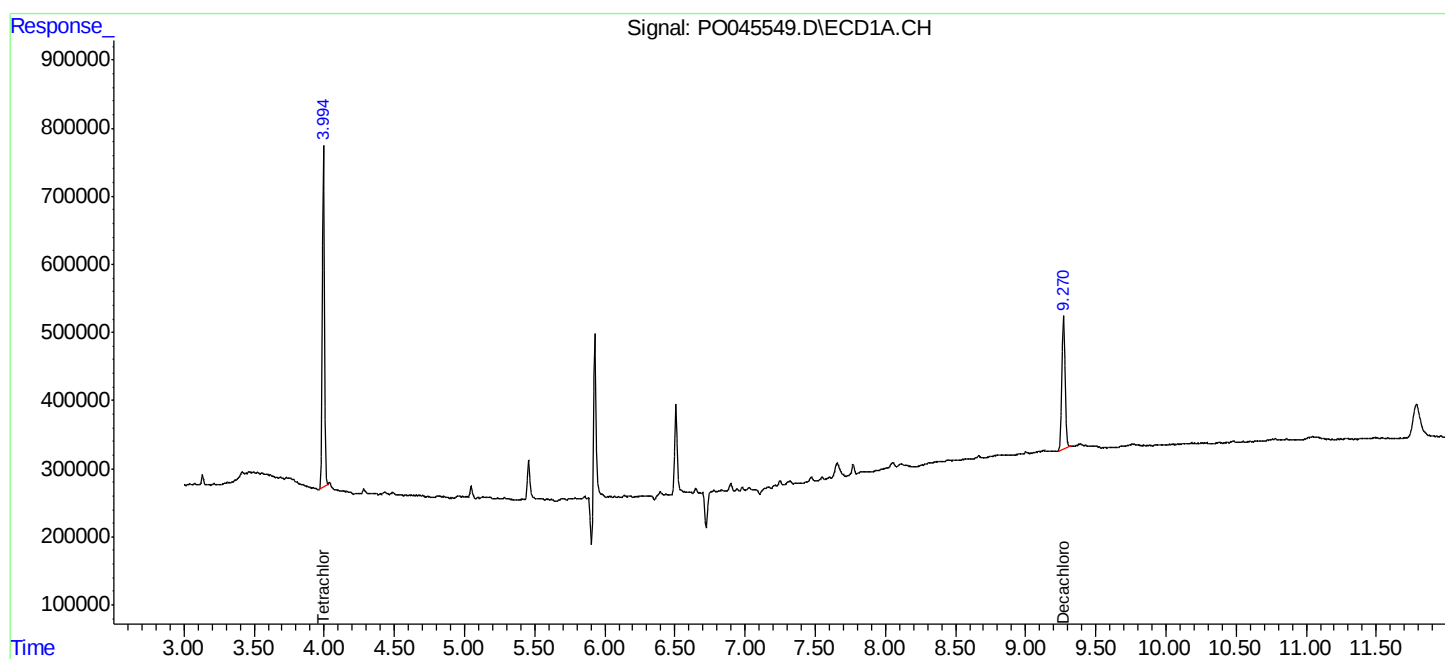

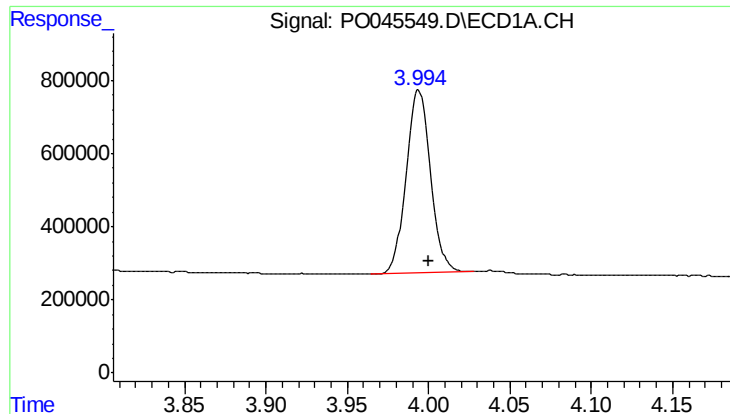


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.006 min
Response: 5218696
Conc: 24.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
INSIDE-WELL-SP


Manual Integrations
APPROVED

UGO
6/6/2018 1:45:51 PM

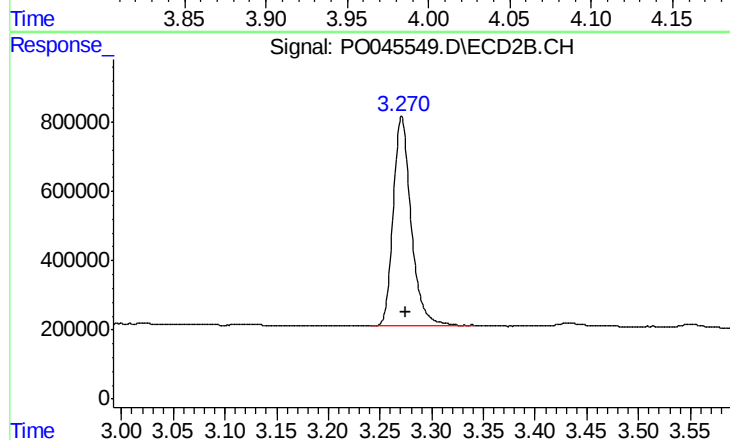


#1 Tetrachloro-m-xylene

R.T.: 3.271 min
Delta R.T.: -0.004 min
Response: 7198546
Conc: 25.96 ng/ml

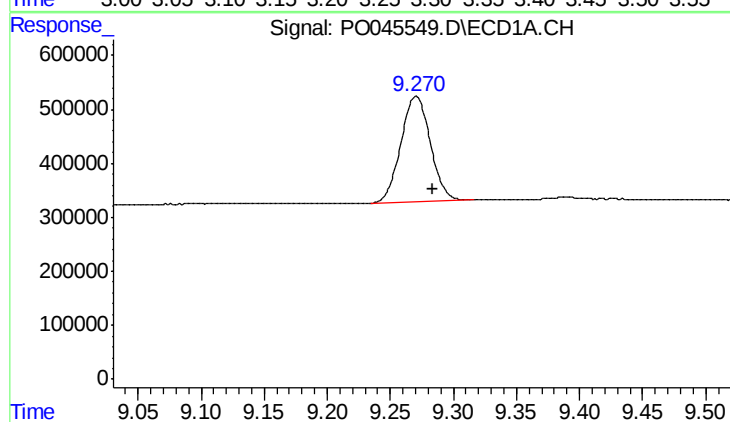

#2 Decachlorobiphenyl

R.T.: 9.270 min
Delta R.T.: -0.013 min
Response: 3187126
Conc: 13.88 ng/ml m

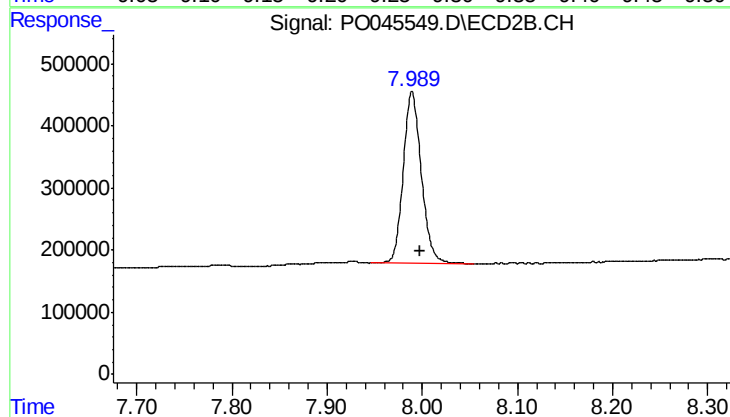

#2 Decachlorobiphenyl

R.T.: 7.989 min
Delta R.T.: -0.009 min
Response: 3658143
Conc: 12.98 ng/ml m