

Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060618\
 Data File : P0045551.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jun 2018 20:31
 Operator : SM/UA
 Sample : J3271-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-7A-WC-2

Manual Integrations
 APPROVED

UGO
 6/6/2018 1:45:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 00:44:39 2018
 Quant Method : Y:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 31 04:53:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.995	3.271	5063378	6734190	24.241	24.286
2) SA Decachlor...	9.272	7.991	3402474	3938196	14.815m	13.973

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\PO060618\
Data File : PO045551.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jun 2018 20:31
Operator : SM/UA
Sample : J3271-03
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-7A-WC-2


Manual Integrations
APPROVED

UGO
6/6/2018 1:45:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 00:44:39 2018
Quant Method : Y:\PESTPCBSRV\HPCHEM1\ECD_0\methods\PO053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

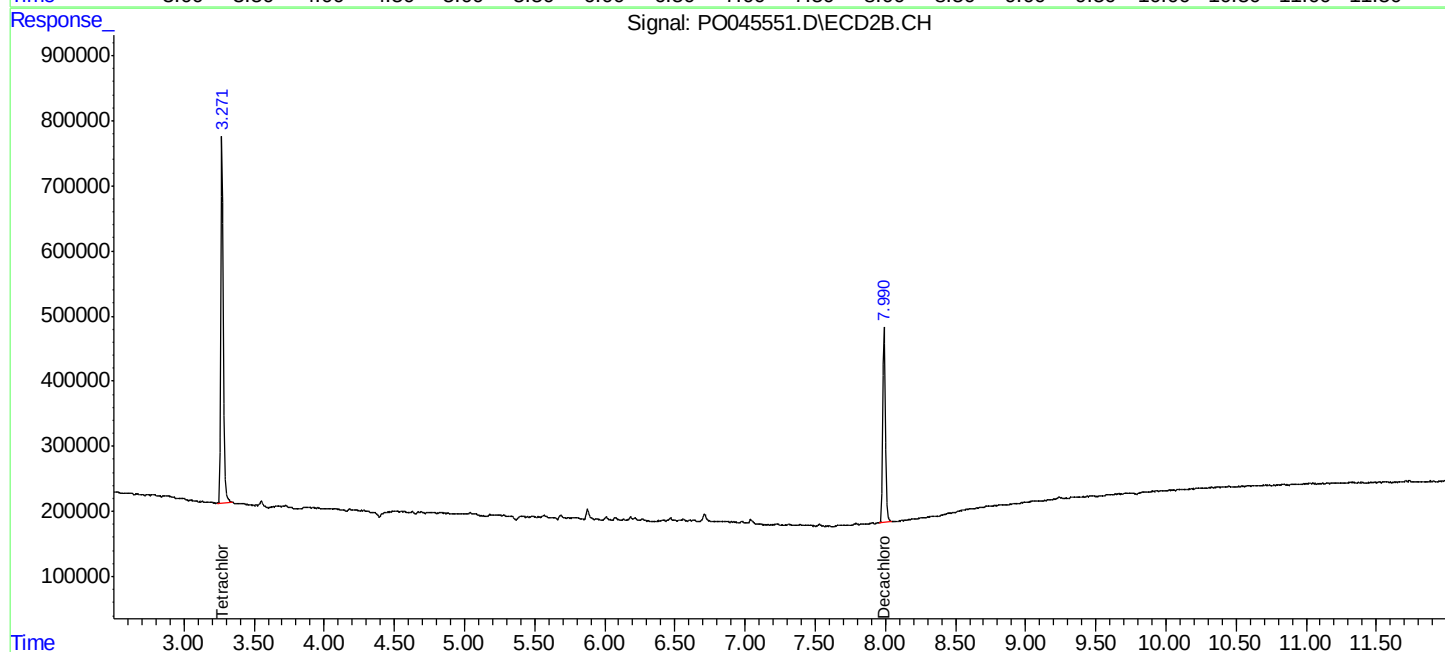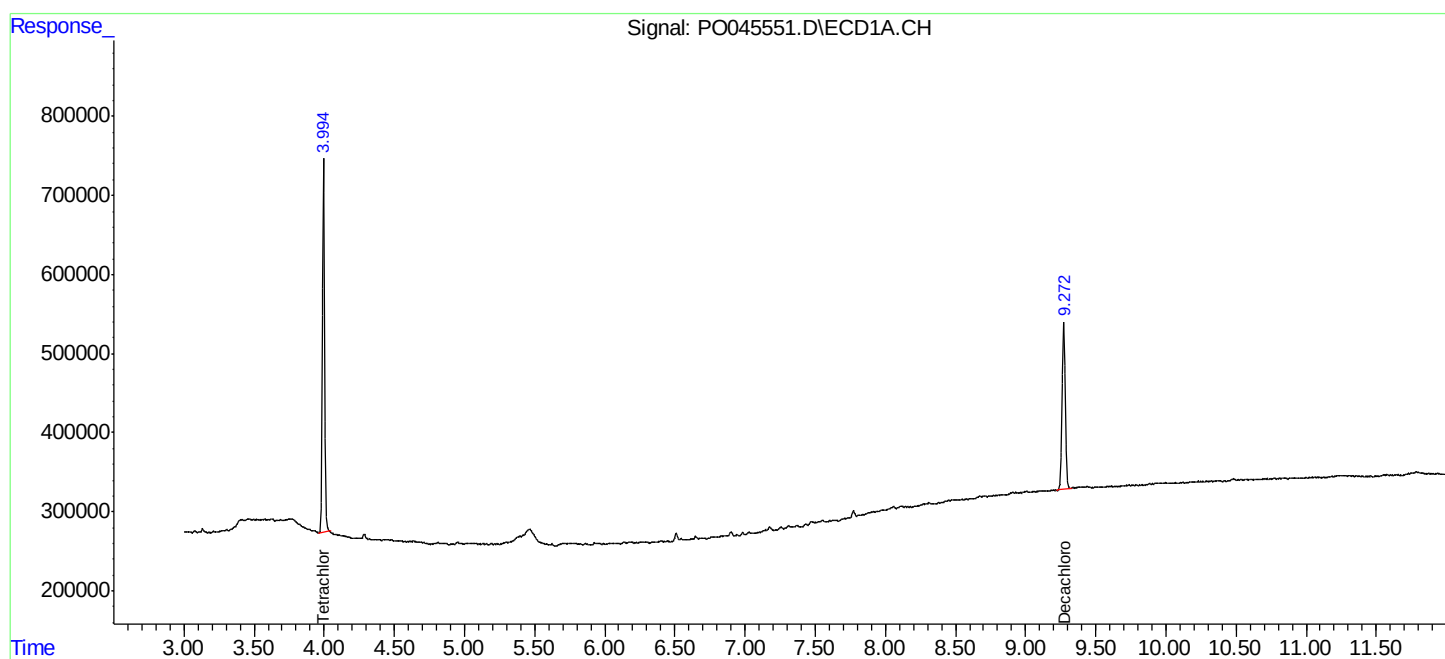

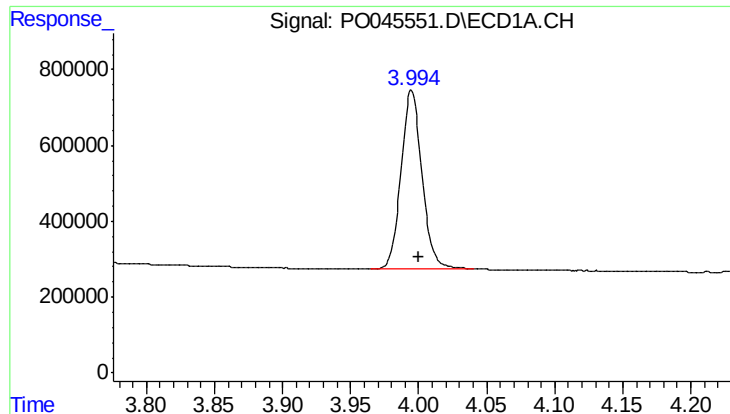


#1 Tetrachloro-m-xylene

R.T.: 3.995 min
Delta R.T.: -0.006 min
Response: 5063378
Conc: 24.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-7A-WC-2


Manual Integrations
APPROVED

UGO
6/6/2018 1:45:54 PM

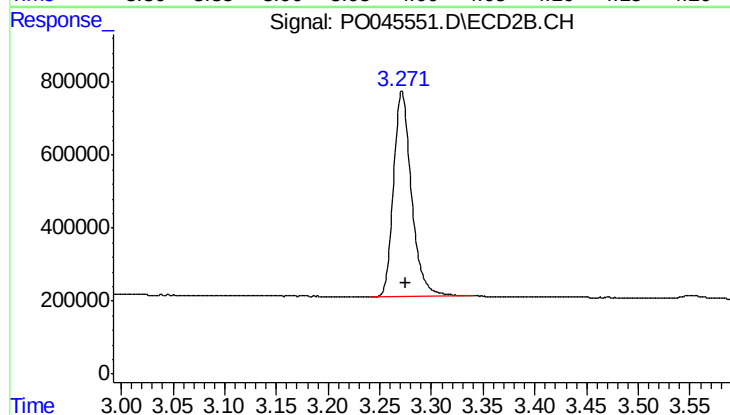


#1 Tetrachloro-m-xylene

R.T.: 3.271 min
Delta R.T.: -0.004 min
Response: 6734190
Conc: 24.29 ng/ml

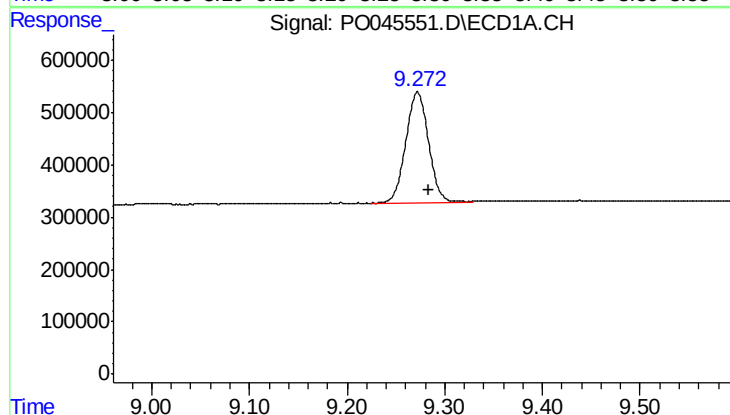

#2 Decachlorobiphenyl

R.T.: 9.272 min
Delta R.T.: -0.012 min
Response: 3402474
Conc: 14.81 ng/ml m

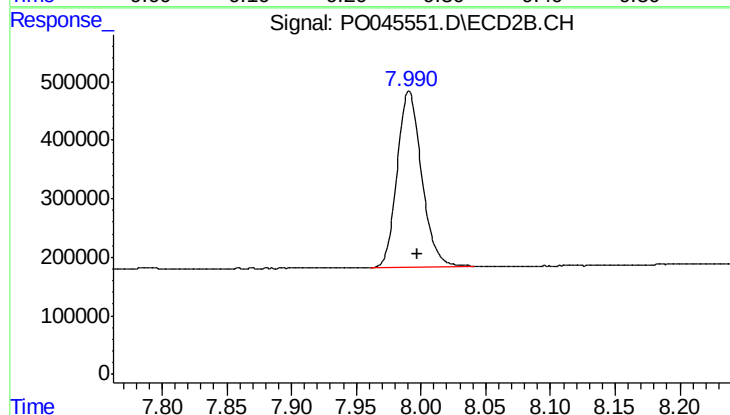

#2 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: -0.006 min
Response: 3938196
Conc: 13.97 ng/ml