

Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\P0060618\
Data File : P0045564.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jun 2018 23:53
Operator : SM/UA
Sample : J3271-07
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-7A-WC-4

Manual Integrations
APPROVED

UGO
6/6/2018 1:46:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 01:21:10 2018
Quant Method : Y:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.993	3.270	5134792	7016767	24.583	25.305
2) SA Decachlor...	9.267	7.988	3079924	3514039	13.410m	12.468

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\PESTPCBSRV\HPCHEM1\ECD 0\Data\PO060618\
Data File : PO045564.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jun 2018 23:53
Operator : SM/UA
Sample : J3271-07
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-7A-WC-4


Manual Integrations
APPROVED

UGO
6/6/2018 1:46:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 01:21:10 2018
Quant Method : Y:\PESTPCBSRV\HPCHEM1\ECD_0\methods\PO053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

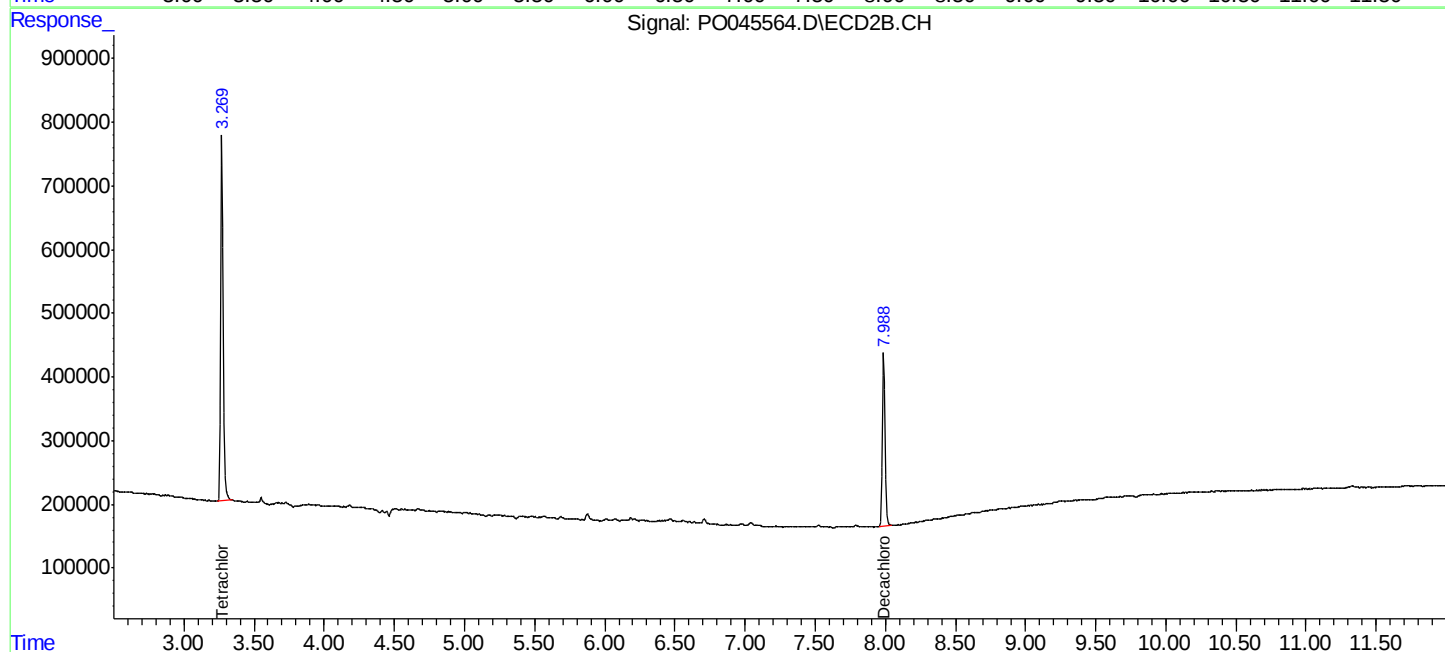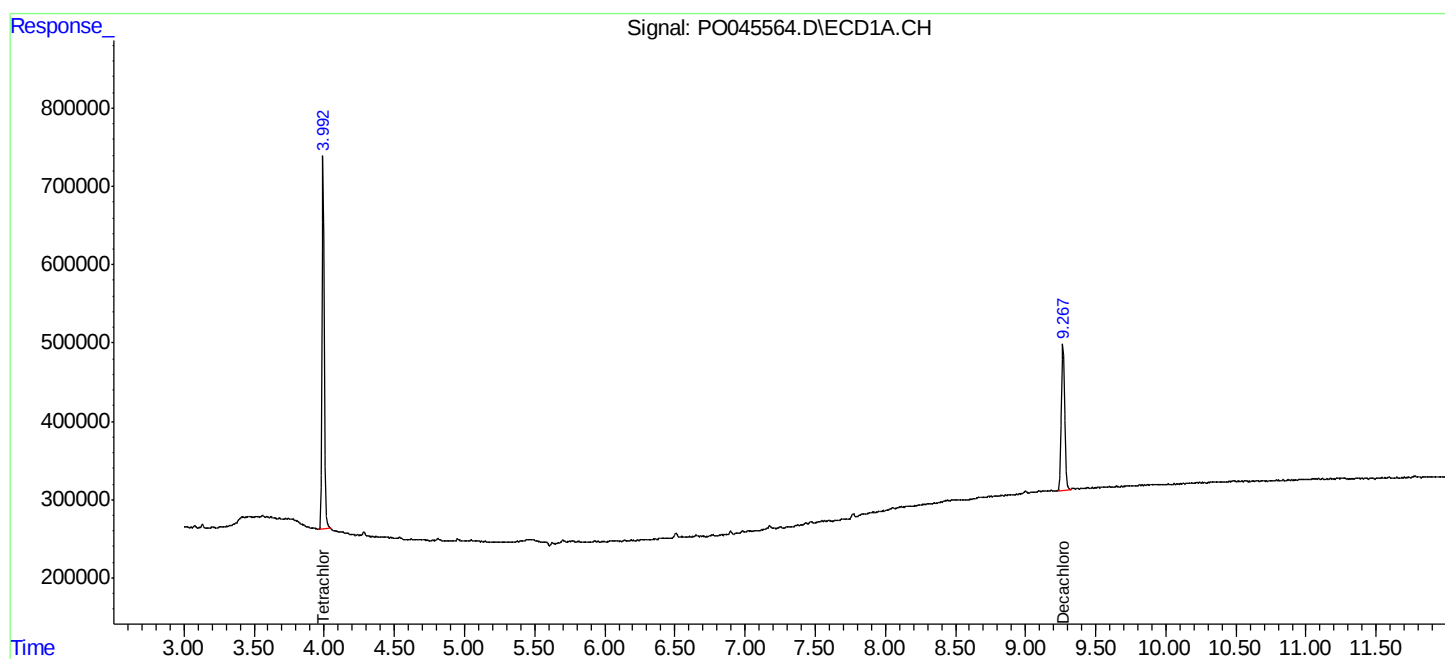

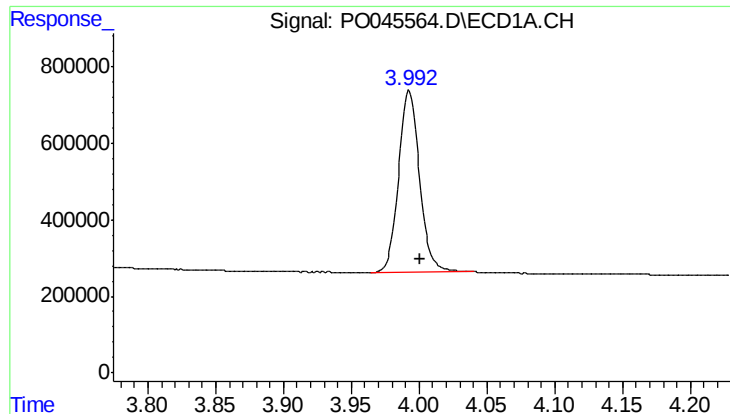


#1 Tetrachloro-m-xylene

R.T.: 3.993 min
Delta R.T.: -0.008 min
Response: 5134792
Conc: 24.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-7A-WC-4


Manual Integrations
APPROVED

UGO
6/6/2018 1:46:46 PM

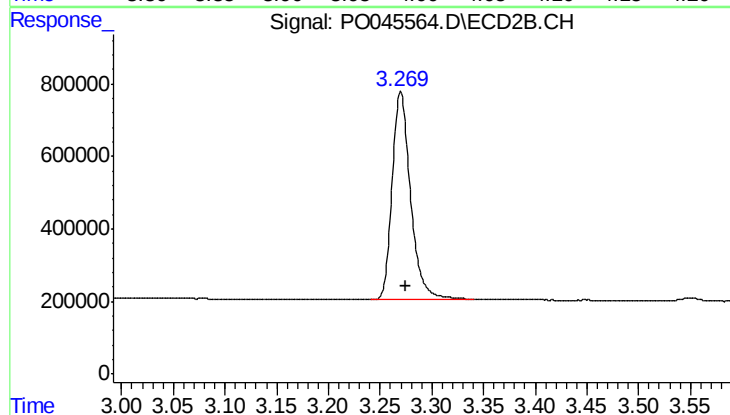


#1 Tetrachloro-m-xylene

R.T.: 3.270 min
Delta R.T.: -0.005 min
Response: 7016767
Conc: 25.30 ng/ml

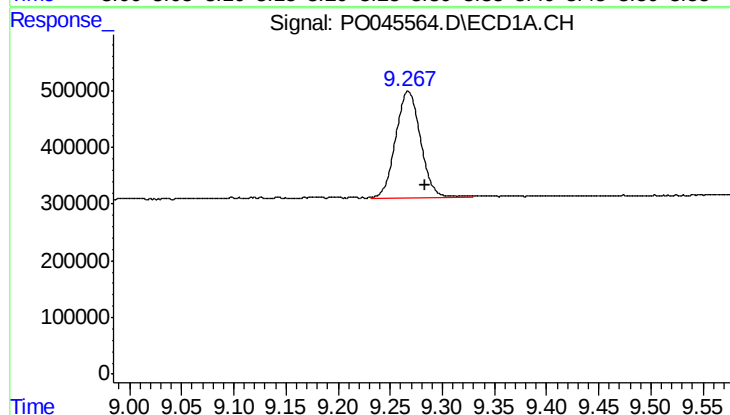

#2 Decachlorobiphenyl

R.T.: 9.267 min
Delta R.T.: -0.017 min
Response: 3079924
Conc: 13.41 ng/ml m

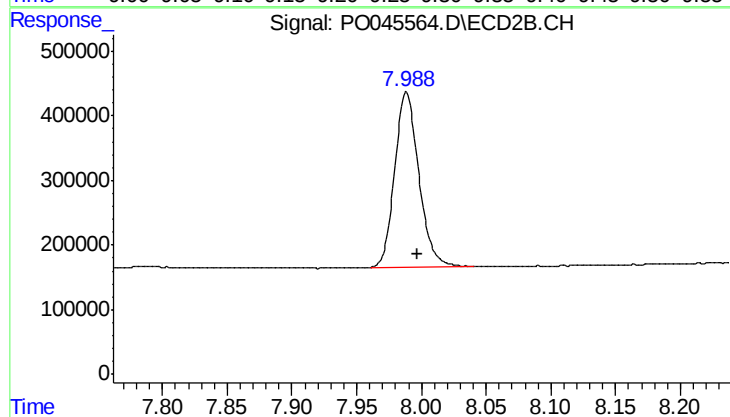

#2 Decachlorobiphenyl

R.T.: 7.988 min
Delta R.T.: -0.009 min
Response: 3514039
Conc: 12.47 ng/ml