

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0060619\
 Data File : P0056918.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jun 2019 12:01
 Operator : SM/SJ
 Sample : K3175-01MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-03-007-ABCDMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 12:47:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.254	3.566	990497	781987	25.873	23.712
2)	SA Decachlor...	9.829	8.502	990716	673181	20.184	18.879
Target Compounds							
3)	L1 AR-1016-1	0.000	4.635	0	172945	N.D.	137.423 #
4)	L1 AR-1016-2	0.000	4.653	0	236708	N.D.	131.386 #
5)	L1 AR-1016-3	0.000	4.828	0	127620	N.D.	129.439 #
6)	L1 AR-1016-4	0.000	4.868	0	105512	N.D.	127.455 #
7)	L1 AR-1016-5	0.000	5.080	0	106872	N.D.	99.627 #
9)	L2 AR-1221-2	0.000	3.862	0	26786	N.D.	71.075 #
10)	L2 AR-1221-3	0.000	3.936	0	77360	N.D.	64.625 #
11)	L3 AR-1232-1	0.000	3.936	0	77360	N.D.	86.112 #
12)	L3 AR-1232-2	0.000	4.653	0	236708	N.D.	243.557 #
13)	L3 AR-1232-3	0.000	4.828	0	127620	N.D.	243.879 #
14)	L3 AR-1232-4	0.000	4.909	0	124827	N.D.	253.360 #
15)	L3 AR-1232-5	0.000	5.080	0	106872	N.D.	189.740 #
16)	L4 AR-1242-1	0.000	4.635	0	172945	N.D.	139.631 #
17)	L4 AR-1242-2	0.000	4.653	0	236708	N.D.	131.620 #
18)	L4 AR-1242-3	0.000	4.828	0	127620	N.D.	129.813 #
19)	L4 AR-1242-4	0.000	4.909	0	124827	N.D.	128.278 #
20)	L4 AR-1242-5	0.000	5.427	0	100858	N.D.	85.309 #
21)	L5 AR-1248-1	0.000	4.635	0	172945	N.D.	184.668 #
22)	L5 AR-1248-2	0.000	4.868	0	105512	N.D.	83.051 #
23)	L5 AR-1248-3	0.000	4.909	0	124827	N.D.	95.587 #
24)	L5 AR-1248-4	0.000	5.080	0	106872	N.D.	67.486 #
25)	L5 AR-1248-5	0.000	5.427	0	100858	N.D.	60.939 #
26)	L6 AR-1254-1	0.000	5.427	0	100858	N.D.	38.136 #
27)	L6 AR-1254-2	0.000	5.573	0	100172	N.D.	46.466 #
28)	L6 AR-1254-3	0.000	5.986	0	186727	N.D.	51.003 #
29)	L6 AR-1254-4	0.000	6.229	0	55504	N.D.	25.264 #
30)	L6 AR-1254-5	7.542	6.613	534202	340333	141.862	107.353
31)	L7 AR-1260-1	7.004	6.101	314892	262561	122.708	131.255
32)	L7 AR-1260-2	7.260	6.289	398073	333558	131.631	135.320
33)	L7 AR-1260-3	0.000	6.440	0	293139	N.D.	130.677 #
34)	L7 AR-1260-4	0.000	6.907	0	217085	N.D.	116.648 #
35)	L7 AR-1260-5	8.148	7.149	578144	470256	120.898	109.049
36)	L8 AR-1262-1	0.000	6.649	0	264379	N.D.	63.339 #
37)	L8 AR-1262-2	8.148	7.149	578144	470256	75.834	68.444
38)	L8 AR-1262-3	0.000	7.427	0	107030	N.D.	36.239 #
39)	L8 AR-1262-4	0.000	7.492	0	349246	N.D.	67.026 #
40)	L8 AR-1262-5	0.000	7.986	0	107038	N.D.	46.094 #
41)	L9 AR-1268-1	0.000	7.427	0	107030	N.D.	14.337 #
42)	L9 AR-1268-2	0.000	7.492	0	349246	N.D.	50.013 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060619\
Data File : P0056918.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2019 12:01
Operator : SM/SJ
Sample : K3175-01MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 12:47:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44)	L9 AR-1268-4	0.000	7.986	0	107038	N.D.	45.855 #
45)	L9 AR-1268-5	0.000	8.263	0	33172	N.D.	1.917 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060619\
Data File : P0056918.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2019 12:01
Operator : SM/SJ
Sample : K3175-01MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 12:47:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

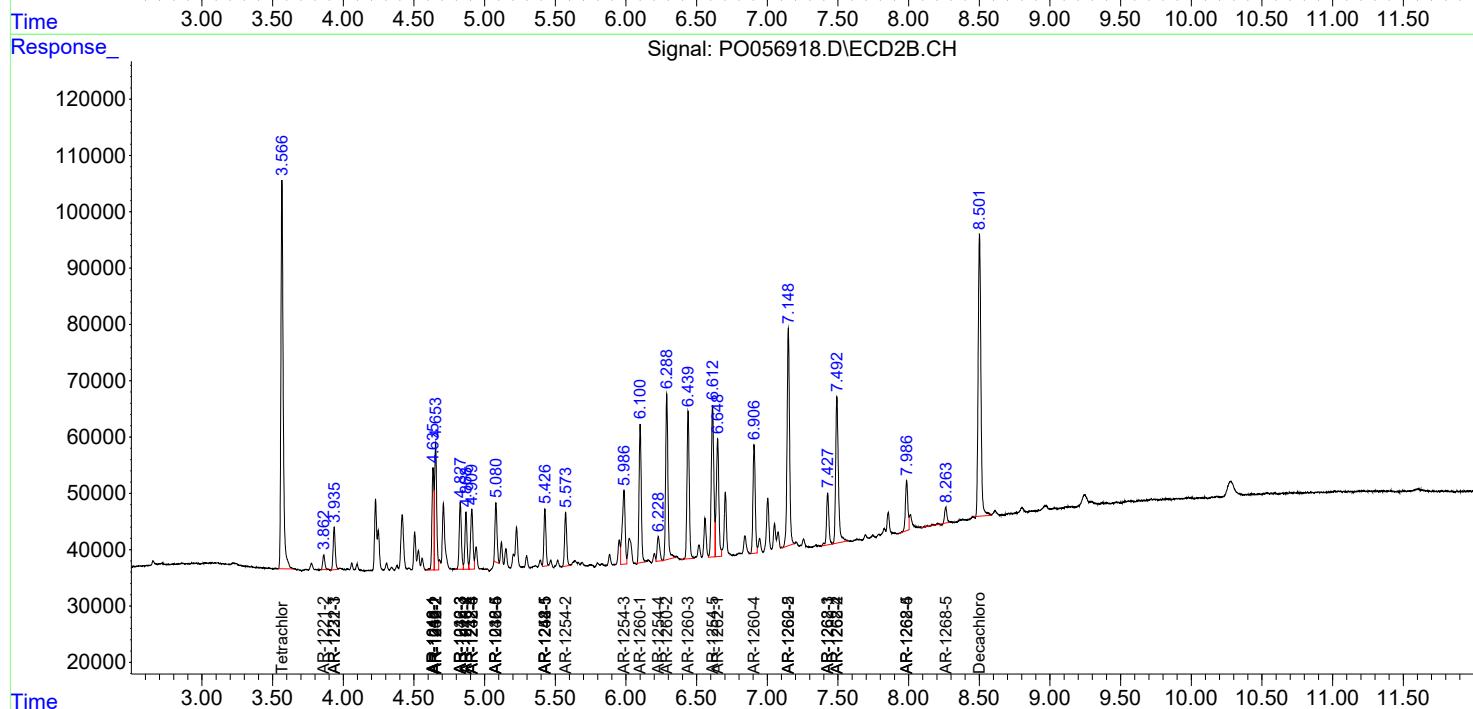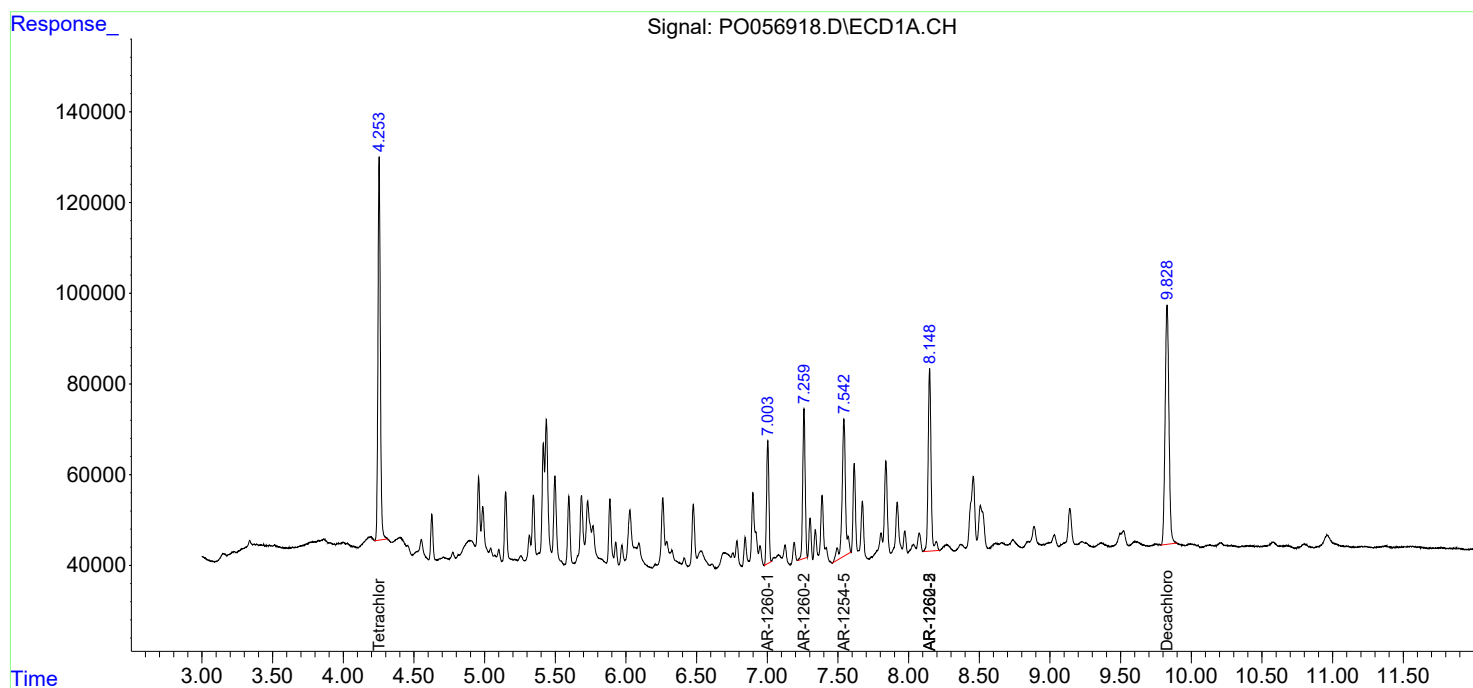


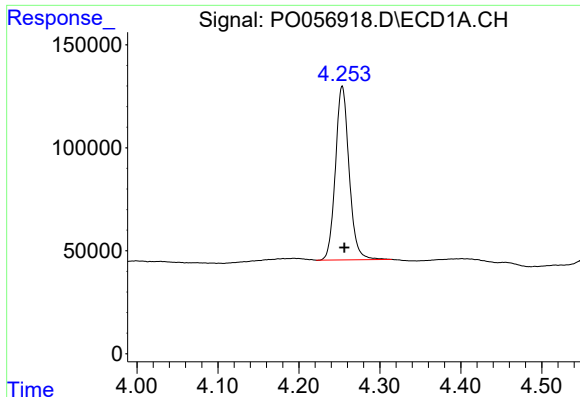

#1 Tetrachloro-m-xylene


R.T.: 4.254 min
Delta R.T.: -0.002 min
Response: 990497
Conc: 25.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

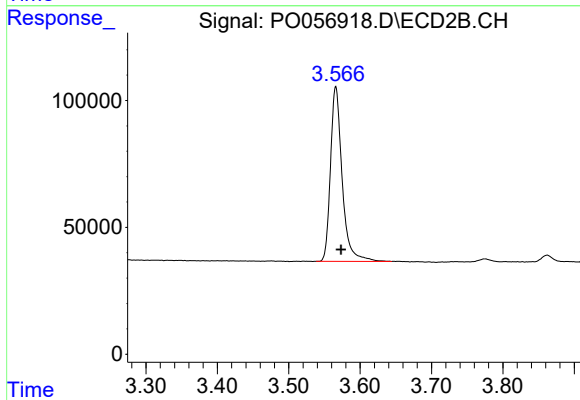


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: -0.007 min
Response: 781987
Conc: 23.71 ng/ml

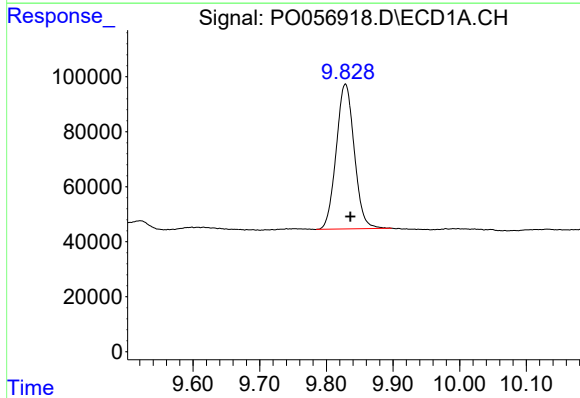


#2 Decachlorobiphenyl

R.T.: 9.829 min
Delta R.T.: -0.008 min
Response: 990716
Conc: 20.18 ng/ml

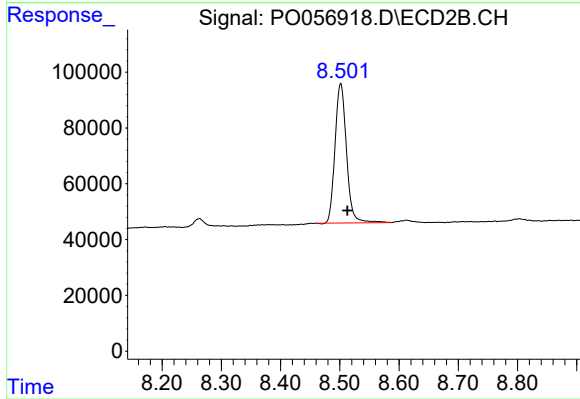

#2 Decachlorobiphenyl


R.T.: 8.502 min
Delta R.T.: -0.011 min
Response: 673181
Conc: 18.88 ng/ml

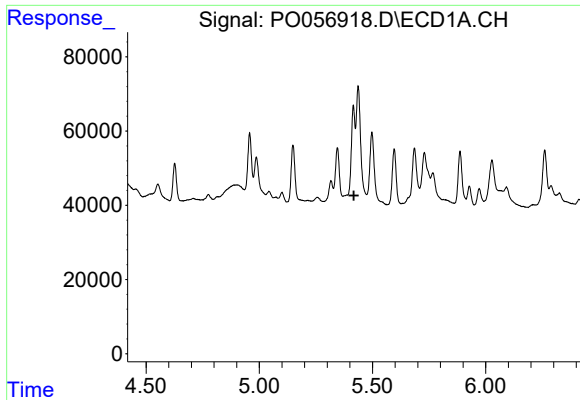

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

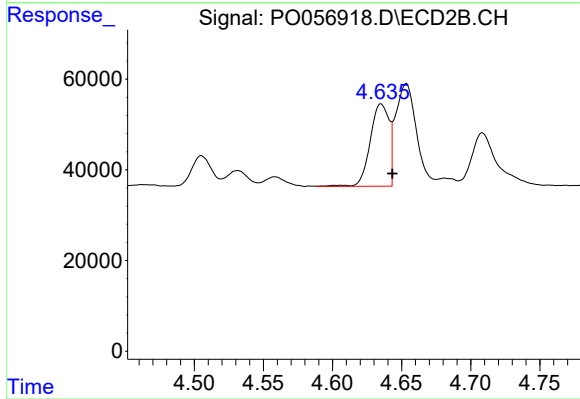


#3 AR-1016-1

R.T.: 4.635 min
Delta R.T.: -0.008 min
Response: 172945
Conc: 137.42 ng/ml

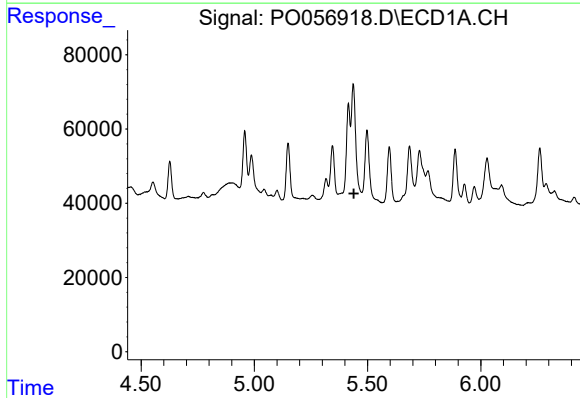


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.440 min
Response: 0
Conc: N.D.

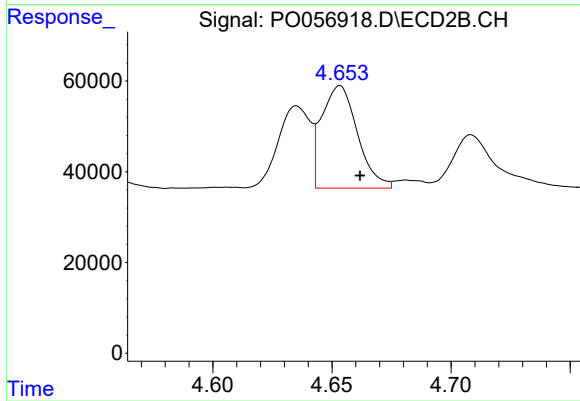

#4 AR-1016-2


R.T.: 4.653 min
Delta R.T.: -0.008 min
Response: 236708
Conc: 131.39 ng/ml

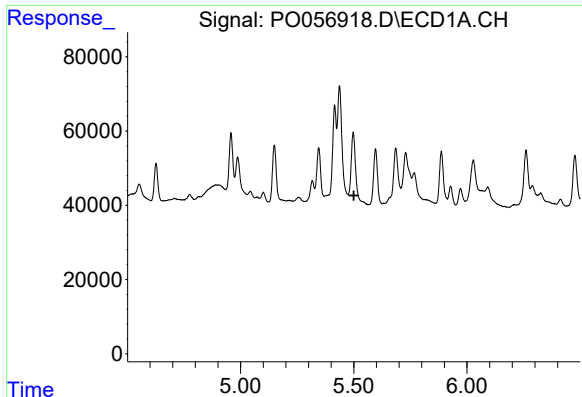

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.500 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

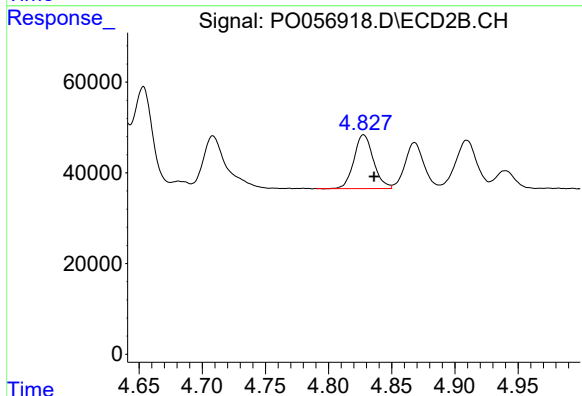


#5 AR-1016-3

R.T.: 4.828 min
Delta R.T.: -0.008 min
Response: 127620
Conc: 129.44 ng/ml

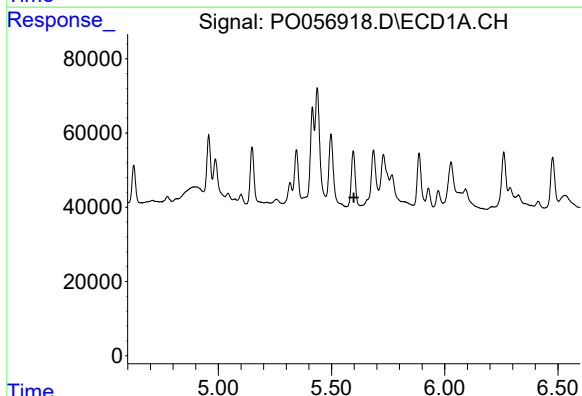


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.599 min
Response: 0
Conc: N.D.

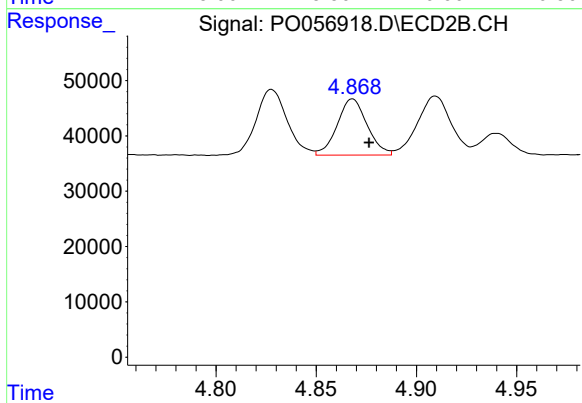

#6 AR-1016-4


R.T.: 4.868 min
Delta R.T.: -0.008 min
Response: 105512
Conc: 127.45 ng/ml

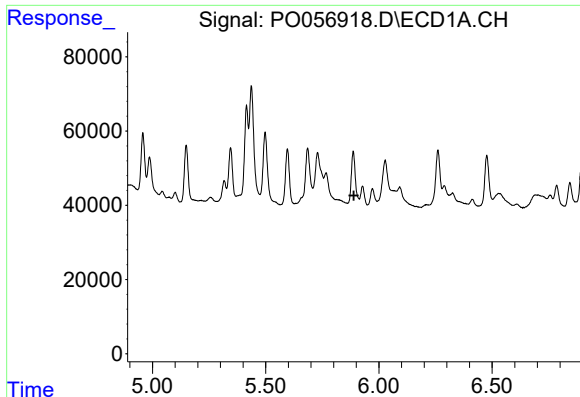

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.890 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

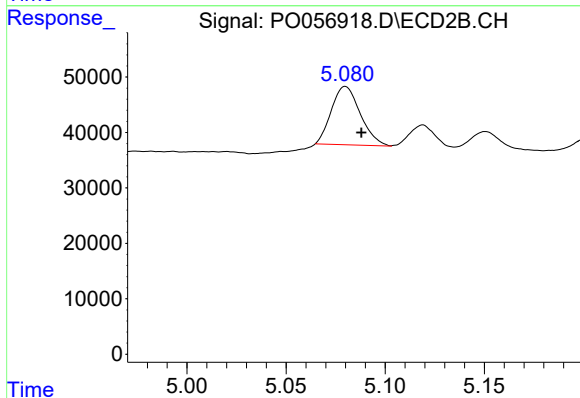


#7 AR-1016-5

R.T.: 5.080 min
Delta R.T.: -0.008 min
Response: 106872
Conc: 99.63 ng/ml

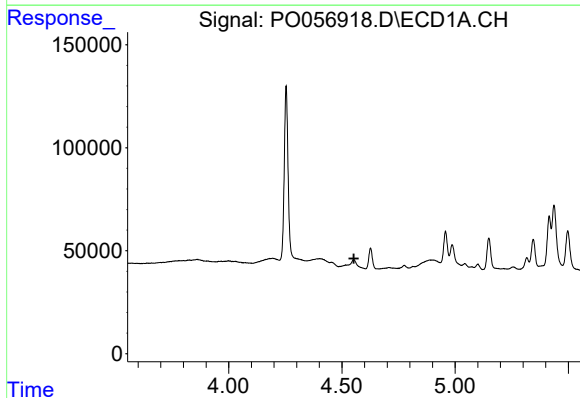


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 4.553 min
Response: 0
Conc: N.D.

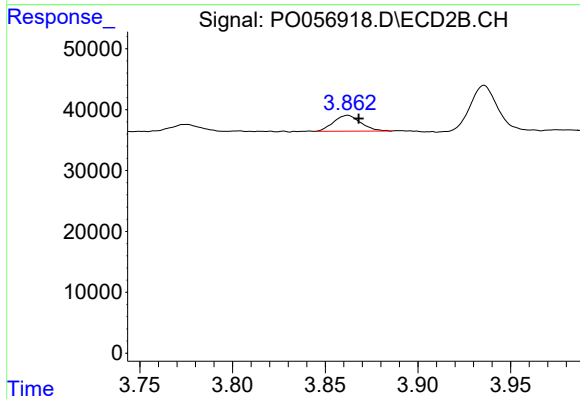

#9 AR-1221-2


R.T.: 3.862 min
Delta R.T.: -0.006 min
Response: 26786
Conc: 71.07 ng/ml

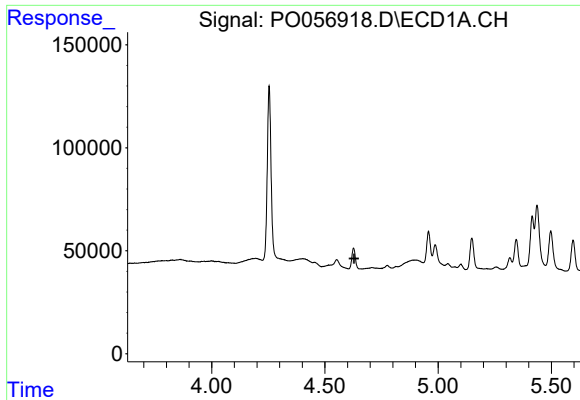

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.628 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

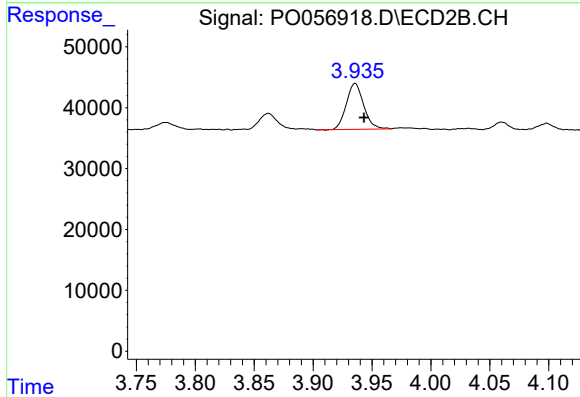


#10 AR-1221-3

R.T.: 3.936 min
Delta R.T.: -0.007 min
Response: 77360
Conc: 64.63 ng/ml

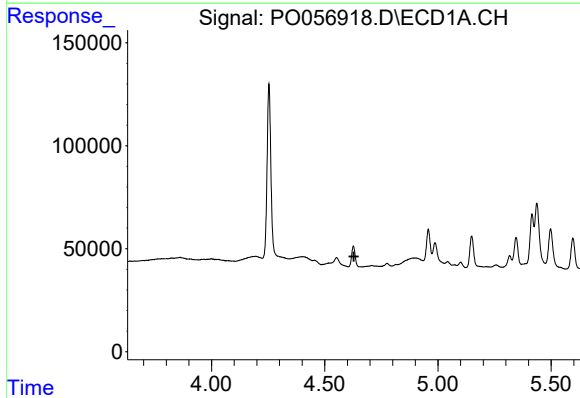


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.629 min
Response: 0
Conc: N.D.

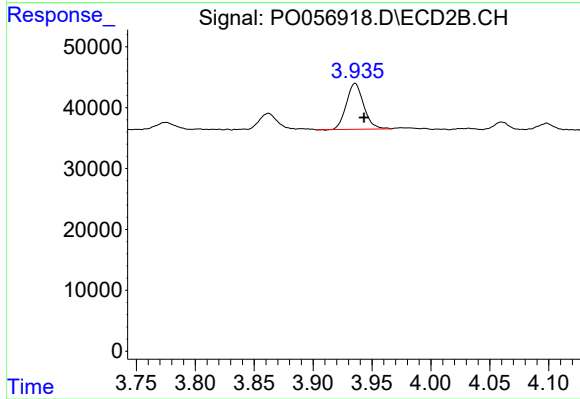

#11 AR-1232-1


R.T.: 3.936 min
Delta R.T.: -0.007 min
Response: 77360
Conc: 86.11 ng/ml

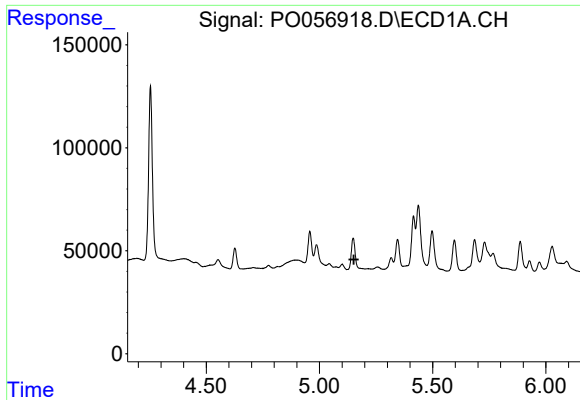

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 5.152 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

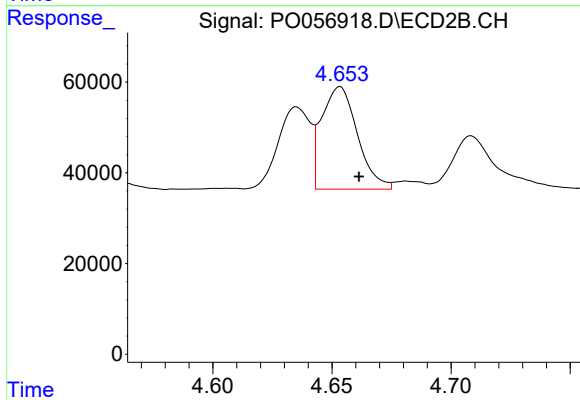


#12 AR-1232-2

R.T.: 4.653 min
Delta R.T.: -0.008 min
Response: 236708
Conc: 243.56 ng/ml

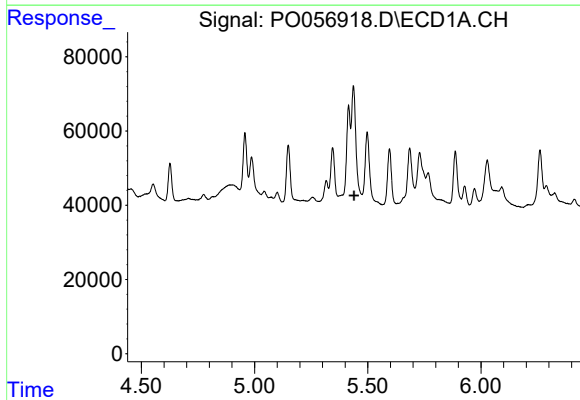


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T.: 5.439 min
Response: 0
Conc: N.D.

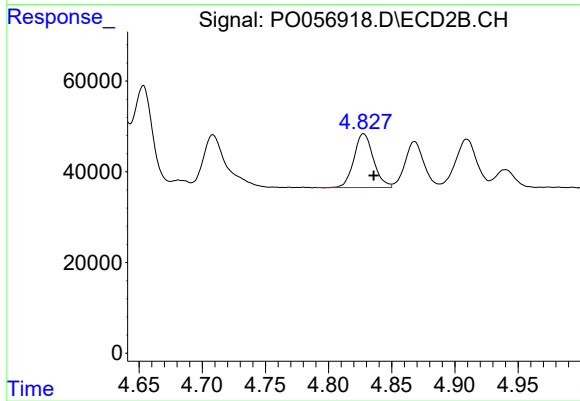

#13 AR-1232-3


R.T.: 4.828 min
Delta R.T.: -0.008 min
Response: 127620
Conc: 243.88 ng/ml

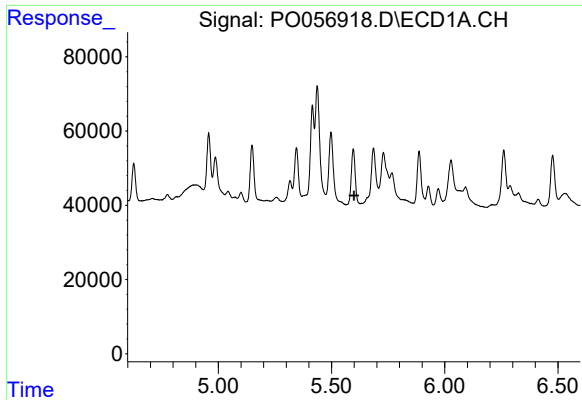

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 5.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

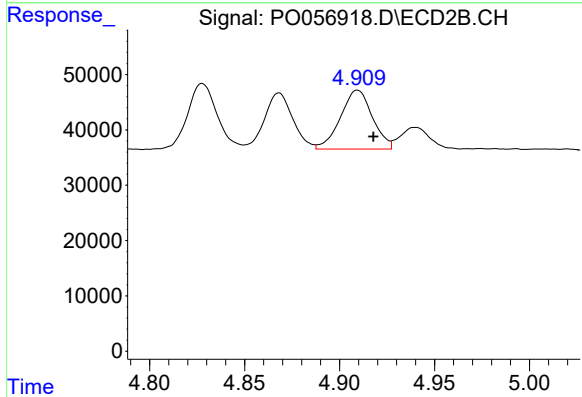


#14 AR-1232-4

R.T.: 4.909 min
Delta R.T.: -0.008 min
Response: 124827
Conc: 253.36 ng/ml

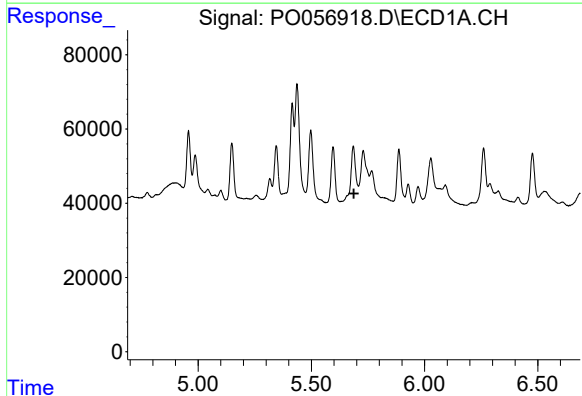


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.688 min
Response: 0
Conc: N.D.

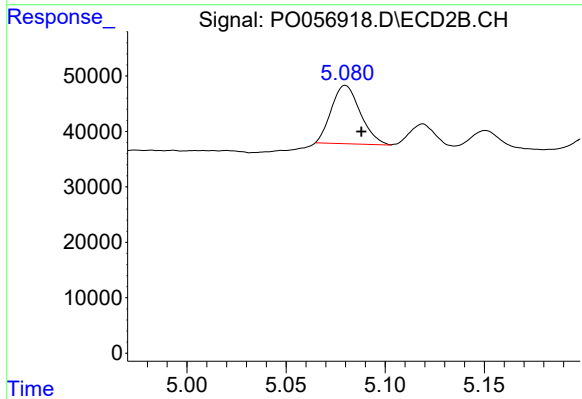

#15 AR-1232-5


R.T.: 5.080 min
Delta R.T.: -0.008 min
Response: 106872
Conc: 189.74 ng/ml

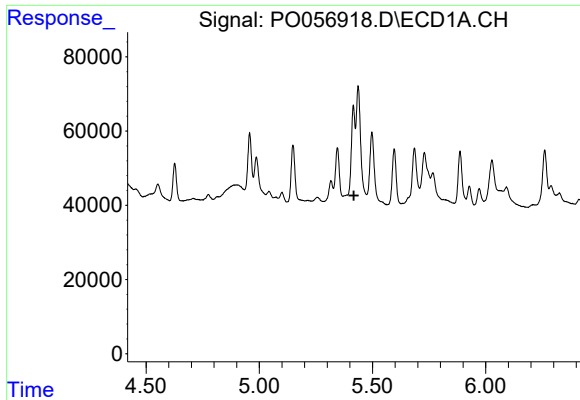

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T.: 5.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

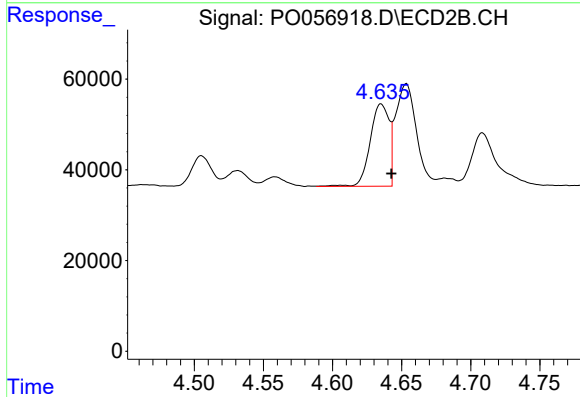


#16 AR-1242-1

R.T.: 4.635 min
Delta R.T.: -0.007 min
Response: 172945
Conc: 139.63 ng/ml

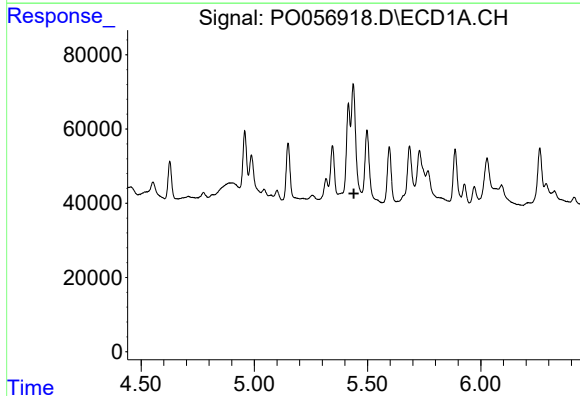


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T.: 5.440 min
Response: 0
Conc: N.D.

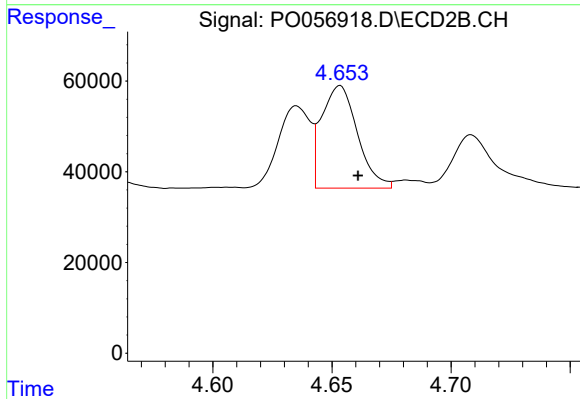

#17 AR-1242-2


R.T.: 4.653 min
Delta R.T.: -0.008 min
Response: 236708
Conc: 131.62 ng/ml

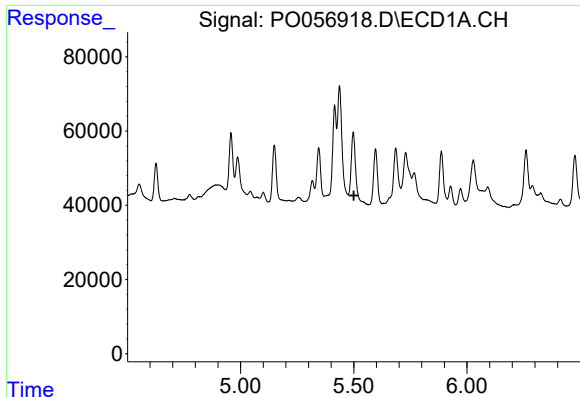

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 5.500 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

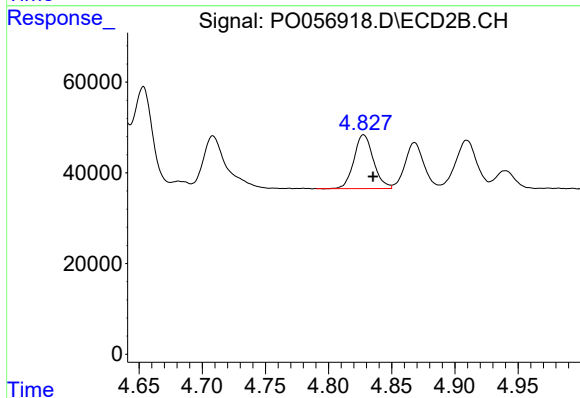


#18 AR-1242-3

R.T.: 4.828 min
Delta R.T.: -0.007 min
Response: 127620
Conc: 129.81 ng/ml

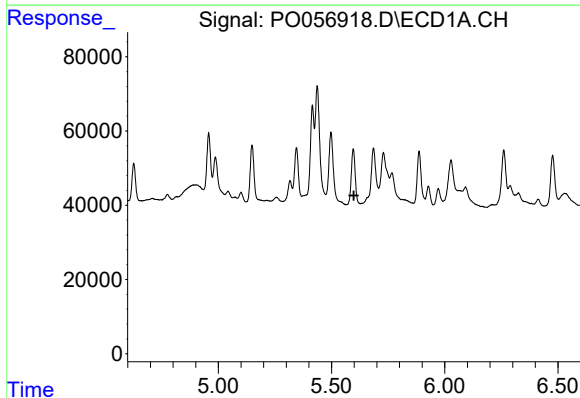


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T.: 5.599 min
Response: 0
Conc: N.D.

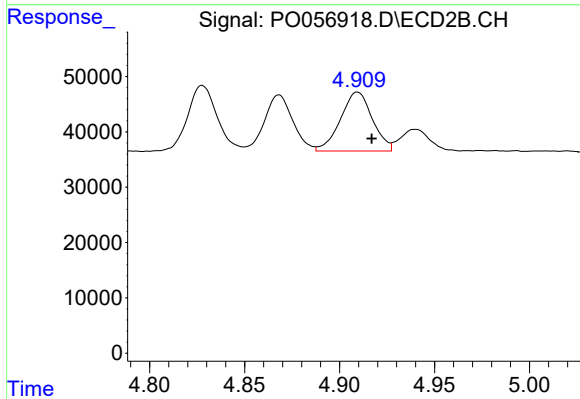

#19 AR-1242-4


R.T.: 4.909 min
Delta R.T.: -0.008 min
Response: 124827
Conc: 128.28 ng/ml

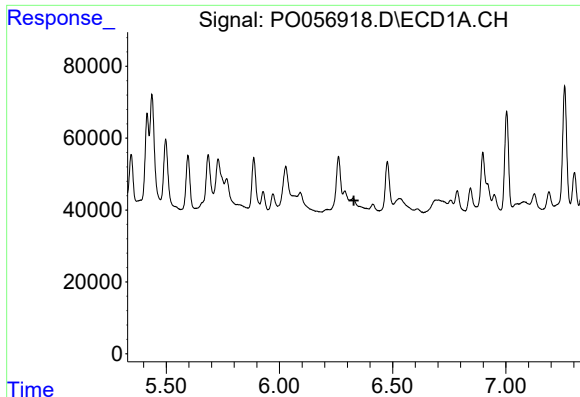

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.329 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

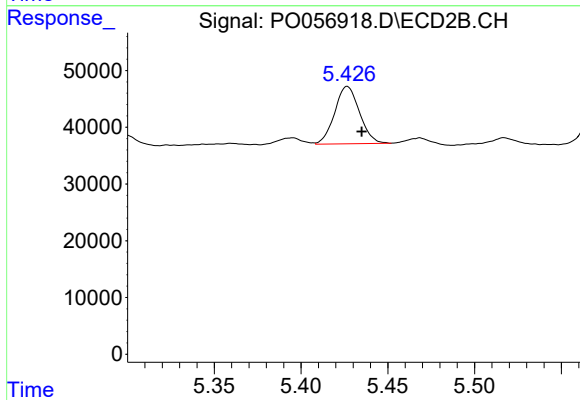


#20 AR-1242-5

R.T.: 5.427 min
Delta R.T.: -0.008 min
Response: 100858
Conc: 85.31 ng/ml

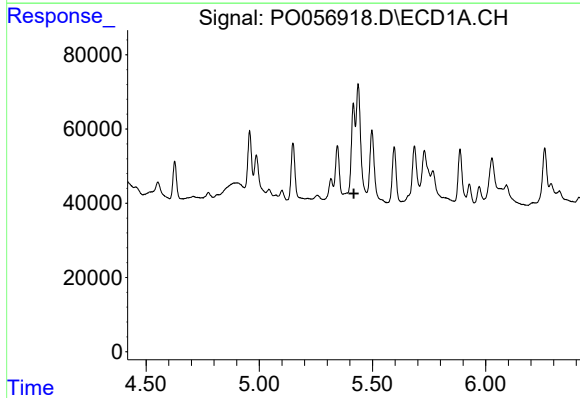


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T.: 5.418 min
Response: 0
Conc: N.D.

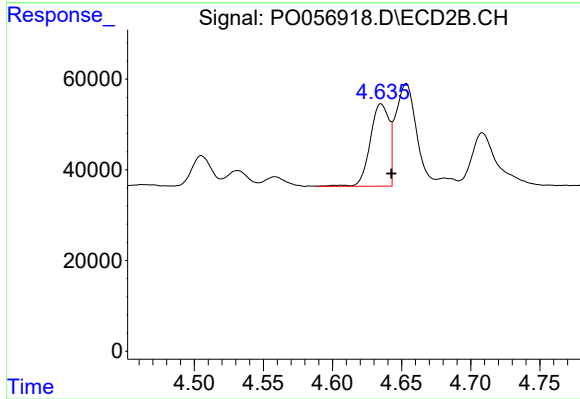

#21 AR-1248-1


R.T.: 4.635 min
Delta R.T.: -0.008 min
Response: 172945
Conc: 184.67 ng/ml

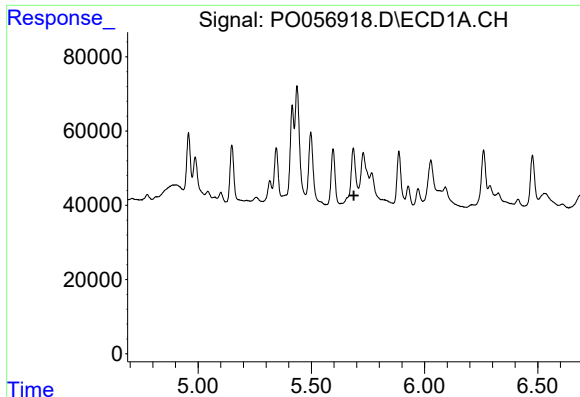

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T.: 5.688 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

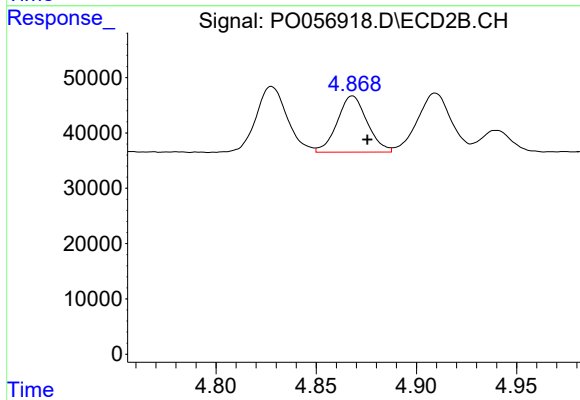


#22 AR-1248-2

R.T.: 4.868 min
Delta R.T.: -0.007 min
Response: 105512
Conc: 83.05 ng/ml

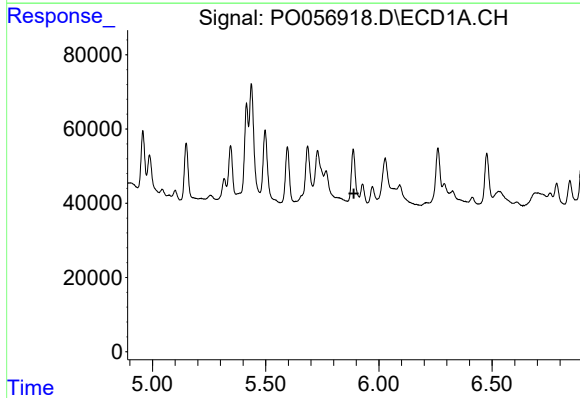


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T.: 5.890 min
Response: 0
Conc: N.D.

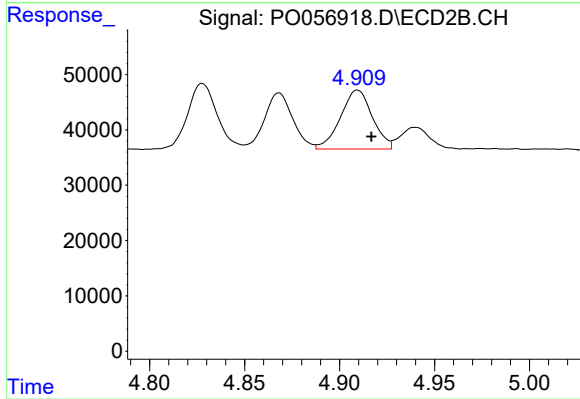

#23 AR-1248-3


R.T.: 4.909 min
Delta R.T.: -0.007 min
Response: 124827
Conc: 95.59 ng/ml

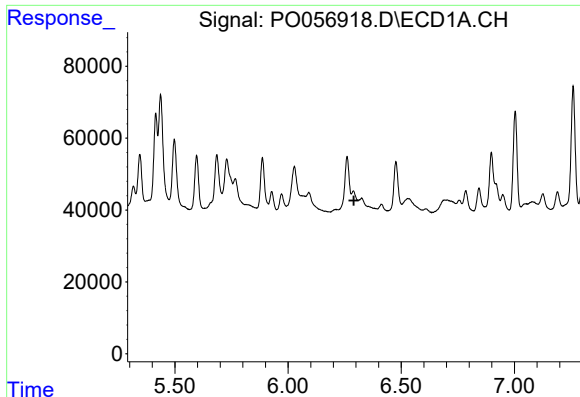

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 6.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

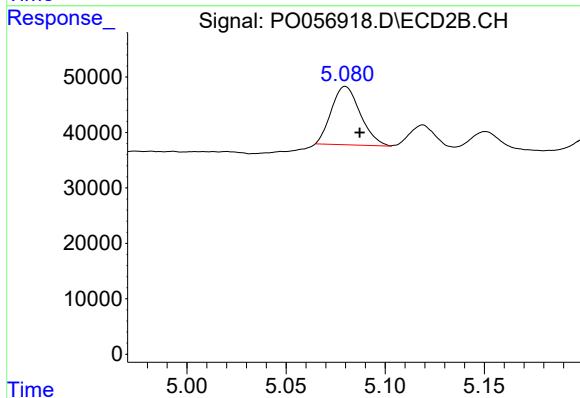


#24 AR-1248-4

R.T.: 5.080 min
Delta R.T.: -0.007 min
Response: 106872
Conc: 67.49 ng/ml

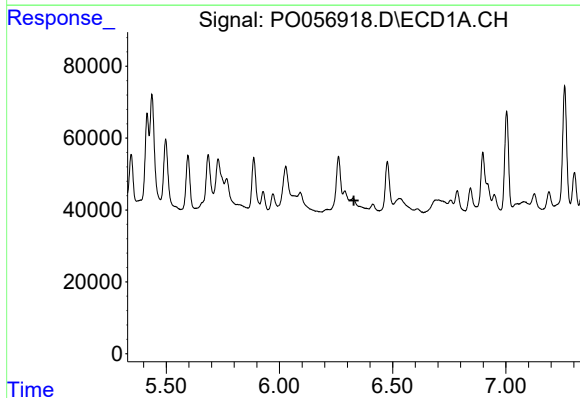


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 6.329 min
Response: 0
Conc: N.D.

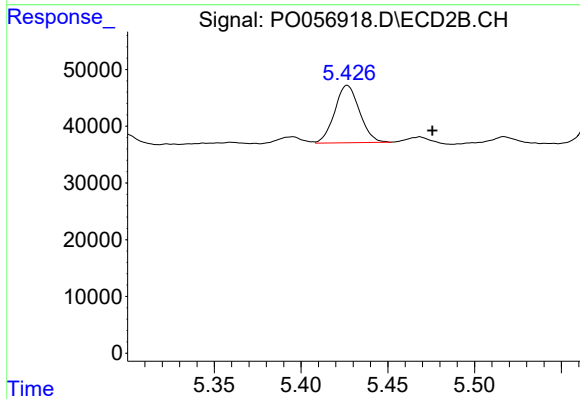

#25 AR-1248-5


R.T.: 5.427 min
Delta R.T.: -0.049 min
Response: 100858
Conc: 60.94 ng/ml

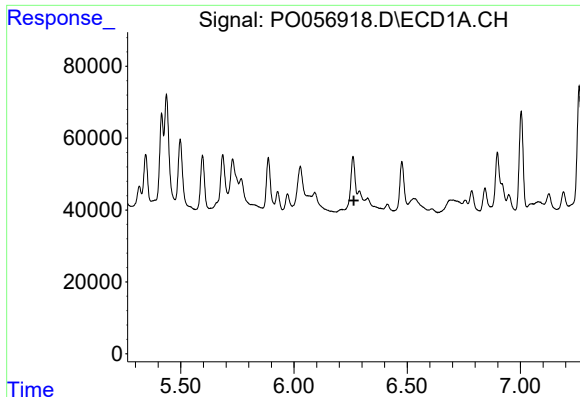

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 6.264 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

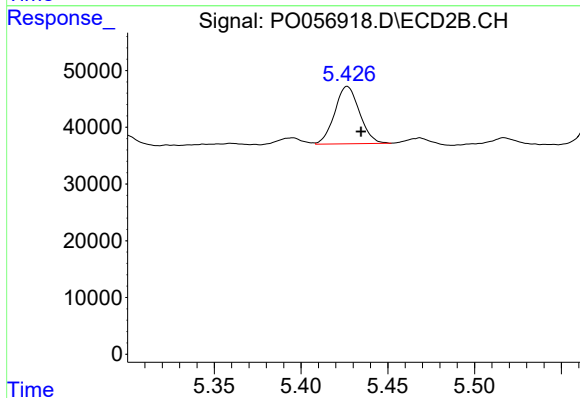


#26 AR-1254-1

R.T.: 5.427 min
Delta R.T.: -0.008 min
Response: 100858
Conc: 38.14 ng/ml

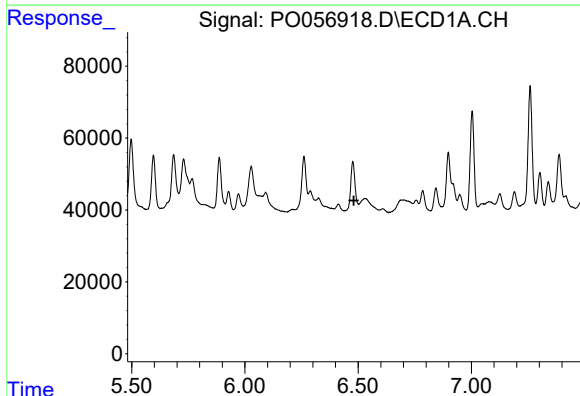


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T.: 6.481 min
Response: 0
Conc: N.D.

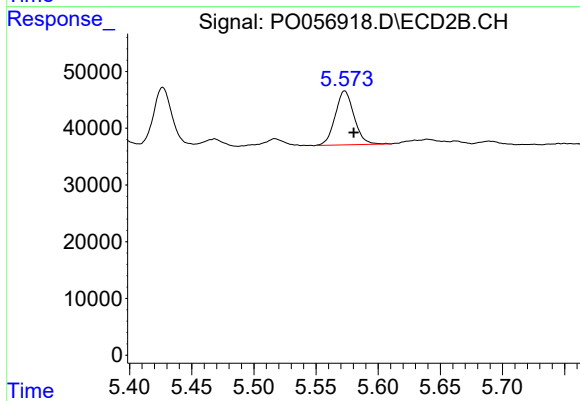

#27 AR-1254-2


R.T.: 5.573 min
Delta R.T.: -0.007 min
Response: 100172
Conc: 46.47 ng/ml

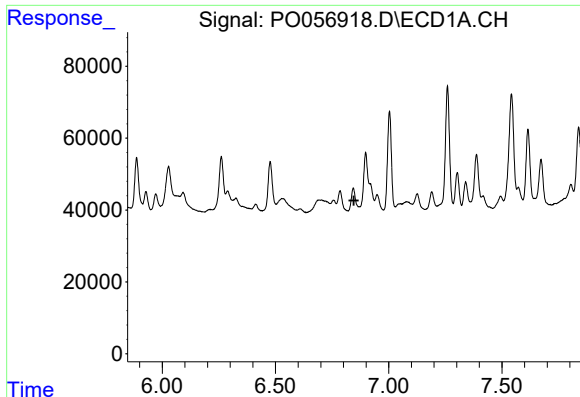

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

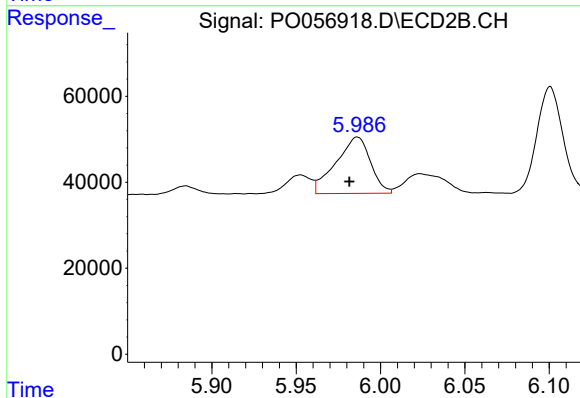


#28 AR-1254-3

R.T.: 5.986 min
Delta R.T.: 0.005 min
Response: 186727
Conc: 51.00 ng/ml

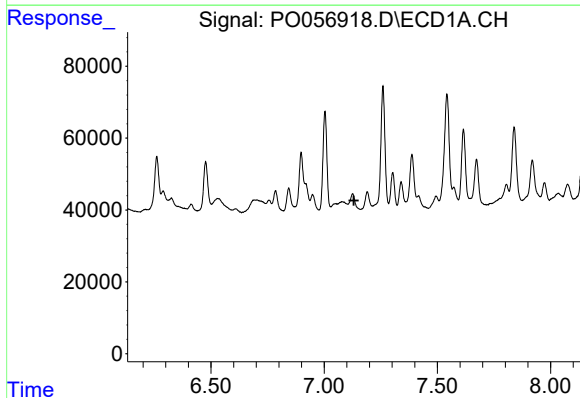


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T.: 7.131 min
Response: 0
Conc: N.D.

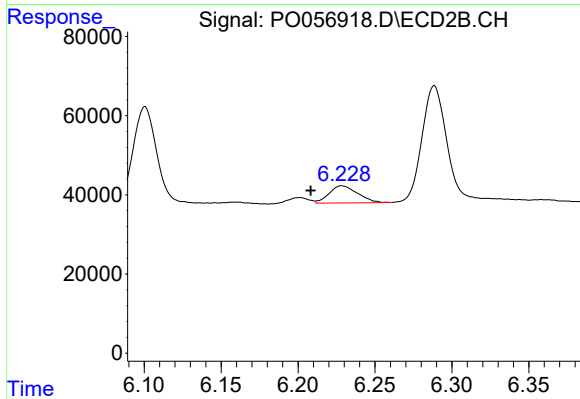

#29 AR-1254-4


R.T.: 6.229 min
Delta R.T.: 0.020 min
Response: 55504
Conc: 25.26 ng/ml

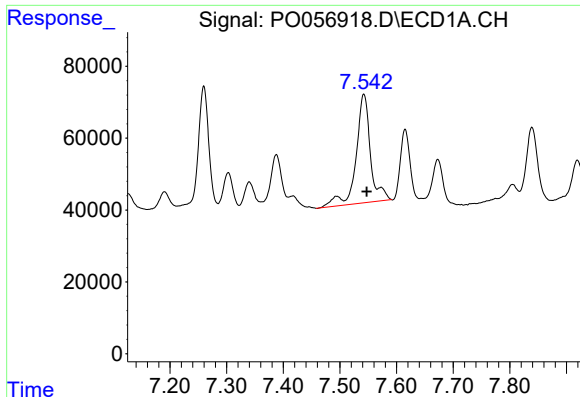

#30 AR-1254-5


R.T.: 7.542 min
Delta R.T.: -0.005 min
Response: 534202
Conc: 141.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

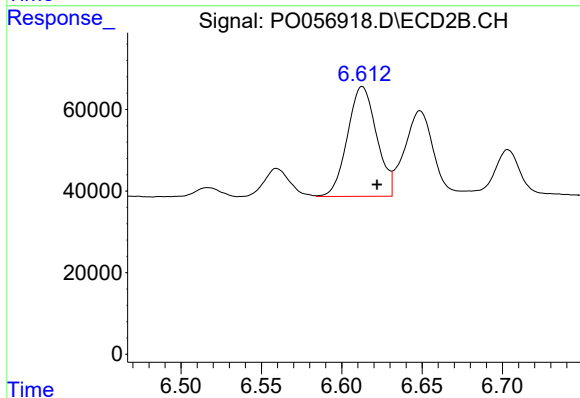


#30 AR-1254-5

R.T.: 6.613 min
Delta R.T.: -0.009 min
Response: 340333
Conc: 107.35 ng/ml

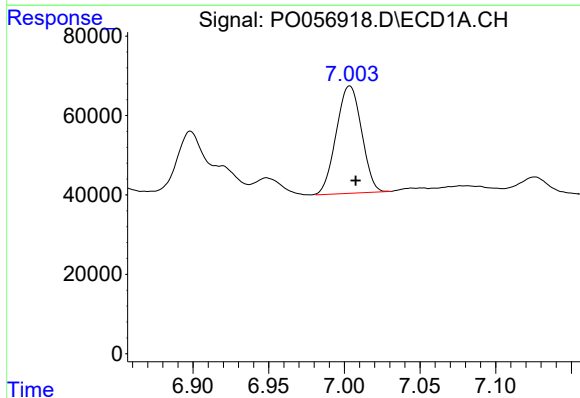


#31 AR-1260-1

R.T.: 7.004 min
Delta R.T.: -0.004 min
Response: 314892
Conc: 122.71 ng/ml

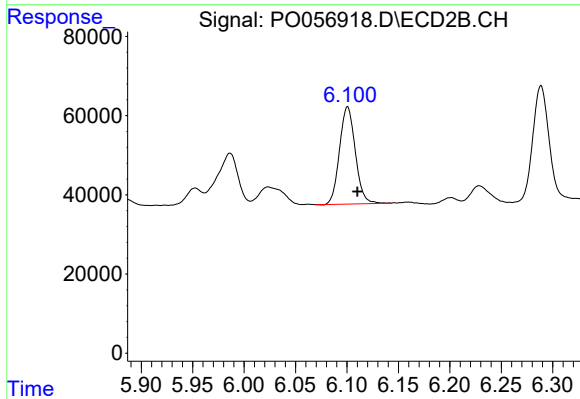

#31 AR-1260-1


R.T.: 6.101 min
Delta R.T.: -0.009 min
Response: 262561
Conc: 131.26 ng/ml

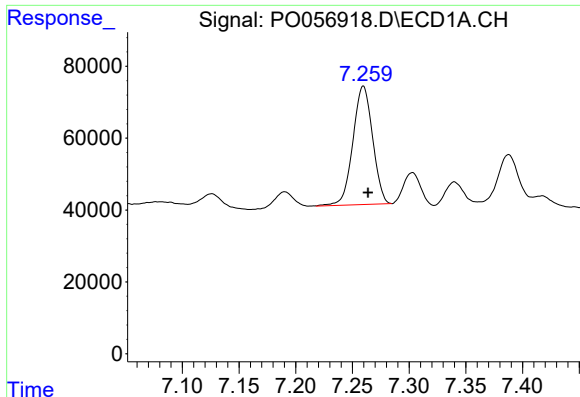

#32 AR-1260-2


R.T.: 7.260 min
Delta R.T.: -0.004 min
Response: 398073
Conc: 131.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

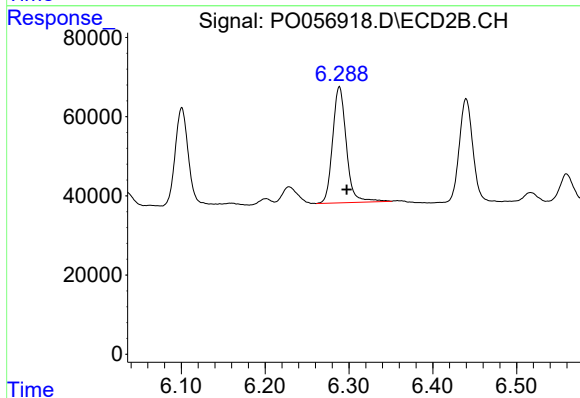


#32 AR-1260-2

R.T.: 6.289 min
Delta R.T.: -0.009 min
Response: 333558
Conc: 135.32 ng/ml

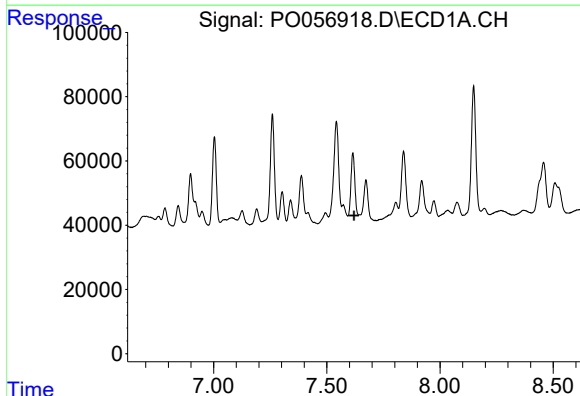


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.620 min
Response: 0
Conc: N.D.

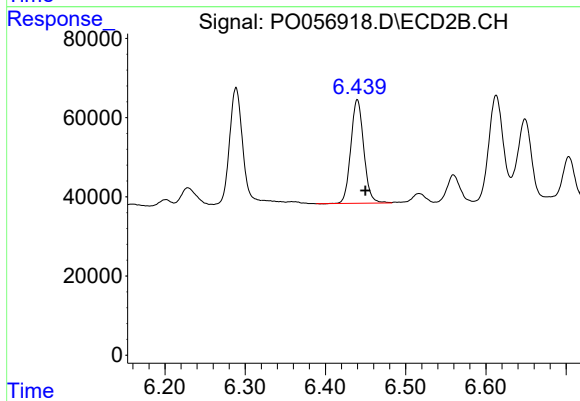

#33 AR-1260-3


R.T.: 6.440 min
Delta R.T.: -0.010 min
Response: 293139
Conc: 130.68 ng/ml

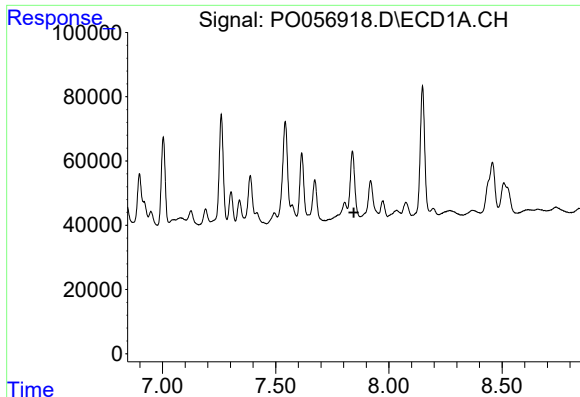

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 7.845 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

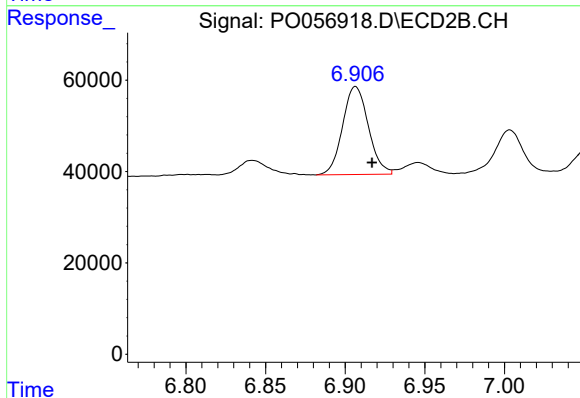


#34 AR-1260-4

R.T.: 6.907 min
Delta R.T.: -0.010 min
Response: 217085
Conc: 116.65 ng/ml

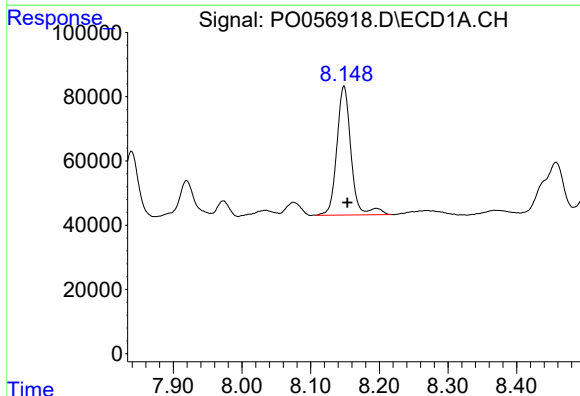


#35 AR-1260-5

R.T.: 8.148 min
Delta R.T.: -0.005 min
Response: 578144
Conc: 120.90 ng/ml

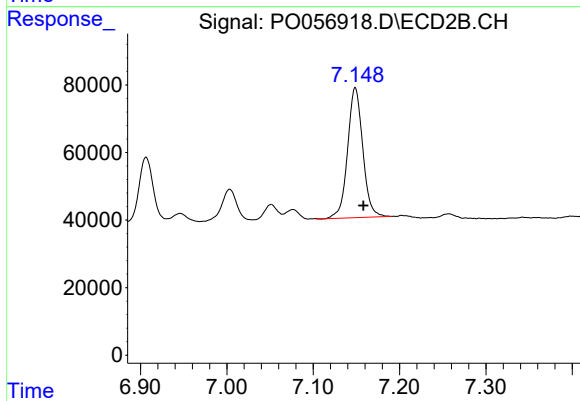

#35 AR-1260-5


R.T.: 7.149 min
Delta R.T.: -0.009 min
Response: 470256
Conc: 109.05 ng/ml

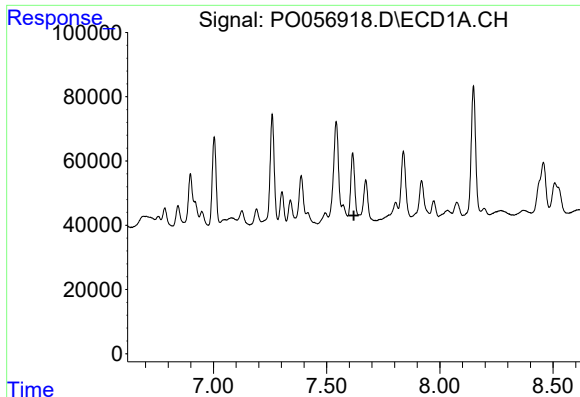

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 7.620 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

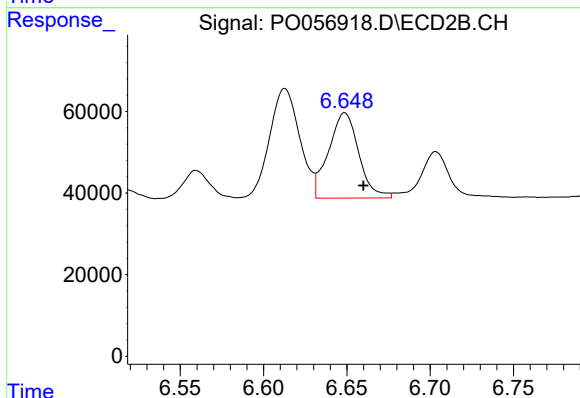


#36 AR-1262-1

R.T.: 6.649 min
Delta R.T.: -0.011 min
Response: 264379
Conc: 63.34 ng/ml

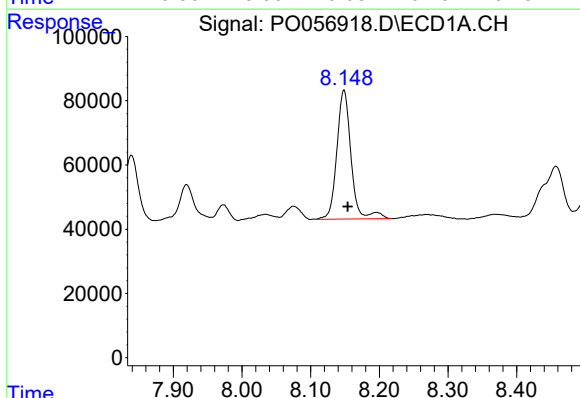


#37 AR-1262-2

R.T.: 8.148 min
Delta R.T.: -0.006 min
Response: 578144
Conc: 75.83 ng/ml

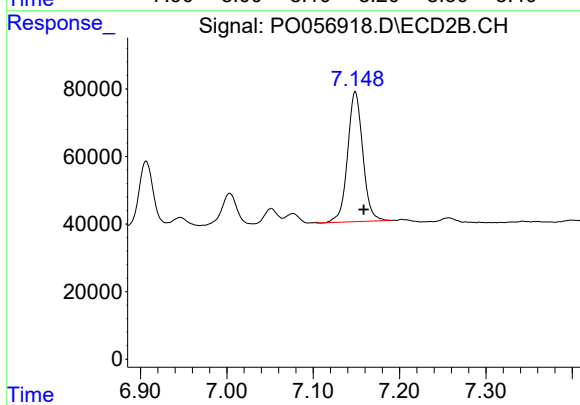

#37 AR-1262-2


R.T.: 7.149 min
Delta R.T.: -0.010 min
Response: 470256
Conc: 68.44 ng/ml

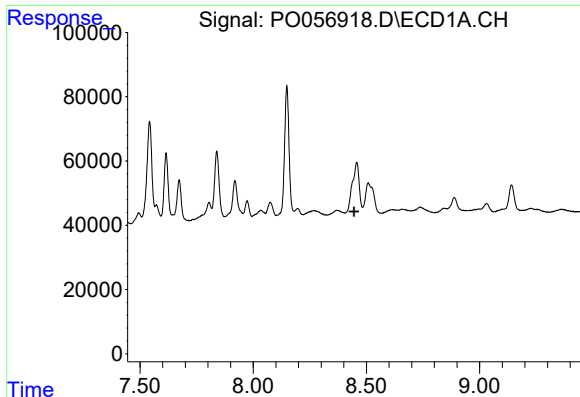

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.445 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

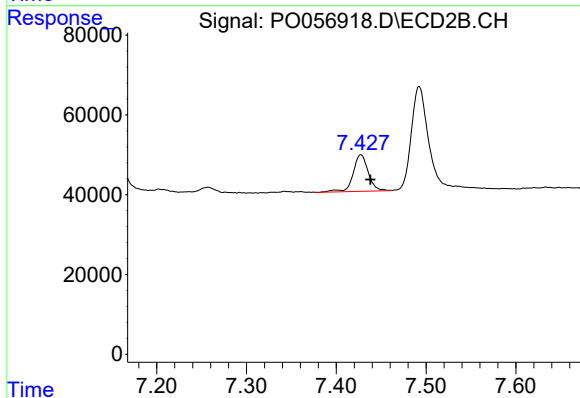


#38 AR-1262-3

R.T.: 7.427 min
Delta R.T.: -0.011 min
Response: 107030
Conc: 36.24 ng/ml

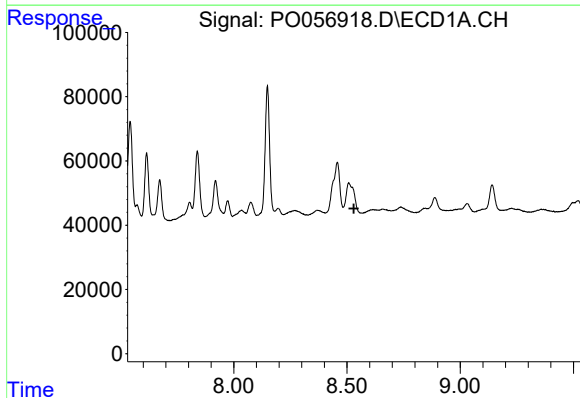


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.530 min
Response: 0
Conc: N.D.

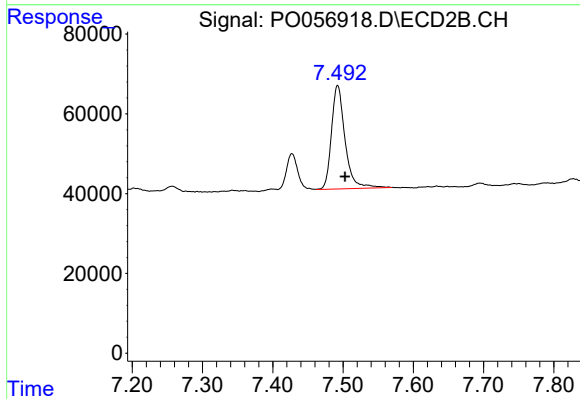

#39 AR-1262-4


R.T.: 7.492 min
Delta R.T.: -0.011 min
Response: 349246
Conc: 67.03 ng/ml

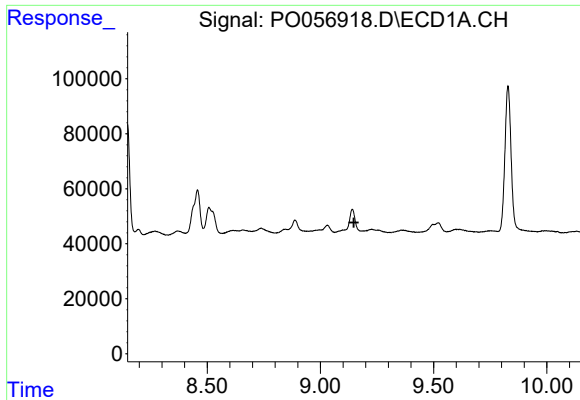

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 9.148 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

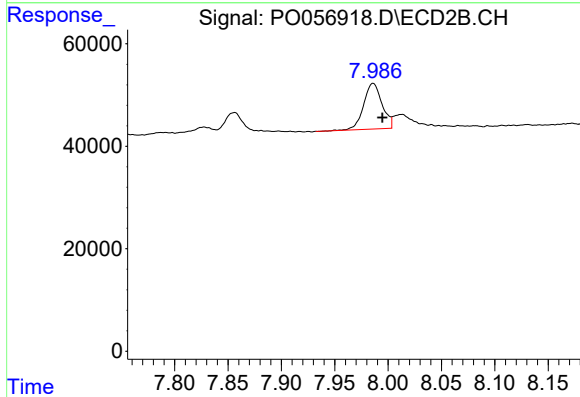


#40 AR-1262-5

R.T.: 7.986 min
Delta R.T.: -0.009 min
Response: 107038
Conc: 46.09 ng/ml

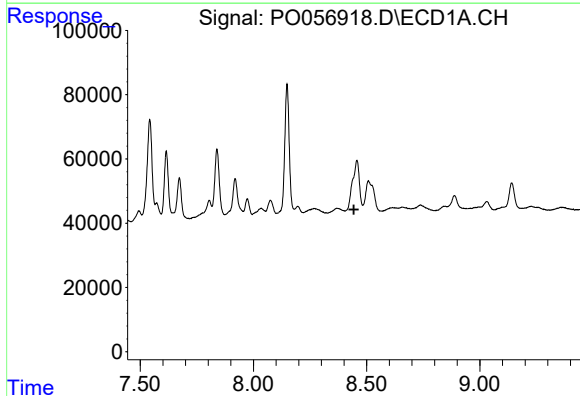


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 8.444 min
Response: 0
Conc: N.D.

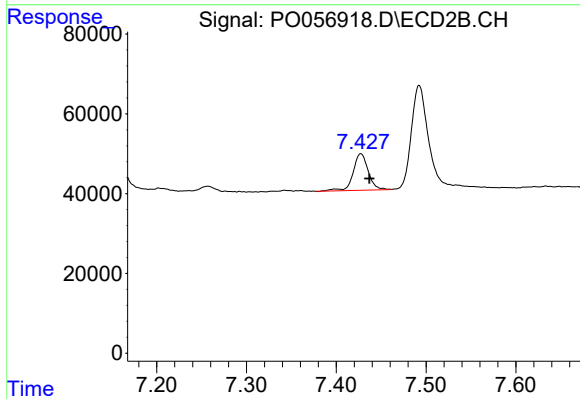

#41 AR-1268-1


R.T.: 7.427 min
Delta R.T.: -0.010 min
Response: 107030
Conc: 14.34 ng/ml

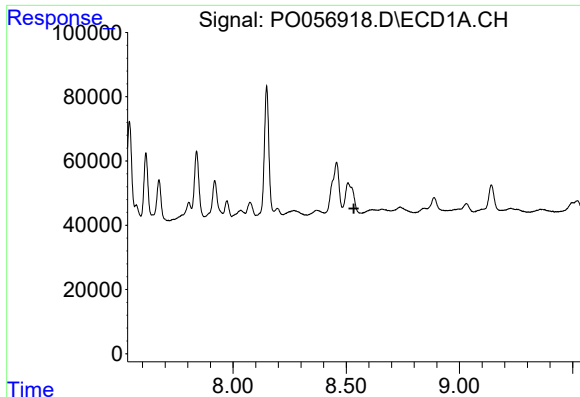

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 8.534 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

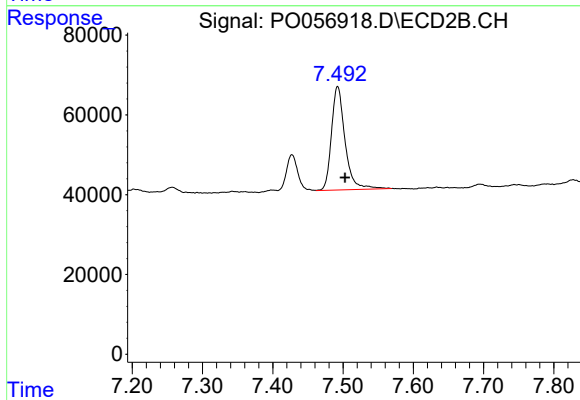


#42 AR-1268-2

R.T.: 7.492 min
Delta R.T.: -0.010 min
Response: 349246
Conc: 50.01 ng/ml

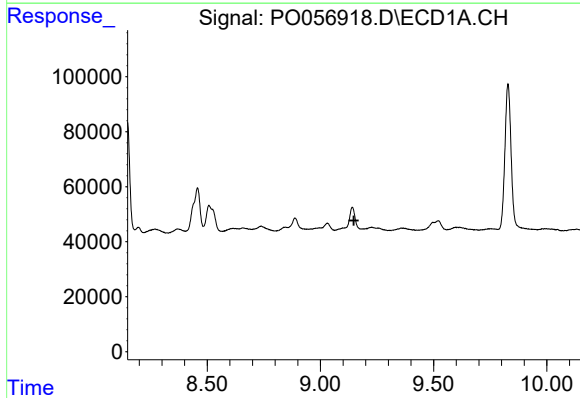


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.148 min
Response: 0
Conc: N.D.

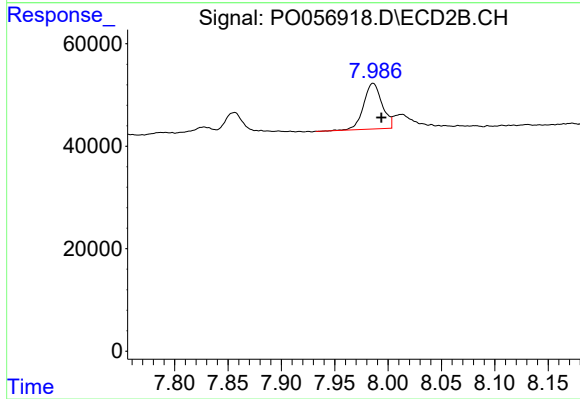

#44 AR-1268-4


R.T.: 7.986 min
Delta R.T.: -0.008 min
Response: 107038
Conc: 45.86 ng/ml

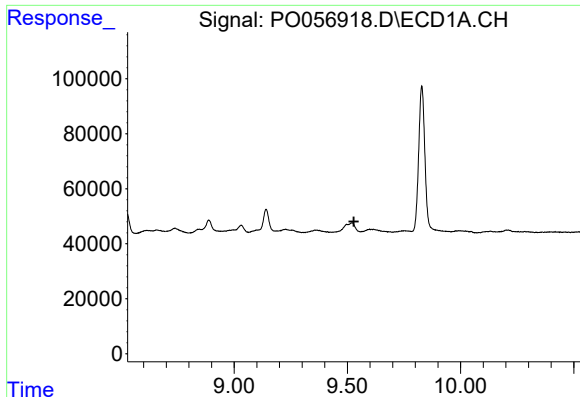

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS

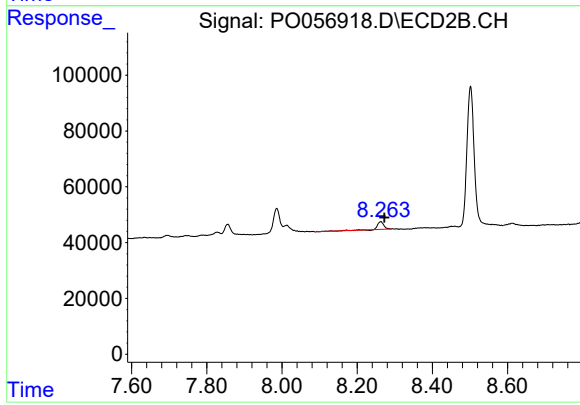

#45 AR-1268-5

R.T.: 8.263 min
Delta R.T.: -0.009 min
Response: 33172
Conc: 1.92 ng/ml