

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0060619\
 Data File : P0056919.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jun 2019 12:21
 Operator : SM/SJ
 Sample : K3175-01MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-03-007-ABCDMSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 12:47:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.254	3.566	952638	779302	24.884	23.631
2)	SA Decachlor...	9.829	8.502	980730	663387	19.981	18.605
Target Compounds							
3)	L1 AR-1016-1	0.000	4.635	0	167323	N.D.	132.956 #
4)	L1 AR-1016-2	0.000	4.653	0	234728	N.D.	130.287 #
5)	L1 AR-1016-3	0.000	4.827	0	124457	N.D.	126.231 #
6)	L1 AR-1016-4	0.000	4.868	0	103774	N.D.	125.355 #
7)	L1 AR-1016-5	0.000	5.079	0	102596	N.D.	95.641 #
9)	L2 AR-1221-2	0.000	3.862	0	27314	N.D.	72.477 #
10)	L2 AR-1221-3	0.000	3.935	0	76420	N.D.	63.840 #
11)	L3 AR-1232-1	0.000	3.935	0	76420	N.D.	85.066 #
12)	L3 AR-1232-2	0.000	4.653	0	234728	N.D.	241.520 #
13)	L3 AR-1232-3	0.000	4.827	0	124457	N.D.	237.835 #
14)	L3 AR-1232-4	0.000	4.909	0	123076	N.D.	249.804 #
15)	L3 AR-1232-5	0.000	5.079	0	102596	N.D.	182.148 #
16)	L4 AR-1242-1	0.000	4.635	0	167323	N.D.	135.092 #
17)	L4 AR-1242-2	0.000	4.653	0	234728	N.D.	130.519 #
18)	L4 AR-1242-3	0.000	4.827	0	124457	N.D.	126.596 #
19)	L4 AR-1242-4	0.000	4.909	0	123076	N.D.	126.478 #
20)	L4 AR-1242-5	0.000	5.427	0	92275	N.D.	78.049 #
21)	L5 AR-1248-1	0.000	4.635	0	167323	N.D.	178.665 #
22)	L5 AR-1248-2	0.000	4.868	0	103774	N.D.	81.683 #
23)	L5 AR-1248-3	0.000	4.909	0	123076	N.D.	94.246 #
24)	L5 AR-1248-4	0.000	5.079	0	102596	N.D.	64.785 #
25)	L5 AR-1248-5	0.000	5.427	0	92275	N.D.	55.753 #
26)	L6 AR-1254-1	0.000	5.427	0	92275	N.D.	34.890 #
27)	L6 AR-1254-2	0.000	5.572	0	97356	N.D.	45.160 #
28)	L6 AR-1254-3	0.000	5.986	0	184005	N.D.	50.260 #
29)	L6 AR-1254-4	0.000	6.228	0	57915	N.D.	26.362 #
30)	L6 AR-1254-5	7.542	6.613	439259	335196	116.649	105.732
31)	L7 AR-1260-1	7.004	6.100	348570	260549	135.832	130.250
32)	L7 AR-1260-2	7.259	6.288	368621	322103	121.892	130.673
33)	L7 AR-1260-3	0.000	6.440	0	290265	N.D.	129.396 #
34)	L7 AR-1260-4	0.000	6.906	0	211927	N.D.	113.877 #
35)	L7 AR-1260-5	8.149	7.148	491215	463417	102.720	107.463
36)	L8 AR-1262-1	0.000	6.648	0	260309	N.D.	62.364 #
37)	L8 AR-1262-2	8.149	7.148	491215	463417	64.432	67.449
38)	L8 AR-1262-3	0.000	7.427	0	99873	N.D.	33.816 #
39)	L8 AR-1262-4	0.000	7.492	0	343085	N.D.	65.844 #
40)	L8 AR-1262-5	0.000	7.986	0	103314	N.D.	44.491 #
41)	L9 AR-1268-1	0.000	7.427	0	99873	N.D.	13.379 #
42)	L9 AR-1268-2	0.000	7.492	0	343085	N.D.	49.131 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060619\
 Data File : P0056919.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jun 2019 12:21
 Operator : SM/SJ
 Sample : K3175-01MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-03-007-ABCDMSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 12:47:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	0.000	7.986	0	103314	N.D.	44.260 #
45) L9	AR-1268-5	0.000	8.262	0	36574	N.D.	2.113 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060619\
Data File : P0056919.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2019 12:21
Operator : SM/SJ
Sample : K3175-01MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 12:47:2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

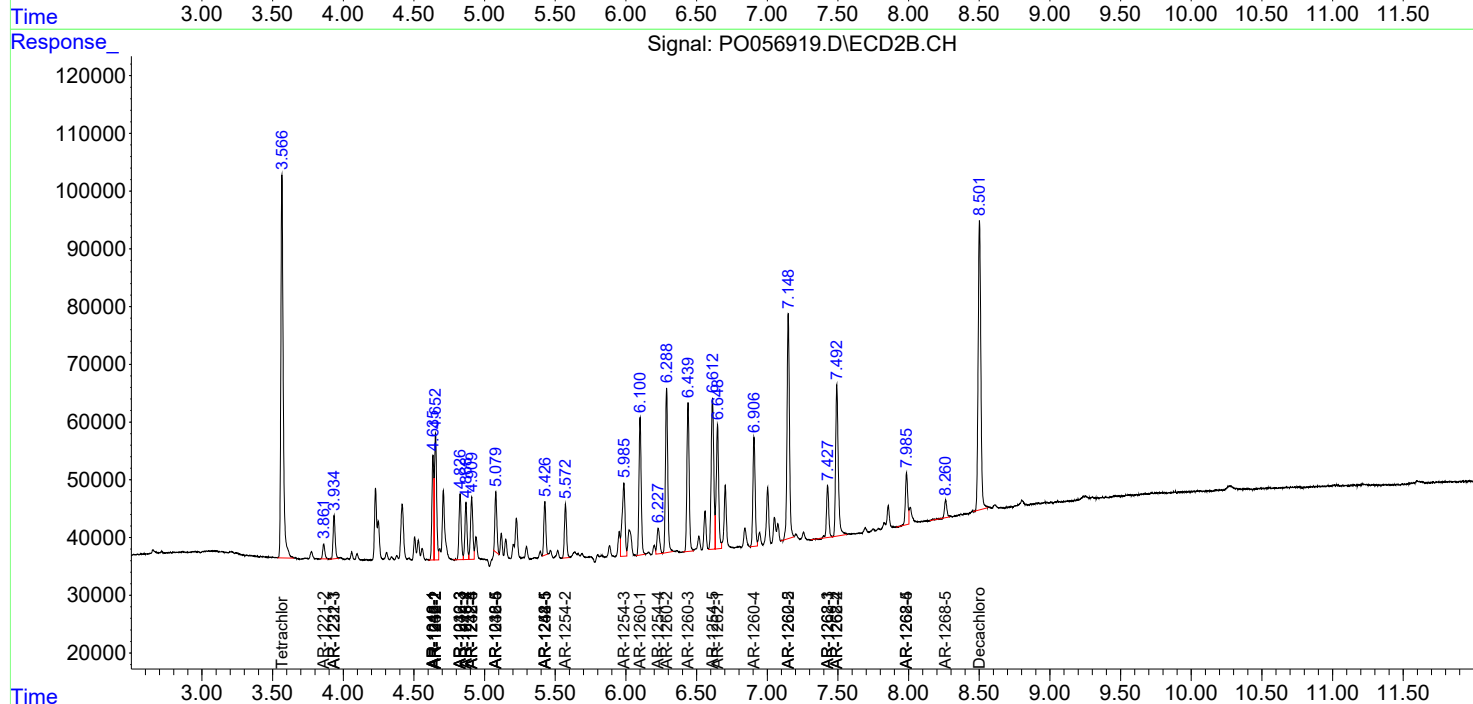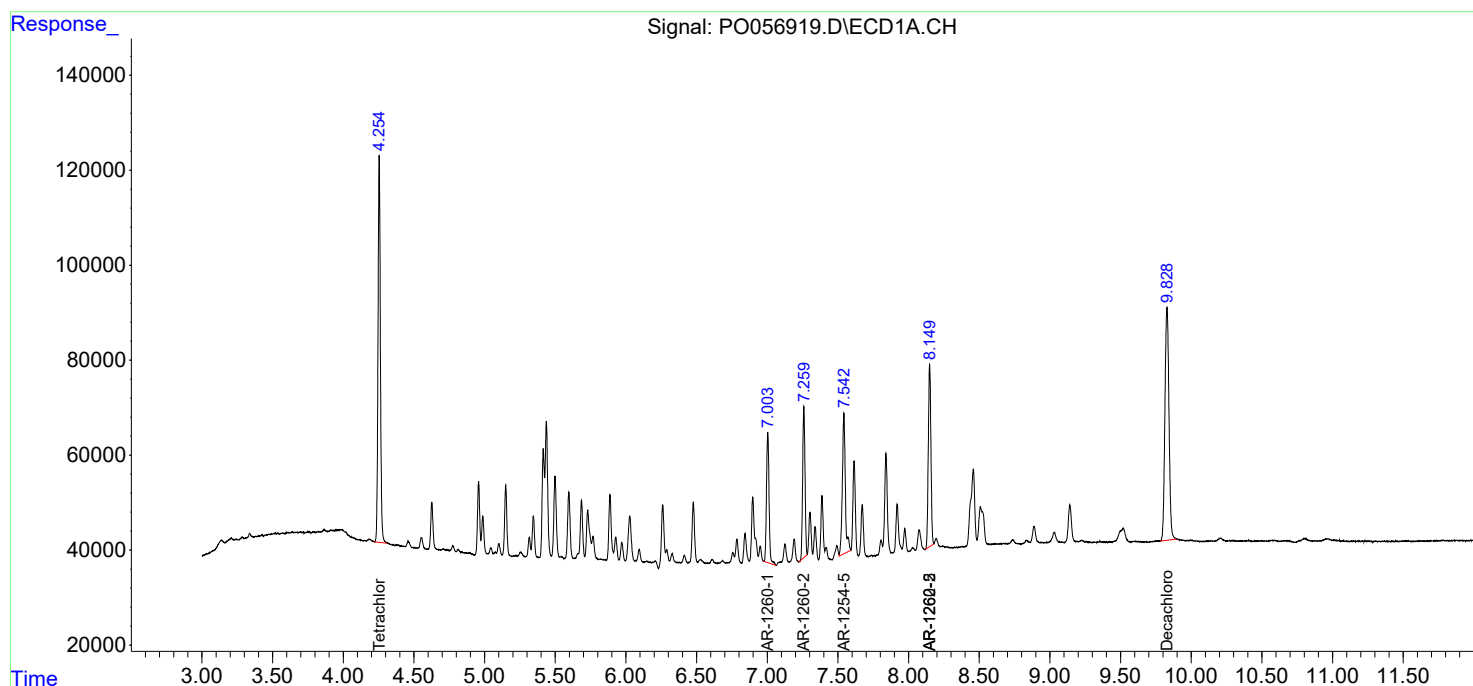


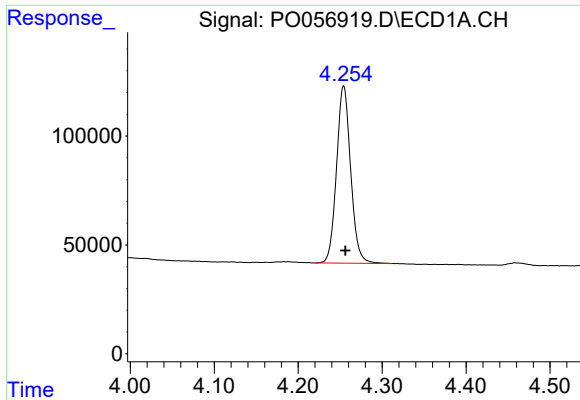

#1 Tetrachloro-m-xylene


R.T.: 4.254 min
Delta R.T.: -0.002 min
Response: 952638
Conc: 24.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

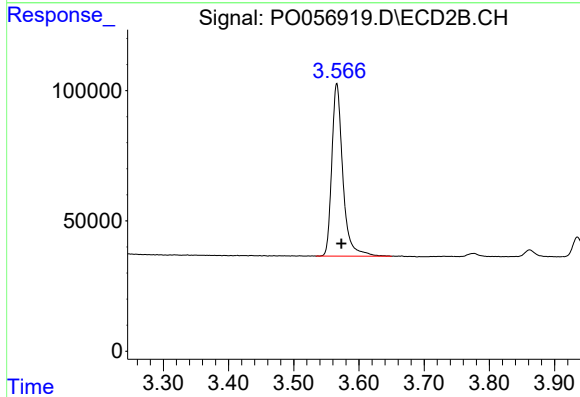


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: -0.007 min
Response: 779302
Conc: 23.63 ng/ml

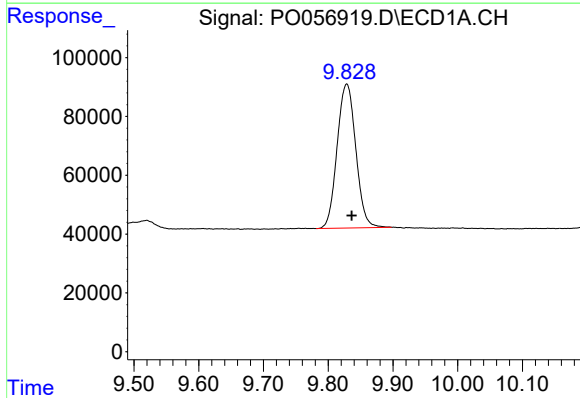


#2 Decachlorobiphenyl

R.T.: 9.829 min
Delta R.T.: -0.008 min
Response: 980730
Conc: 19.98 ng/ml

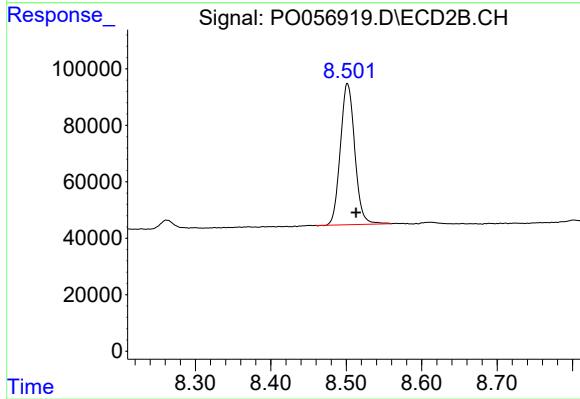

#2 Decachlorobiphenyl


R.T.: 8.502 min
Delta R.T.: -0.011 min
Response: 663387
Conc: 18.60 ng/ml

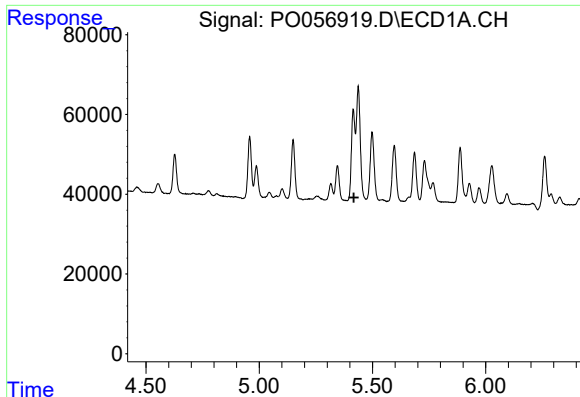

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

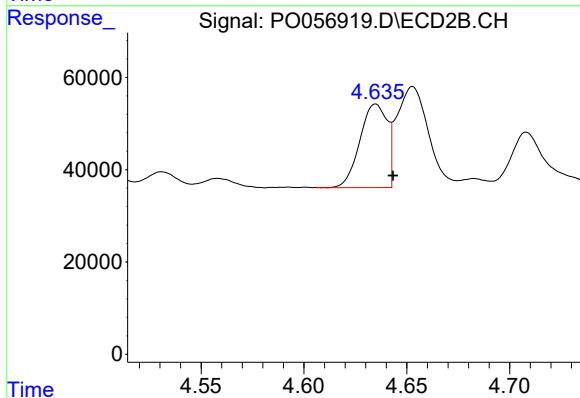


#3 AR-1016-1

R.T.: 4.635 min
Delta R.T.: -0.008 min
Response: 167323
Conc: 132.96 ng/ml

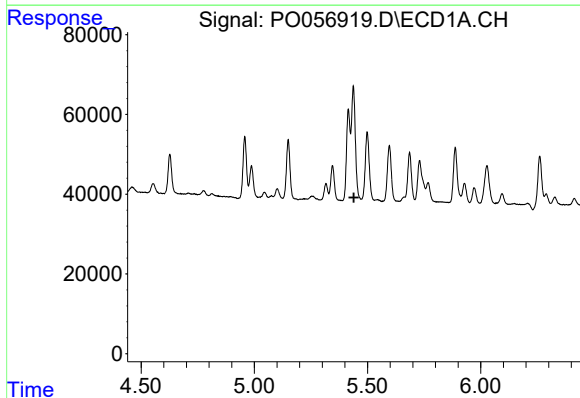


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.440 min
Response: 0
Conc: N.D.

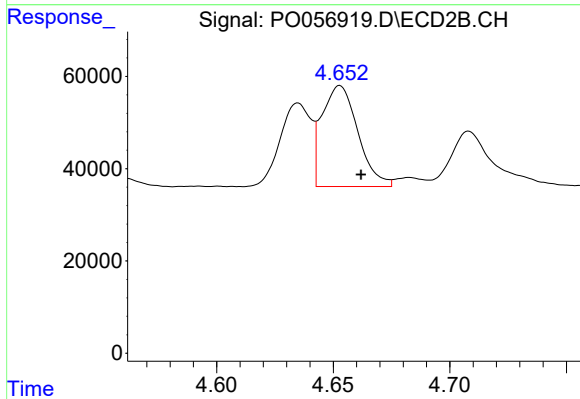

#4 AR-1016-2


R.T.: 4.653 min
Delta R.T.: -0.009 min
Response: 234728
Conc: 130.29 ng/ml

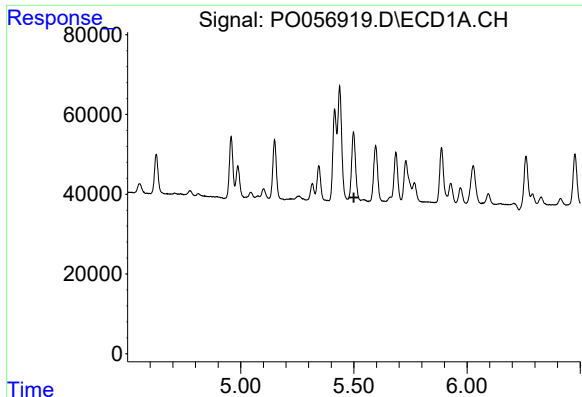

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.500 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

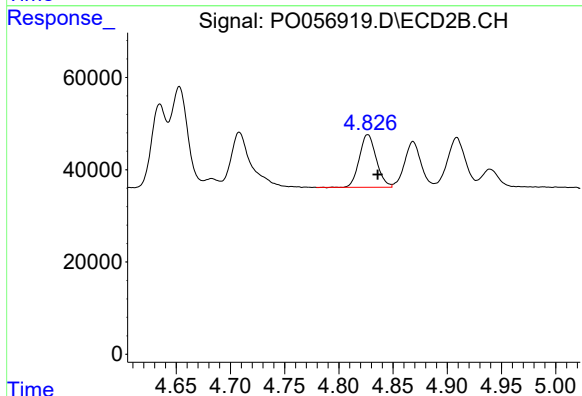


#5 AR-1016-3

R.T.: 4.827 min
Delta R.T.: -0.009 min
Response: 124457
Conc: 126.23 ng/ml

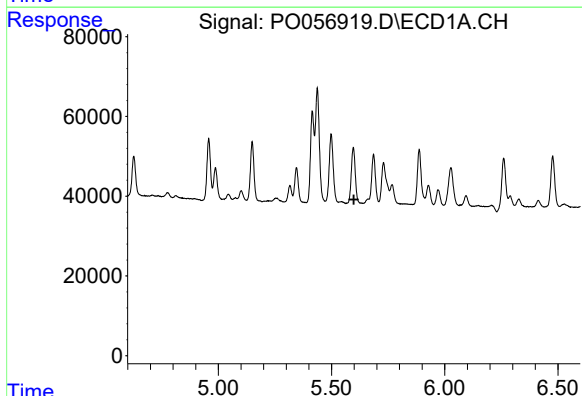


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.599 min
Response: 0
Conc: N.D.

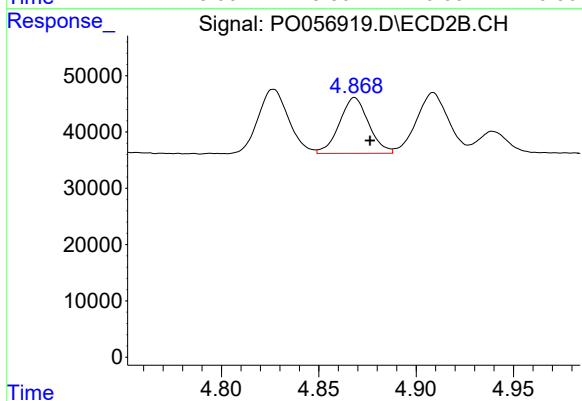

#6 AR-1016-4


R.T.: 4.868 min
Delta R.T.: -0.008 min
Response: 103774
Conc: 125.35 ng/ml

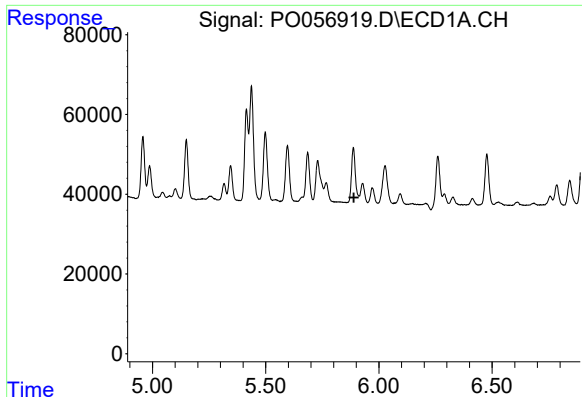

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.890 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

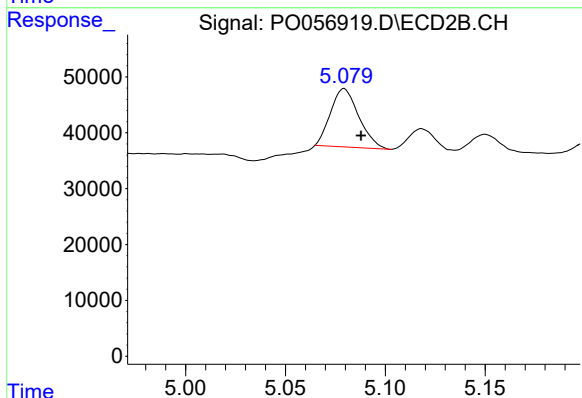


#7 AR-1016-5

R.T.: 5.079 min
Delta R.T.: -0.008 min
Response: 102596
Conc: 95.64 ng/ml

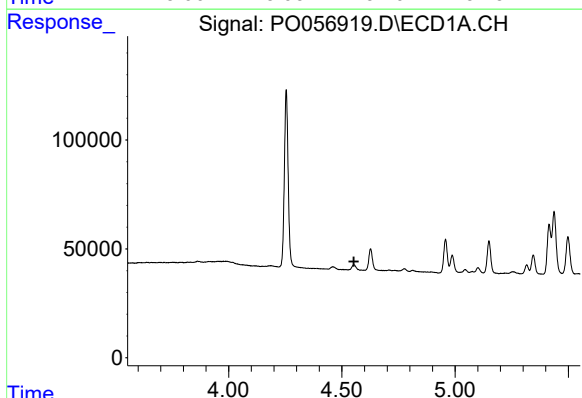


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 4.553 min
Response: 0
Conc: N.D.

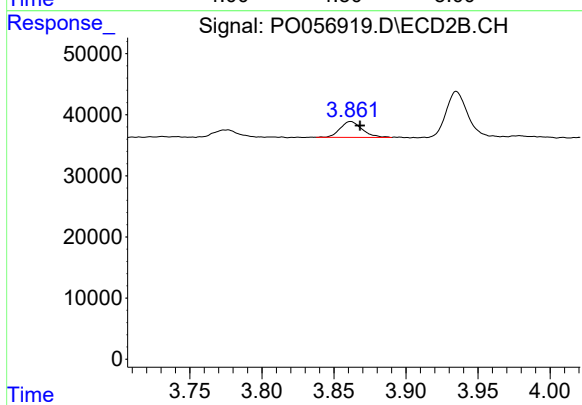

#9 AR-1221-2


R.T.: 3.862 min
Delta R.T.: -0.006 min
Response: 27314
Conc: 72.48 ng/ml

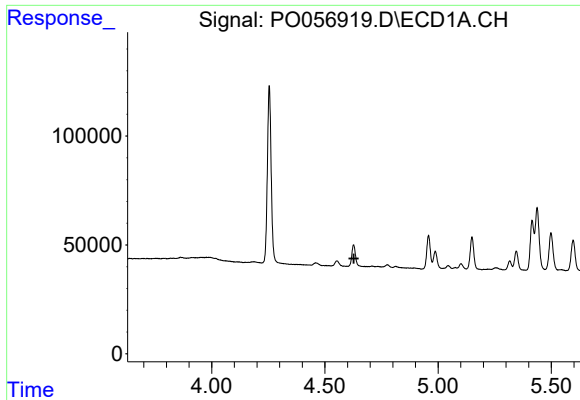

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 4.628 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

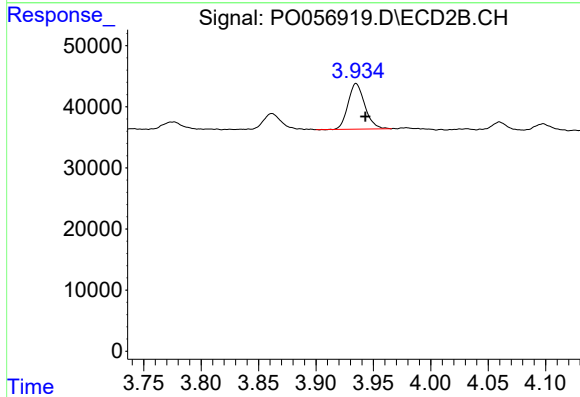


#10 AR-1221-3

R.T.: 3.935 min
Delta R.T.: -0.008 min
Response: 76420
Conc: 63.84 ng/ml

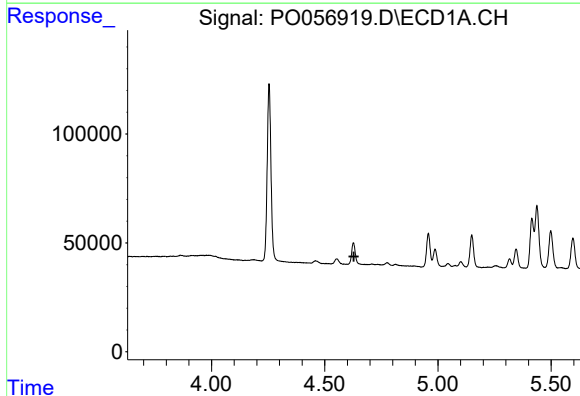


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 4.629 min
Response: 0
Conc: N.D.

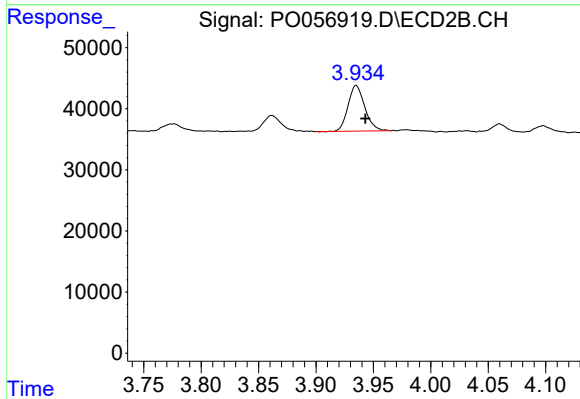

#11 AR-1232-1


R.T.: 3.935 min
Delta R.T.: -0.008 min
Response: 76420
Conc: 85.07 ng/ml

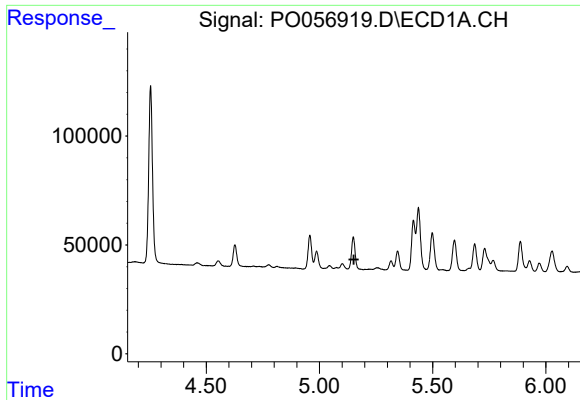

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 5.152 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

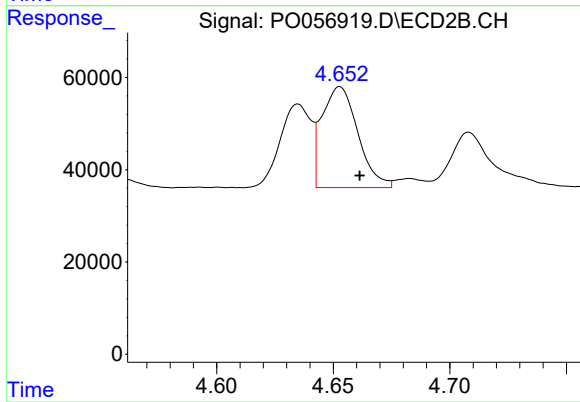


#12 AR-1232-2

R.T.: 4.653 min
Delta R.T.: -0.009 min
Response: 234728
Conc: 241.52 ng/ml

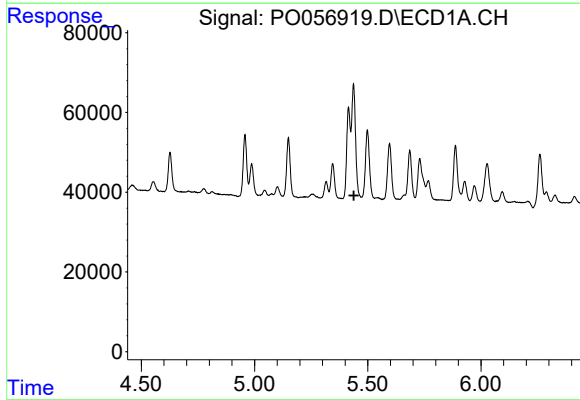


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T.: 5.439 min
Response: 0
Conc: N.D.

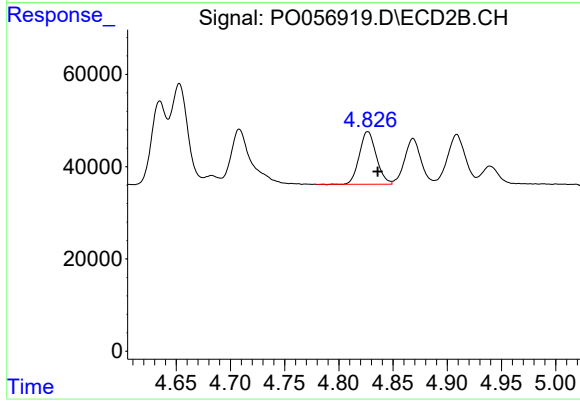

#13 AR-1232-3


R.T.: 4.827 min
Delta R.T.: -0.009 min
Response: 124457
Conc: 237.83 ng/ml

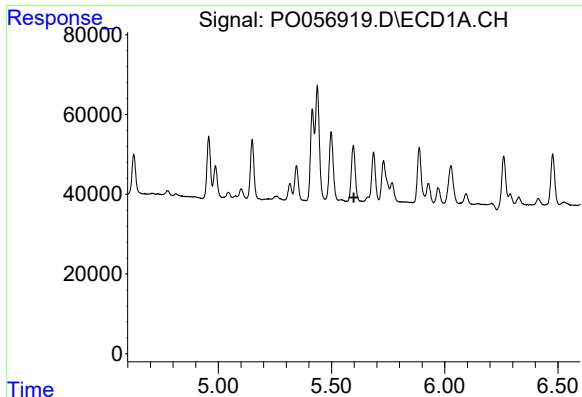

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T.: 5.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

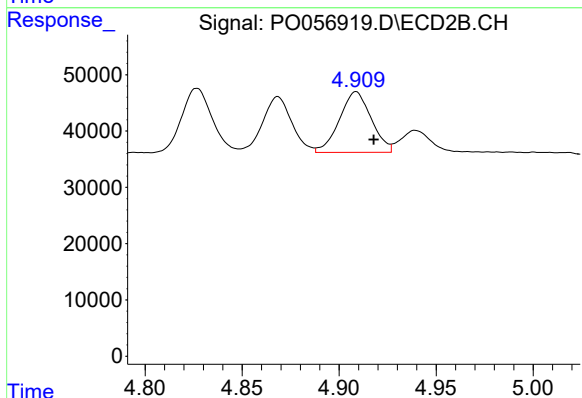


#14 AR-1232-4

R.T.: 4.909 min
Delta R.T.: -0.009 min
Response: 123076
Conc: 249.80 ng/ml

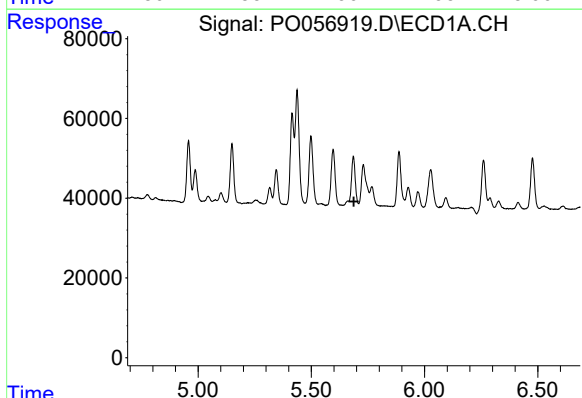


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 5.688 min
Response: 0
Conc: N.D.

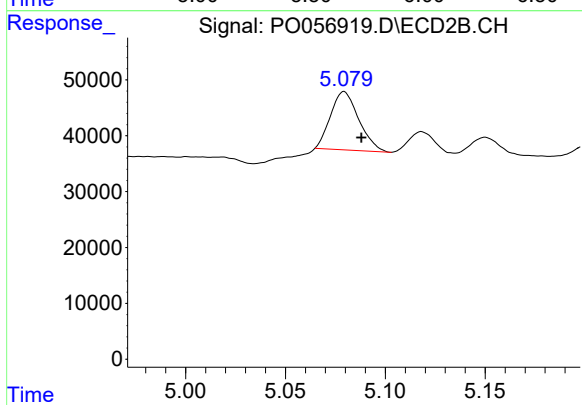

#15 AR-1232-5


R.T.: 5.079 min
Delta R.T.: -0.009 min
Response: 102596
Conc: 182.15 ng/ml

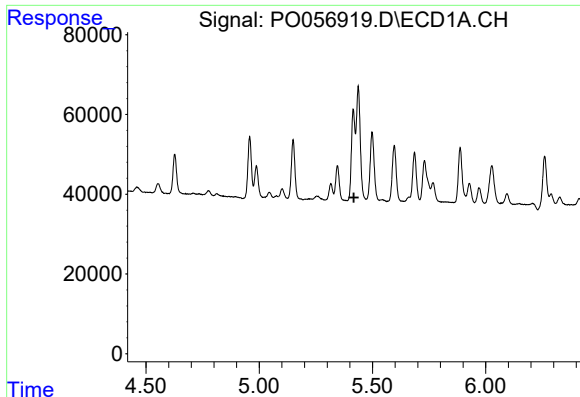

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T.: 5.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

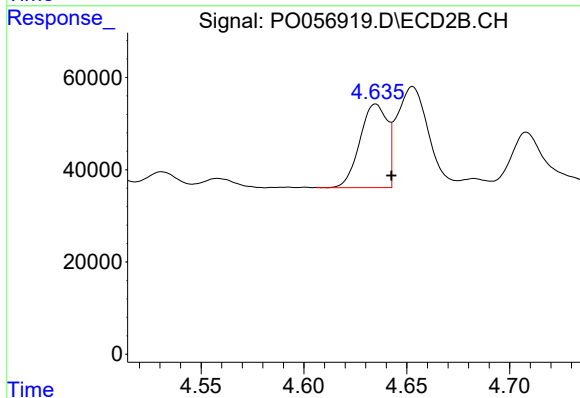


#16 AR-1242-1

R.T.: 4.635 min
Delta R.T.: -0.008 min
Response: 167323
Conc: 135.09 ng/ml

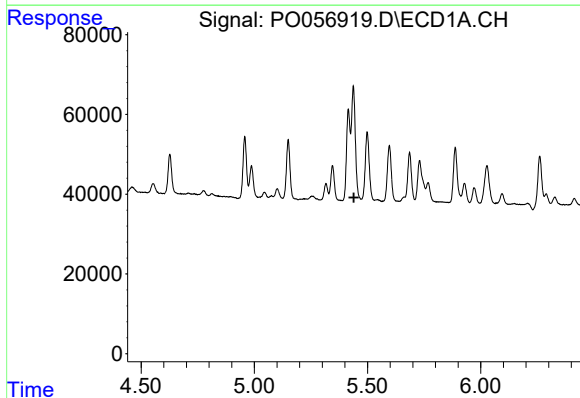


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T.: 5.440 min
Response: 0
Conc: N.D.

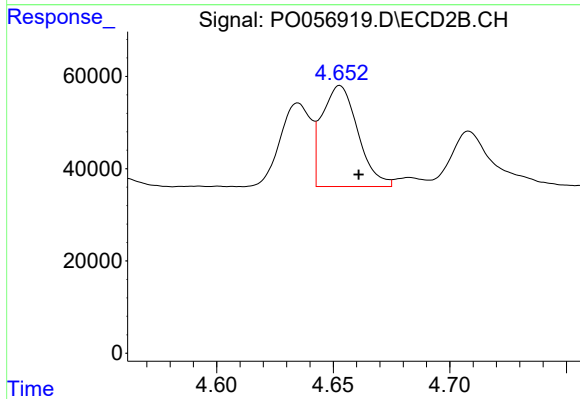

#17 AR-1242-2


R.T.: 4.653 min
Delta R.T.: -0.008 min
Response: 234728
Conc: 130.52 ng/ml

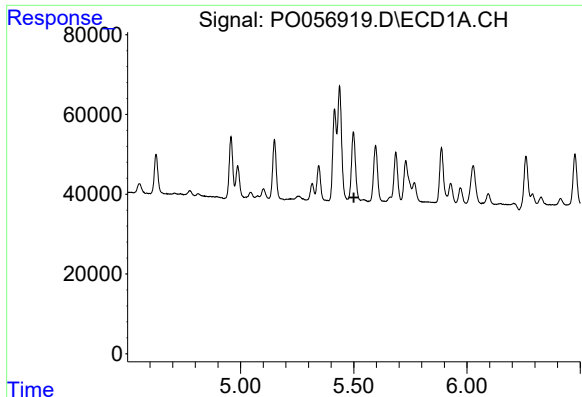

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 5.500 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

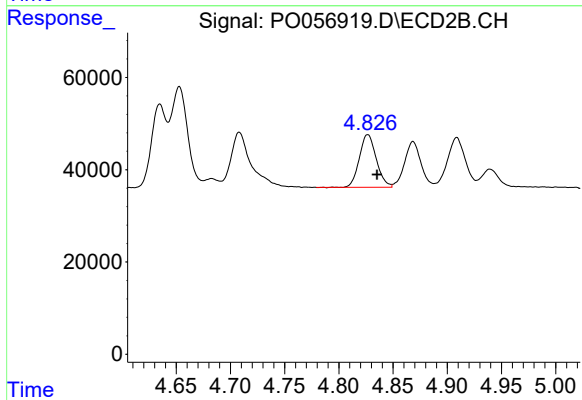


#18 AR-1242-3

R.T.: 4.827 min
Delta R.T.: -0.008 min
Response: 124457
Conc: 126.60 ng/ml

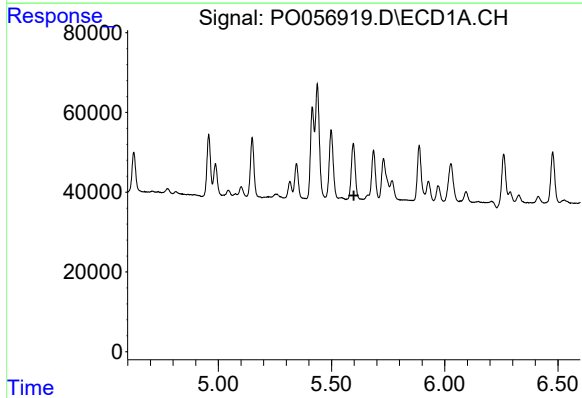


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T.: 5.599 min
Response: 0
Conc: N.D.

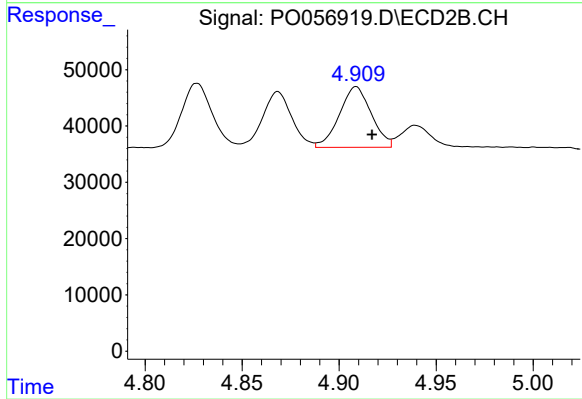

#19 AR-1242-4


R.T.: 4.909 min
Delta R.T.: -0.008 min
Response: 123076
Conc: 126.48 ng/ml

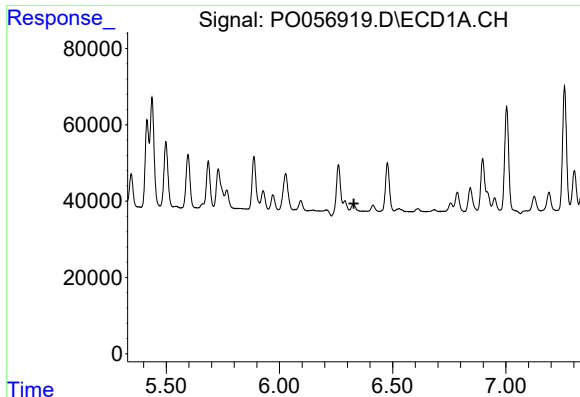

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.329 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

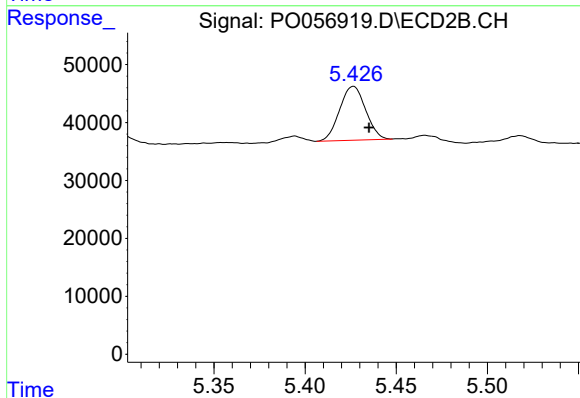


#20 AR-1242-5

R.T.: 5.427 min
Delta R.T.: -0.008 min
Response: 92275
Conc: 78.05 ng/ml

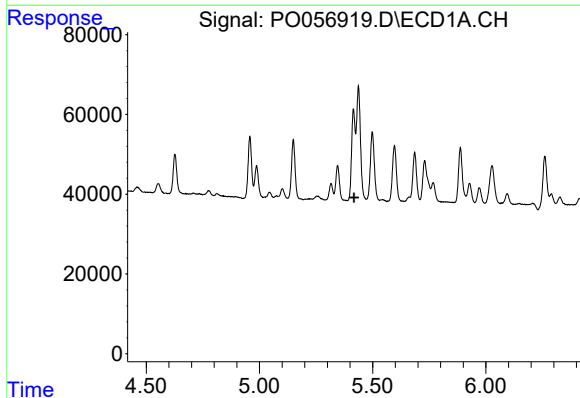


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T.: 5.418 min
Response: 0
Conc: N.D.

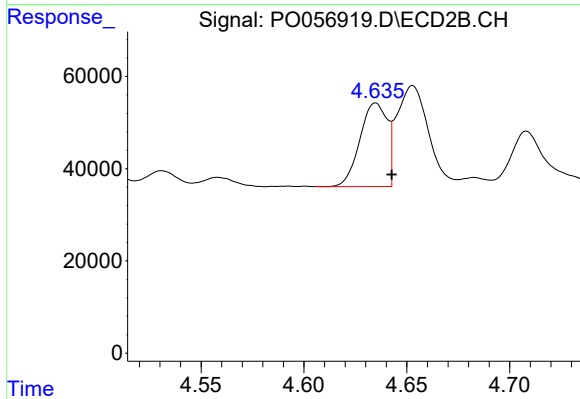

#21 AR-1248-1


R.T.: 4.635 min
Delta R.T.: -0.008 min
Response: 167323
Conc: 178.66 ng/ml

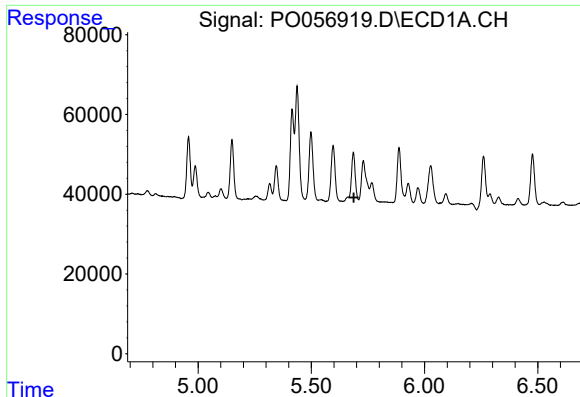

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T.: 5.688 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

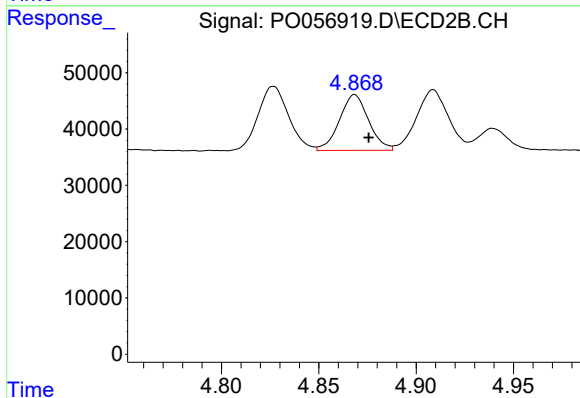


#22 AR-1248-2

R.T.: 4.868 min
Delta R.T.: -0.007 min
Response: 103774
Conc: 81.68 ng/ml

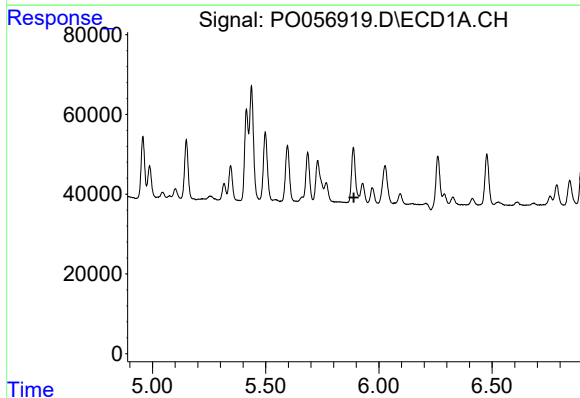


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T.: 5.890 min
Response: 0
Conc: N.D.

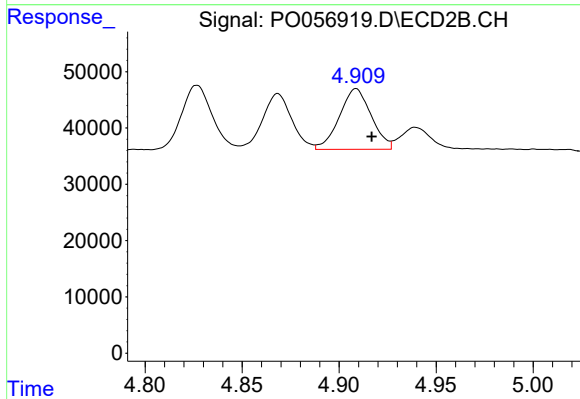

#23 AR-1248-3


R.T.: 4.909 min
Delta R.T.: -0.008 min
Response: 123076
Conc: 94.25 ng/ml

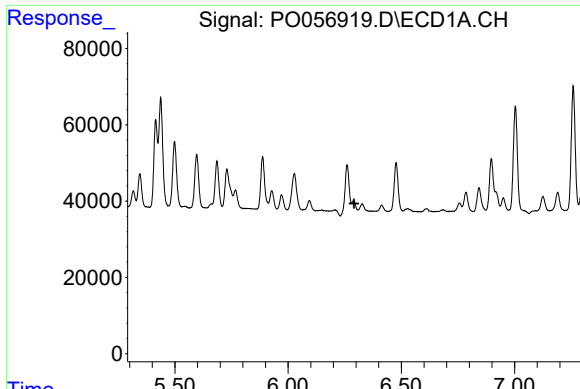

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 6.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

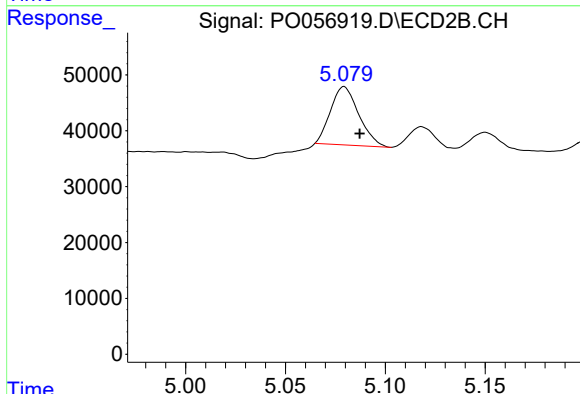


#24 AR-1248-4

R.T.: 5.079 min
Delta R.T.: -0.008 min
Response: 102596
Conc: 64.79 ng/ml

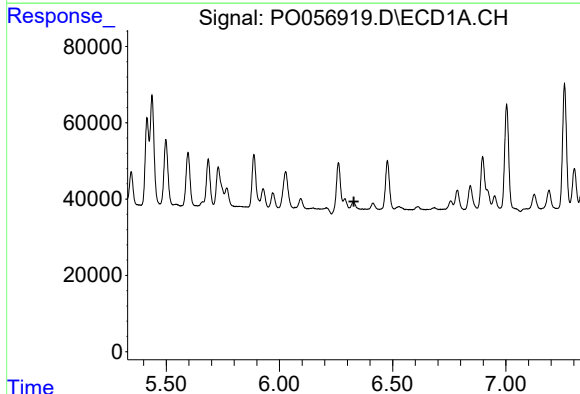


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 6.329 min
Response: 0
Conc: N.D.

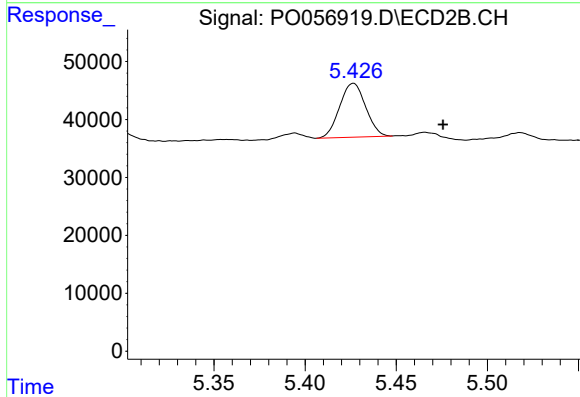

#25 AR-1248-5


R.T.: 5.427 min
Delta R.T.: -0.049 min
Response: 92275
Conc: 55.75 ng/ml

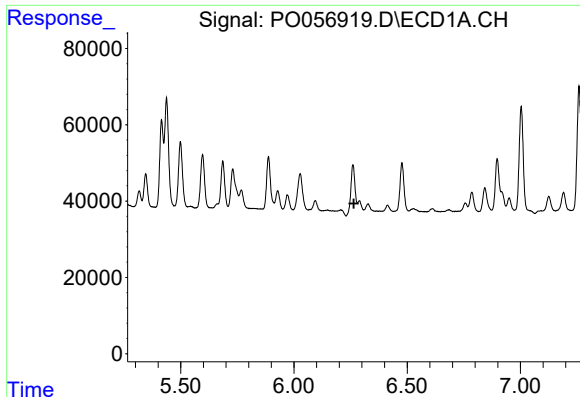

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 6.264 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

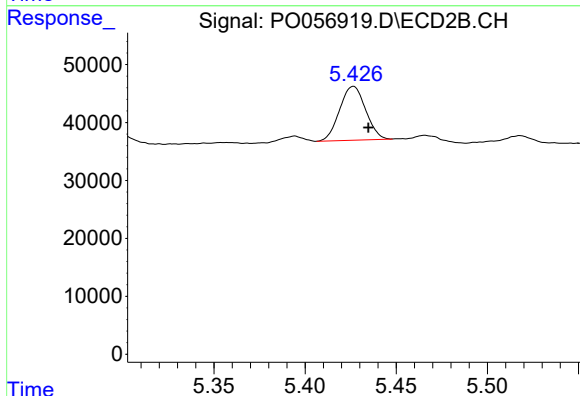


#26 AR-1254-1

R.T.: 5.427 min
Delta R.T.: -0.008 min
Response: 92275
Conc: 34.89 ng/ml

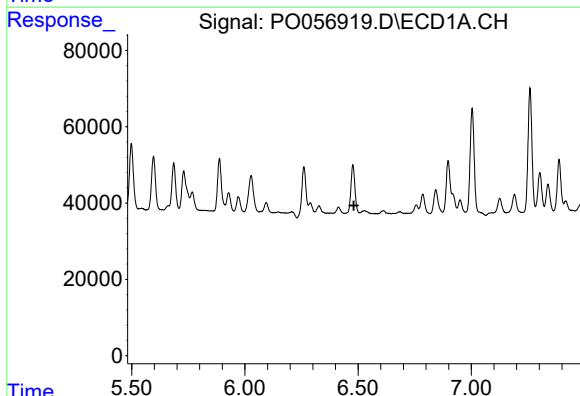


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T.: 6.481 min
Response: 0
Conc: N.D.

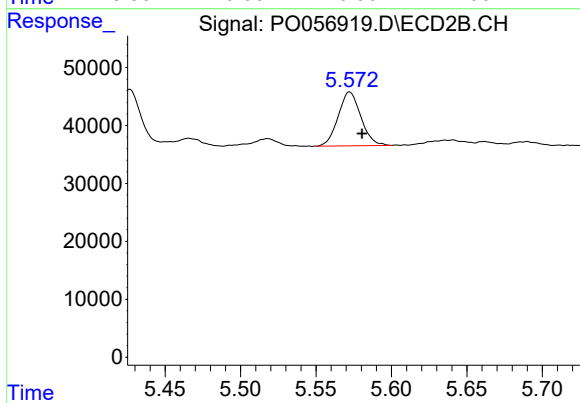

#27 AR-1254-2


R.T.: 5.572 min
Delta R.T.: -0.008 min
Response: 97356
Conc: 45.16 ng/ml

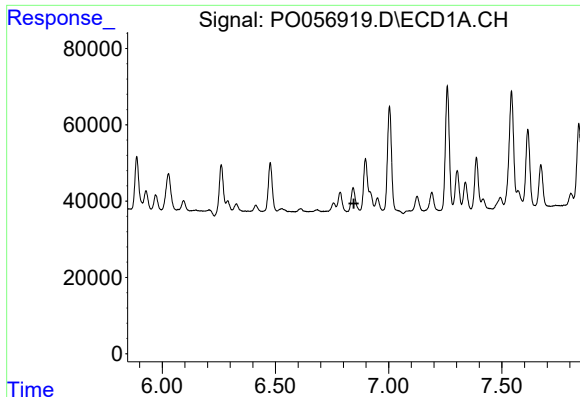

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

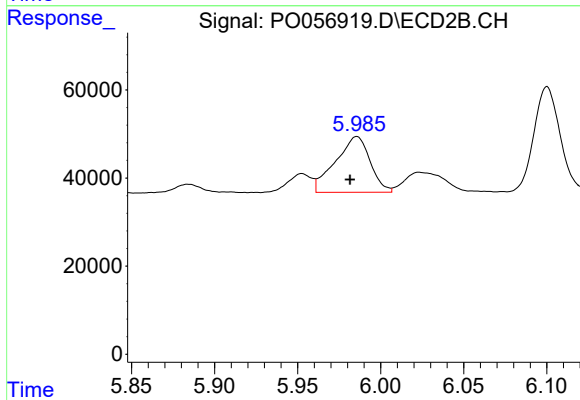


#28 AR-1254-3

R.T.: 5.986 min
Delta R.T.: 0.004 min
Response: 184005
Conc: 50.26 ng/ml

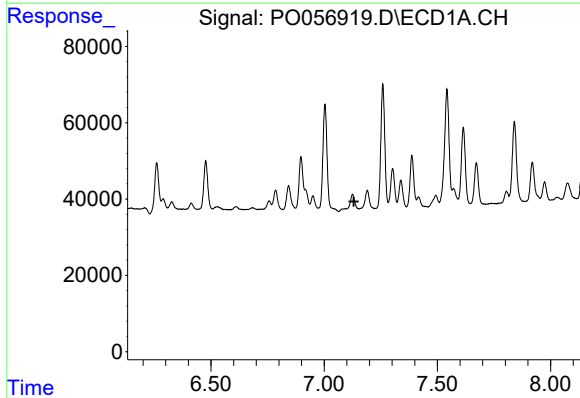


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T.: 7.131 min
Response: 0
Conc: N.D.

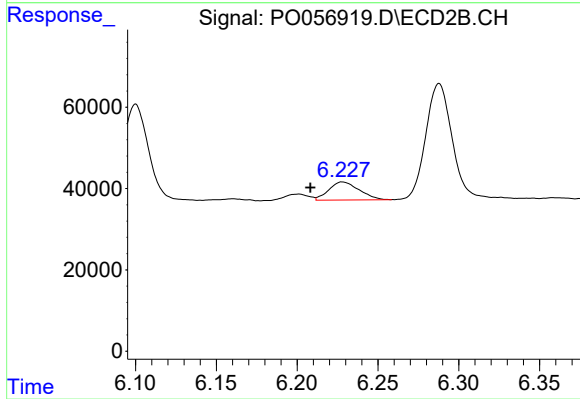

#29 AR-1254-4


R.T.: 6.228 min
Delta R.T.: 0.020 min
Response: 57915
Conc: 26.36 ng/ml

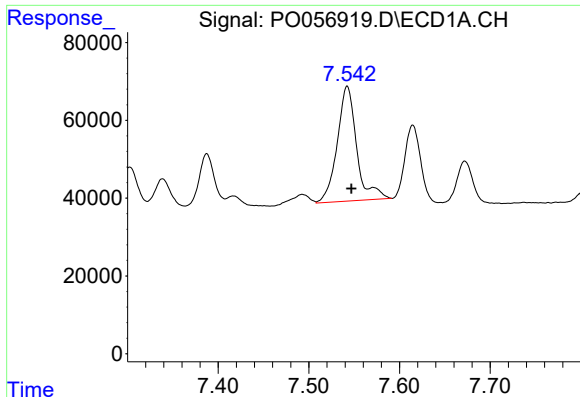

#30 AR-1254-5


R.T.: 7.542 min
Delta R.T.: -0.005 min
Response: 439259
Conc: 116.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

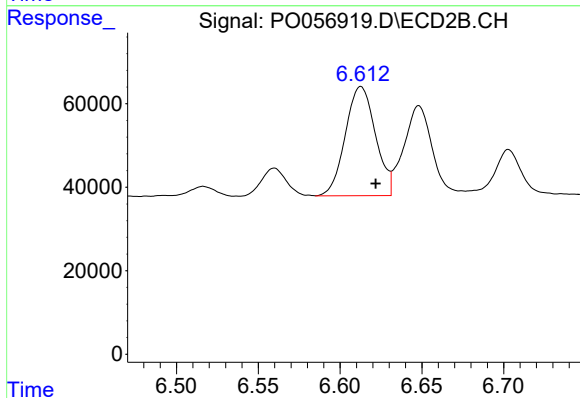


#30 AR-1254-5

R.T.: 6.613 min
Delta R.T.: -0.009 min
Response: 335196
Conc: 105.73 ng/ml

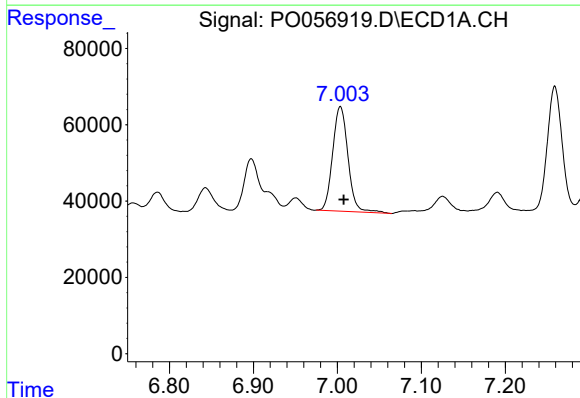


#31 AR-1260-1

R.T.: 7.004 min
Delta R.T.: -0.004 min
Response: 348570
Conc: 135.83 ng/ml

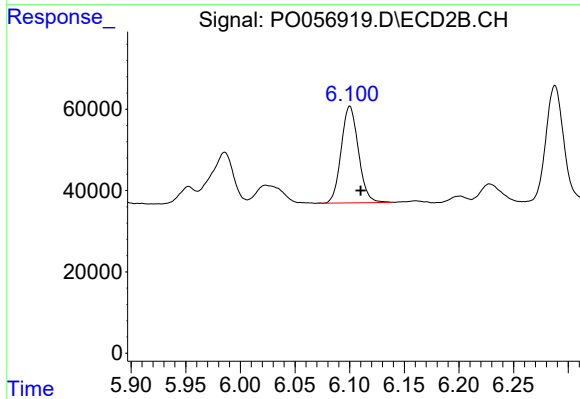

#31 AR-1260-1


R.T.: 6.100 min
Delta R.T.: -0.010 min
Response: 260549
Conc: 130.25 ng/ml

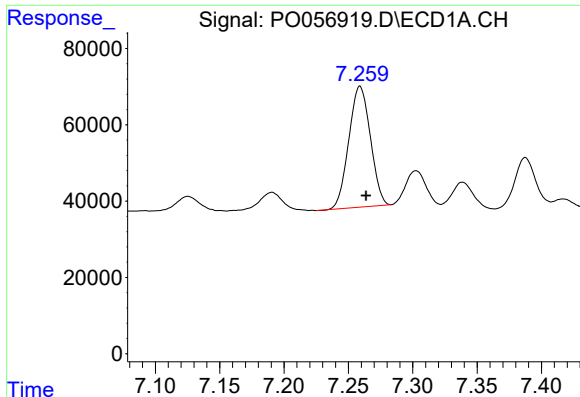

#32 AR-1260-2


R.T.: 7.259 min
Delta R.T.: -0.005 min
Response: 368621
Conc: 121.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

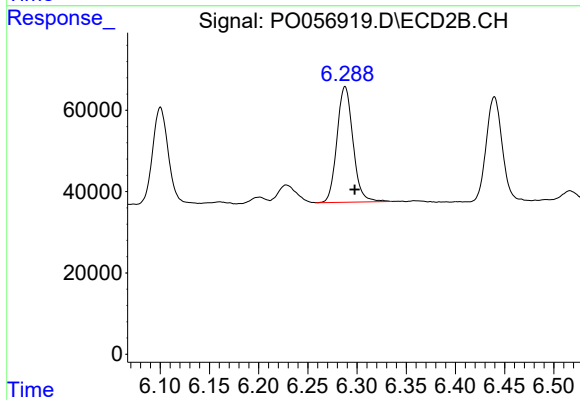


#32 AR-1260-2

R.T.: 6.288 min
Delta R.T.: -0.010 min
Response: 322103
Conc: 130.67 ng/ml

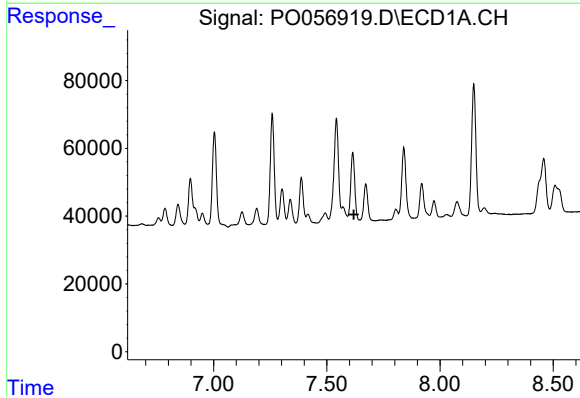


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.620 min
Response: 0
Conc: N.D.

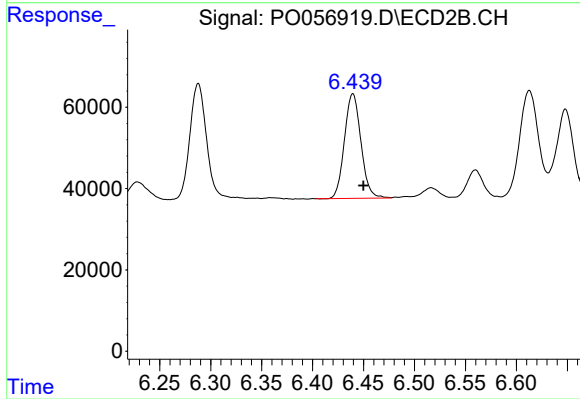

#33 AR-1260-3


R.T.: 6.440 min
Delta R.T.: -0.010 min
Response: 290265
Conc: 129.40 ng/ml

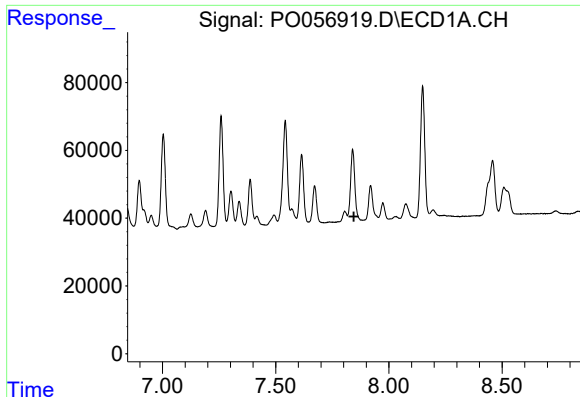

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 7.845 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

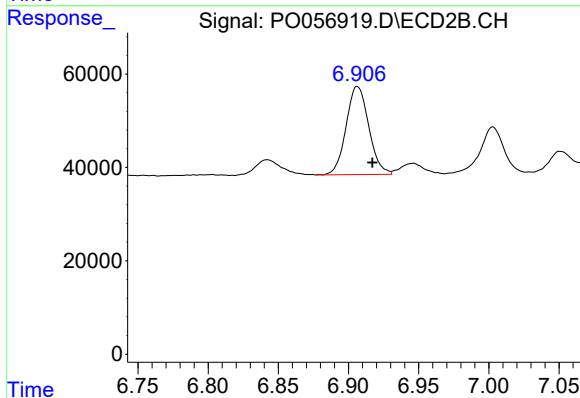


#34 AR-1260-4

R.T.: 6.906 min
Delta R.T.: -0.010 min
Response: 211927
Conc: 113.88 ng/ml

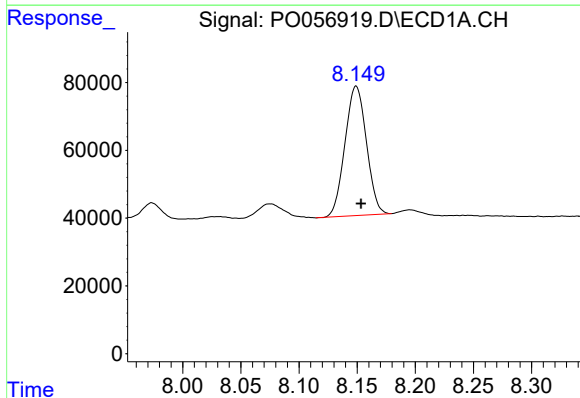


#35 AR-1260-5

R.T.: 8.149 min
Delta R.T.: -0.004 min
Response: 491215
Conc: 102.72 ng/ml

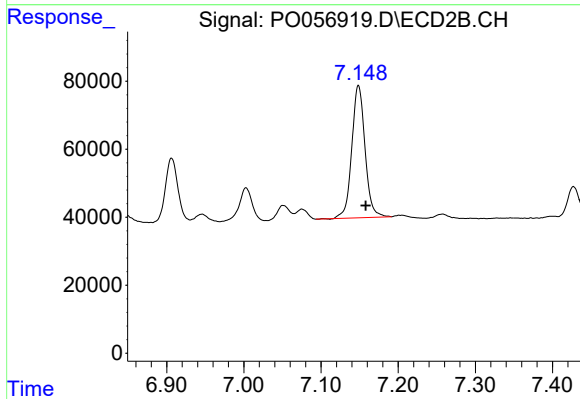

#35 AR-1260-5


R.T.: 7.148 min
Delta R.T.: -0.010 min
Response: 463417
Conc: 107.46 ng/ml

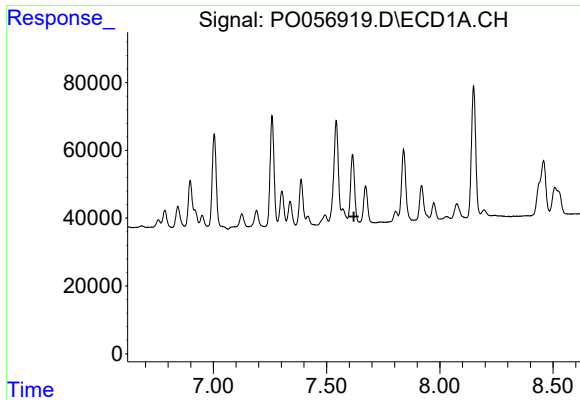

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 7.620 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

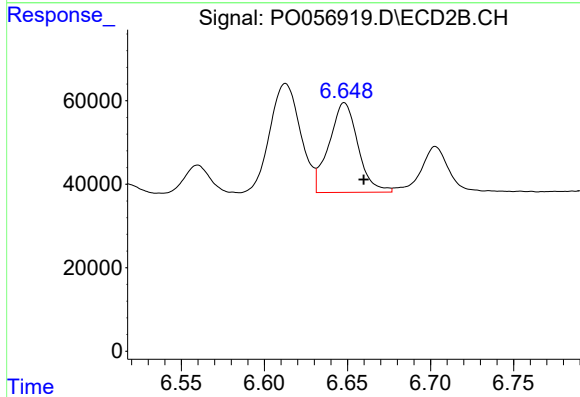


#36 AR-1262-1

R.T.: 6.648 min
Delta R.T.: -0.012 min
Response: 260309
Conc: 62.36 ng/ml

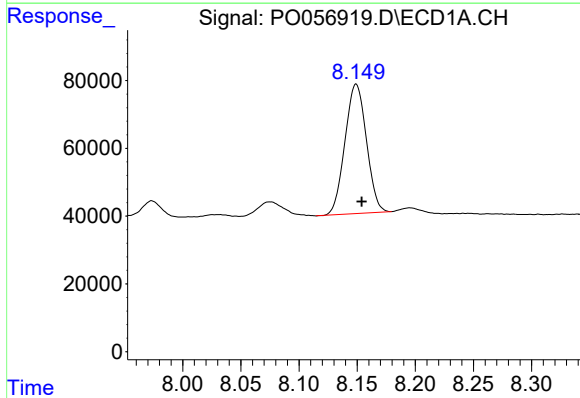


#37 AR-1262-2

R.T.: 8.149 min
Delta R.T.: -0.005 min
Response: 491215
Conc: 64.43 ng/ml

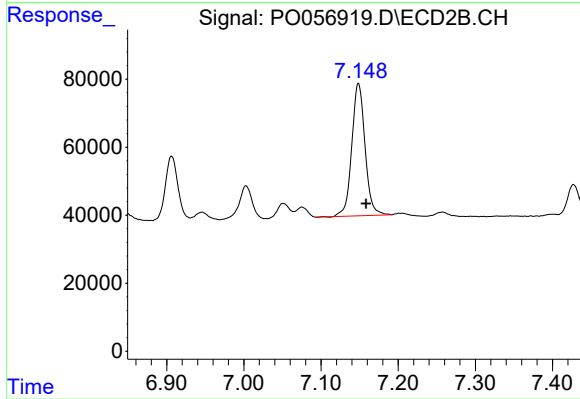

#37 AR-1262-2


R.T.: 7.148 min
Delta R.T.: -0.010 min
Response: 463417
Conc: 67.45 ng/ml

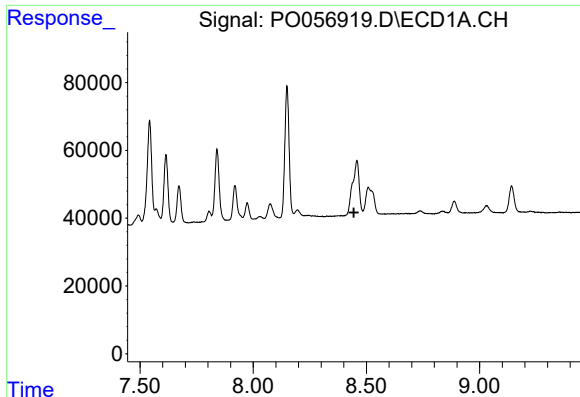

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.445 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

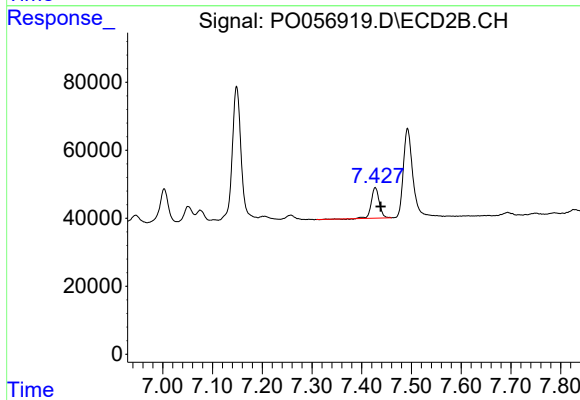


#38 AR-1262-3

R.T.: 7.427 min
Delta R.T.: -0.011 min
Response: 99873
Conc: 33.82 ng/ml

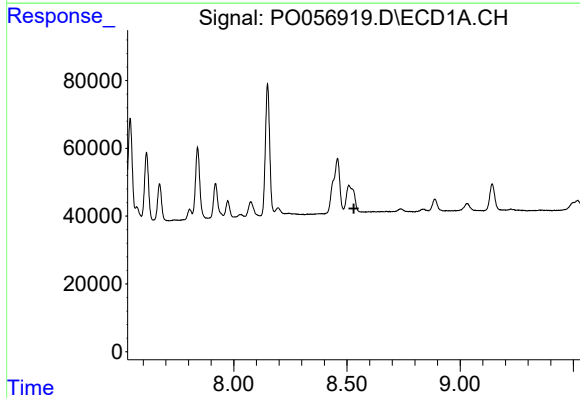


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.530 min
Response: 0
Conc: N.D.

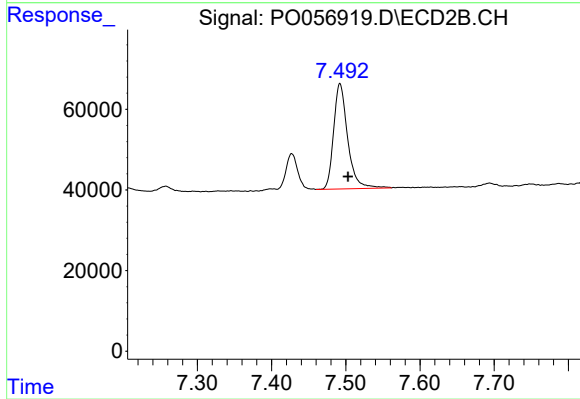

#39 AR-1262-4


R.T.: 7.492 min
Delta R.T.: -0.011 min
Response: 343085
Conc: 65.84 ng/ml

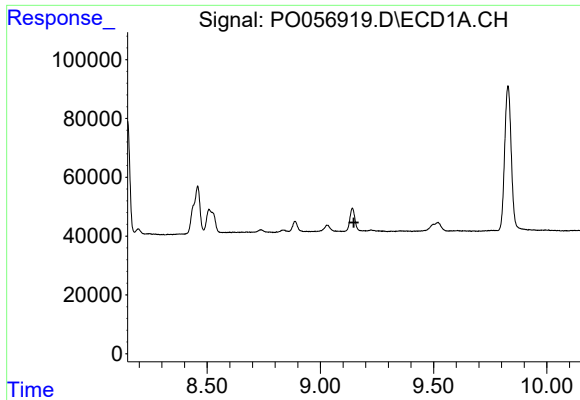

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 9.148 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

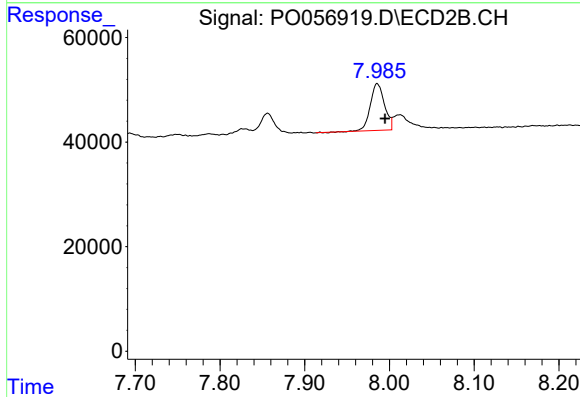


#40 AR-1262-5

R.T.: 7.986 min
Delta R.T.: -0.009 min
Response: 103314
Conc: 44.49 ng/ml

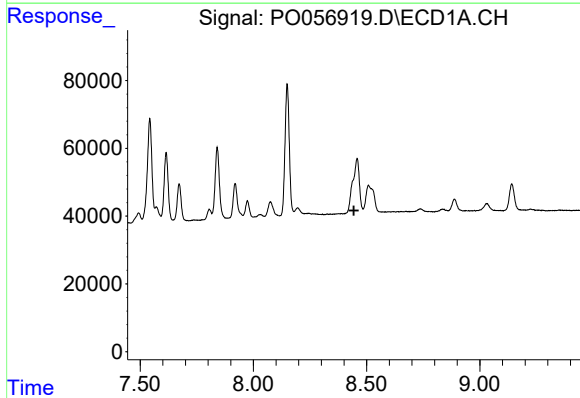


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 8.444 min
Response: 0
Conc: N.D.

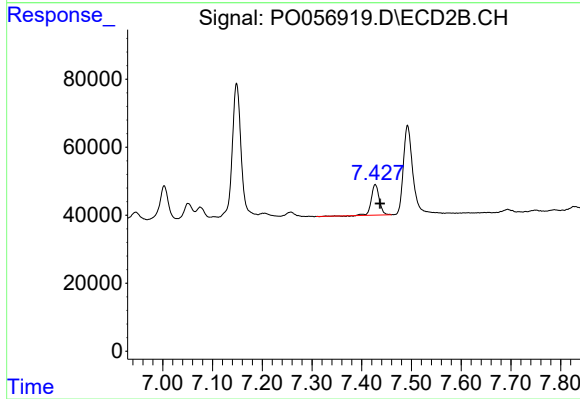

#41 AR-1268-1


R.T.: 7.427 min
Delta R.T.: -0.010 min
Response: 99873
Conc: 13.38 ng/ml

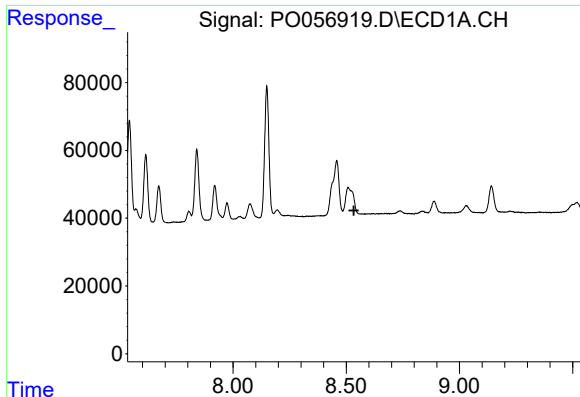

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 8.534 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

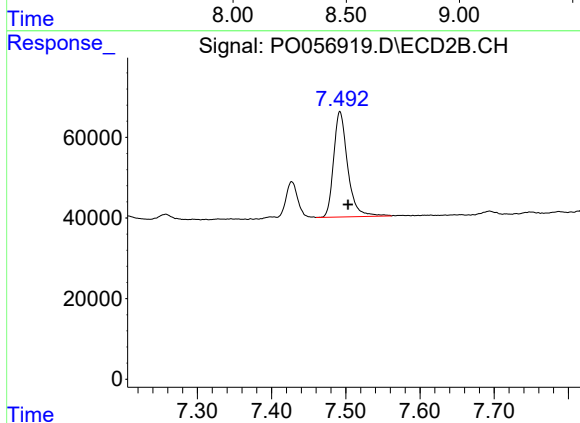


#42 AR-1268-2

R.T.: 7.492 min
Delta R.T.: -0.011 min
Response: 343085
Conc: 49.13 ng/ml

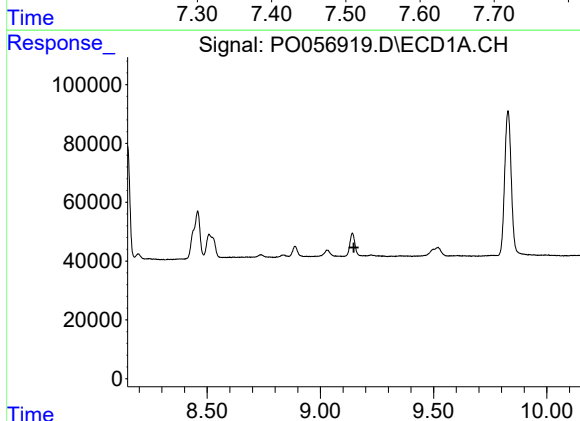


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.148 min
Response: 0
Conc: N.D.

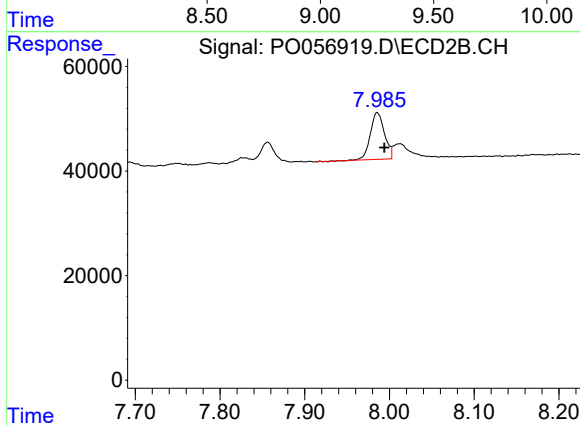

#44 AR-1268-4


R.T.: 7.986 min
Delta R.T.: -0.008 min
Response: 103314
Conc: 44.26 ng/ml

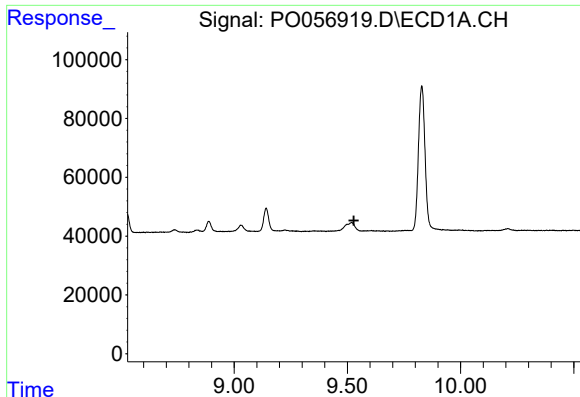

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD

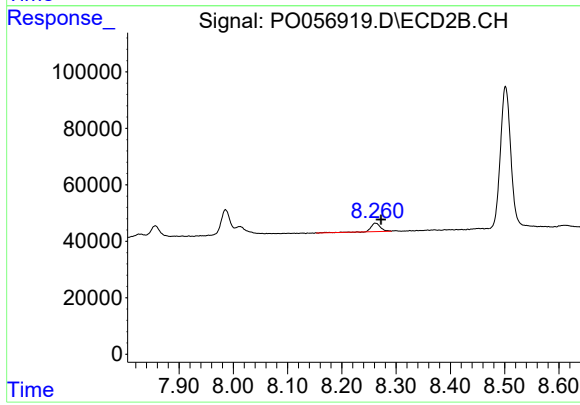

#45 AR-1268-5

R.T.: 8.262 min
Delta R.T.: -0.010 min
Response: 36574
Conc: 2.11 ng/ml