

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060619\
 Data File : P0056932.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jun 2019 17:17
 Operator : SM/SJ
 Sample : K3183-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SP-COMP-1


Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 02:30:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.255	3.565	981396	759845	25.635	23.041
2)	SA Decachlor...	9.828	8.501	875240	614723	17.832	17.240
Target Compounds							
10)	L2 AR-1221-3	0.000	3.979	0	45457	N.D.	37.974 #
11)	L3 AR-1232-1	0.000	3.979	0	45457	N.D.	50.600 #
29)	L6 AR-1254-4	0.000	6.156	0	21663	N.D.	9.860 #
30)	L6 AR-1254-5	0.000	6.612	0	78287	N.D.	24.694 #
31)	L7 AR-1260-1	0.000	6.101	0	52451	N.D.	26.220 #
32)	L7 AR-1260-2	0.000	6.288	0	30520	N.D.	12.382 #
33)	L7 AR-1260-3	0.000	6.439	0	31489	N.D.	14.037 #
34)	L7 AR-1260-4	0.000	6.905	0	23538	N.D.	12.648 #
35)	L7 AR-1260-5	0.000	7.148	0	73914	N.D.	17.140 #
36)	L8 AR-1262-1	0.000	6.647	0	40911	N.D.	9.801 #
37)	L8 AR-1262-2	0.000	7.148	0	73914	N.D.	10.758 #
38)	L8 AR-1262-3	0.000	7.428	0	25791	N.D.	8.732 #
39)	L8 AR-1262-4	0.000	7.491	0	47245	N.D.	9.067 #
40)	L8 AR-1262-5	0.000	7.985	0	15874	N.D.	6.836 #
41)	L9 AR-1268-1	0.000	7.428	0	25791	N.D.	3.455 #
42)	L9 AR-1268-2	0.000	7.491	0	47245	N.D.	6.766 #
43)	L9 AR-1268-3	0.000	7.694	0	22763	N.D.	3.835 #
44)	L9 AR-1268-4	0.000	7.985	0	15874	N.D.	6.801 #
45)	L9 AR-1268-5	0.000	8.262	0	42337	N.D.	2.446 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

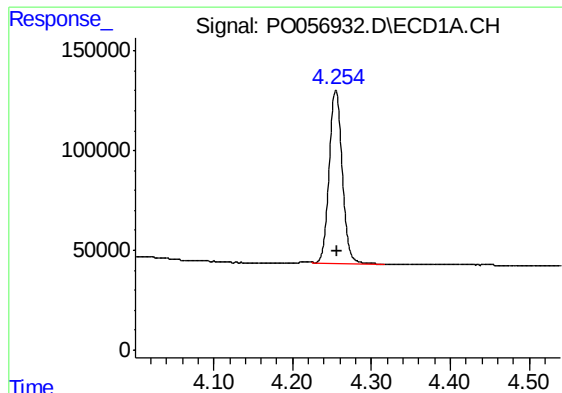

#1 Tetrachloro-m-xylene


R.T.: 4.255 min
Delta R.T.: -0.001 min
Response: 981396
Conc: 25.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-COMP-1

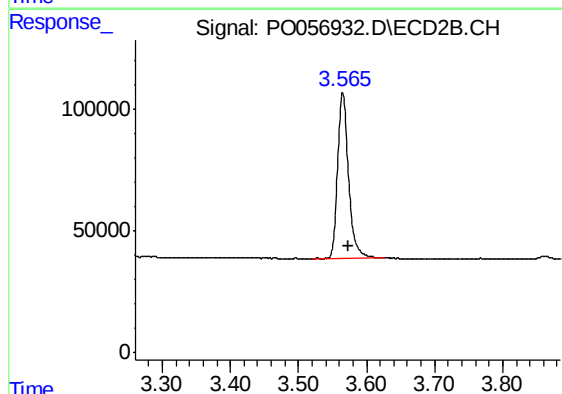


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: -0.008 min
Response: 759845
Conc: 23.04 ng/ml

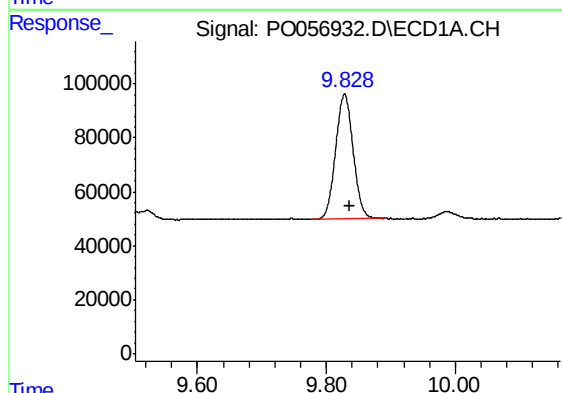


#2 Decachlorobiphenyl

R.T.: 9.828 min
Delta R.T.: -0.008 min
Response: 875240
Conc: 17.83 ng/ml

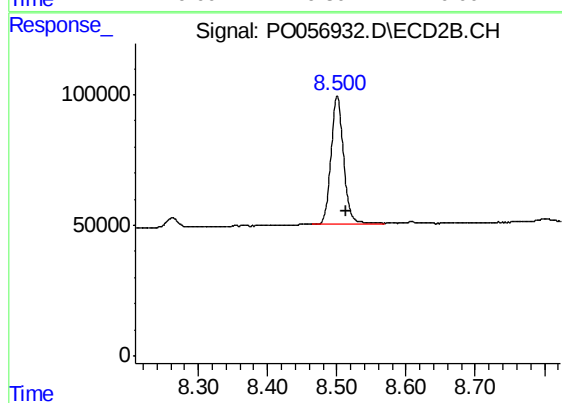

#2 Decachlorobiphenyl


R.T.: 8.501 min
Delta R.T.: -0.012 min
Response: 614723
Conc: 17.24 ng/ml

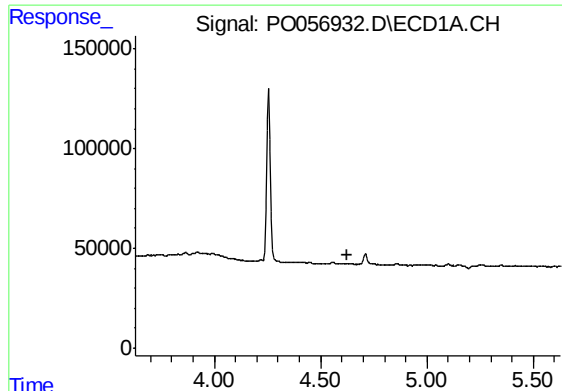

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.628 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SP-COMP-1

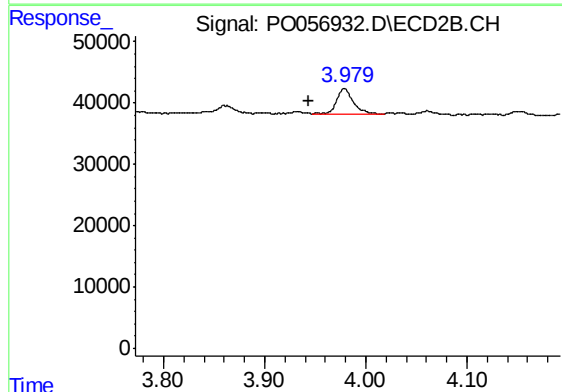


#10 AR-1221-3

R.T.: 3.979 min
Delta R.T.: 0.036 min
Response: 45457
Conc: 37.97 ng/ml

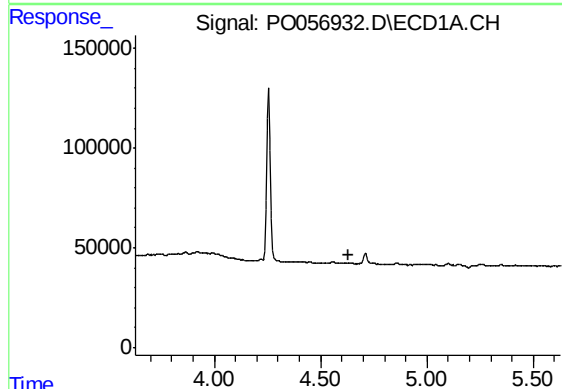


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.629 min
Response: 0
Conc: N.D.

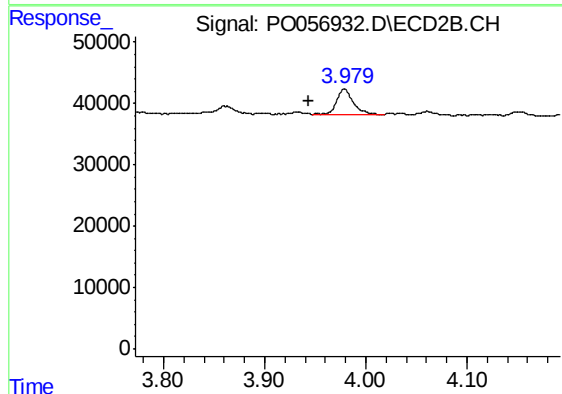

#11 AR-1232-1


R.T.: 3.979 min
Delta R.T.: 0.036 min
Response: 45457
Conc: 50.60 ng/ml

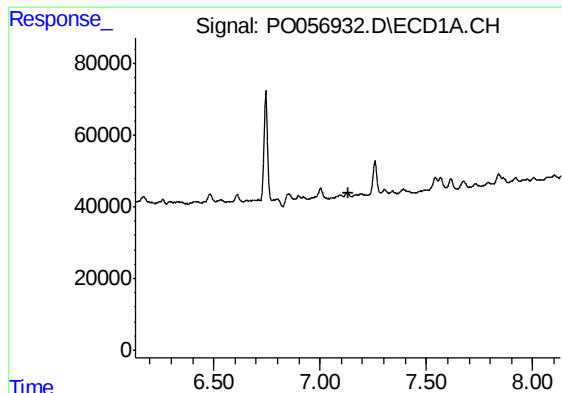

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 7.131 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SP-COMP-1

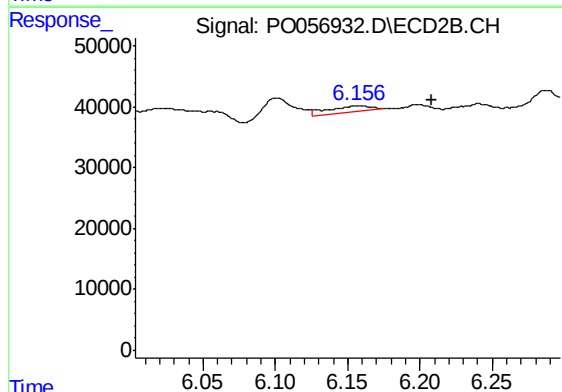


#29 AR-1254-4

R.T.: 6.156 min
Delta R.T.: -0.052 min
Response: 21663
Conc: 9.86 ng/ml

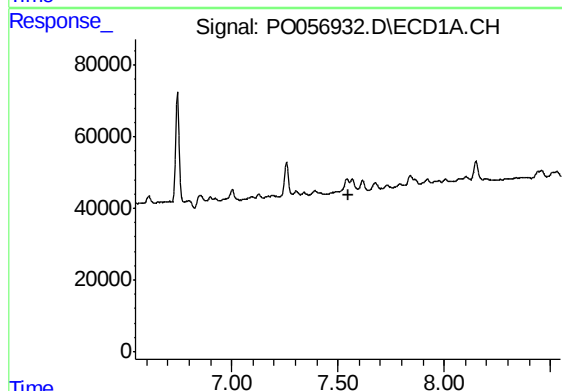


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.547 min
Response: 0
Conc: N.D.

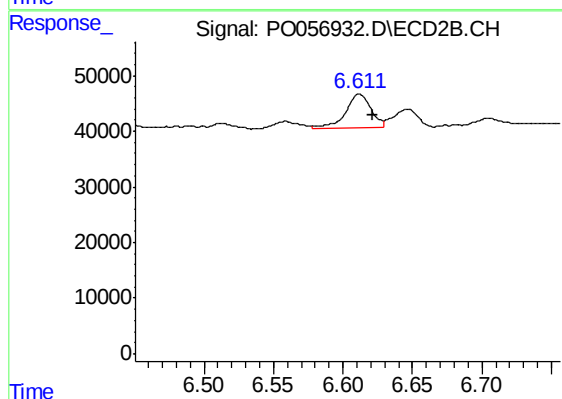

#30 AR-1254-5


R.T.: 6.612 min
Delta R.T.: -0.010 min
Response: 78287
Conc: 24.69 ng/ml

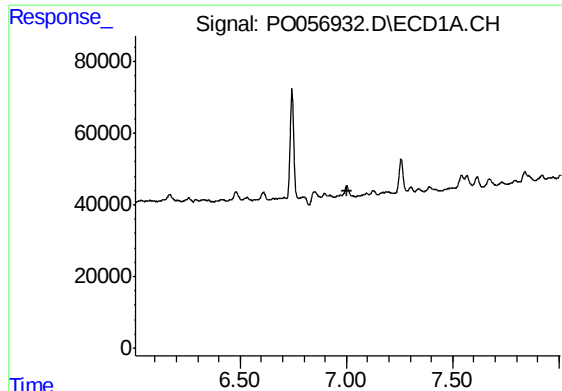

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 7.008 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SP-COMP-1

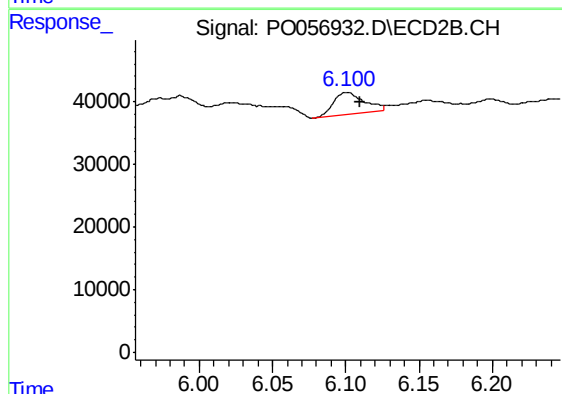


#31 AR-1260-1

R.T.: 6.101 min
Delta R.T.: -0.009 min
Response: 52451
Conc: 26.22 ng/ml

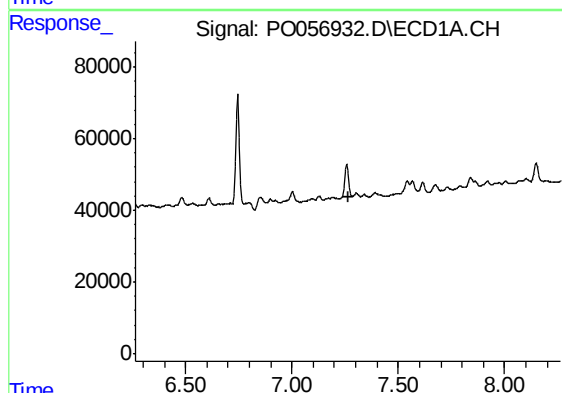


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.264 min
Response: 0
Conc: N.D.

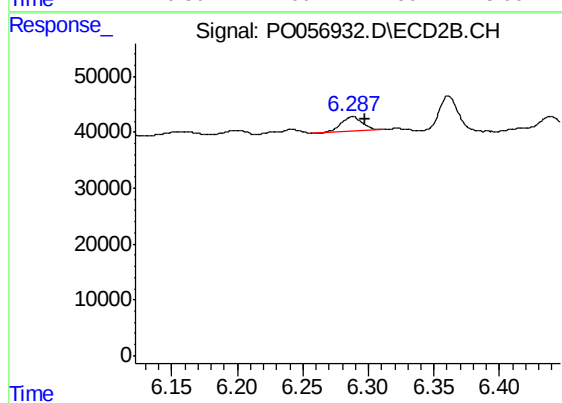

#32 AR-1260-2


R.T.: 6.288 min
Delta R.T.: -0.009 min
Response: 30520
Conc: 12.38 ng/ml

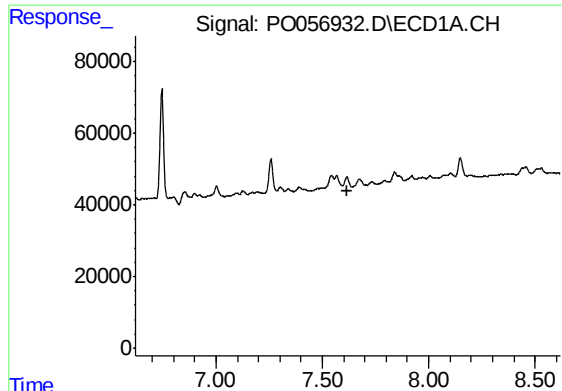

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.620 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SP-COMP-1

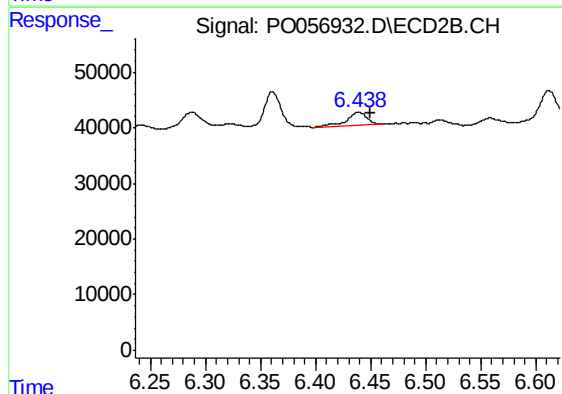


#33 AR-1260-3

R.T.: 6.439 min
Delta R.T.: -0.011 min
Response: 31489
Conc: 14.04 ng/ml

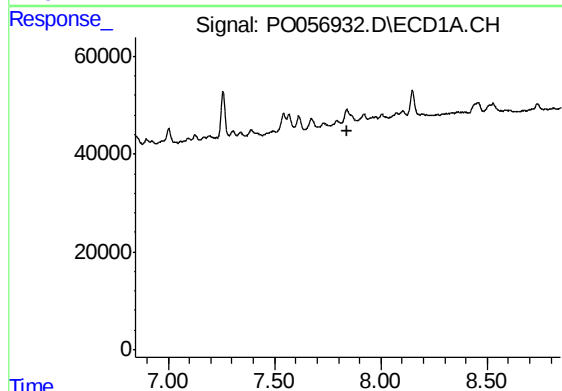


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.845 min
Response: 0
Conc: N.D.

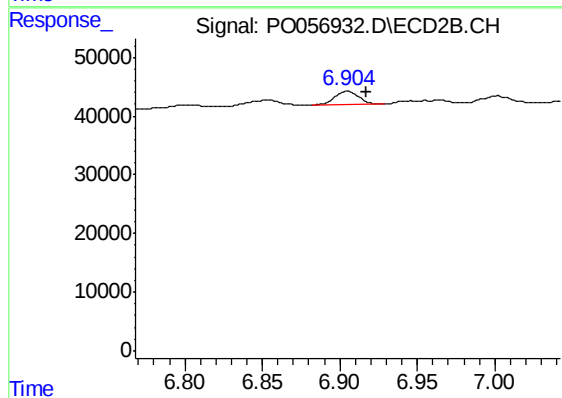

#34 AR-1260-4


R.T.: 6.905 min
Delta R.T.: -0.012 min
Response: 23538
Conc: 12.65 ng/ml

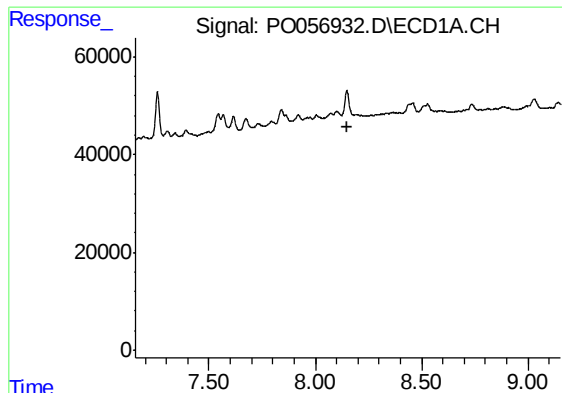

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.153 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SP-COMP-1

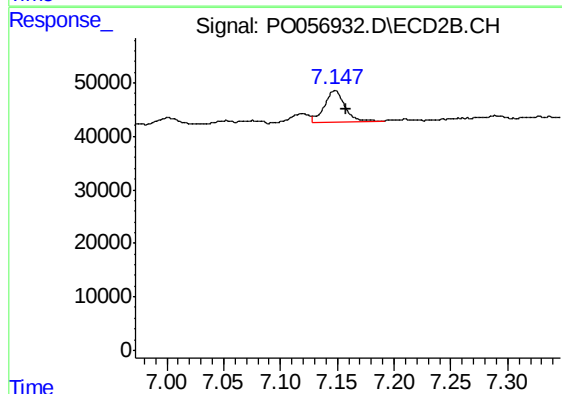


#35 AR-1260-5

R.T.: 7.148 min
Delta R.T.: -0.010 min
Response: 73914
Conc: 17.14 ng/ml

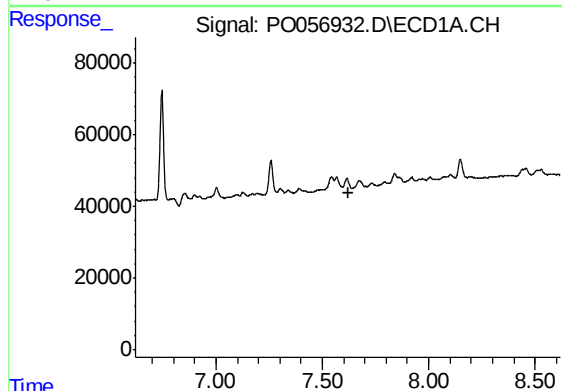


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.620 min
Response: 0
Conc: N.D.

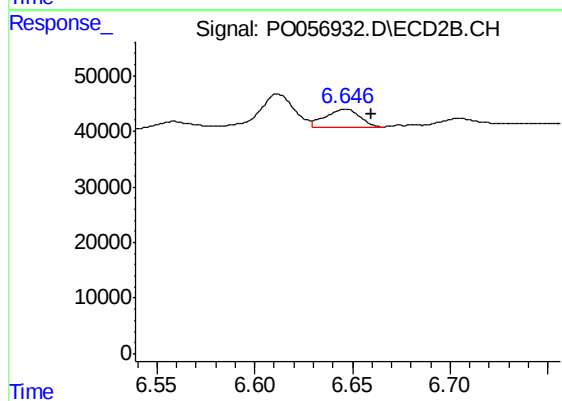

#36 AR-1262-1


R.T.: 6.647 min
Delta R.T.: -0.013 min
Response: 40911
Conc: 9.80 ng/ml

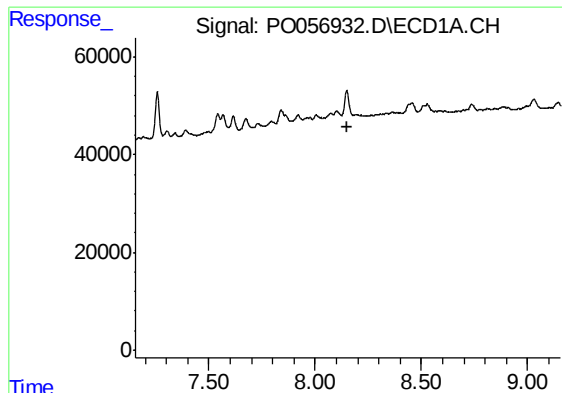

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 8.154 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SP-COMP-1

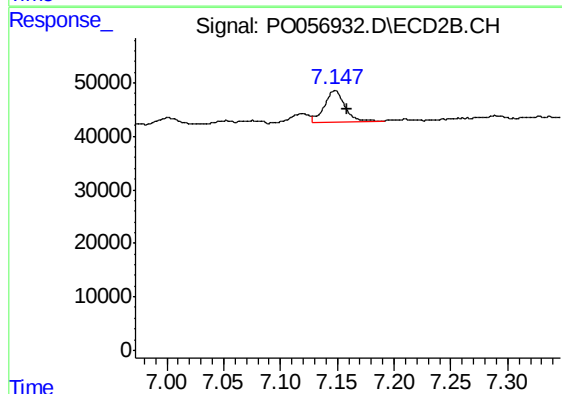


#37 AR-1262-2

R.T.: 7.148 min
Delta R.T.: -0.011 min
Response: 73914
Conc: 10.76 ng/ml

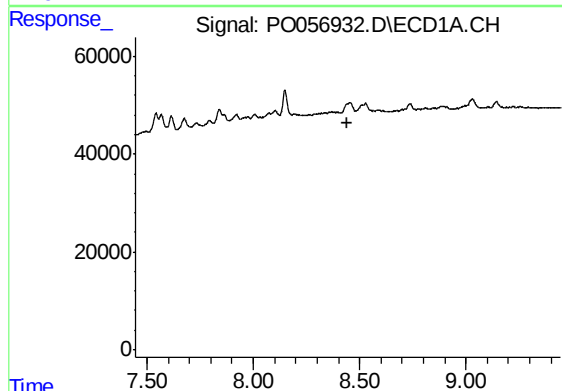


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.445 min
Response: 0
Conc: N.D.

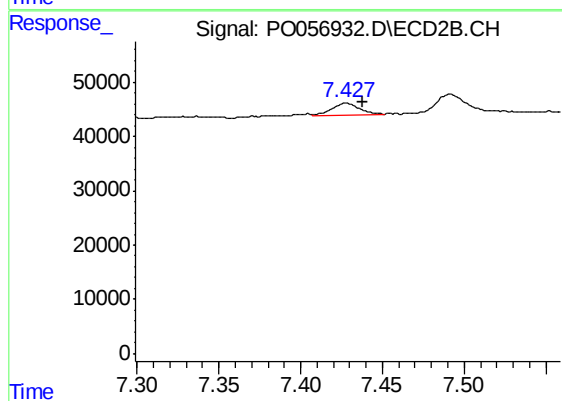

#38 AR-1262-3


R.T.: 7.428 min
Delta R.T.: -0.010 min
Response: 25791
Conc: 8.73 ng/ml

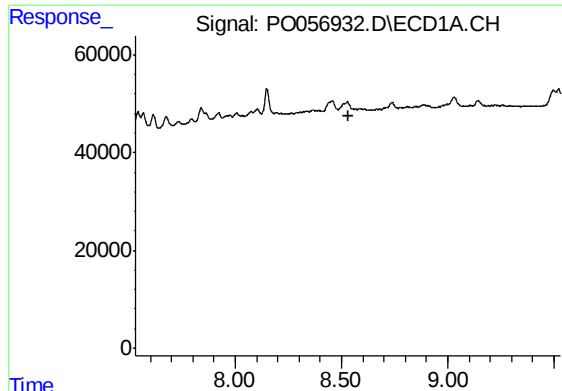

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.530 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SP-COMP-1

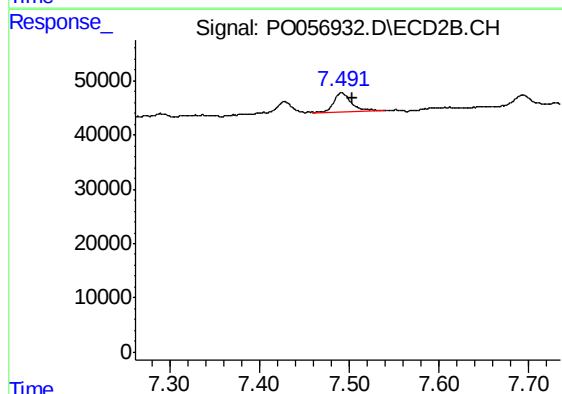


#39 AR-1262-4

R.T.: 7.491 min
Delta R.T.: -0.012 min
Response: 47245
Conc: 9.07 ng/ml

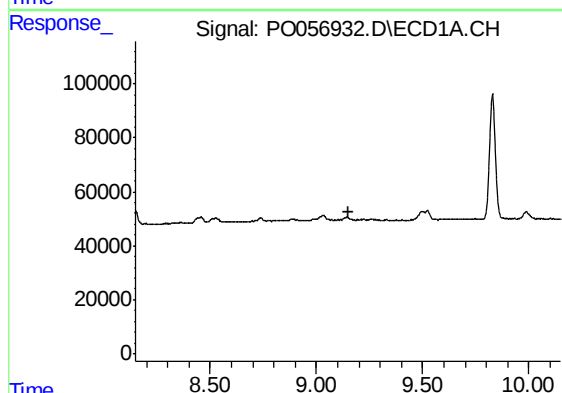


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.148 min
Response: 0
Conc: N.D.

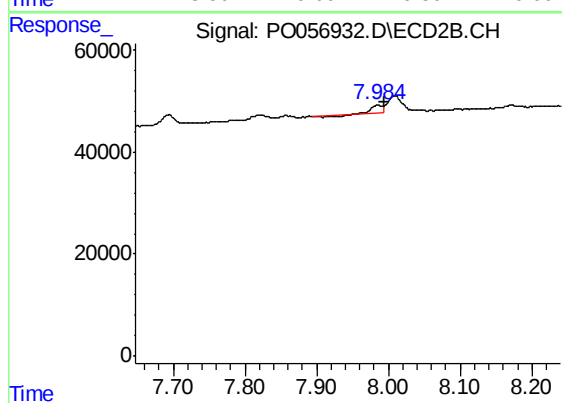

#40 AR-1262-5


R.T.: 7.985 min
Delta R.T.: -0.010 min
Response: 15874
Conc: 6.84 ng/ml

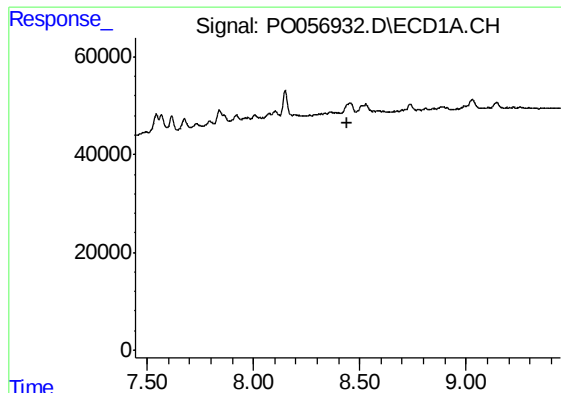

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.444 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SP-COMP-1

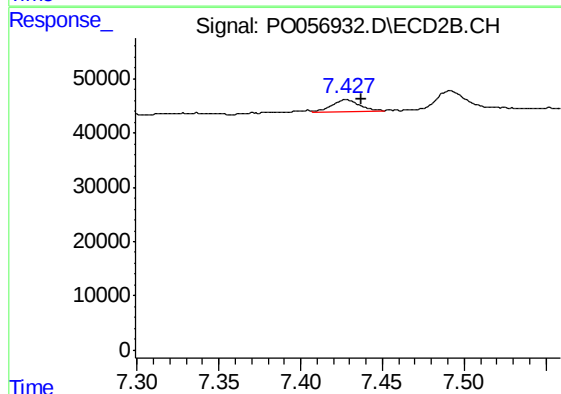


#41 AR-1268-1

R.T.: 7.428 min
Delta R.T.: -0.009 min
Response: 25791
Conc: 3.45 ng/ml

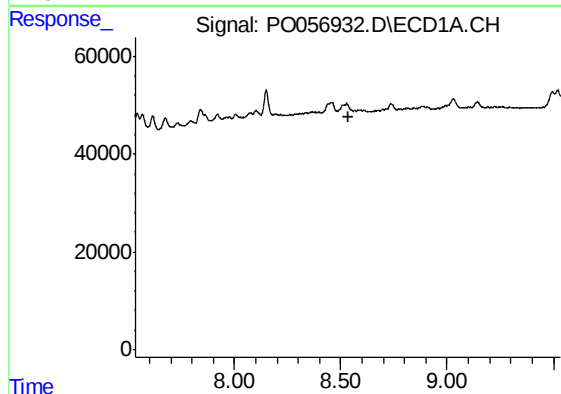


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.534 min
Response: 0
Conc: N.D.

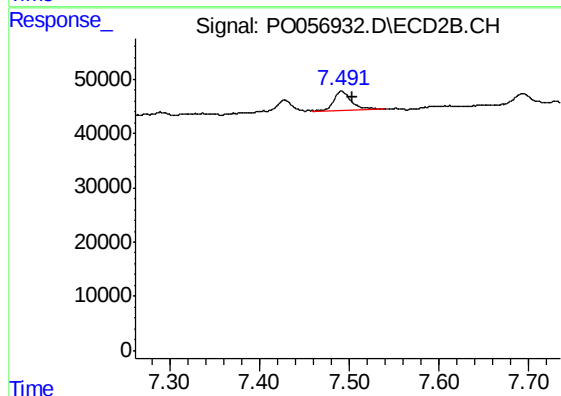

#42 AR-1268-2


R.T.: 7.491 min
Delta R.T.: -0.012 min
Response: 47245
Conc: 6.77 ng/ml

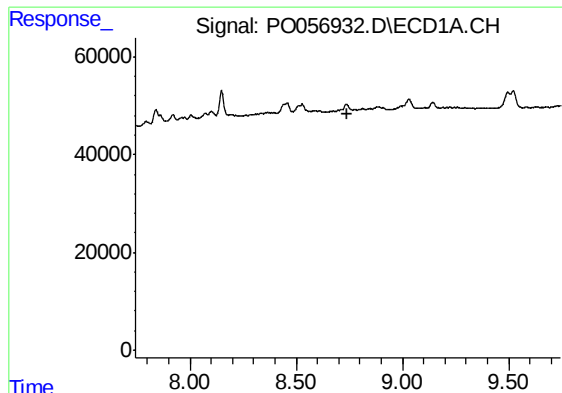

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 8.743 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SP-COMP-1

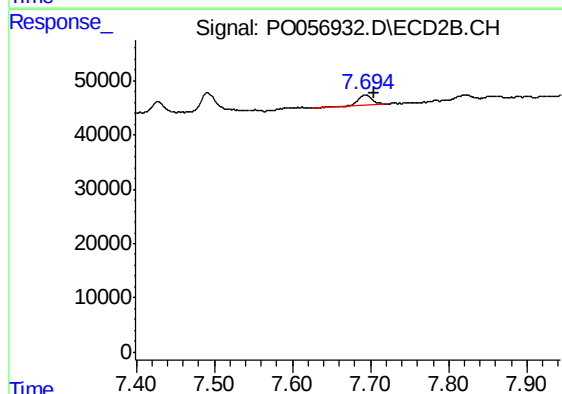


#43 AR-1268-3

R.T.: 7.694 min
Delta R.T.: -0.011 min
Response: 22763
Conc: 3.84 ng/ml

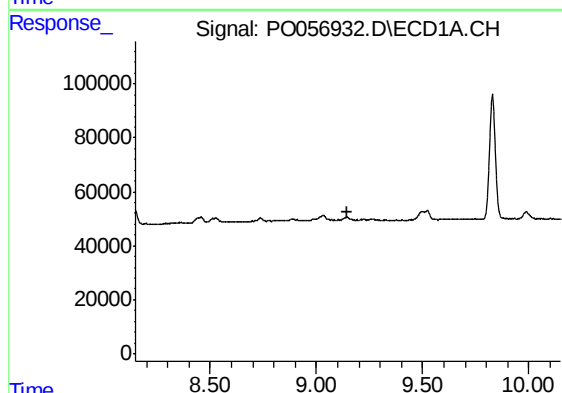


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.148 min
Response: 0
Conc: N.D.

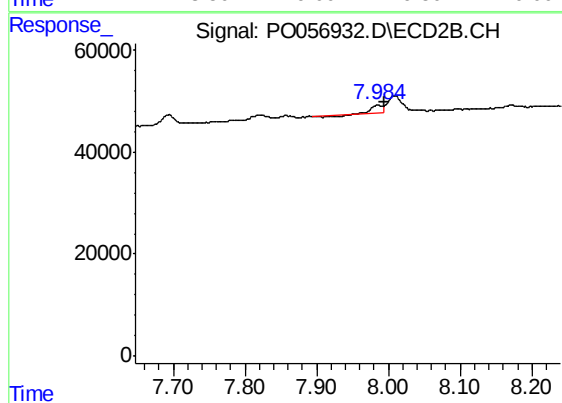

#44 AR-1268-4


R.T.: 7.985 min
Delta R.T.: -0.009 min
Response: 15874
Conc: 6.80 ng/ml

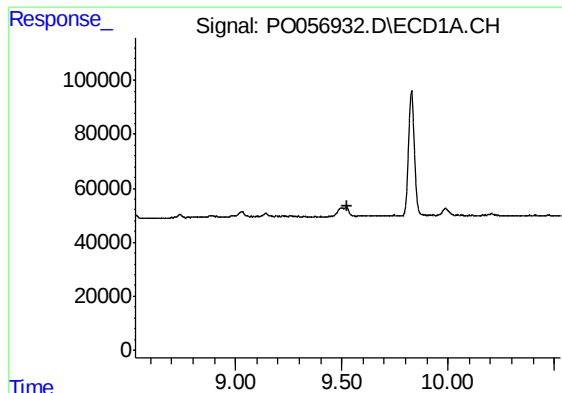

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SP-COMP-1

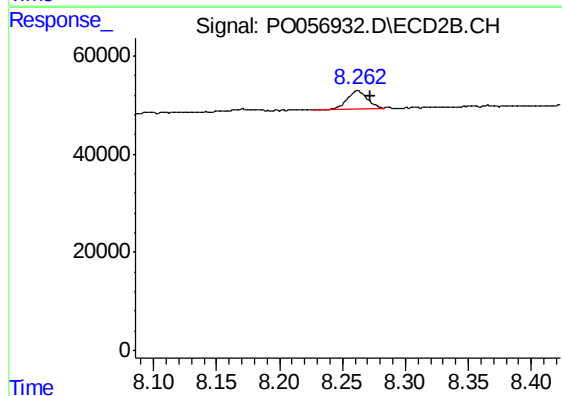

#45 AR-1268-5

R.T.: 8.262 min
Delta R.T.: -0.010 min
Response: 42337
Conc: 2.45 ng/ml