

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060619\
 Data File : P0056941.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jun 2019 19:51
 Operator : SM/SJ
 Sample : K3192-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLVR-AVEX-WC1B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 02:33:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.244	3.564	1440724	1055438	37.633	32.004
2) SA Decachlor...	9.814	8.496	1258430	896926	25.638	25.154
Target Compounds						
40) L8 AR-1262-5	0.000	8.012	0	23740	N.D.	10.223 #
44) L9 AR-1268-4	0.000	8.012	0	23740	N.D.	10.170 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO060619\
Data File : PO056941.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2019 19:51
Operator : SM/SJ
Sample : K3192-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLVR-AVEX-WC1B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 02:33:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

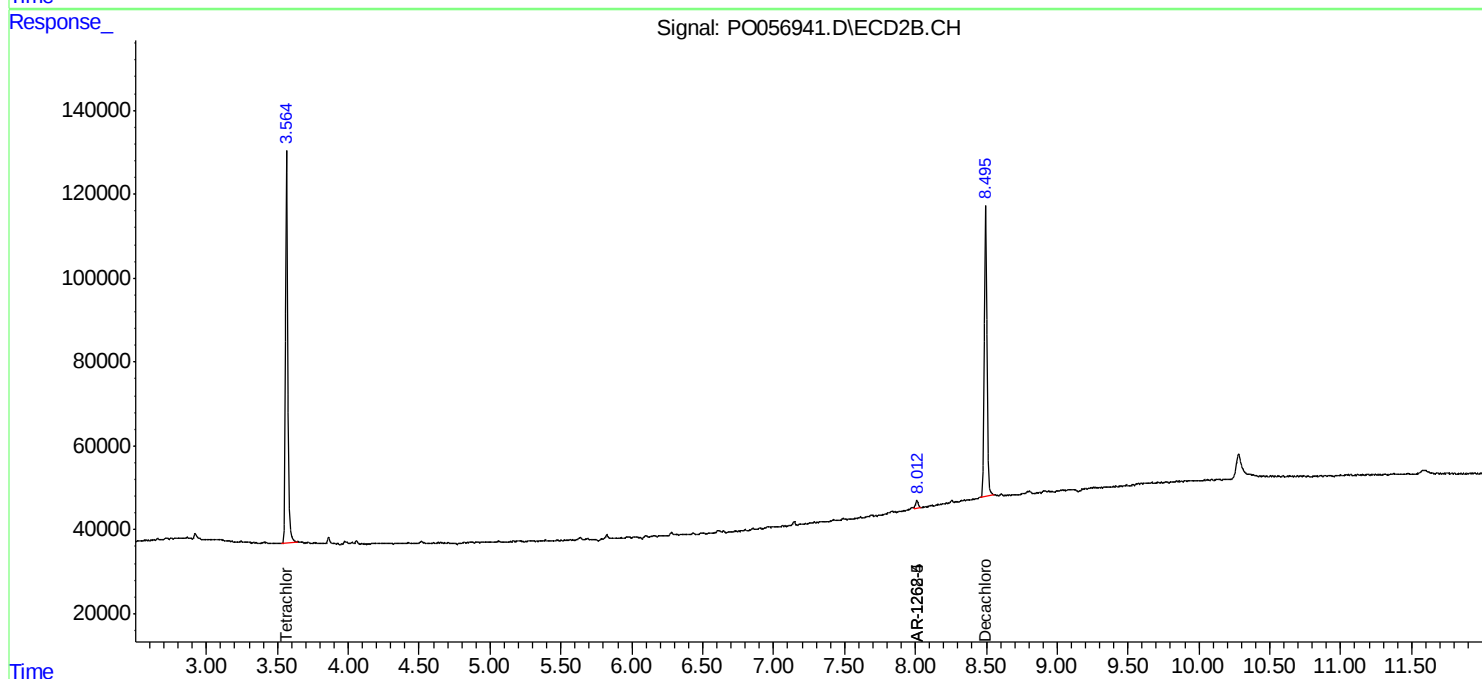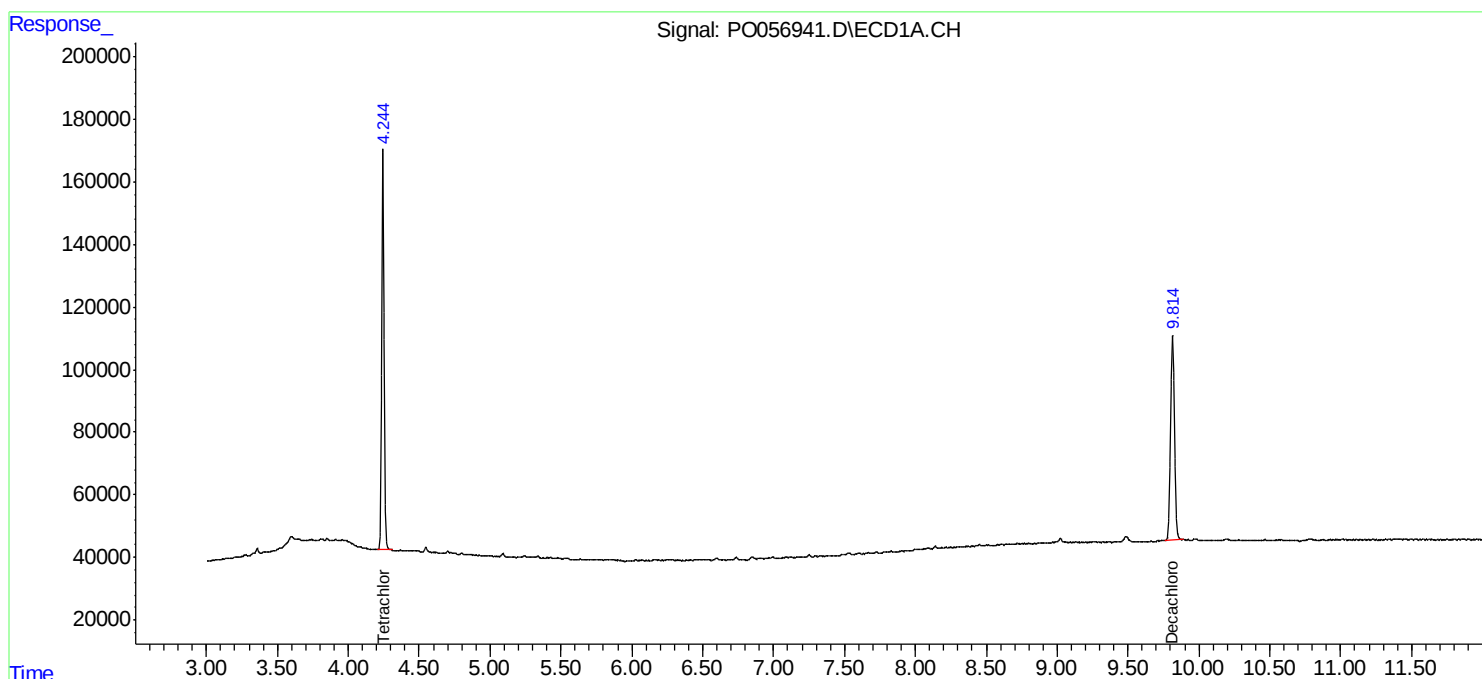


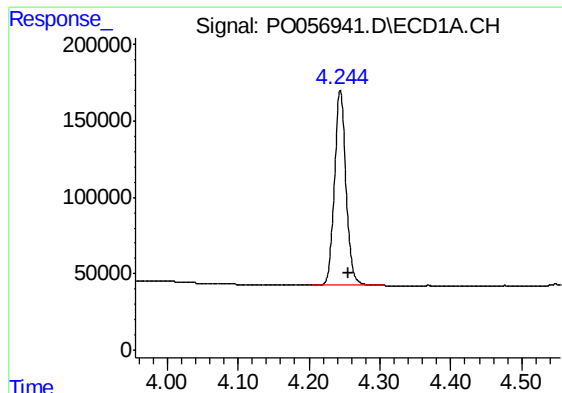

#1 Tetrachloro-m-xylene


R.T.: 4.244 min
Delta R.T.: -0.012 min
Response: 1440724
Conc: 37.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLVR-AVEX-WC1B

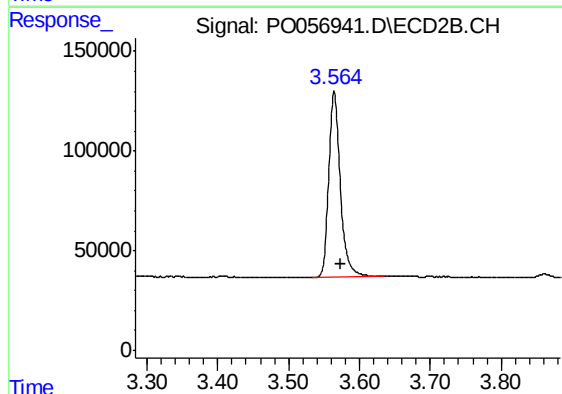


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: -0.009 min
Response: 1055438
Conc: 32.00 ng/ml

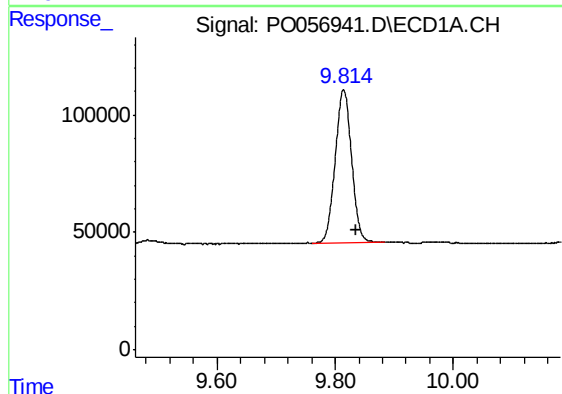


#2 Decachlorobiphenyl

R.T.: 9.814 min
Delta R.T.: -0.022 min
Response: 1258430
Conc: 25.64 ng/ml

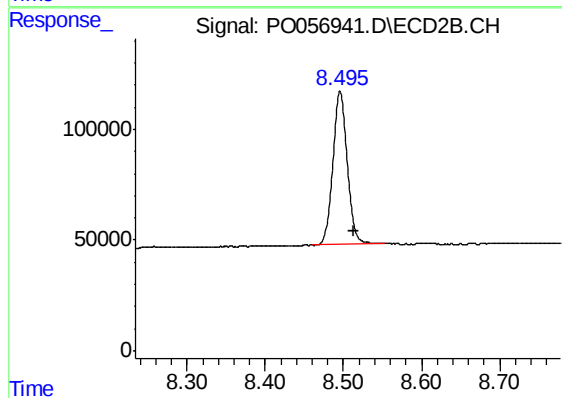

#2 Decachlorobiphenyl


R.T.: 8.496 min
Delta R.T.: -0.017 min
Response: 896926
Conc: 25.15 ng/ml

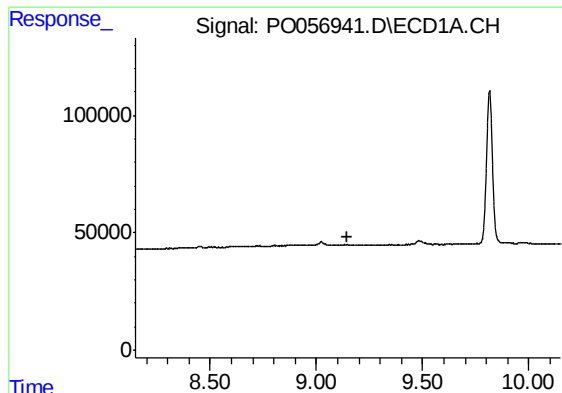

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 9.148 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CLVR-AVEX-WC1B

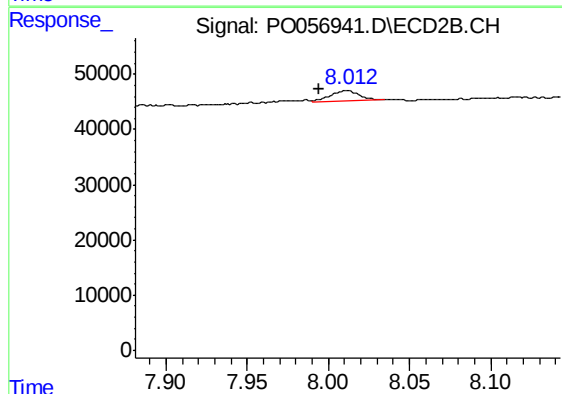


#40 AR-1262-5

R.T.: 8.012 min
Delta R.T.: 0.018 min
Response: 23740
Conc: 10.22 ng/ml

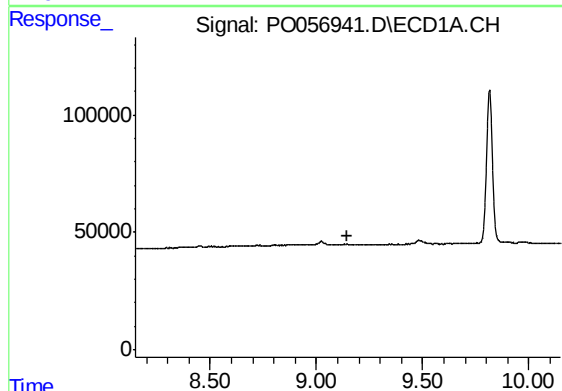

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.148 min
Response: 0
Conc: N.D.

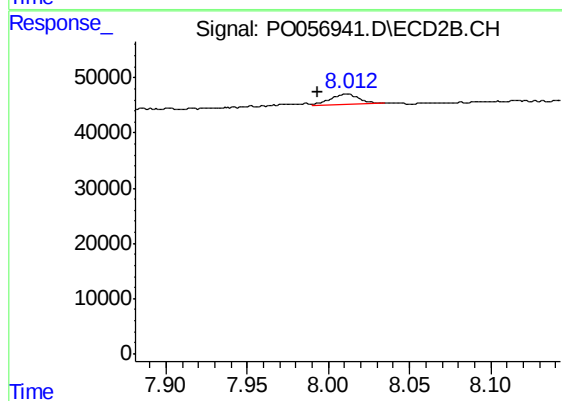

#44 AR-1268-4

R.T.: 8.012 min
Delta R.T.: 0.019 min
Response: 23740
Conc: 10.17 ng/ml