

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0060619\
 Data File : P0056918.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jun 2019 12:01
 Operator : SM/SJ
 Sample : K3175-01MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 FK-BPM-03-007-ABCDMS

Manual Integrations
 APPROVED

Ankita
 6/7/2019 4:20:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 12:47:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.254	3.566	990497	781987	25.873	23.712
2)	SA Decachlor...	9.829	8.502	990716	673181	20.184	18.879
Target Compounds							
3)	L1 AR-1016-1	5.415	4.635	245739	172945	136.626m	137.423
4)	L1 AR-1016-2	5.436	4.653	364974	236708	145.346m	131.386
5)	L1 AR-1016-3	5.497	4.828	208959	127620	130.007m	129.439
6)	L1 AR-1016-4	5.595	4.868	176762	105512	134.748m	127.455
7)	L1 AR-1016-5	5.886	5.080	163556	126397	118.381m	117.828m
31)	L7 AR-1260-1	7.004	6.101	314892	262561	122.708	131.255
32)	L7 AR-1260-2	7.260	6.289	398073	333558	131.631	135.320
33)	L7 AR-1260-3	7.615	6.440	259835	293139	107.858m	130.677
34)	L7 AR-1260-4	7.839	6.907	280234	217085	106.992m	116.648
35)	L7 AR-1260-5	8.148	7.149	553250	470256	115.692m	109.049

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO056918\
Data File : PO056918.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2019 12:01
Operator : SM/SJ
Sample : K3175-01MS
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS


Manual Integrations
APPROVED

Ankita
6/7/2019 4:20:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 12:47:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

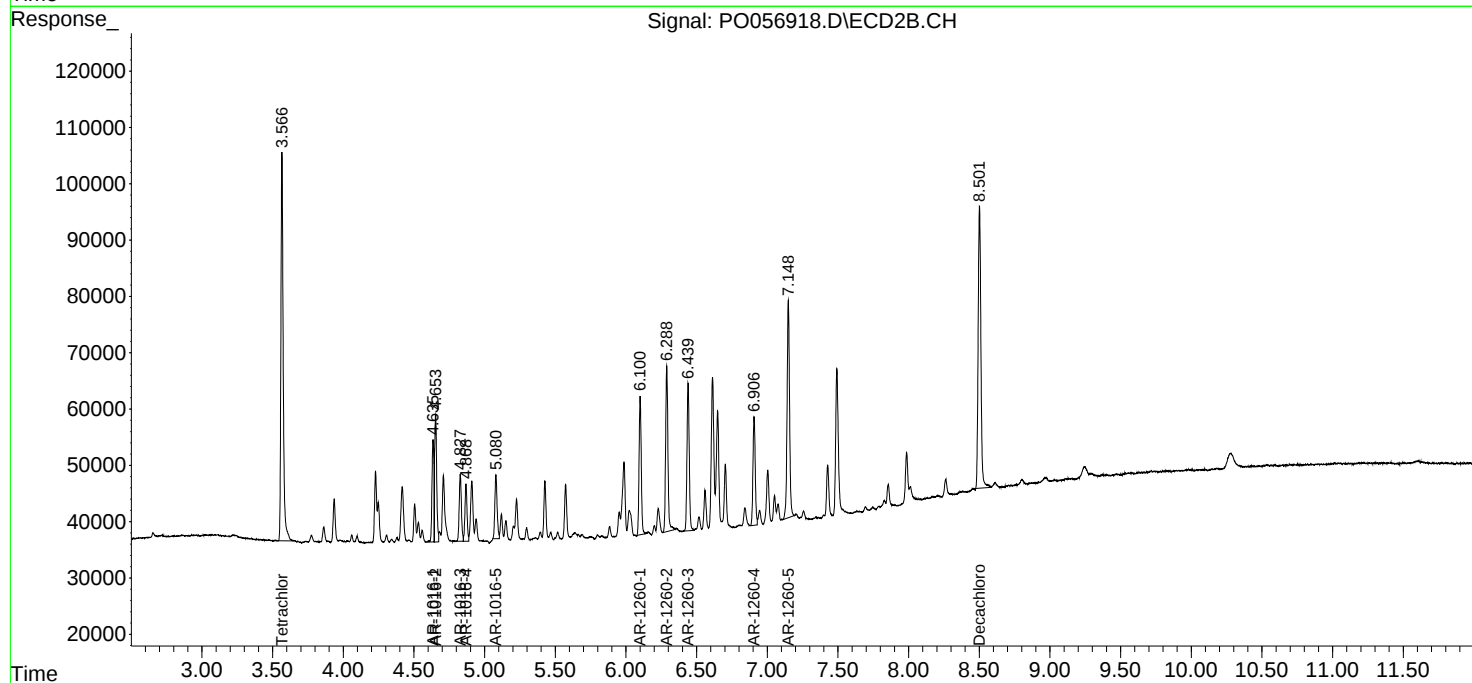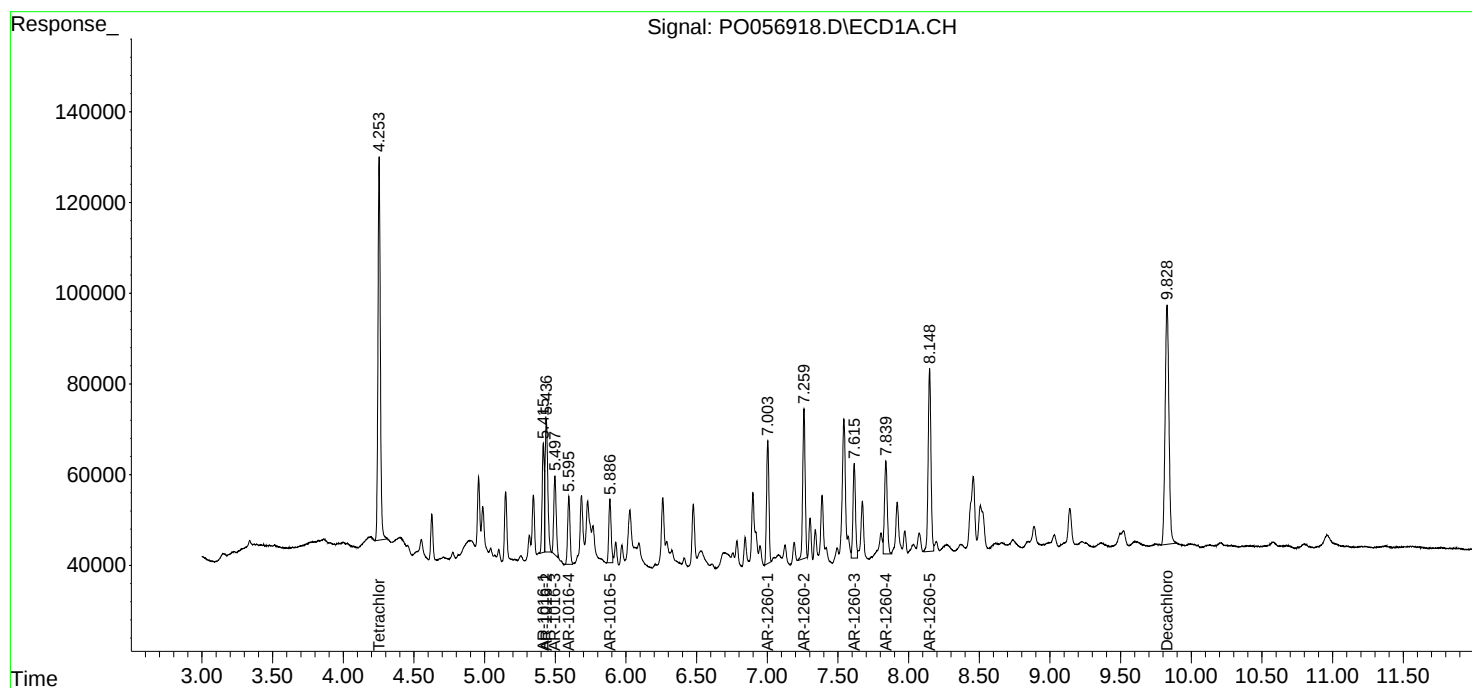

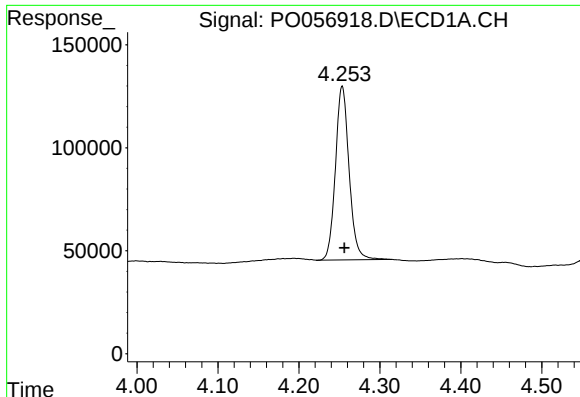


#1 Tetrachloro-m-xylene

R.T.: 4.254 min
Delta R.T.: -0.002 min
Response: 990497
Conc: 25.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS


Manual Integrations
APPROVED

Ankita
6/7/2019 4:20:53 PM

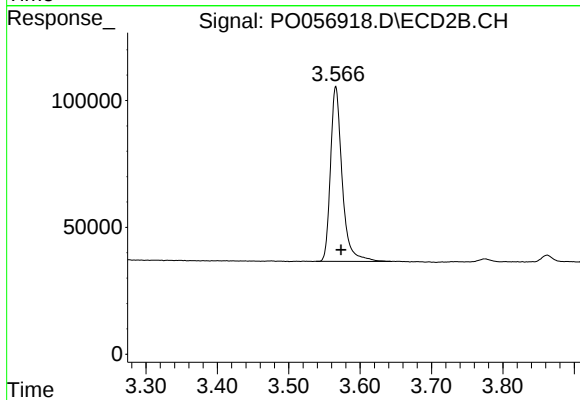


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: -0.007 min
Response: 781987
Conc: 23.71 ng/ml

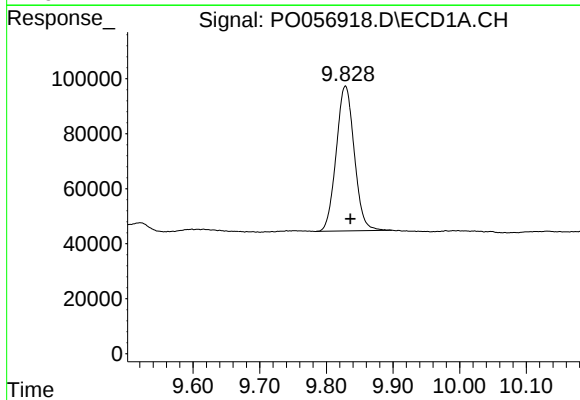


#2 Decachlorobiphenyl

R.T.: 9.829 min
Delta R.T.: -0.008 min
Response: 990716
Conc: 20.18 ng/ml

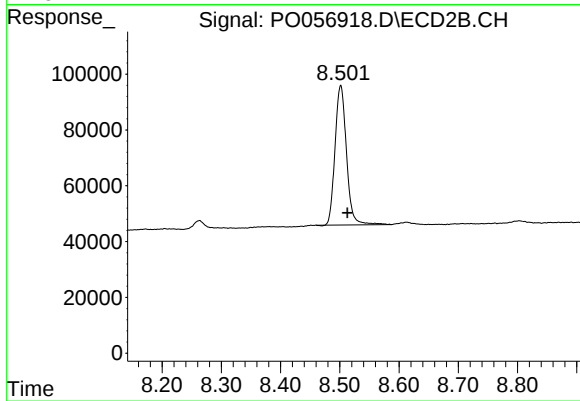

#2 Decachlorobiphenyl

R.T.: 8.502 min
Delta R.T.: -0.011 min
Response: 673181
Conc: 18.88 ng/ml

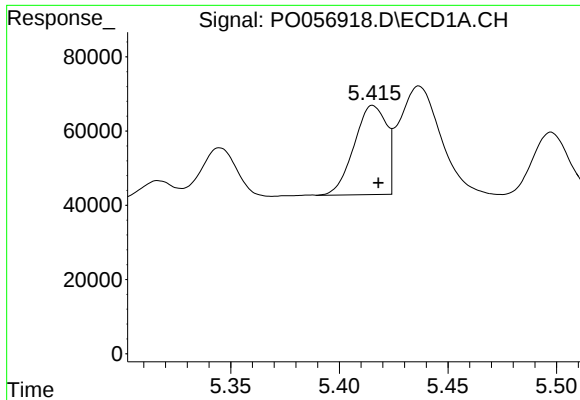


#3 AR-1016-1

R.T.: 5.415 min
Delta R.T.: -0.003 min
Response: 245739
Conc: 136.63 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS


Manual Integrations
APPROVED

Ankita
6/7/2019 4:20:53 PM

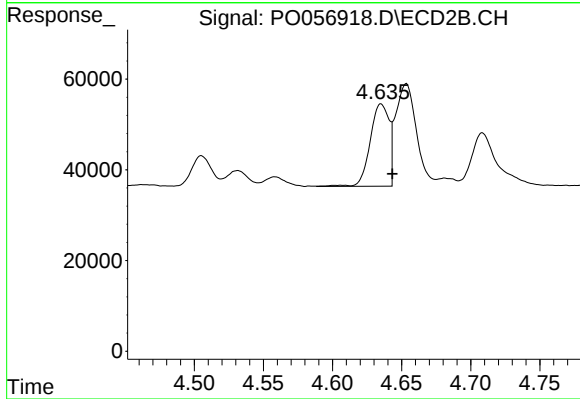


#3 AR-1016-1

R.T.: 4.635 min
Delta R.T.: -0.008 min
Response: 172945
Conc: 137.42 ng/ml

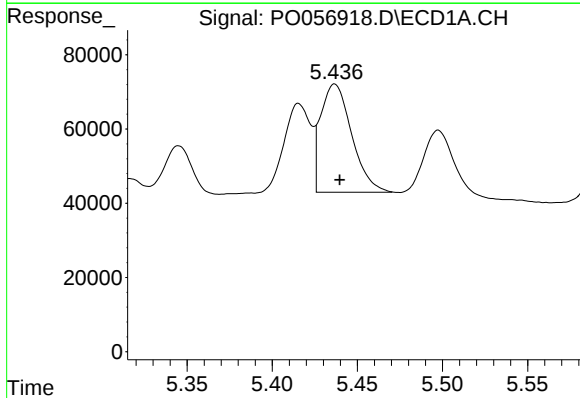


#4 AR-1016-2

R.T.: 5.436 min
Delta R.T.: -0.003 min
Response: 364974
Conc: 145.35 ng/ml m

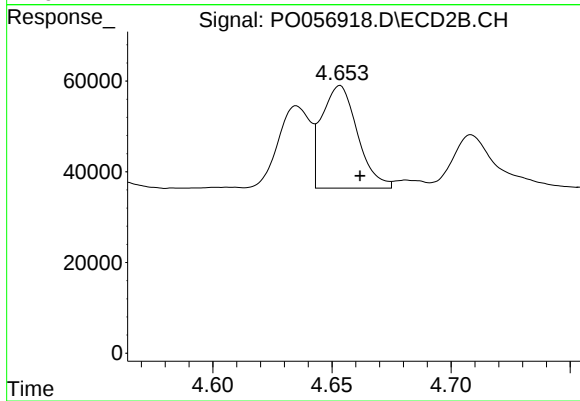

#4 AR-1016-2

R.T.: 4.653 min
Delta R.T.: -0.008 min
Response: 236708
Conc: 131.39 ng/ml

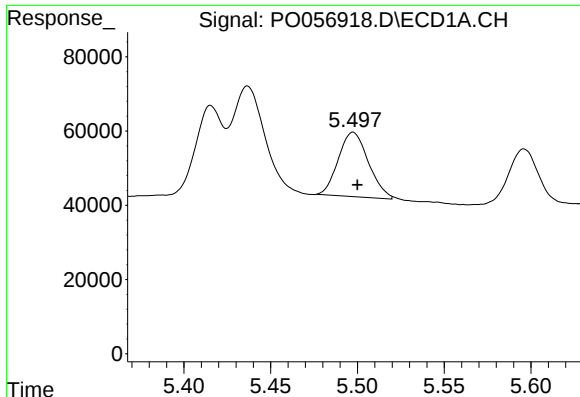


#5 AR-1016-3

R.T.: 5.497 min
Delta R.T.: -0.003 min
Response: 208959
Conc: 130.01 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS


Manual Integrations
APPROVED

Ankita
6/7/2019 4:20:53 PM

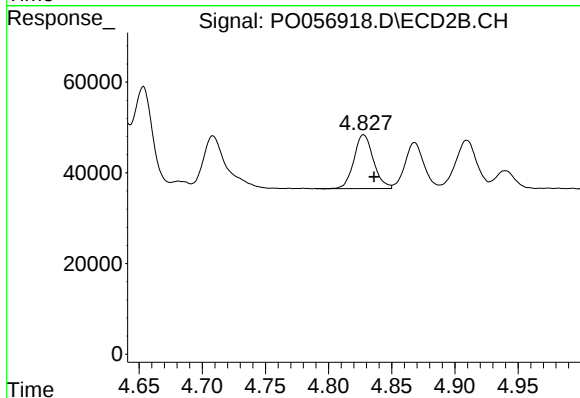


#5 AR-1016-3

R.T.: 4.828 min
Delta R.T.: -0.008 min
Response: 127620
Conc: 129.44 ng/ml

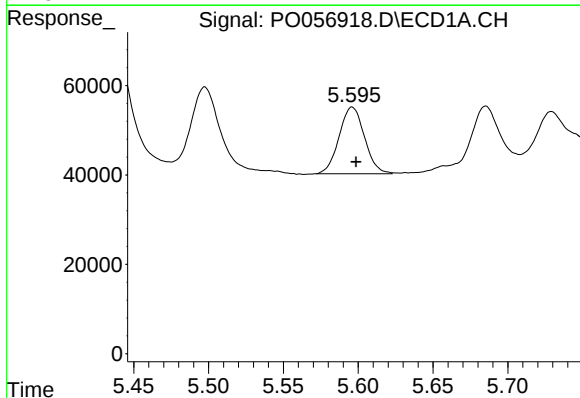


#6 AR-1016-4

R.T.: 5.595 min
Delta R.T.: -0.003 min
Response: 176762
Conc: 134.75 ng/ml m

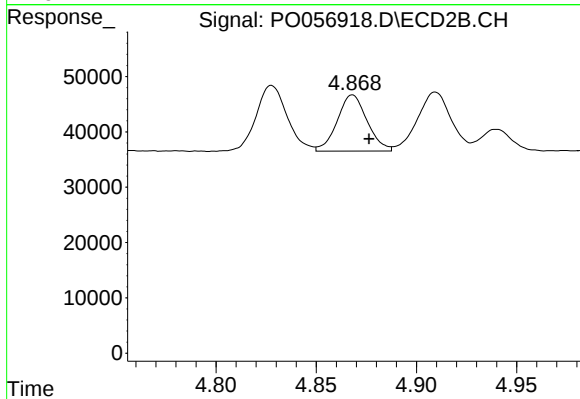

#6 AR-1016-4

R.T.: 4.868 min
Delta R.T.: -0.008 min
Response: 105512
Conc: 127.45 ng/ml

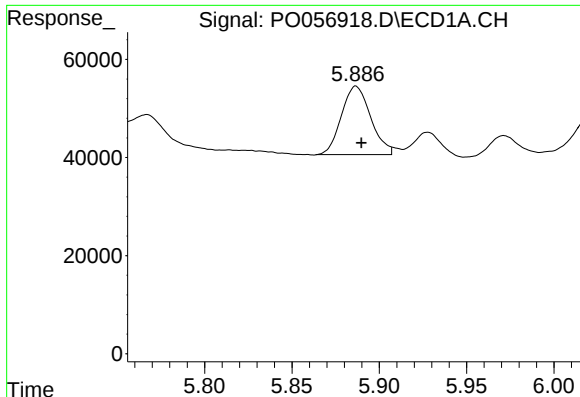


#7 AR-1016-5

R.T.: 5.886 min
Delta R.T.: -0.004 min
Response: 163556
Conc: 118.38 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS


Manual Integrations
APPROVED

Ankita
6/7/2019 4:20:53 PM

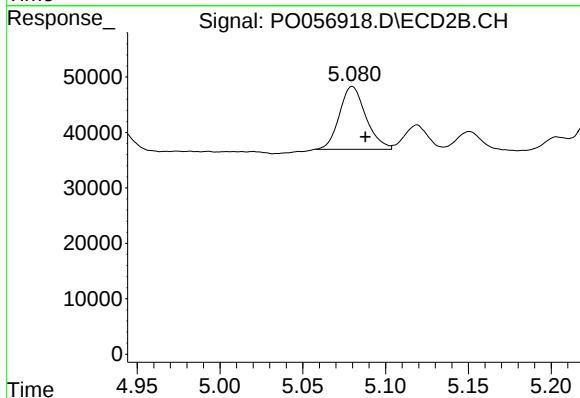


#7 AR-1016-5

R.T.: 5.080 min
Delta R.T.: -0.008 min
Response: 126397
Conc: 117.83 ng/ml m

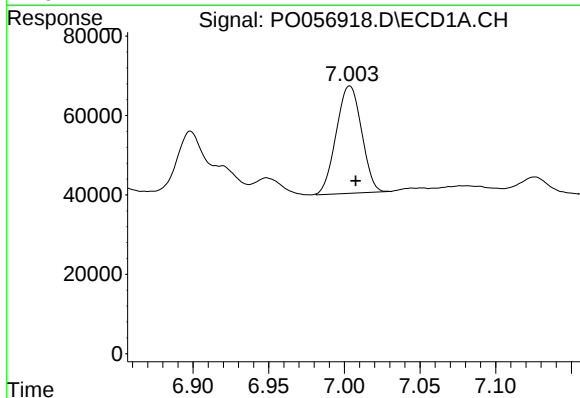


#31 AR-1260-1

R.T.: 7.004 min
Delta R.T.: -0.004 min
Response: 314892
Conc: 122.71 ng/ml

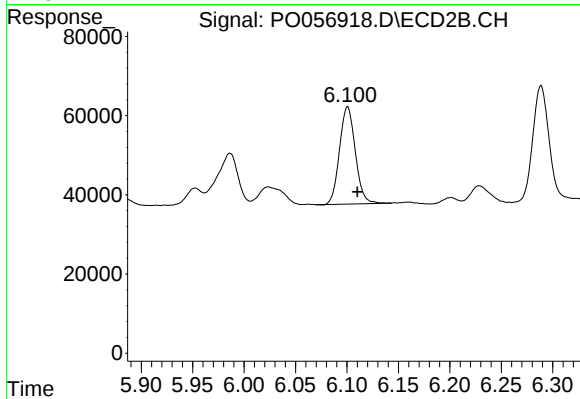

#31 AR-1260-1

R.T.: 6.101 min
Delta R.T.: -0.009 min
Response: 262561
Conc: 131.26 ng/ml

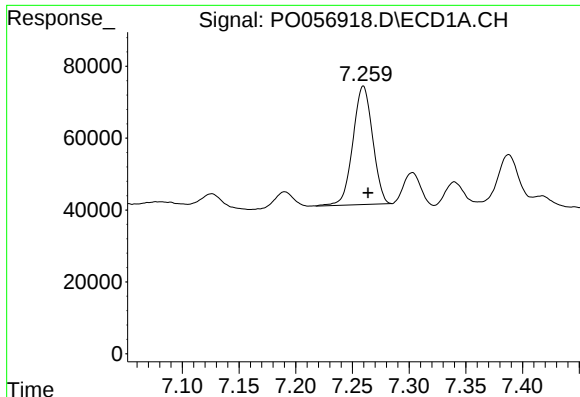


#32 AR-1260-2

R.T.: 7.260 min
Delta R.T.: -0.004 min
Response: 398073
Conc: 131.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS


Manual Integrations
APPROVED

Ankita
6/7/2019 4:20:53 PM

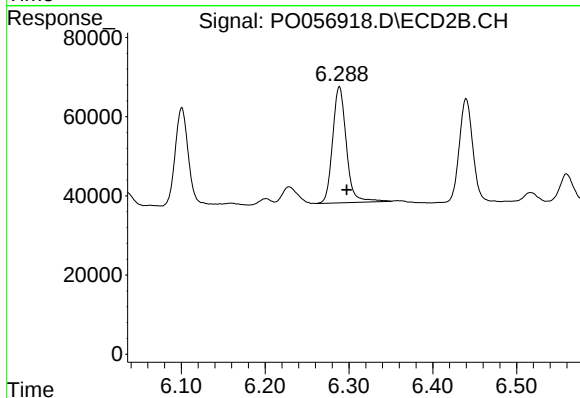


#32 AR-1260-2

R.T.: 6.289 min
Delta R.T.: -0.009 min
Response: 333558
Conc: 135.32 ng/ml

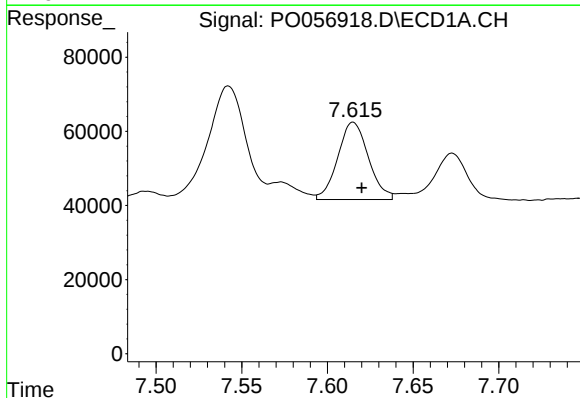


#33 AR-1260-3

R.T.: 7.615 min
Delta R.T.: -0.005 min
Response: 259835
Conc: 107.86 ng/ml m

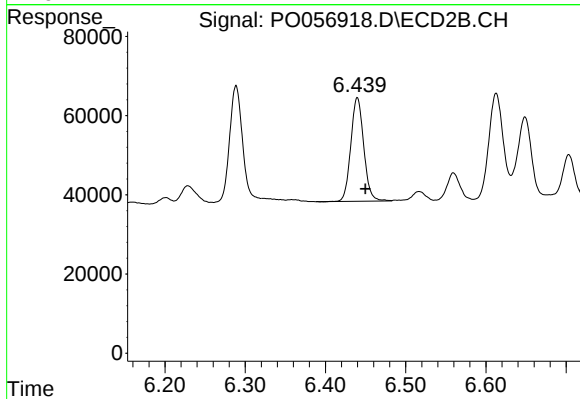

#33 AR-1260-3

R.T.: 6.440 min
Delta R.T.: -0.010 min
Response: 293139
Conc: 130.68 ng/ml

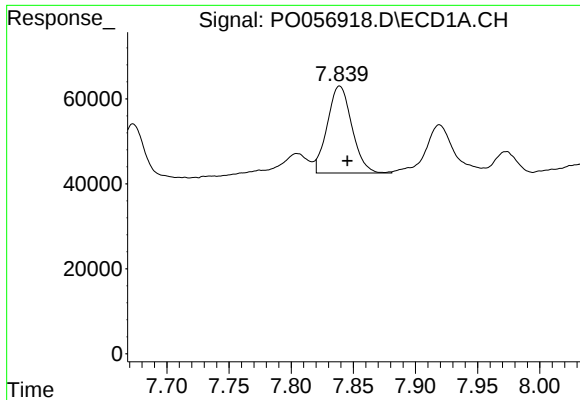


#34 AR-1260-4

R.T.: 7.839 min
Delta R.T.: -0.007 min
Response: 280234
Conc: 106.99 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMS


Manual Integrations
APPROVED

Ankita
6/7/2019 4:20:53 PM

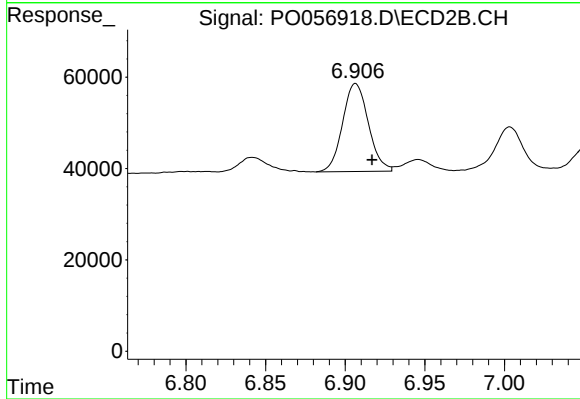


#34 AR-1260-4

R.T.: 6.907 min
Delta R.T.: -0.010 min
Response: 217085
Conc: 116.65 ng/ml

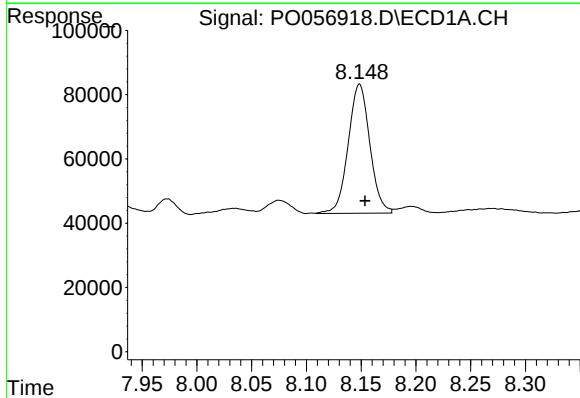

#35 AR-1260-5

R.T.: 8.148 min
Delta R.T.: -0.005 min
Response: 553250
Conc: 115.69 ng/ml m

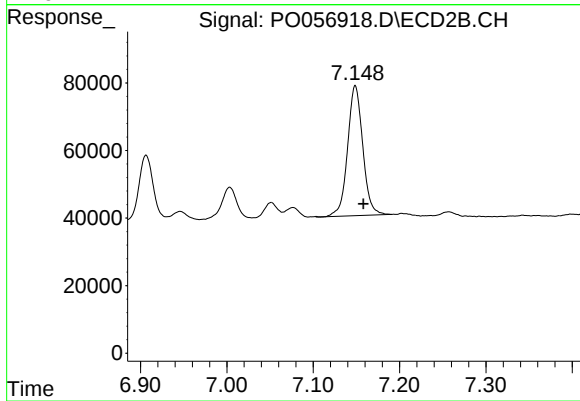

#35 AR-1260-5

R.T.: 7.149 min
Delta R.T.: -0.009 min
Response: 470256
Conc: 109.05 ng/ml