

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060619\
 Data File : P0056919.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jun 2019 12:21
 Operator : SM/SJ
 Sample : K3175-01MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-03-007-ABCDMSD

Manual Integrations
 APPROVED

Ankita
 6/7/2019 4:20:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 12:47:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.254	3.566	952638	779302	24.884	23.631
2) SA Decachlor...	9.829	8.502	980730	663387	19.981	18.605
Target Compounds						
3) L1 AR-1016-1	5.414	4.635	259749	167323	144.416m	132.956
4) L1 AR-1016-2	5.437	4.653	319473	234728	127.226m	130.287
5) L1 AR-1016-3	5.498	4.827	205793	124457	128.037m	126.231
6) L1 AR-1016-4	5.596	4.868	162951	103774	124.220m	125.355
7) L1 AR-1016-5	5.887	5.079	161105	125876	116.607m	117.342m
31) L7 AR-1260-1	7.004	6.100	348570	260549	135.832	130.250
32) L7 AR-1260-2	7.259	6.288	368621	322103	121.892	130.673
33) L7 AR-1260-3	7.614	6.440	264434	290265	109.767m	129.396
34) L7 AR-1260-4	7.839	6.906	275873	211927	105.327m	113.877
35) L7 AR-1260-5	8.149	7.148	491215	463417	102.720	107.463

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO060619\
Data File : PO056919.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2019 12:21
Operator : SM/SJ
Sample : K3175-01MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD


Manual Integrations
APPROVED

Ankita
6/7/2019 4:20:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 12:47:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

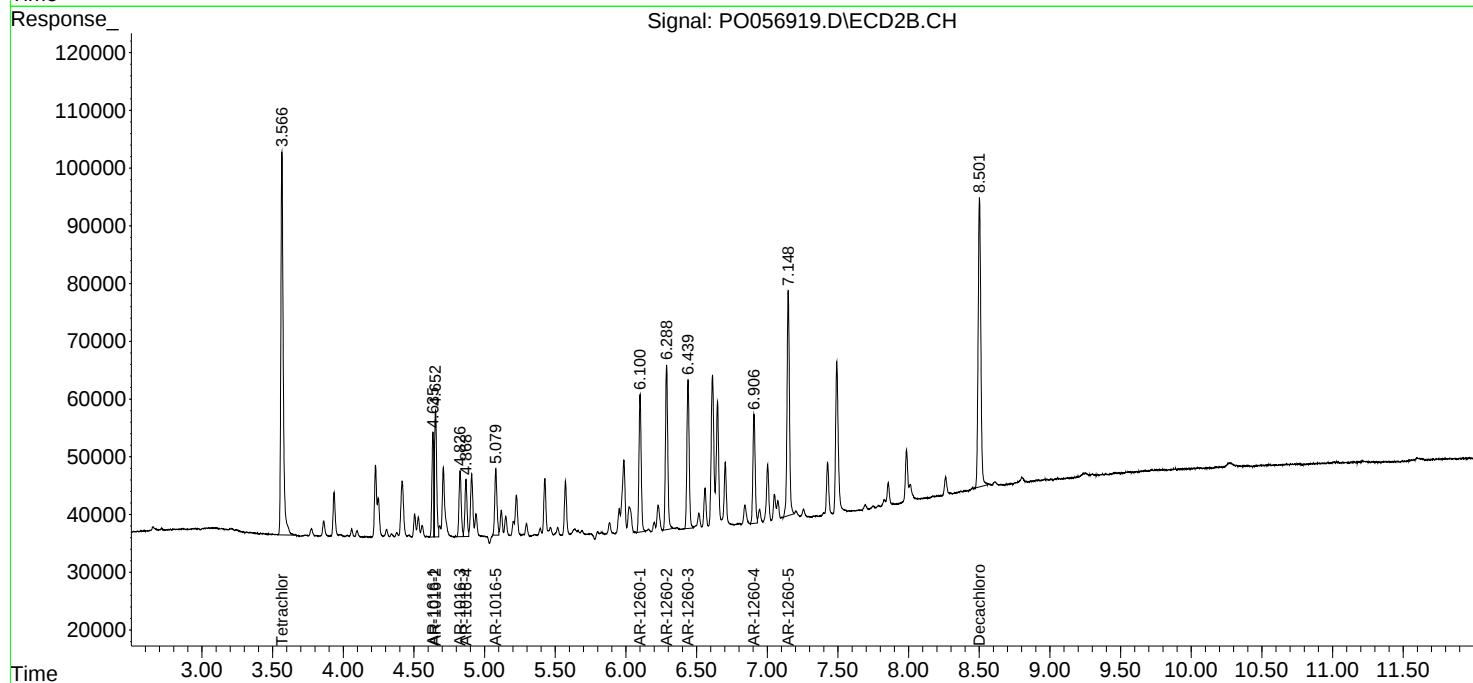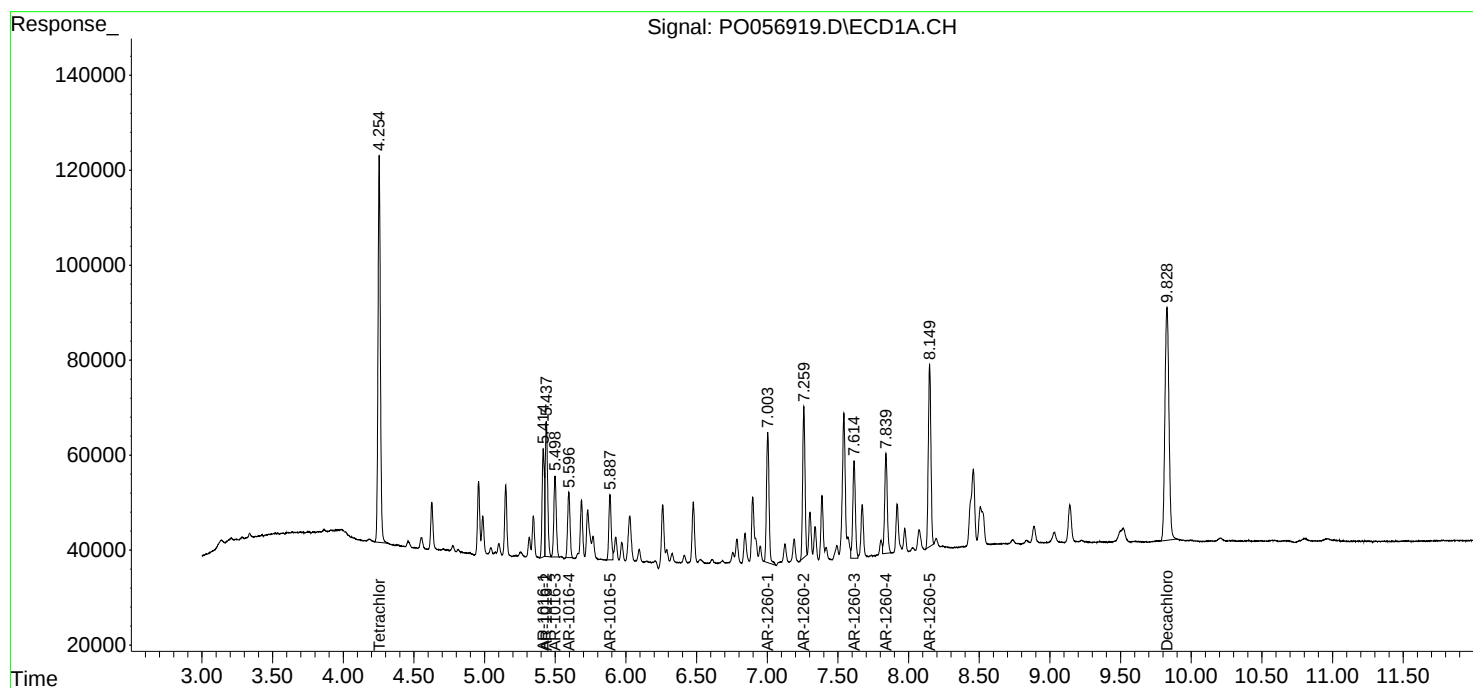

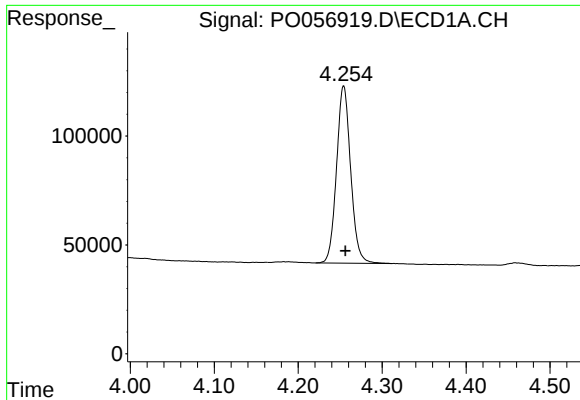


#1 Tetrachloro-m-xylene

R.T.: 4.254 min
Delta R.T.: -0.002 min
Response: 952638
Conc: 24.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD


Manual Integrations
APPROVED

Ankita
6/7/2019 4:20:55 PM

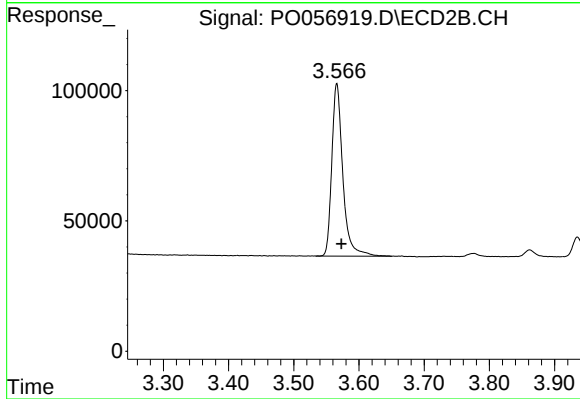


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: -0.007 min
Response: 779302
Conc: 23.63 ng/ml

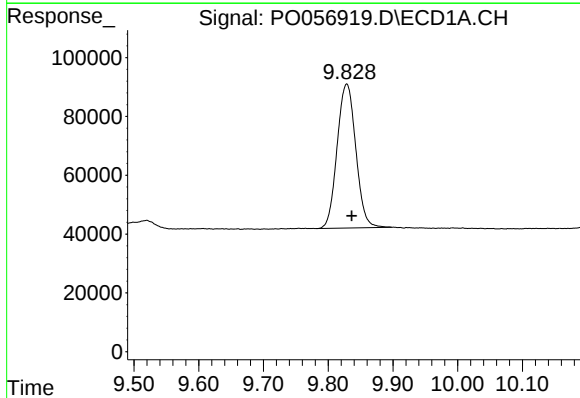


#2 Decachlorobiphenyl

R.T.: 9.829 min
Delta R.T.: -0.008 min
Response: 980730
Conc: 19.98 ng/ml

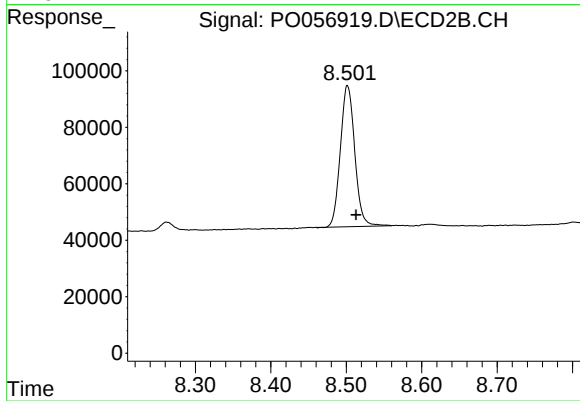

#2 Decachlorobiphenyl

R.T.: 8.502 min
Delta R.T.: -0.011 min
Response: 663387
Conc: 18.60 ng/ml

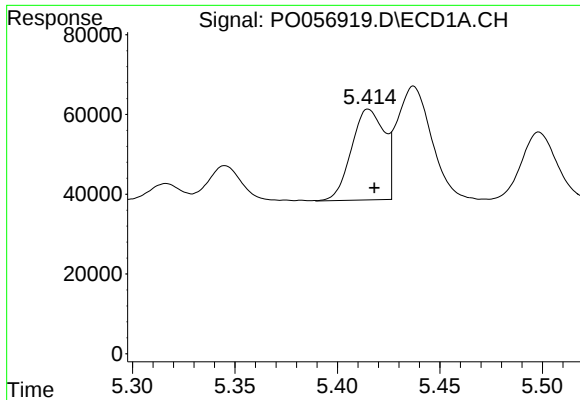


#3 AR-1016-1

R.T.: 5.414 min
Delta R.T.: -0.004 min
Response: 259749
Conc: 144.42 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD


Manual Integrations
APPROVED

Ankita
6/7/2019 4:20:55 PM

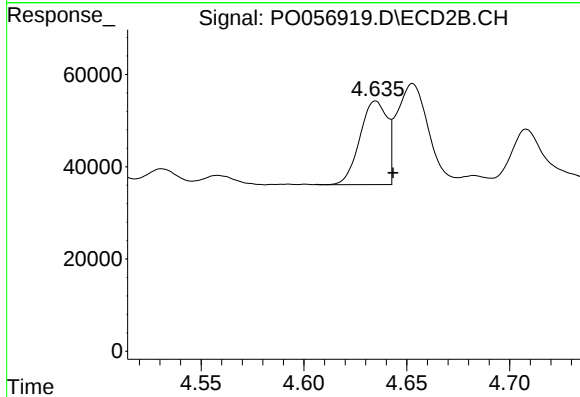


#3 AR-1016-1

R.T.: 4.635 min
Delta R.T.: -0.008 min
Response: 167323
Conc: 132.96 ng/ml

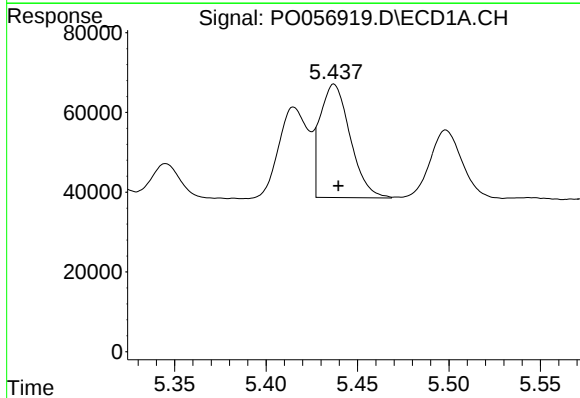


#4 AR-1016-2

R.T.: 5.437 min
Delta R.T.: -0.003 min
Response: 319473
Conc: 127.23 ng/ml m

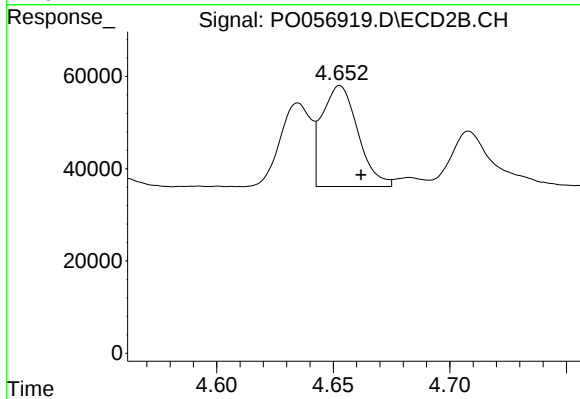

#4 AR-1016-2

R.T.: 4.653 min
Delta R.T.: -0.009 min
Response: 234728
Conc: 130.29 ng/ml

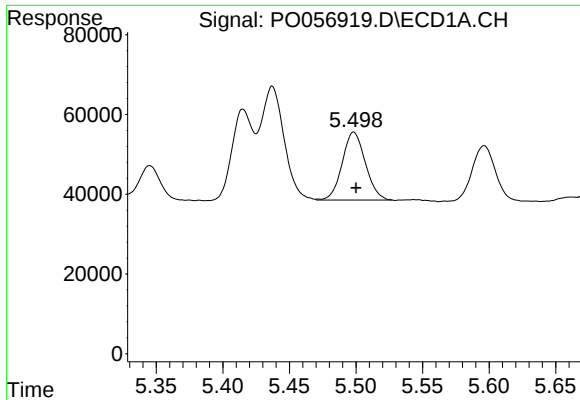


#5 AR-1016-3

R.T.: 5.498 min
Delta R.T.: -0.002 min
Response: 205793
Conc: 128.04 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD


Manual Integrations
APPROVED

Ankita
6/7/2019 4:20:55 PM

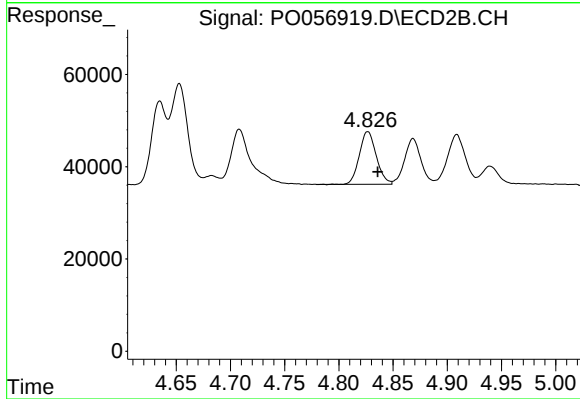


#5 AR-1016-3

R.T.: 4.827 min
Delta R.T.: -0.009 min
Response: 124457
Conc: 126.23 ng/ml

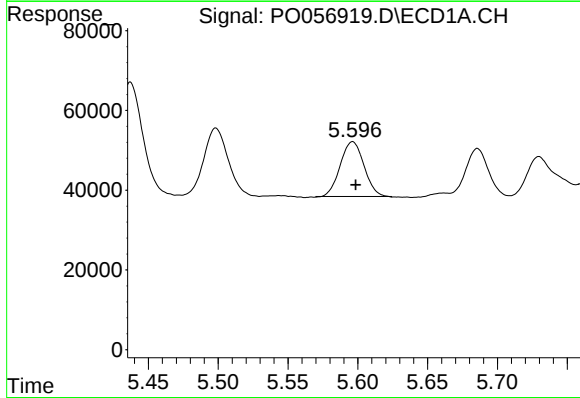


#6 AR-1016-4

R.T.: 5.596 min
Delta R.T.: -0.003 min
Response: 162951
Conc: 124.22 ng/ml m

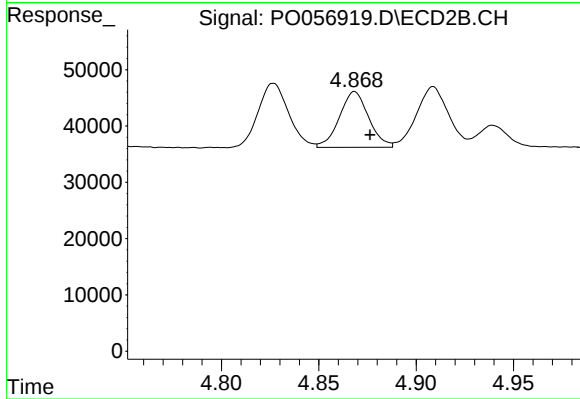

#6 AR-1016-4

R.T.: 4.868 min
Delta R.T.: -0.008 min
Response: 103774
Conc: 125.35 ng/ml

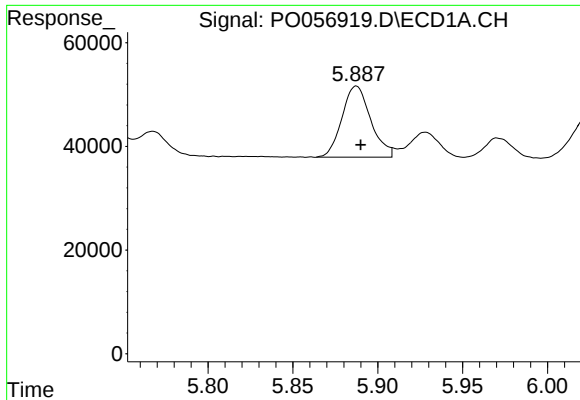


#7 AR-1016-5

R.T.: 5.887 min
Delta R.T.: -0.003 min
Response: 161105
Conc: 116.61 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD


Manual Integrations
APPROVED

Ankita
6/7/2019 4:20:55 PM

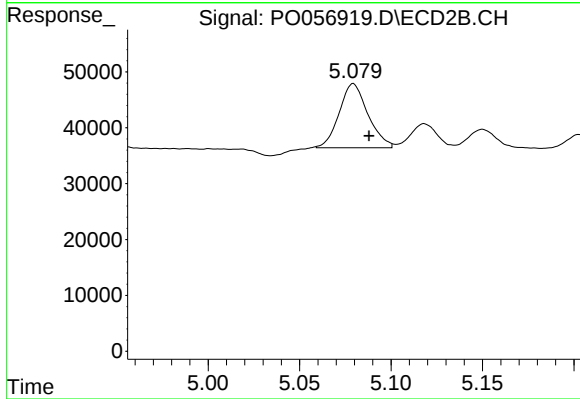


#7 AR-1016-5

R.T.: 5.079 min
Delta R.T.: -0.009 min
Response: 125876
Conc: 117.34 ng/ml m

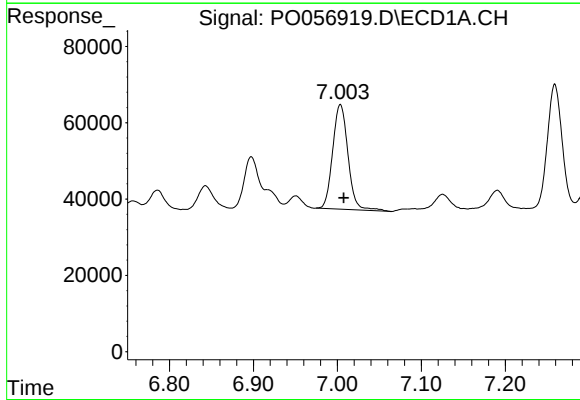


#31 AR-1260-1

R.T.: 7.004 min
Delta R.T.: -0.004 min
Response: 348570
Conc: 135.83 ng/ml

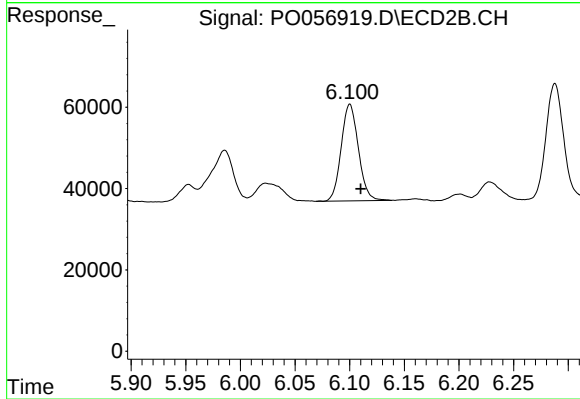

#31 AR-1260-1

R.T.: 6.100 min
Delta R.T.: -0.010 min
Response: 260549
Conc: 130.25 ng/ml

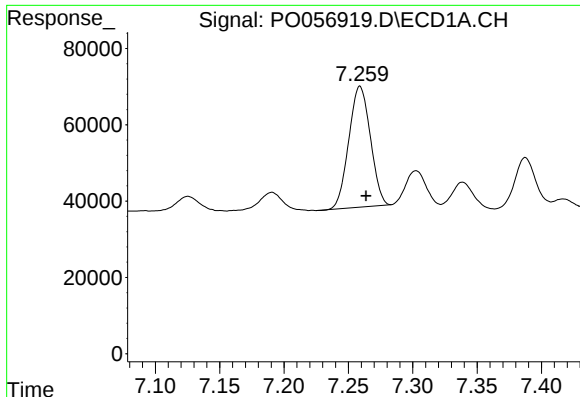


#32 AR-1260-2

R.T.: 7.259 min
Delta R.T.: -0.005 min
Response: 368621
Conc: 121.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD


Manual Integrations
APPROVED

Ankita
6/7/2019 4:20:55 PM

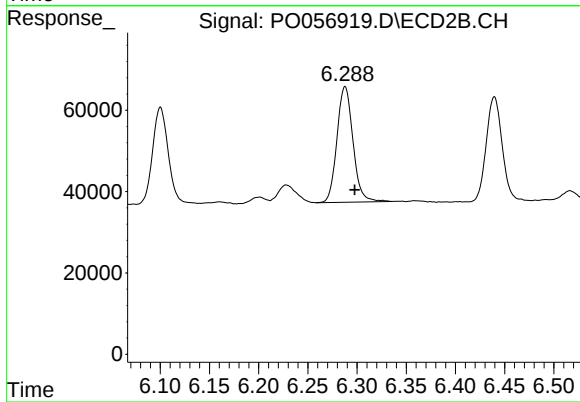


#32 AR-1260-2

R.T.: 6.288 min
Delta R.T.: -0.010 min
Response: 322103
Conc: 130.67 ng/ml

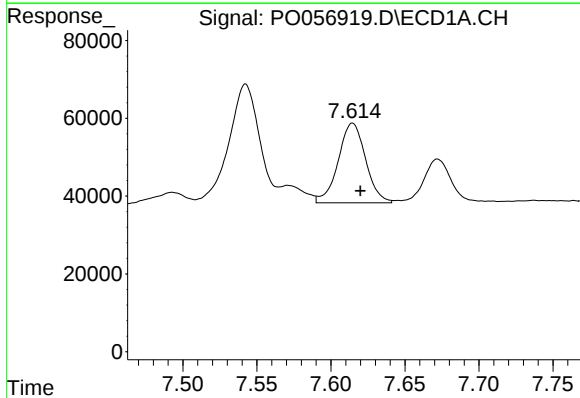


#33 AR-1260-3

R.T.: 7.614 min
Delta R.T.: -0.006 min
Response: 264434
Conc: 109.77 ng/ml m

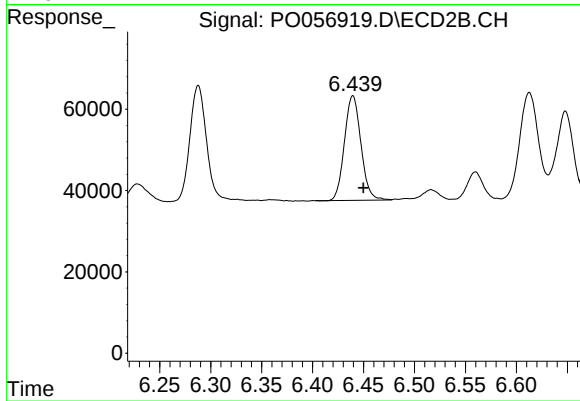

#33 AR-1260-3

R.T.: 6.440 min
Delta R.T.: -0.010 min
Response: 290265
Conc: 129.40 ng/ml

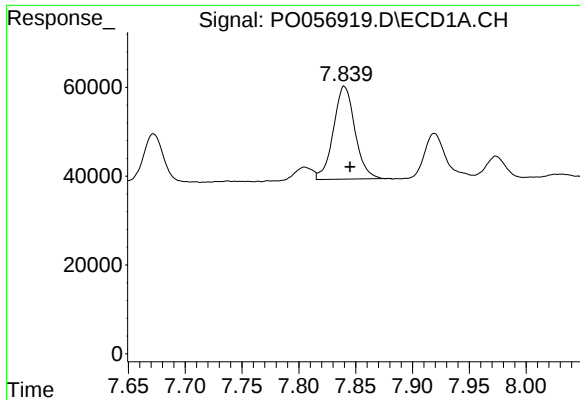


#34 AR-1260-4

R.T.: 7.839 min
Delta R.T.: -0.006 min
Response: 275873
Conc: 105.33 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-007-ABCDMSD


Manual Integrations
APPROVED

Ankita
6/7/2019 4:20:55 PM

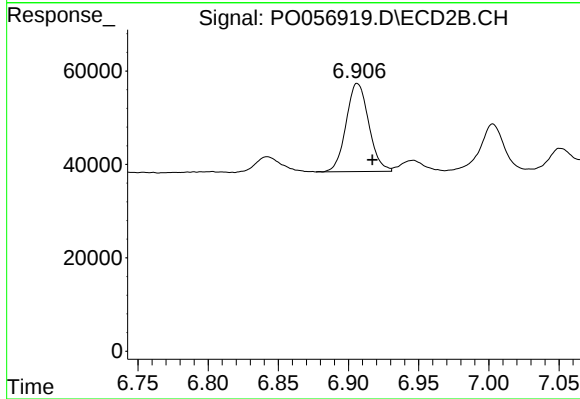


#34 AR-1260-4

R.T.: 6.906 min
Delta R.T.: -0.010 min
Response: 211927
Conc: 113.88 ng/ml

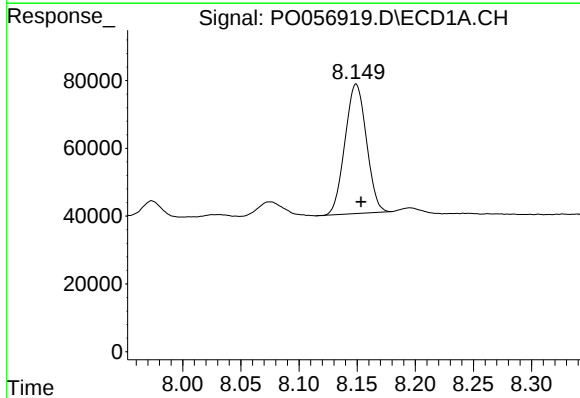

#35 AR-1260-5

R.T.: 8.149 min
Delta R.T.: -0.004 min
Response: 491215
Conc: 102.72 ng/ml

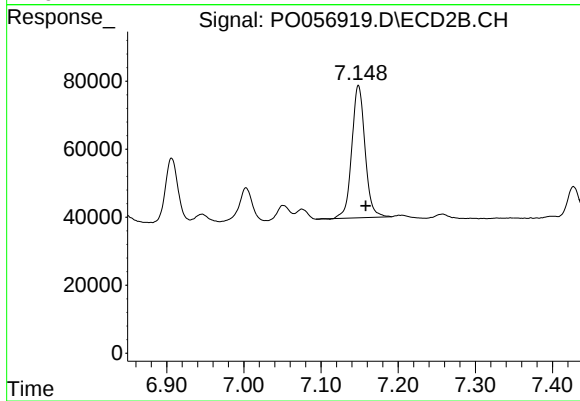

#35 AR-1260-5

R.T.: 7.148 min
Delta R.T.: -0.010 min
Response: 463417
Conc: 107.46 ng/ml