

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060619\
 Data File : P0056935.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jun 2019 18:09
 Operator : SM/SJ
 Sample : K3183-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-2

Manual Integrations
 APPROVED

Ankita
 6/7/2019 4:21:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 02:31:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.245	3.564	1004751	765924	26.245m	23.225
2) SA Decachlor...	9.816	8.497	871689	589874	17.759	16.543

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060619\
Data File : P0056935.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2019 18:09
Operator : SM/SJ
Sample : K3183-07
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-2


Manual Integrations
APPROVED

Ankita
6/7/2019 4:21:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 02:31:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

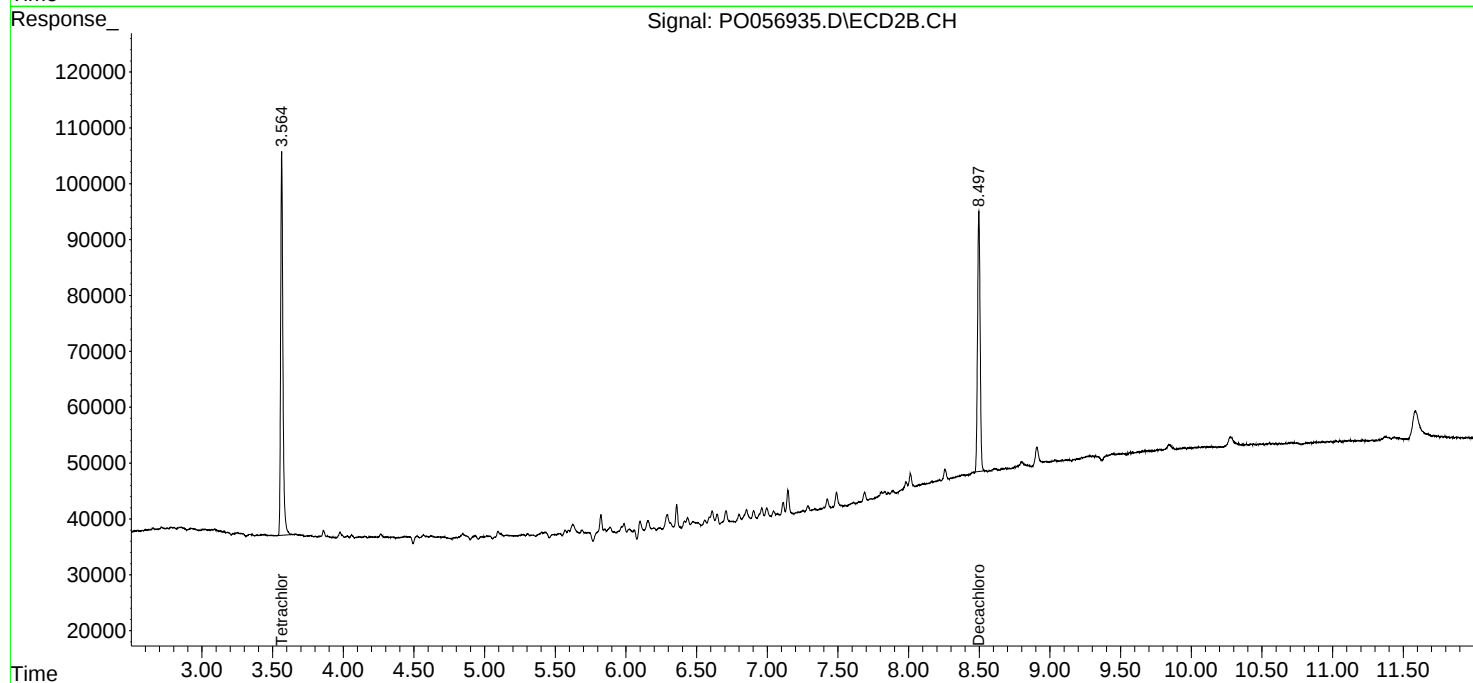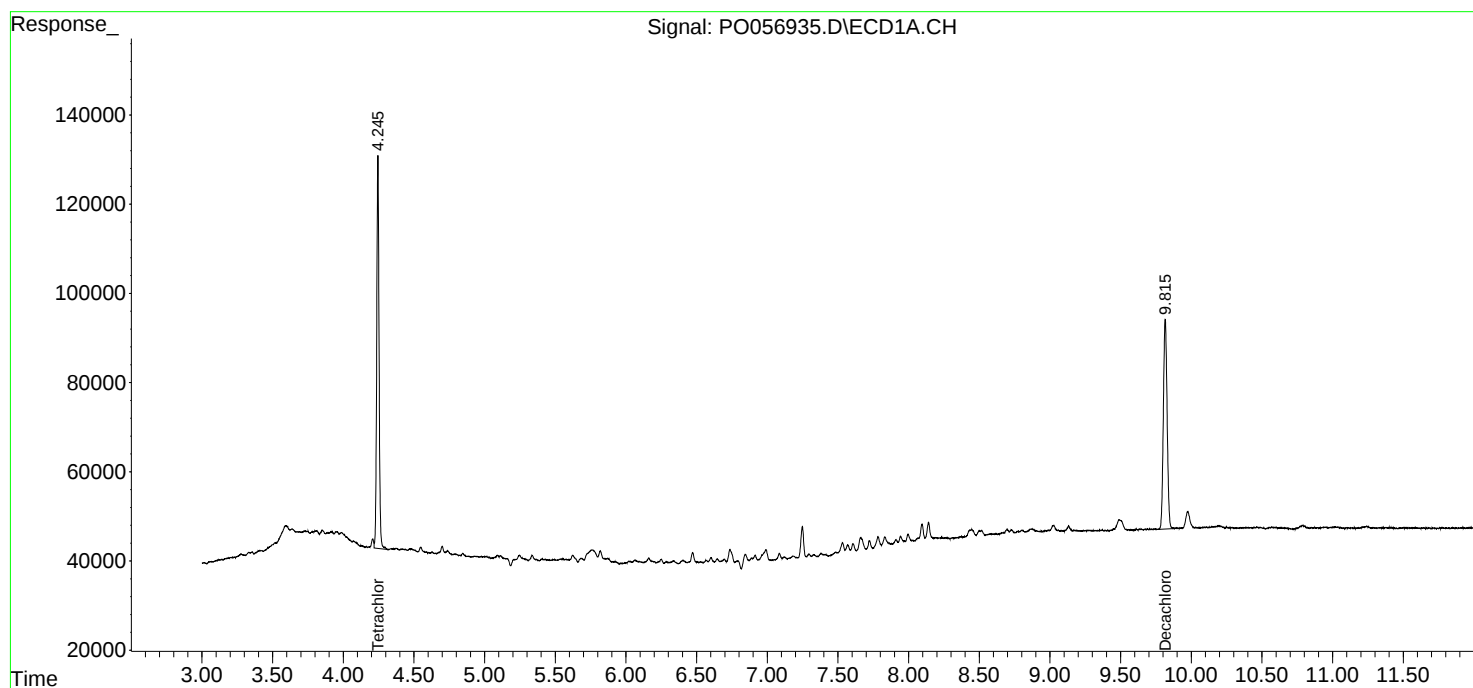

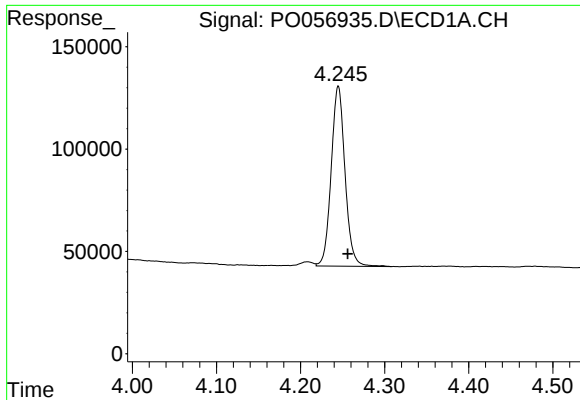


#1 Tetrachloro-m-xylene

R.T.: 4.245 min
Delta R.T.: -0.011 min
Response: 1004751
Conc: 26.25 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
6/7/2019 4:21:38 PM

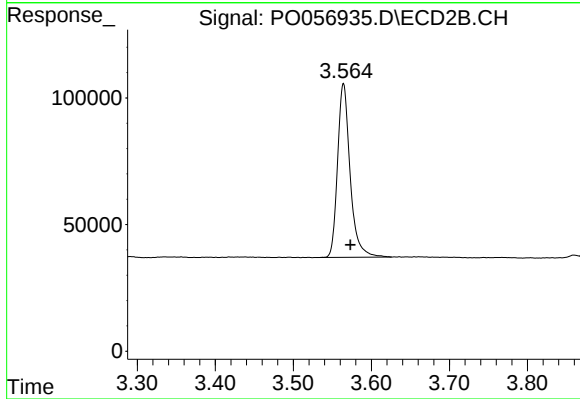


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: -0.009 min
Response: 765924
Conc: 23.22 ng/ml

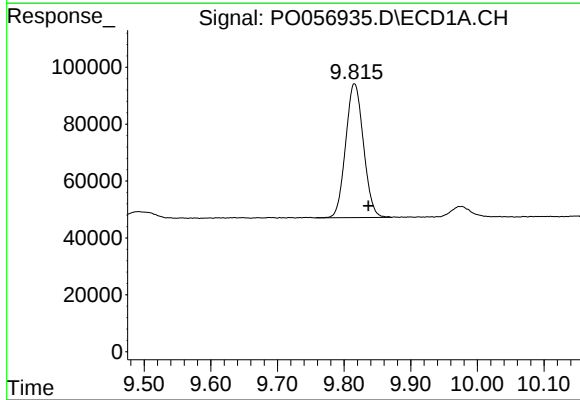

#2 Decachlorobiphenyl

R.T.: 9.816 min
Delta R.T.: -0.021 min
Response: 871689
Conc: 17.76 ng/ml

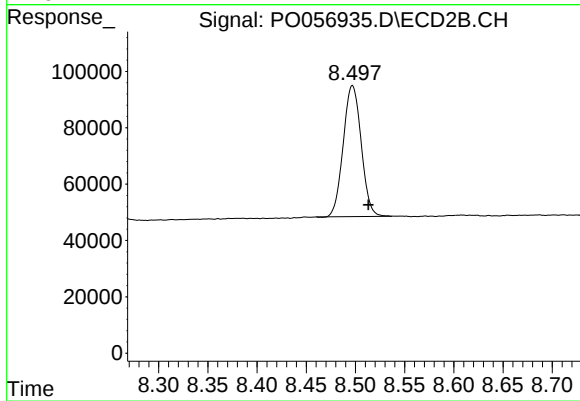

#2 Decachlorobiphenyl

R.T.: 8.497 min
Delta R.T.: -0.016 min
Response: 589874
Conc: 16.54 ng/ml