

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060619\
 Data File : P0056949.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jun 2019 22:07
 Operator : SM/SJ
 Sample : K3182-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MW-10

Manual Integrations
 APPROVED

Ankita
 6/7/2019 4:18:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 02:36:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.245	3.565	1037185	773528	27.092m	23.456
2) SA Decachlor...	9.817	8.499	852066	589161	17.359	16.523

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO060619\
Data File : PO056949.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2019 22:07
Operator : SM/SJ
Sample : K3182-07
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
MW-10


Manual Integrations
APPROVED

Ankita
6/7/2019 4:18:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 02:36:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

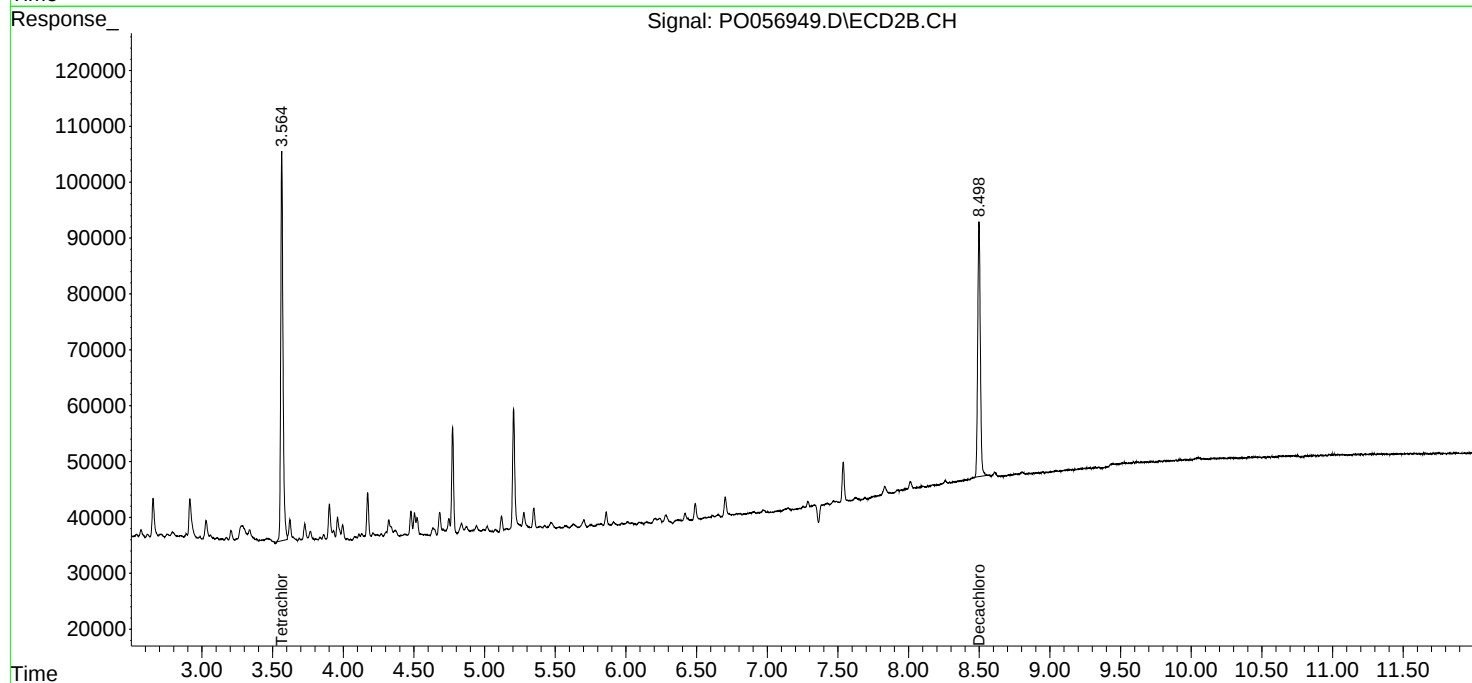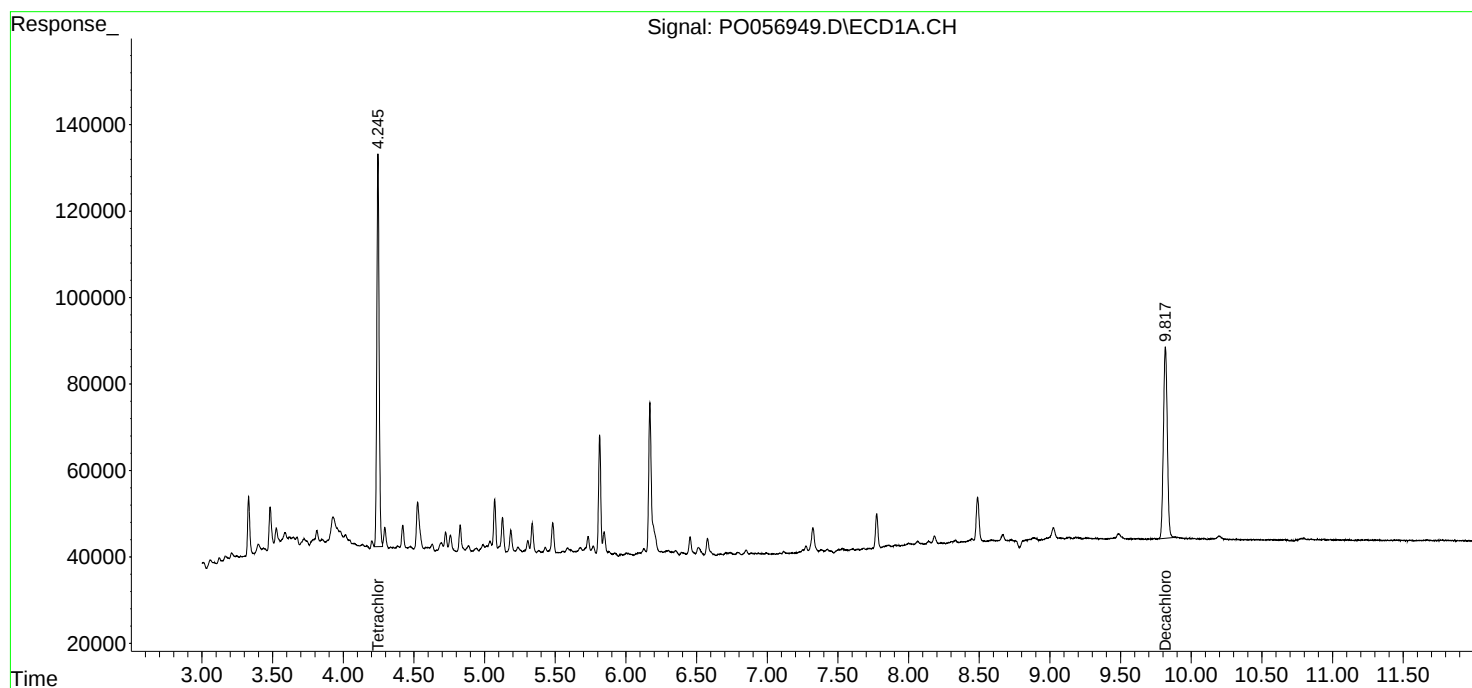

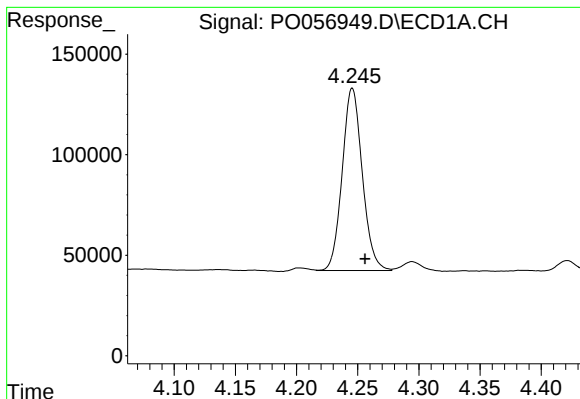


#1 Tetrachloro-m-xylene

R.T.: 4.245 min
Delta R.T.: -0.011 min
Response: 1037185
Conc: 27.09 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MW-10


Manual Integrations
APPROVED

Ankita
6/7/2019 4:18:23 PM

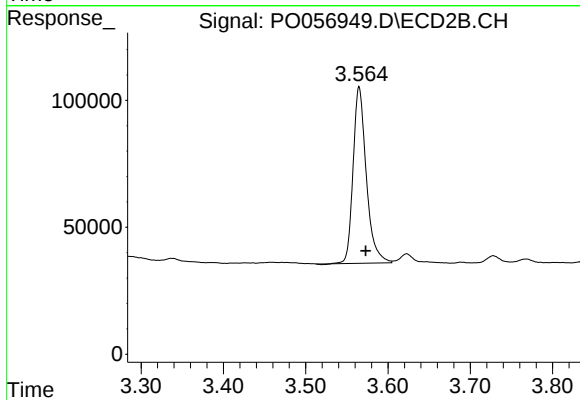


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: -0.008 min
Response: 773528
Conc: 23.46 ng/ml

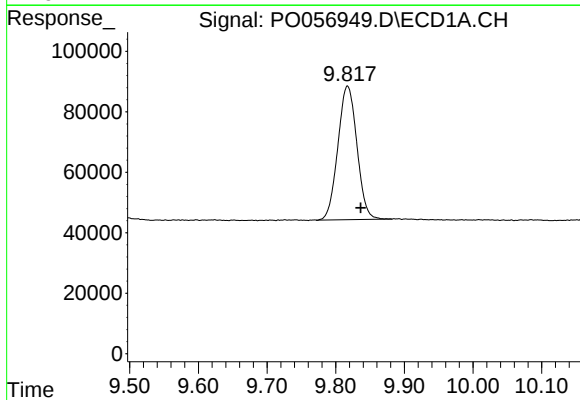

#2 Decachlorobiphenyl

R.T.: 9.817 min
Delta R.T.: -0.019 min
Response: 852066
Conc: 17.36 ng/ml

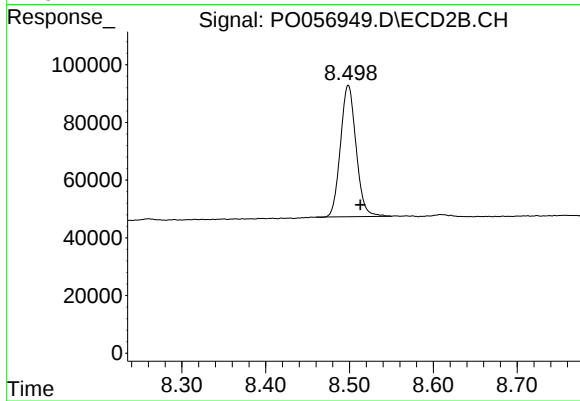

#2 Decachlorobiphenyl

R.T.: 8.499 min
Delta R.T.: -0.014 min
Response: 589161
Conc: 16.52 ng/ml