

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0060718\
Data File : P0045571.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2018 9:34
Operator : SM/UA
Sample : J3271-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-7A-WC-3

Manual Integrations
APPROVED

ugo
6/7/2018 8:14:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 11:17:18 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.993	3.270	3788258	5253370	18.137	18.945
2)	SA Decachlor...	9.268	7.989	2601022	3201038	11.325m	11.358

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0060718\
Data File : P0045571.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2018 9:34
Operator : SM/UA
Sample : J3271-05
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-7A-WC-3


Manual Integrations
APPROVED

ugo
6/7/2018 8:14:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 11:17:18 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

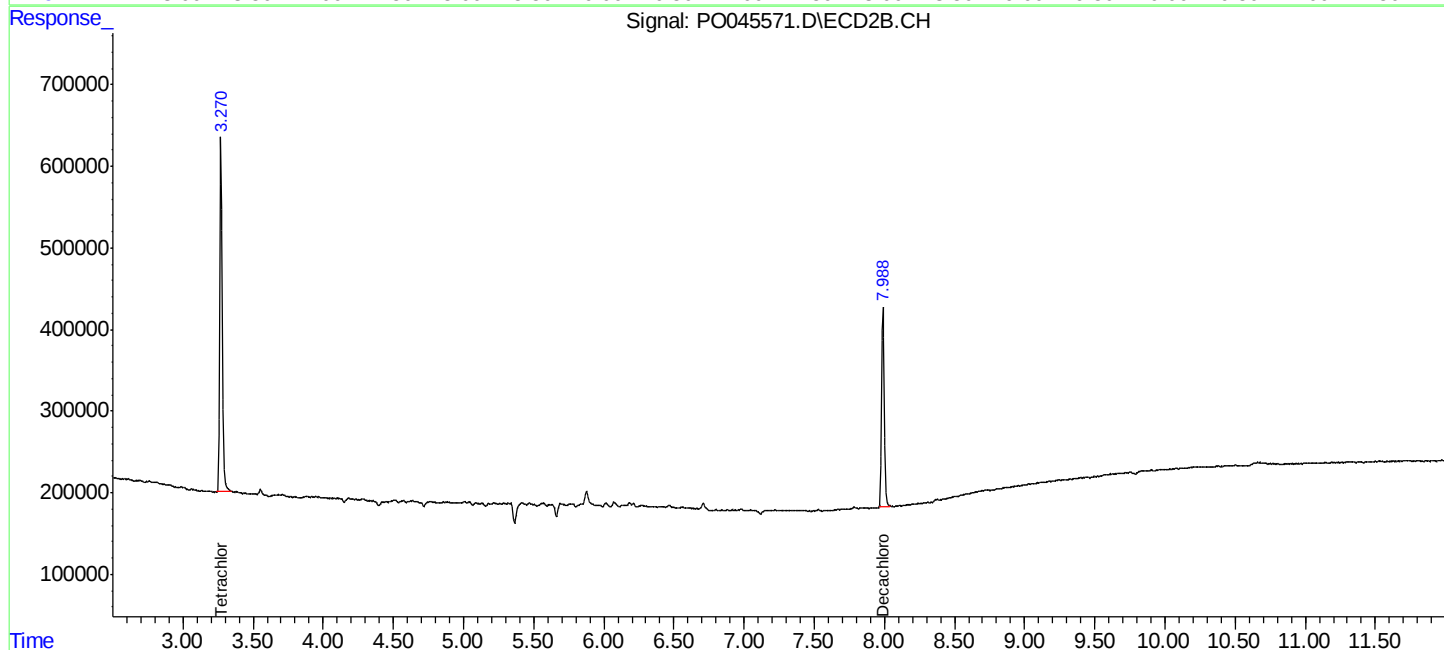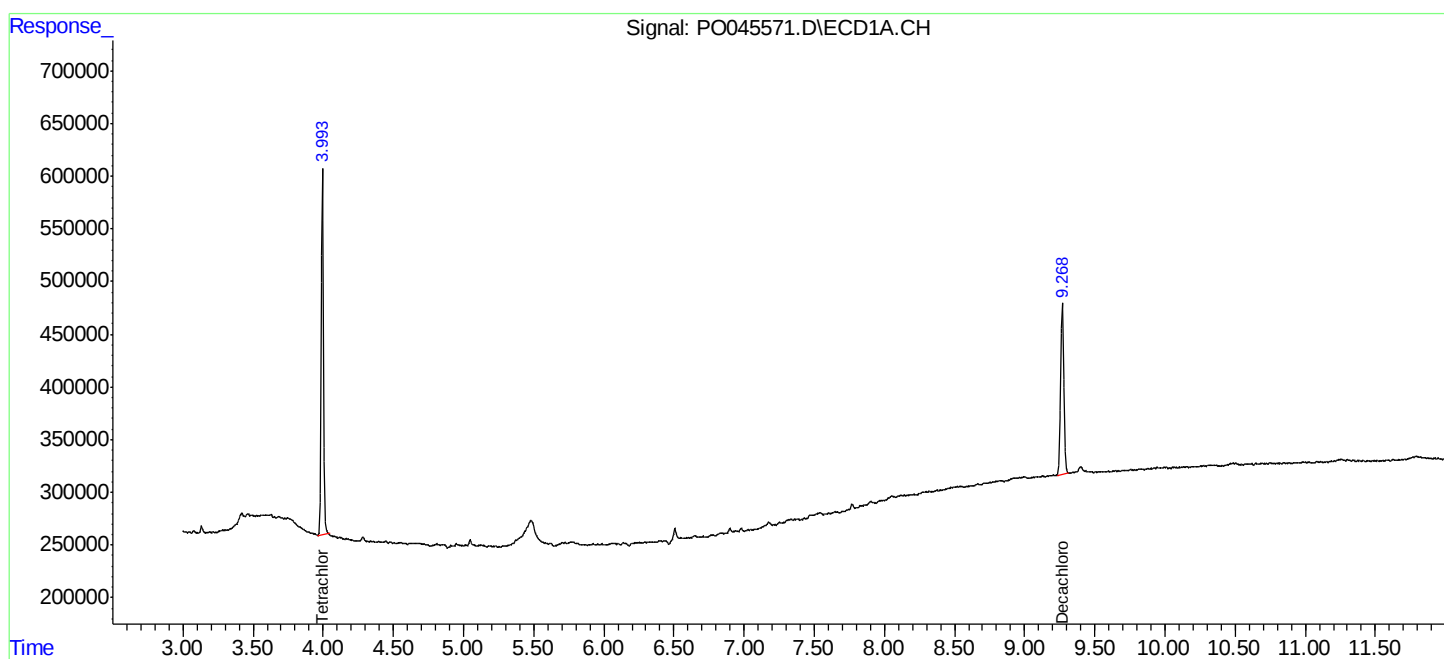

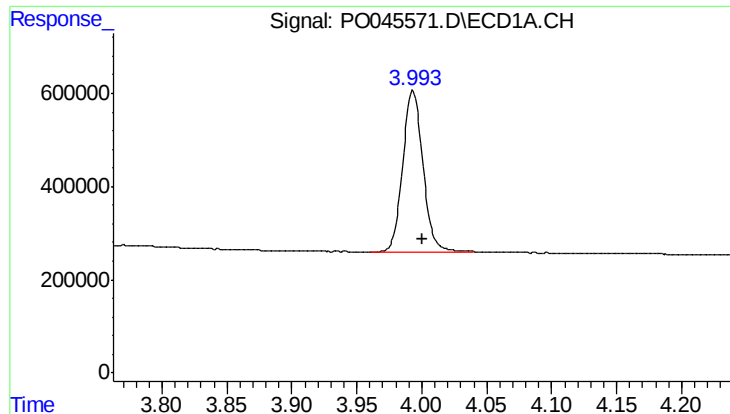


#1 Tetrachloro-m-xylene

R.T.: 3.993 min
Delta R.T.: -0.007 min
Response: 3788258
Conc: 18.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-7A-WC-3


Manual Integrations
APPROVED

ugo
6/7/2018 8:14:59 AM

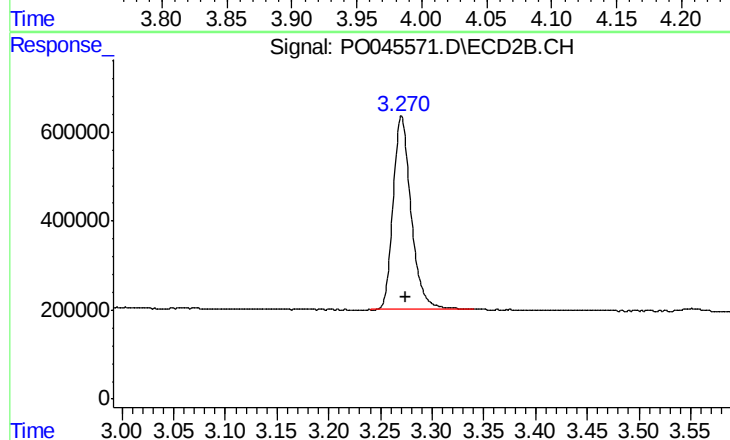


#1 Tetrachloro-m-xylene

R.T.: 3.270 min
Delta R.T.: -0.005 min
Response: 5253370
Conc: 18.95 ng/ml

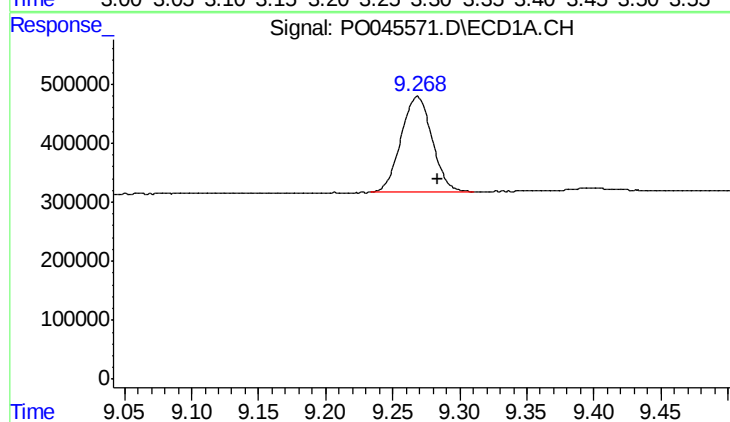

#2 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: -0.015 min
Response: 2601022
Conc: 11.33 ng/ml m

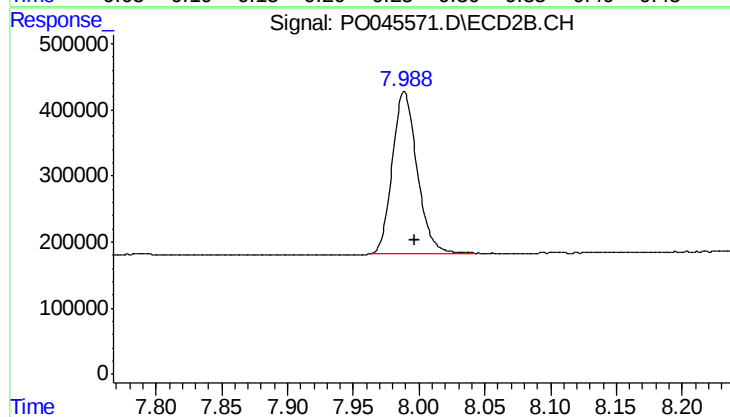

#2 Decachlorobiphenyl

R.T.: 7.989 min
Delta R.T.: -0.008 min
Response: 3201038
Conc: 11.36 ng/ml