

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0060718\
Data File : P0045576.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2018 10:51
Operator : SM/UA
Sample : J3239-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AU-05-060118-C

Manual Integrations
APPROVED

ugo
6/7/2018 8:15:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 11:30:19 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.994	3.271	5013219	6477843	24.001	23.361
2) SA Decachlor...	9.267	7.988	3095815	2915860	13.479m	10.346

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0060718\
Data File : P0045576.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2018 10:51
Operator : SM/UA
Sample : J3239-05
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AU-05-060118-C


Manual Integrations
APPROVED

ugo
6/7/2018 8:15:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 11:30:19 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

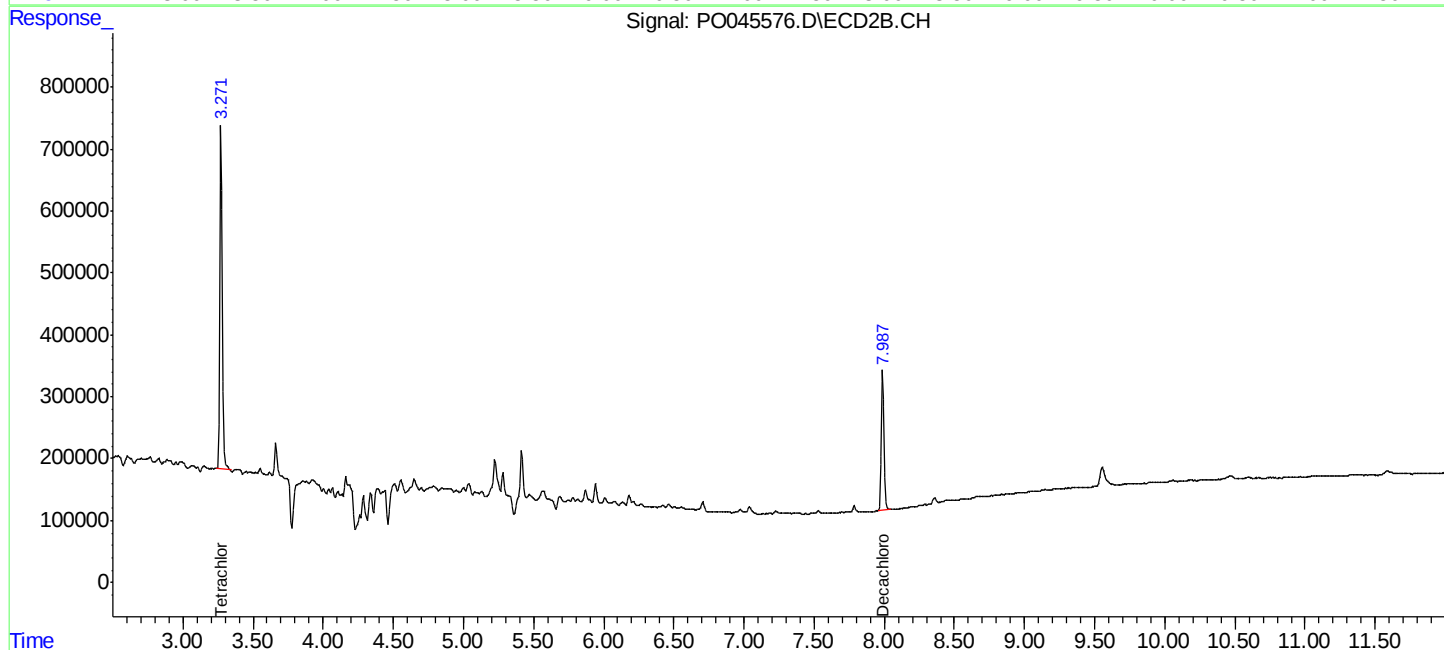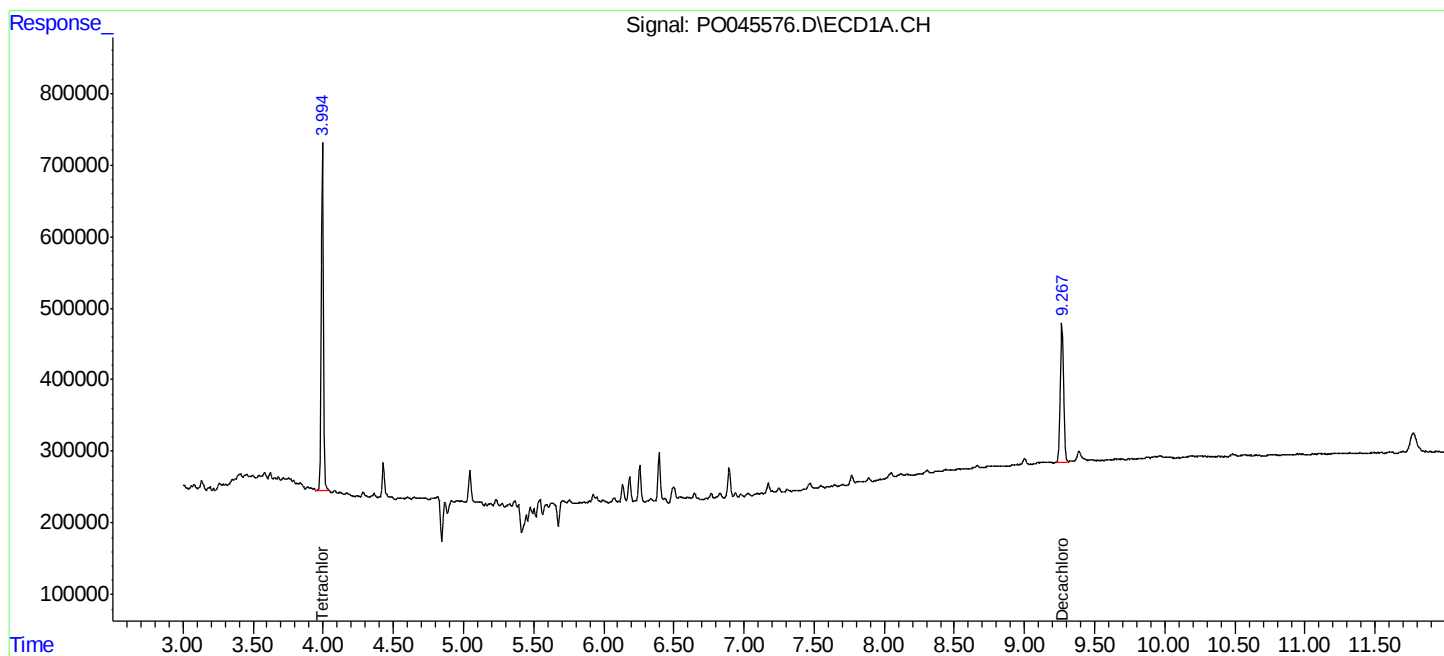

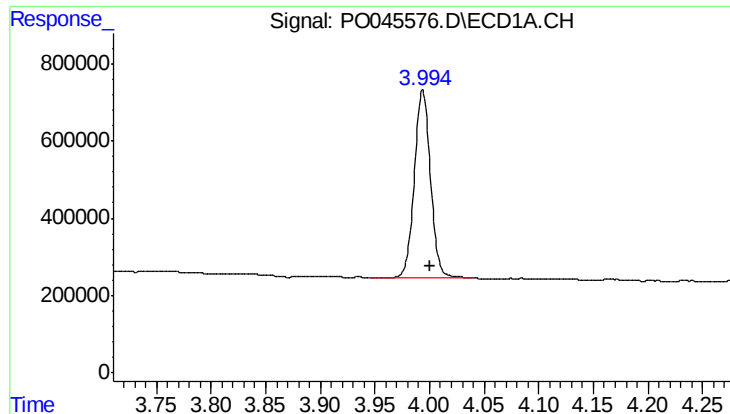


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.007 min
Response: 5013219
Conc: 24.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
AU-05-060118-C


Manual Integrations
APPROVED

ugo
6/7/2018 8:15:21 AM

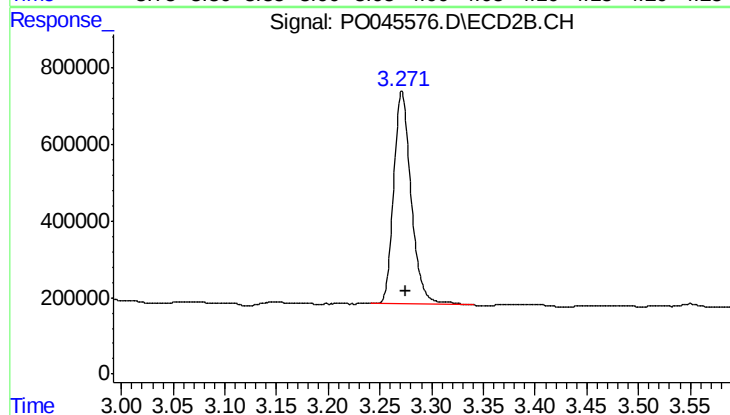


#1 Tetrachloro-m-xylene

R.T.: 3.271 min
Delta R.T.: -0.004 min
Response: 6477843
Conc: 23.36 ng/ml

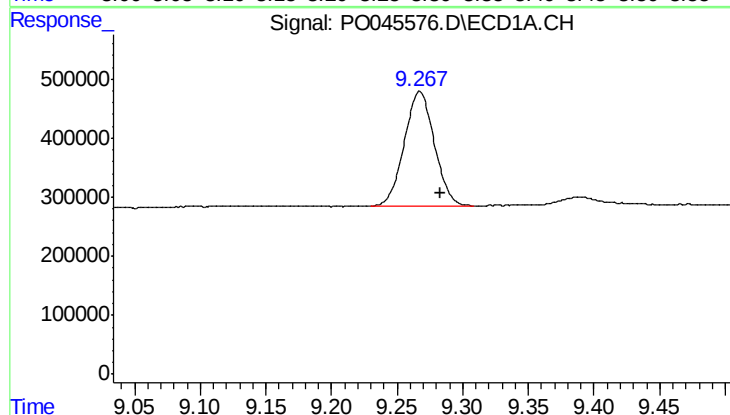

#2 Decachlorobiphenyl

R.T.: 9.267 min
Delta R.T.: -0.017 min
Response: 3095815
Conc: 13.48 ng/ml m

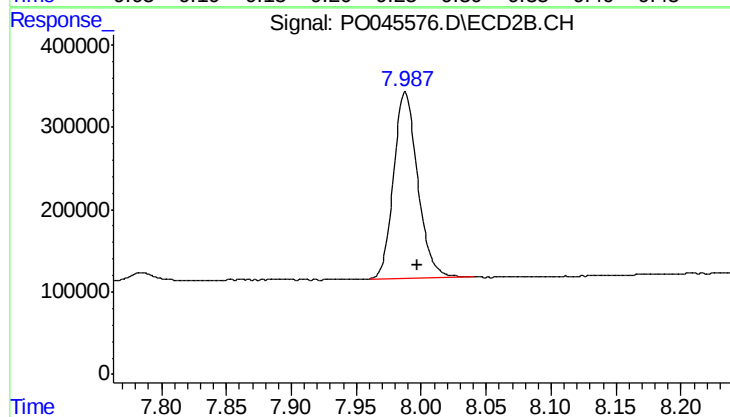

#2 Decachlorobiphenyl

R.T.: 7.988 min
Delta R.T.: -0.010 min
Response: 2915860
Conc: 10.35 ng/ml