

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0060718\
 Data File : P0045577.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jun 2018 11:07
 Operator : SM/UA
 Sample : J3239-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AU-05-060118-D

Manual Integrations
 APPROVED

ugo
 6/7/2018 8:15:24 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 11:32:57 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 31 04:53:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.994	3.272	5082197	5807210	24.331	20.943
2) SA Decachlor...	9.268	7.988	3229389	3055898	14.061m	10.843

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0060718\
Data File : P0045577.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2018 11:07
Operator : SM/UA
Sample : J3239-07
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AU-05-060118-D


Manual Integrations
APPROVED

ugo
6/7/2018 8:15:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 11:32:57 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

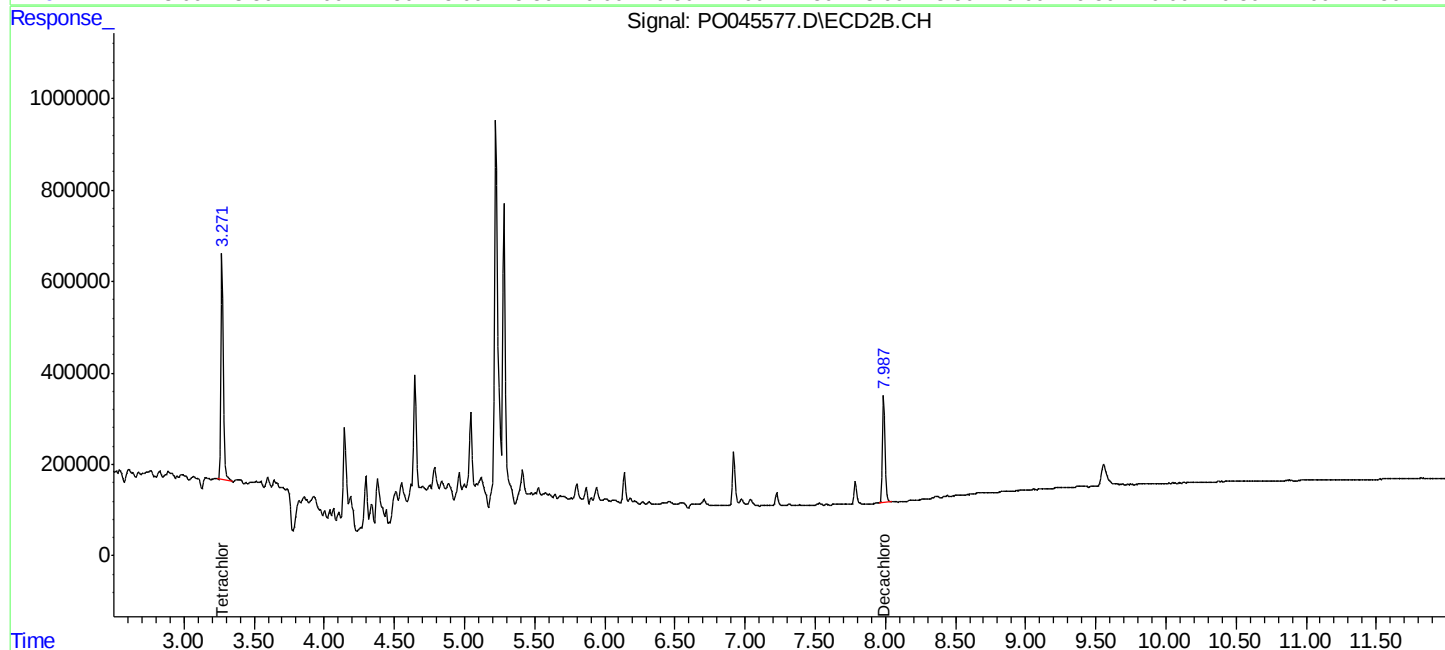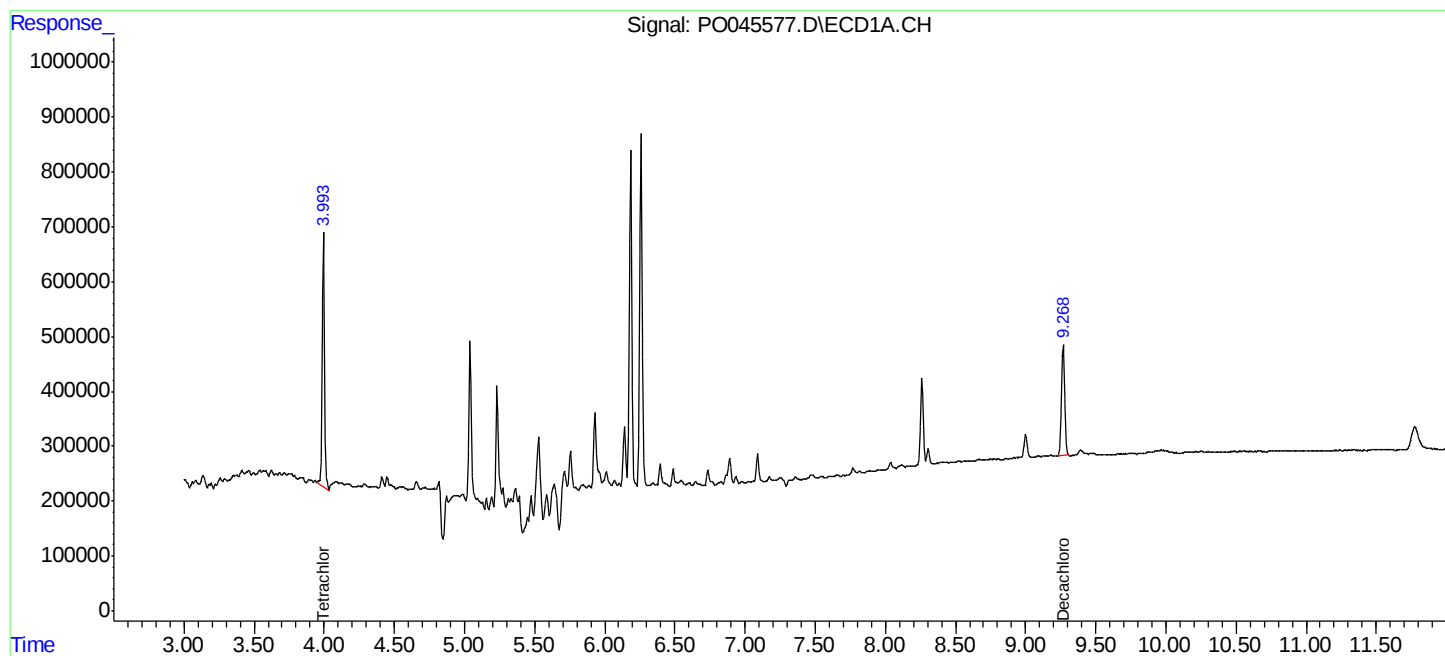

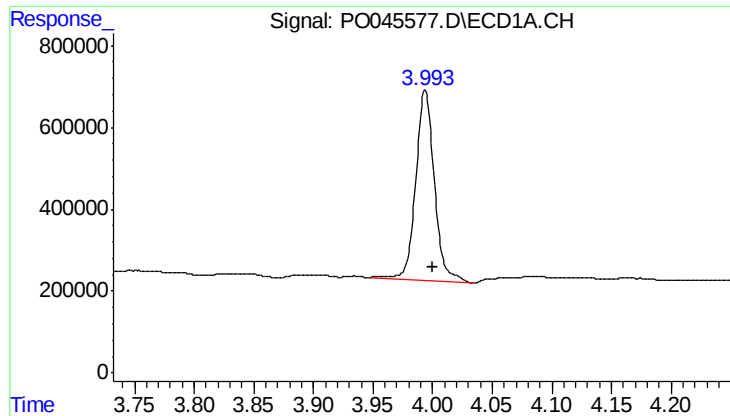


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.007 min
Response: 5082197
Conc: 24.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
AU-05-060118-D


Manual Integrations
APPROVED

ugo
6/7/2018 8:15:24 AM

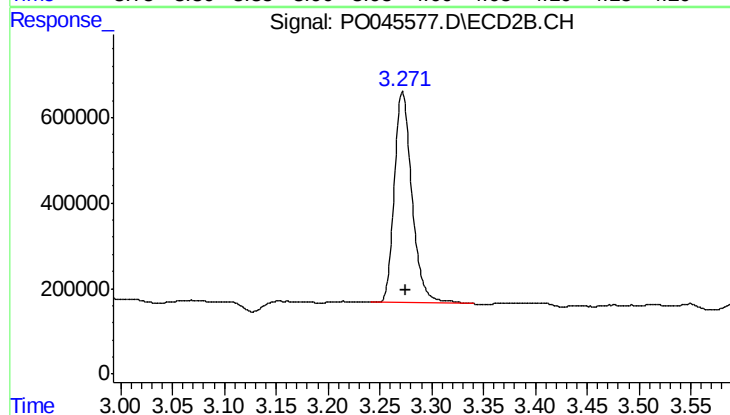


#1 Tetrachloro-m-xylene

R.T.: 3.272 min
Delta R.T.: -0.003 min
Response: 5807210
Conc: 20.94 ng/ml

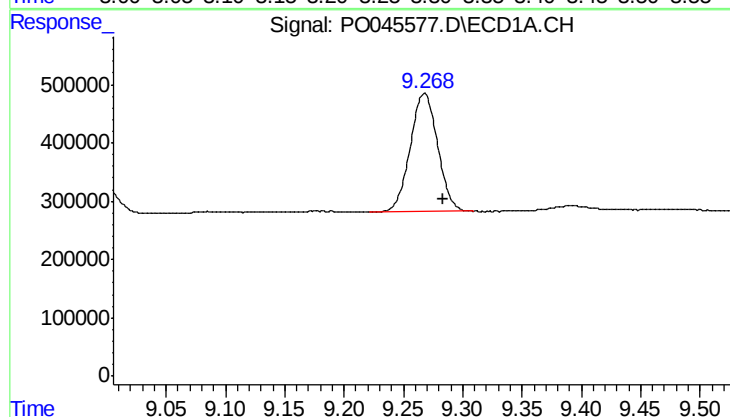

#2 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: -0.016 min
Response: 3229389
Conc: 14.06 ng/ml m

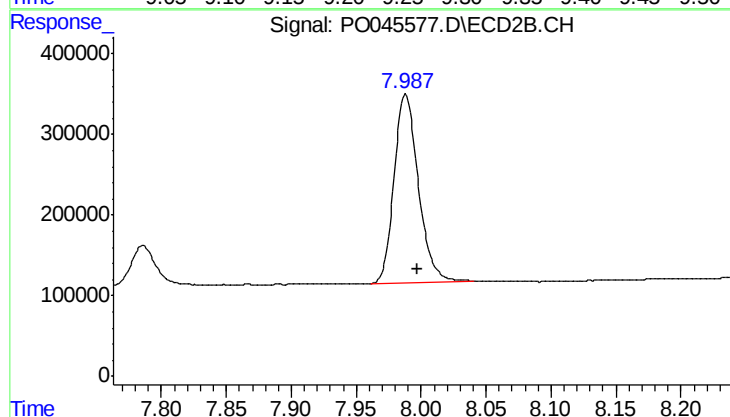

#2 Decachlorobiphenyl

R.T.: 7.988 min
Delta R.T.: -0.009 min
Response: 3055898
Conc: 10.84 ng/ml