

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0060718\
 Data File : P0045585.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jun 2018 13:44
 Operator : SM/UA
 Sample : J3327-02 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B405073

Manual Integrations
 APPROVED

ugo
 6/7/2018 8:15:44 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 14:01:50 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 31 04:53:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.004	3.273	858795	628853	4.112	2.268 #
2) SA Decachlor...	9.274	7.990	544502	350210	2.371	1.243m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0060718\
Data File : P0045585.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2018 13:44
Operator : SM/UA
Sample : J3327-02 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
B405073


Manual Integrations
APPROVED

ugo
6/7/2018 8:15:44 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 14:01:50 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

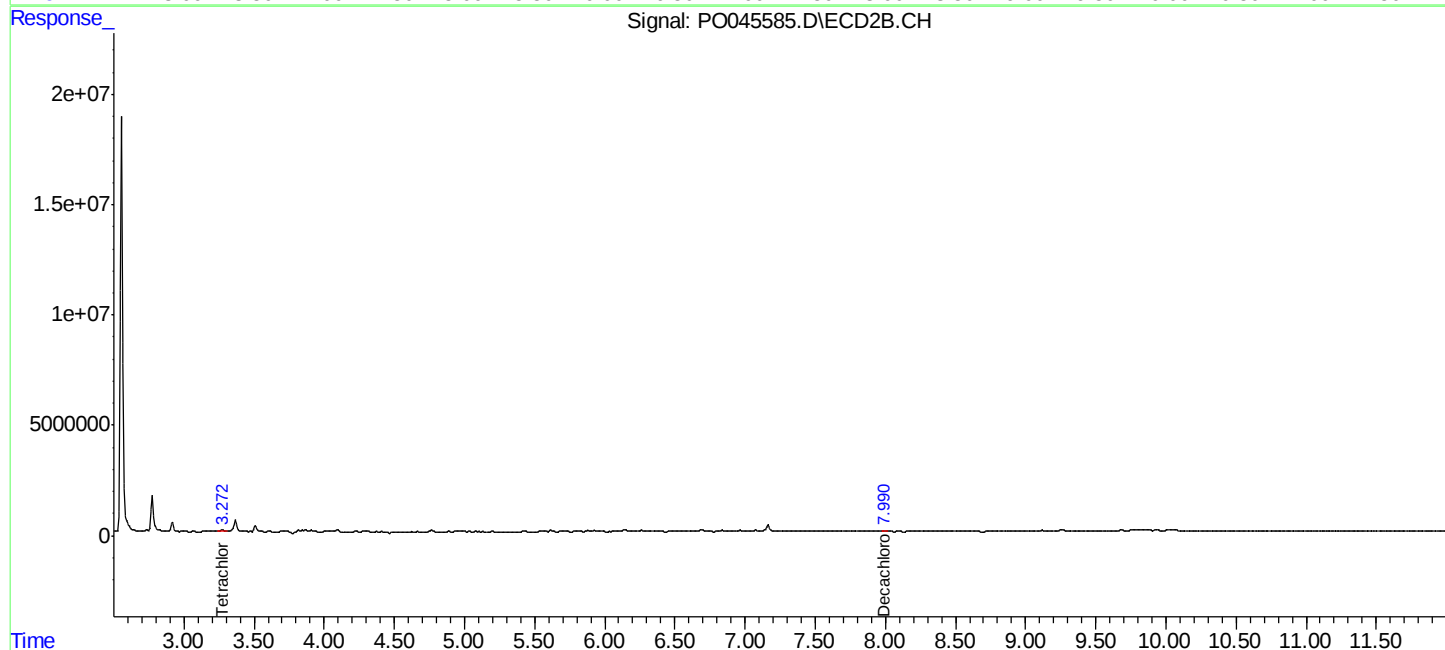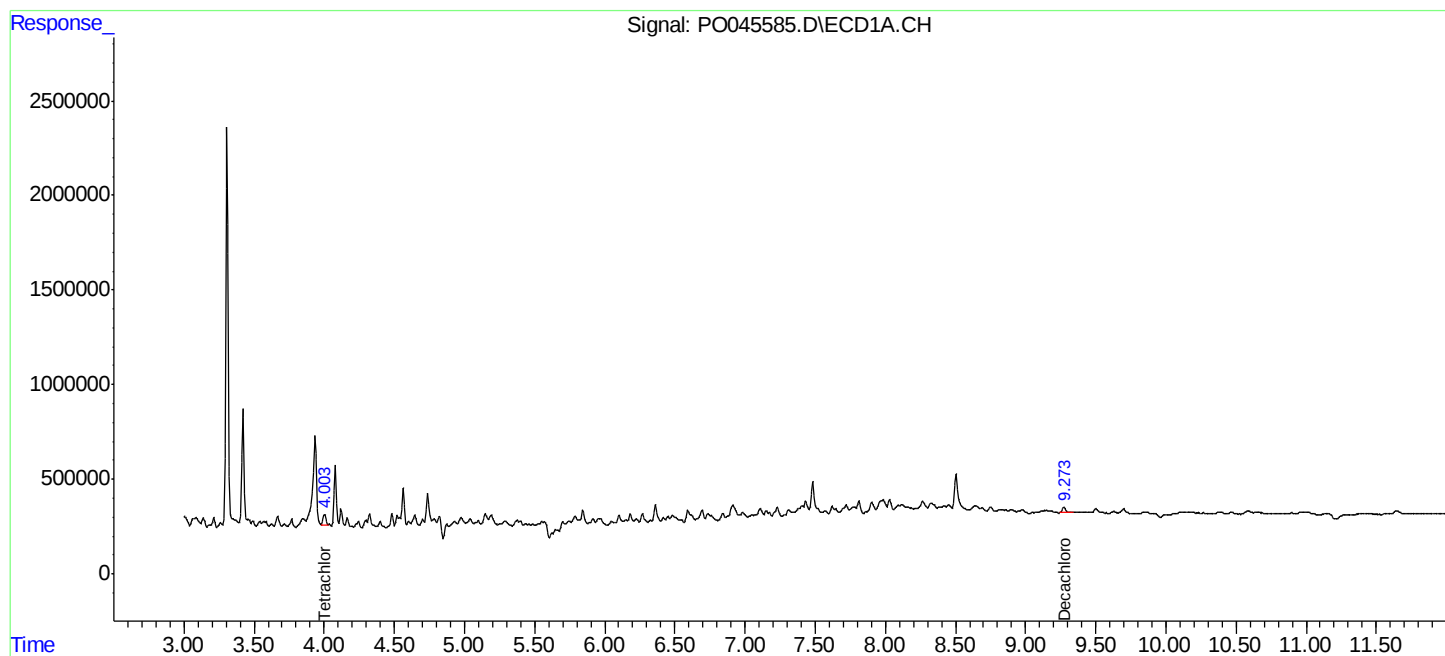

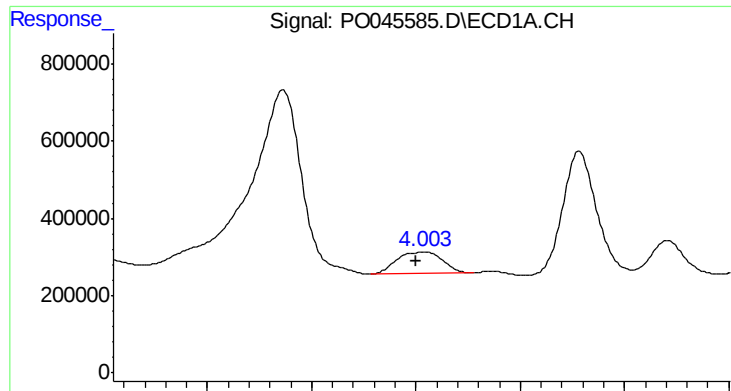


#1 Tetrachloro-m-xylene

R.T.: 4.004 min
Delta R.T.: 0.004 min
Response: 858795
Conc: 4.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
B405073


Manual Integrations
APPROVED

ugo
6/7/2018 8:15:44 AM

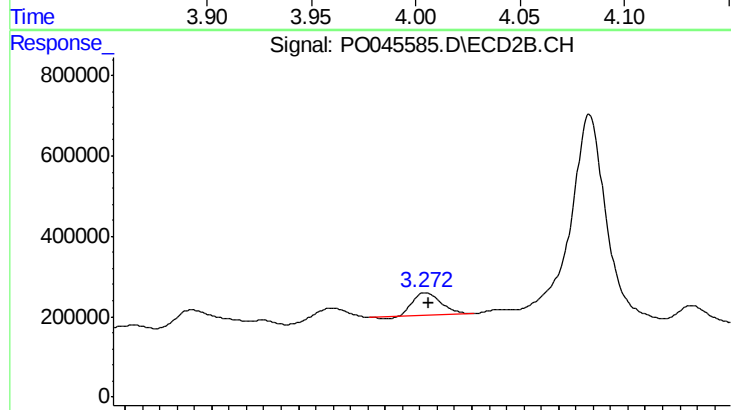


#1 Tetrachloro-m-xylene

R.T.: 3.273 min
Delta R.T.: -0.002 min
Response: 628853
Conc: 2.27 ng/ml

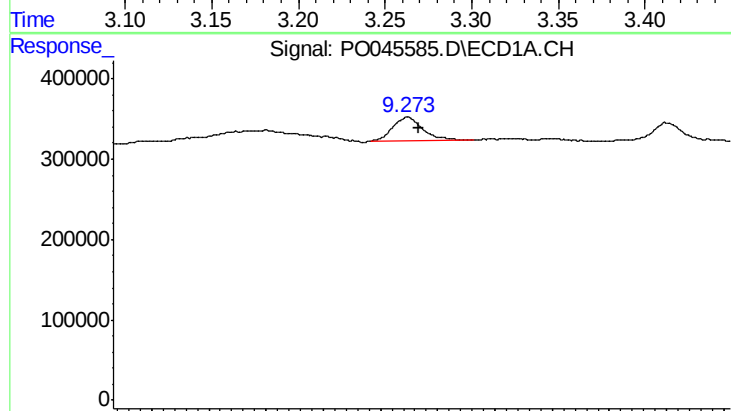

#2 Decachlorobiphenyl

R.T.: 9.274 min
Delta R.T.: -0.010 min
Response: 544502
Conc: 2.37 ng/ml

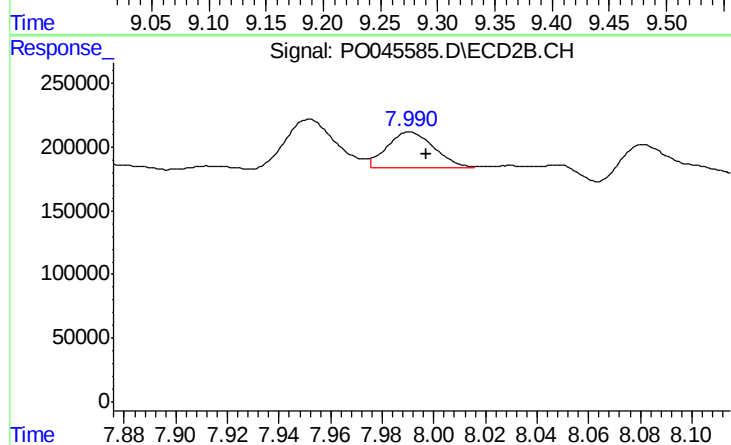

#2 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.007 min
Response: 350210
Conc: 1.24 ng/ml m