

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0060718\
Data File : P0045591.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2018 18:41
Operator : SM/UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

ugo
6/7/2018 4:26:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 00:28:48 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.994	3.269	3635951	4606195	17.407	16.611
2)	SA Decachlor...	9.267	7.986	4335118	4642108	18.875m	16.471

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0060718\
Data File : P0045591.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2018 18:41
Operator : SM/UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

ugo
6/7/2018 4:26:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 00:28:48 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

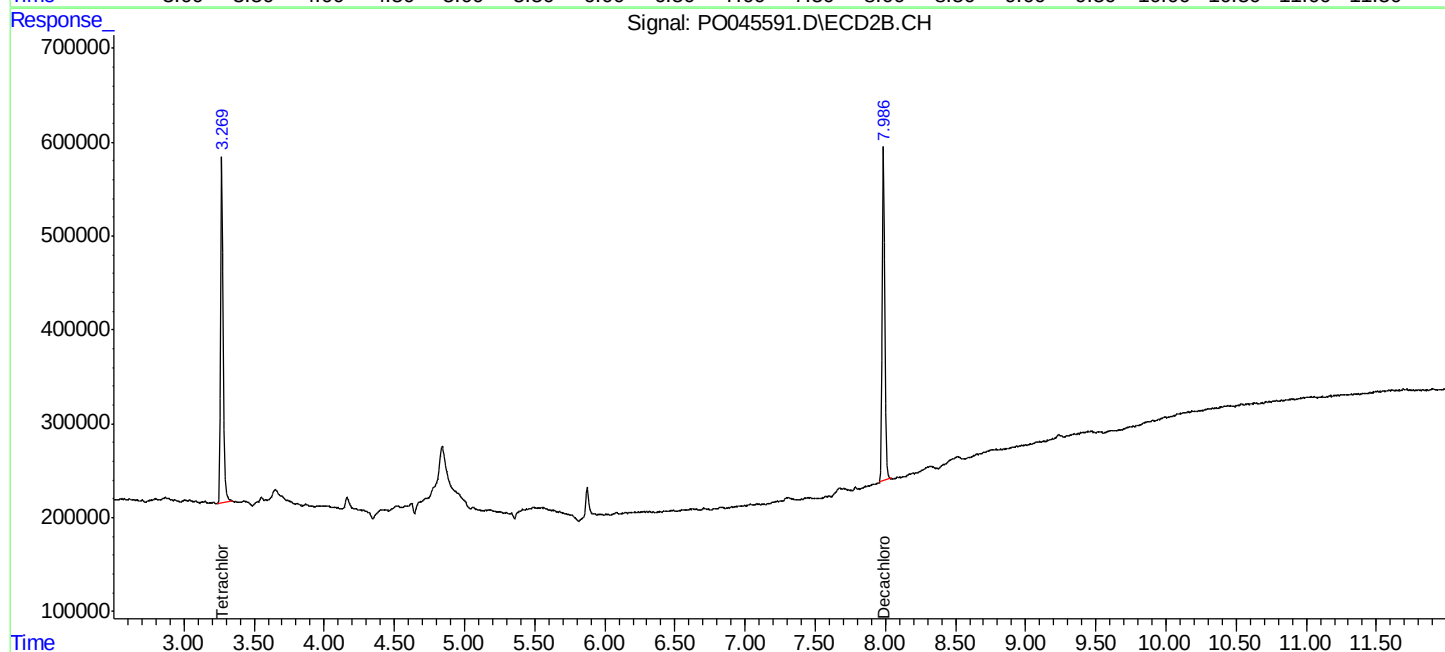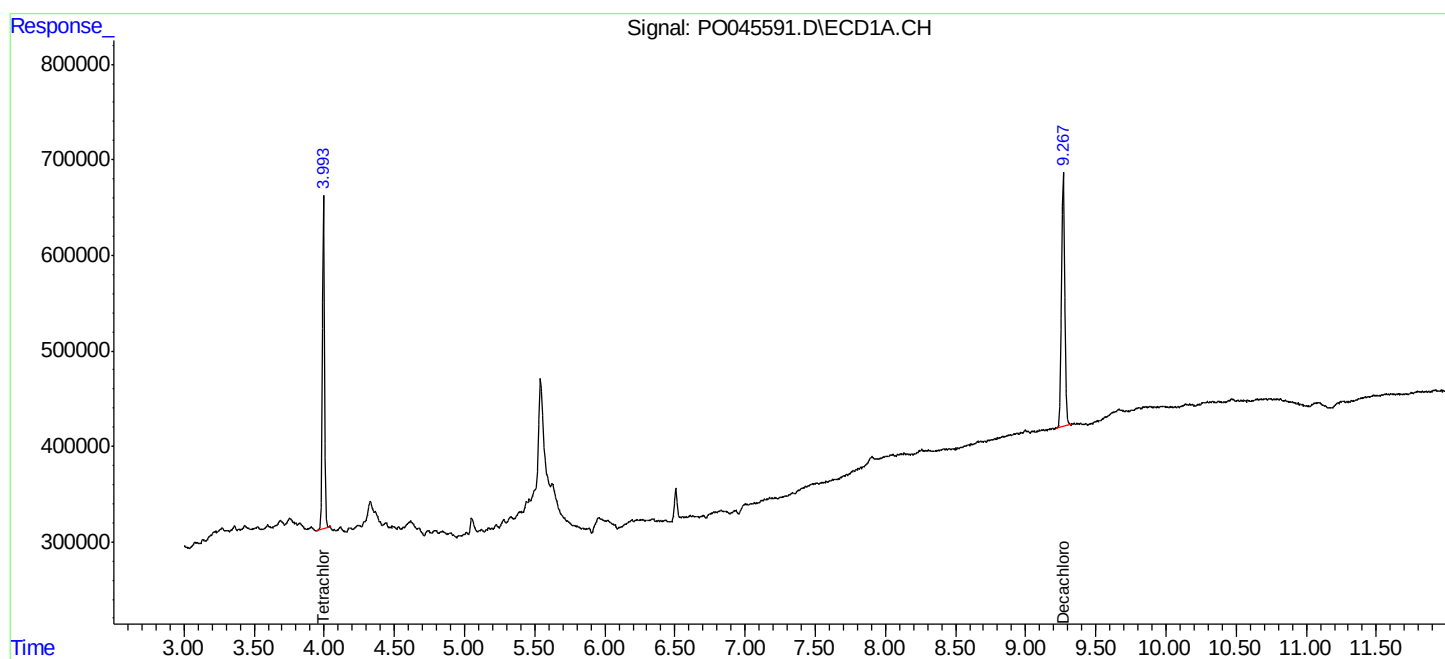

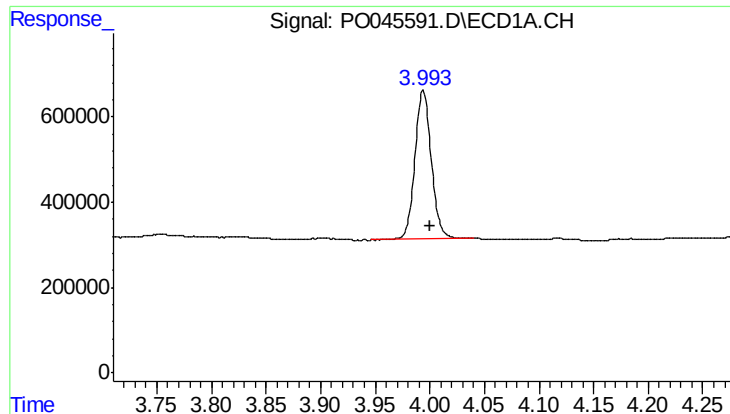


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.006 min
Response: 3635951
Conc: 17.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

ugo
6/7/2018 4:26:06 PM

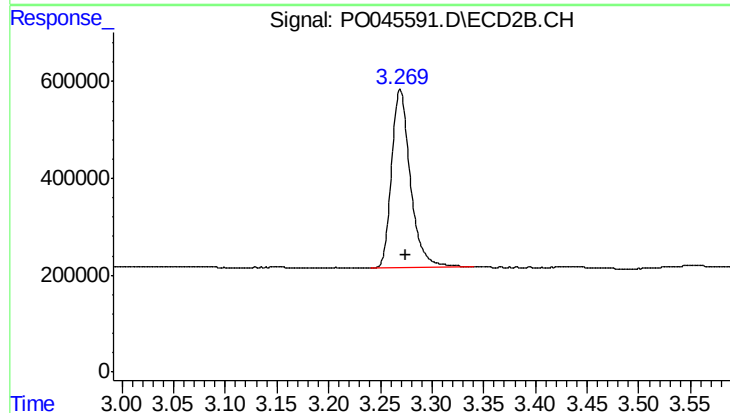


#1 Tetrachloro-m-xylene

R.T.: 3.269 min
Delta R.T.: -0.006 min
Response: 4606195
Conc: 16.61 ng/ml

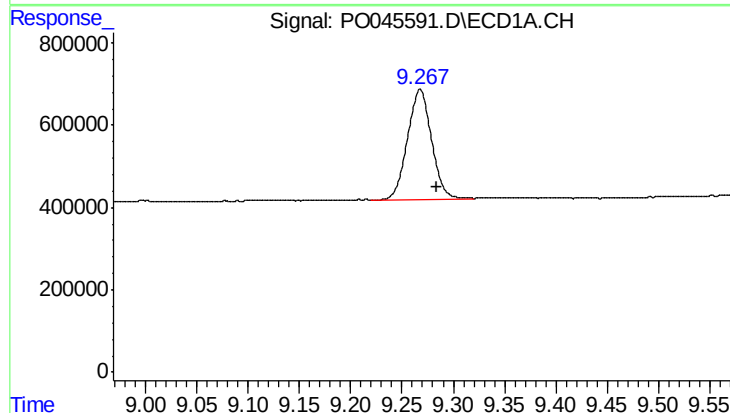

#2 Decachlorobiphenyl

R.T.: 9.267 min
Delta R.T.: -0.016 min
Response: 4335118
Conc: 18.88 ng/ml m

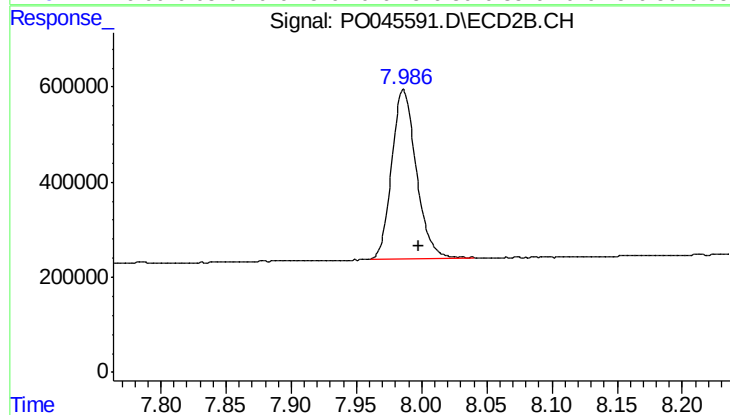

#2 Decachlorobiphenyl

R.T.: 7.986 min
Delta R.T.: -0.011 min
Response: 4642108
Conc: 16.47 ng/ml