

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0060718\
Data File : P0045597.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2018 20:49
Operator : SM/UA
Sample : J3281-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
053118-DBRC-F-U-M

Manual Integrations
APPROVED

ugo
6/7/2018 4:26:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 00:48:17 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.990	3.267	3294243	4145205	15.771	14.949
2)	SA Decachlor...	9.261	7.984	3136847	3853353	13.658m	13.672m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060718\
Data File : P0045597.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2018 20:49
Operator : SM/UA
Sample : J3281-02
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
053118-DBRC-F-U-M


Manual Integrations
APPROVED

ugo
6/7/2018 4:26:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 00:48:17 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_O\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

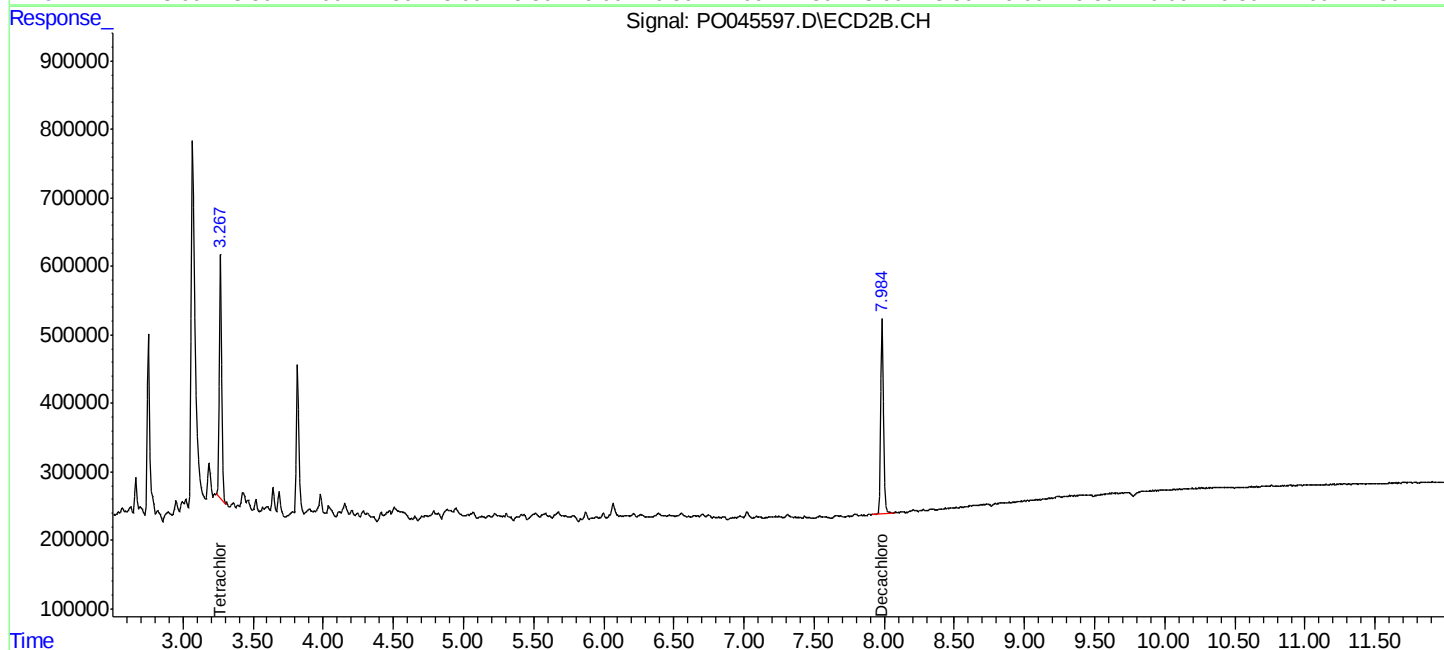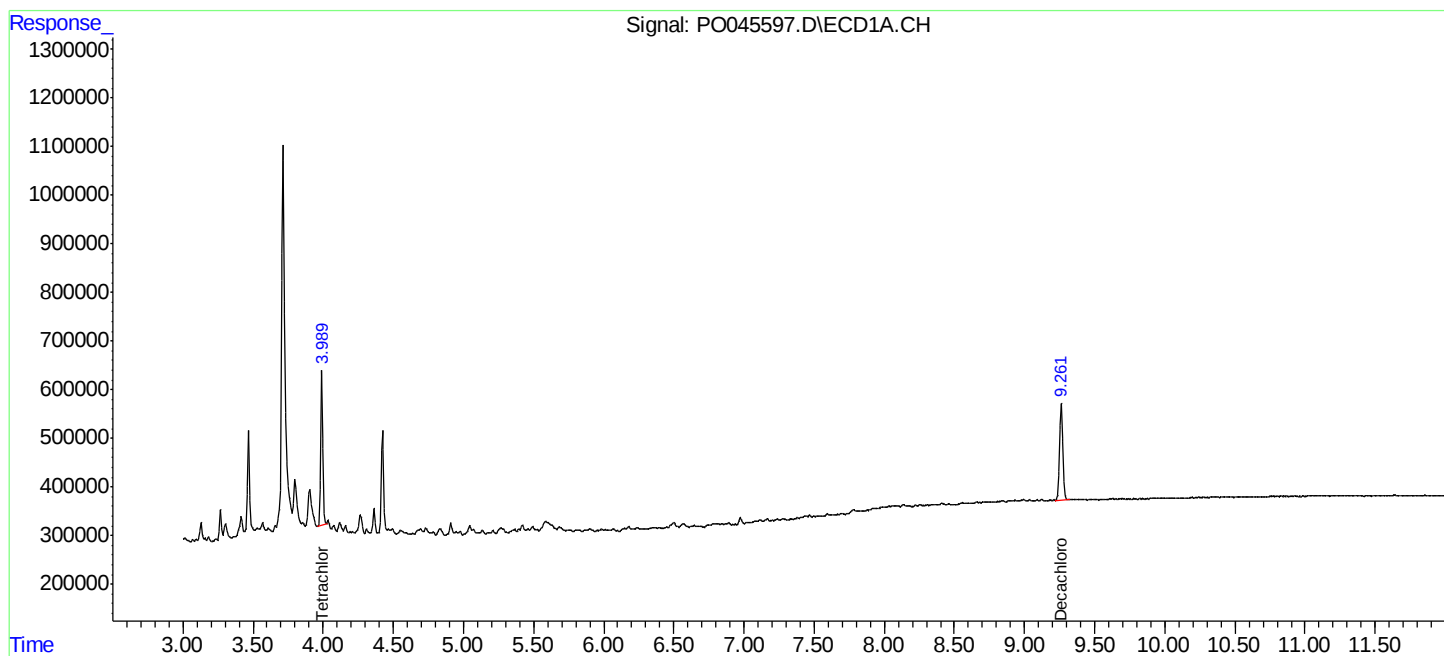

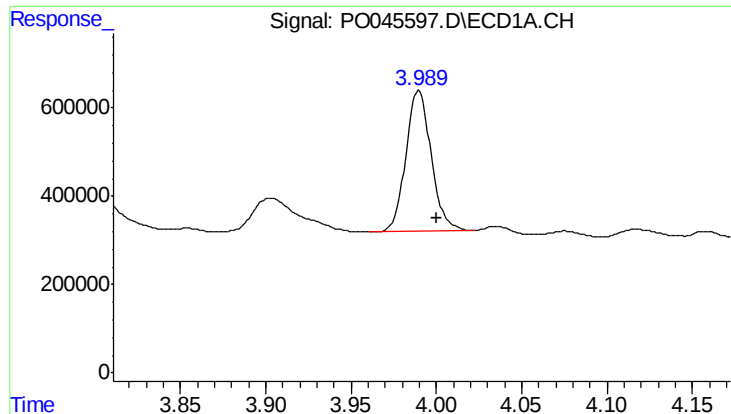


#1 Tetrachloro-m-xylene

R.T.: 3.990 min
Delta R.T.: -0.011 min
Response: 3294243
Conc: 15.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
053118-DBRC-F-U-M


Manual Integrations
APPROVED

ugo
6/7/2018 4:26:35 PM

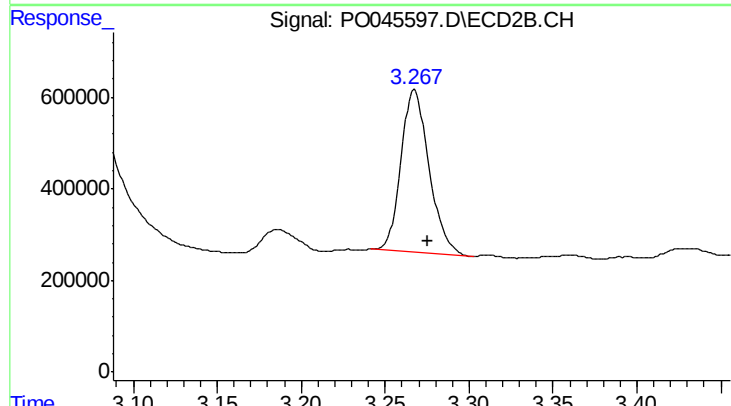


#1 Tetrachloro-m-xylene

R.T.: 3.267 min
Delta R.T.: -0.008 min
Response: 4145205
Conc: 14.95 ng/ml

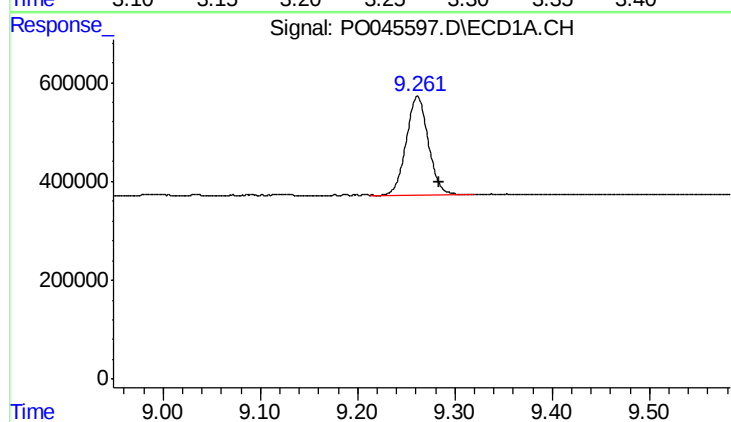

#2 Decachlorobiphenyl

R.T.: 9.261 min
Delta R.T.: -0.022 min
Response: 3136847
Conc: 13.66 ng/ml m

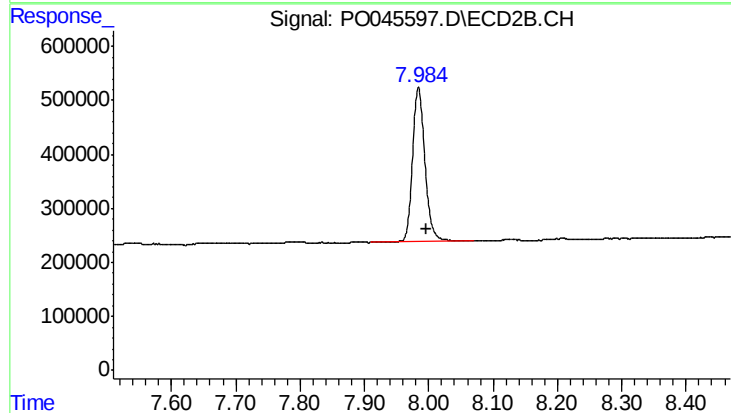

#2 Decachlorobiphenyl

R.T.: 7.984 min
Delta R.T.: -0.014 min
Response: 3853353
Conc: 13.67 ng/ml m