

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0060718\
Data File : P0045613.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jun 2018 00:57
Operator : SM/UA
Sample : J3321-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
060118-JETT-F-D-B

Manual Integrations
APPROVED

ugo
6/7/2018 4:27:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 04:50:07 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.990	3.268	3335934	4124768	15.971	14.875
2) SA Decachlor...	9.259	7.982	2936621	3722998	12.786m	13.210m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060718\
Data File : P0045613.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jun 2018 00:57
Operator : SM/UA
Sample : J3321-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
060118-JETT-F-D-B


Manual Integrations
APPROVED

ugo
6/7/2018 4:27:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 04:50:07 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_O\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

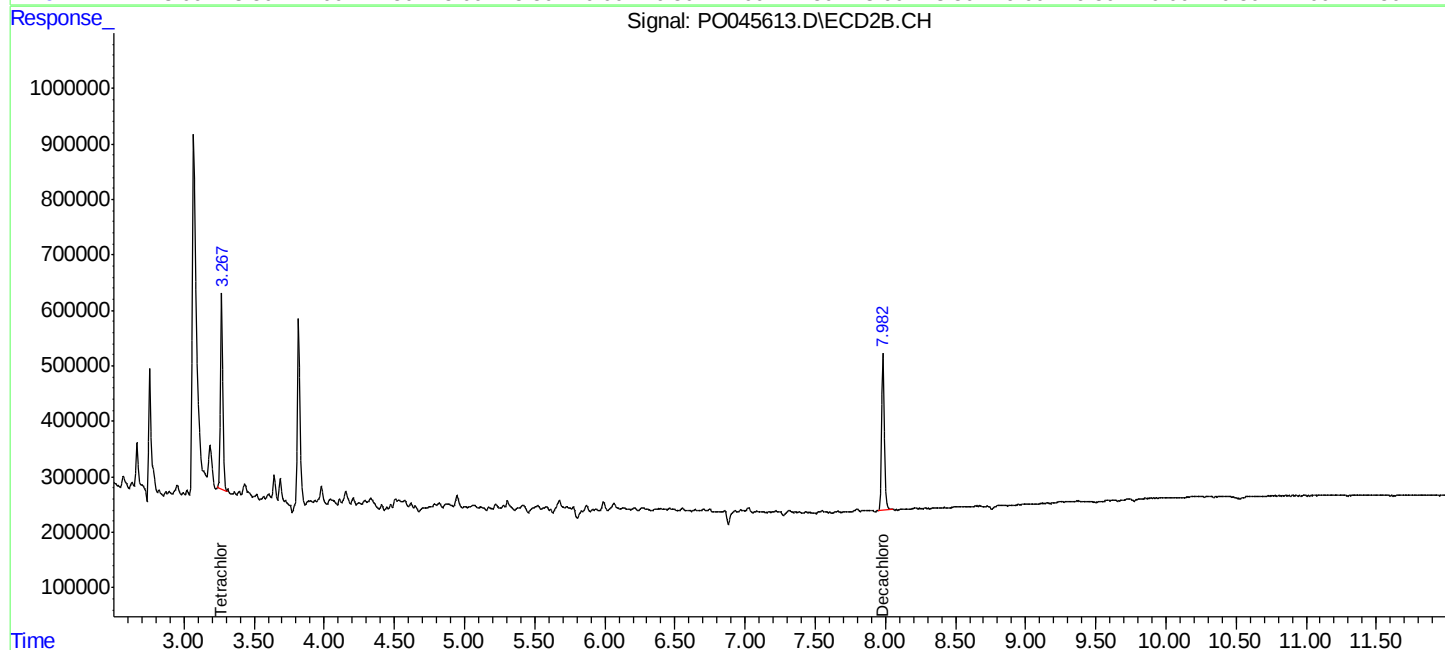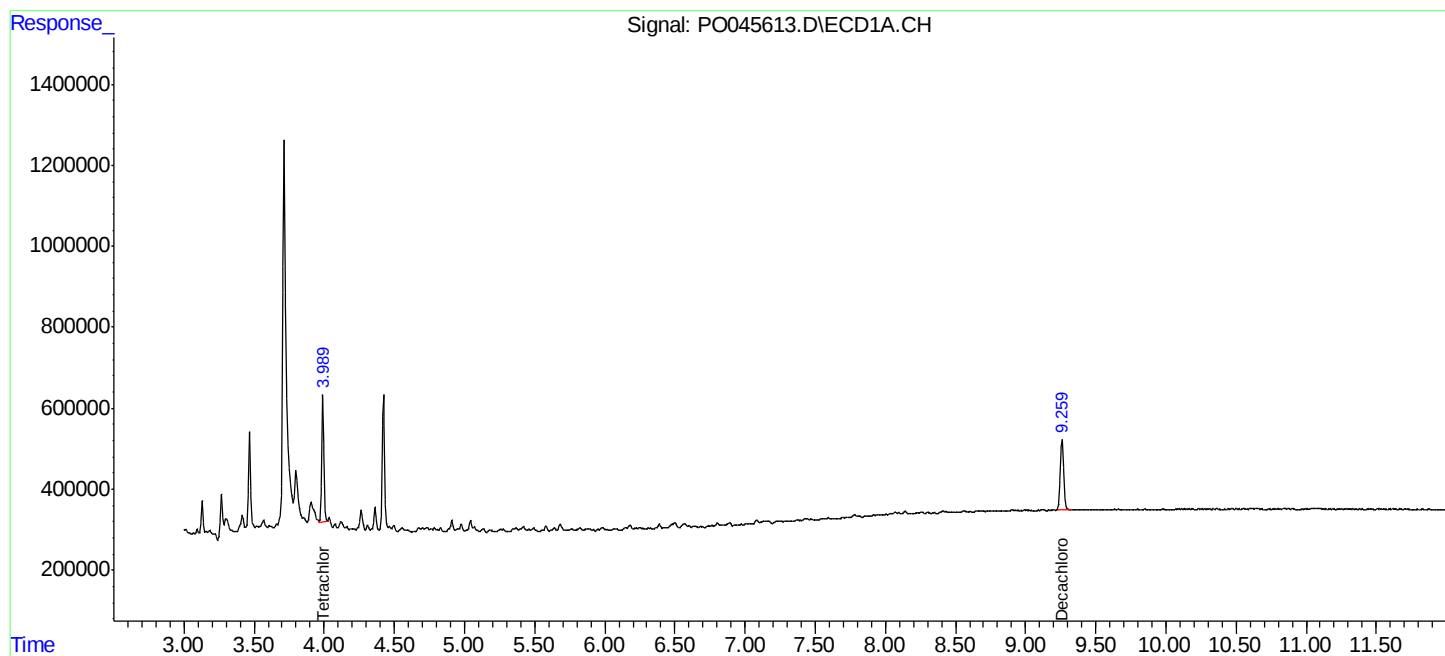

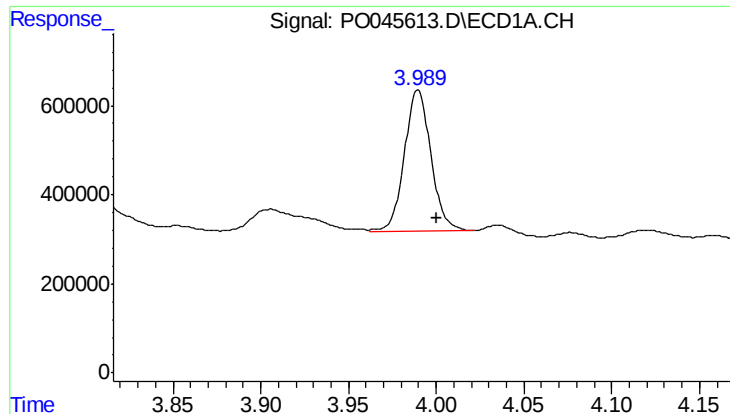


#1 Tetrachloro-m-xylene

R.T.: 3.990 min
Delta R.T.: -0.011 min
Response: 3335934
Conc: 15.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
060118-JETT-F-D-B


Manual Integrations
APPROVED

ugo
6/7/2018 4:27:44 PM

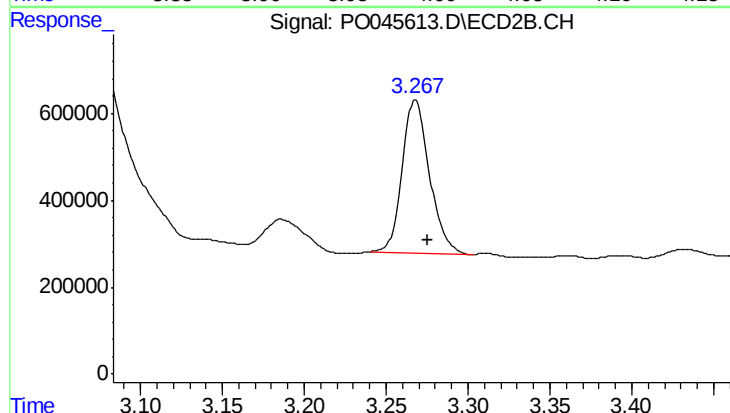


#1 Tetrachloro-m-xylene

R.T.: 3.268 min
Delta R.T.: -0.007 min
Response: 4124768
Conc: 14.88 ng/ml

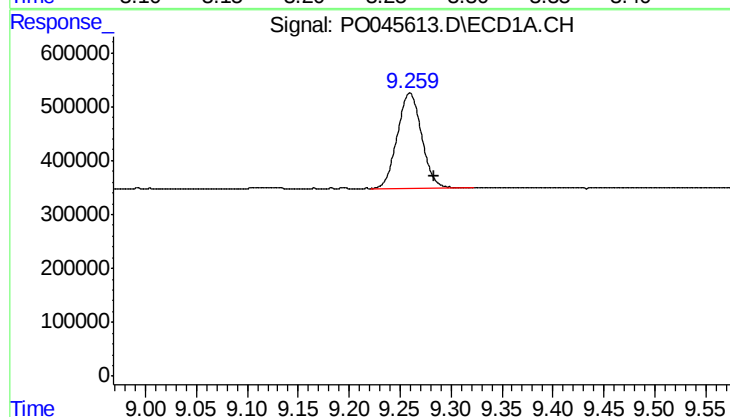

#2 Decachlorobiphenyl

R.T.: 9.259 min
Delta R.T.: -0.024 min
Response: 2936621
Conc: 12.79 ng/ml m

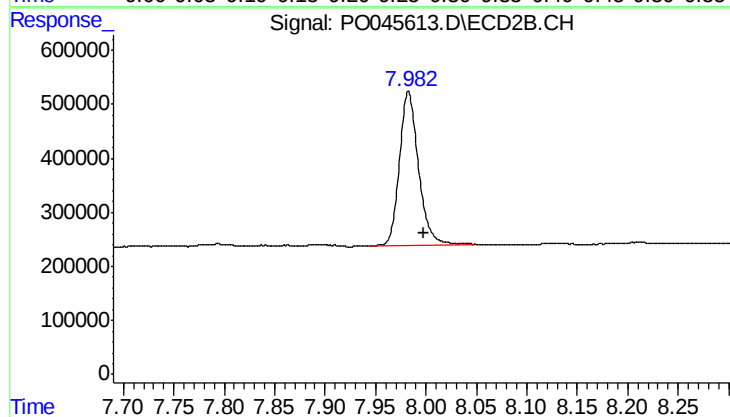

#2 Decachlorobiphenyl

R.T.: 7.982 min
Delta R.T.: -0.015 min
Response: 3722998
Conc: 13.21 ng/ml m