

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0060719\  
 Data File : P0056999.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 08 Jun 2019 00:10  
 Operator : SM/SJ  
 Sample : K3191-07  
 Misc :  
 ALS Vial : 25 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 CULVER-CBTC-TP1-060419

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jun 08 04:05:37 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0052319.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri May 24 00:11:05 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1  | RT#2  | Resp#1 | Resp#2 | ng/ml  | ng/ml  |
|-----------------------------|-------|-------|--------|--------|--------|--------|
| -----                       |       |       |        |        |        |        |
| System Monitoring Compounds |       |       |        |        |        |        |
| 1) SA Tetrachlo...          | 4.245 | 3.564 | 720950 | 617890 | 18.832 | 18.736 |
| 2) SA Decachlor...          | 9.811 | 8.494 | 858317 | 576348 | 17.487 | 16.164 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0060719\  
Data File : P0056999.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 08 Jun 2019 00:10  
Operator : SM/SJ  
Sample : K3191-07  
Misc :  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
CULVER-CBTC-TP1-060419

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jun 08 04:05:37 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0052319.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri May 24 00:11:05 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

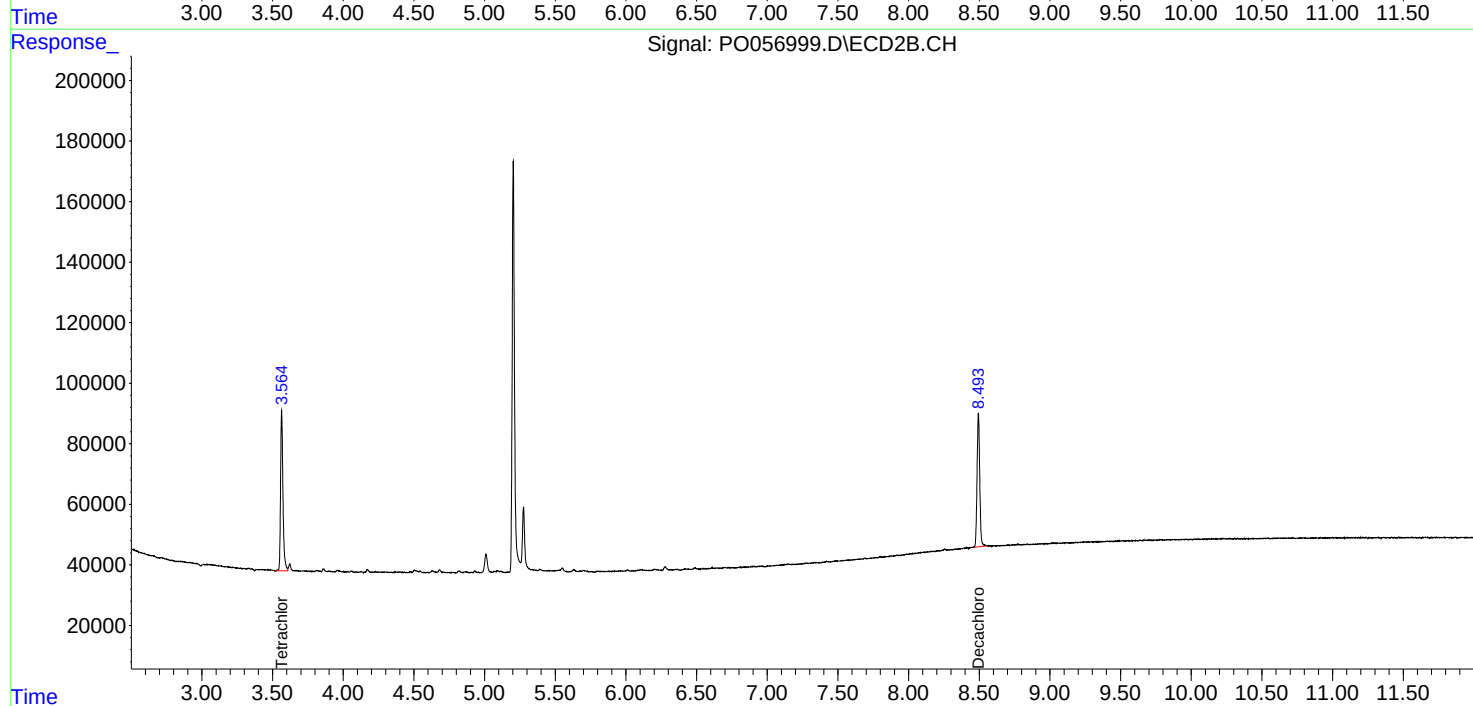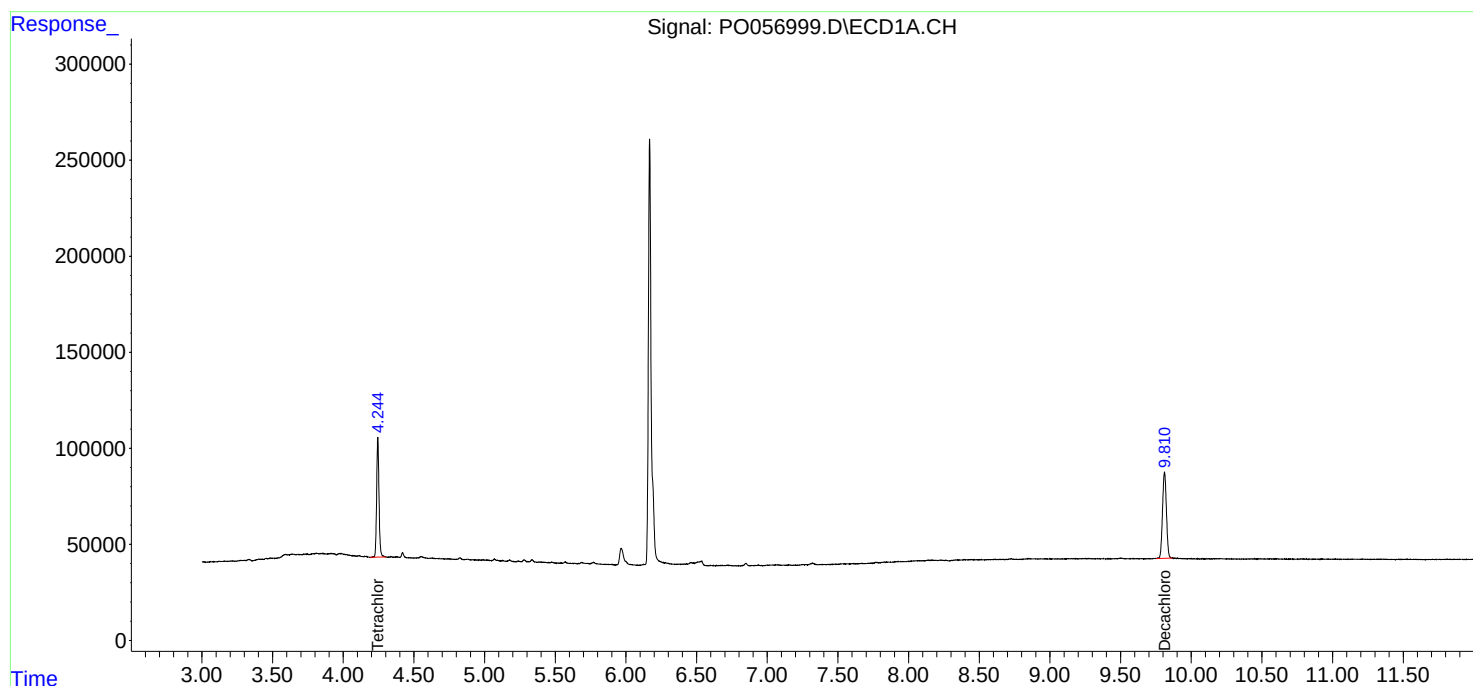


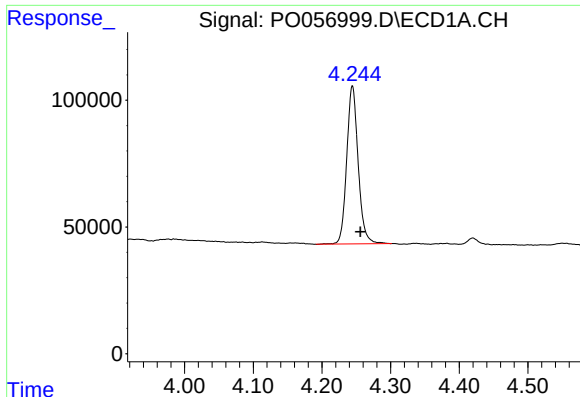

#1 Tetrachloro-m-xylene


R.T.: 4.245 min  
Delta R.T.: -0.011 min  
Response: 720950  
Conc: 18.83 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CULVER-CBTC-TP1-060419

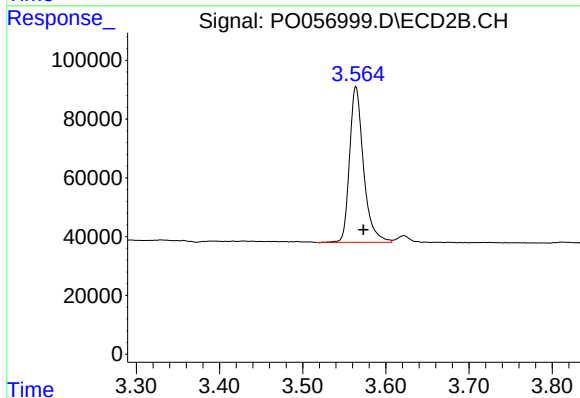


#1 Tetrachloro-m-xylene

R.T.: 3.564 min  
Delta R.T.: -0.009 min  
Response: 617890  
Conc: 18.74 ng/ml

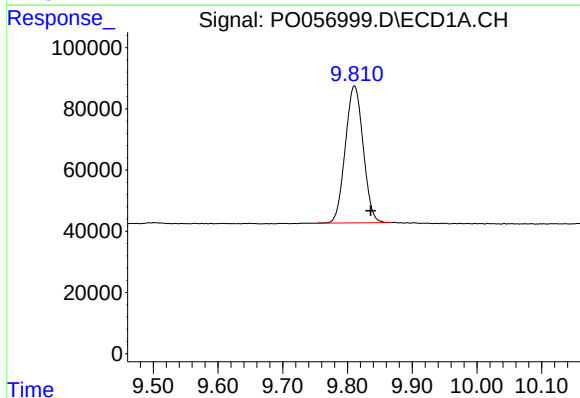

#2 Decachlorobiphenyl

R.T.: 9.811 min  
Delta R.T.: -0.025 min  
Response: 858317  
Conc: 17.49 ng/ml

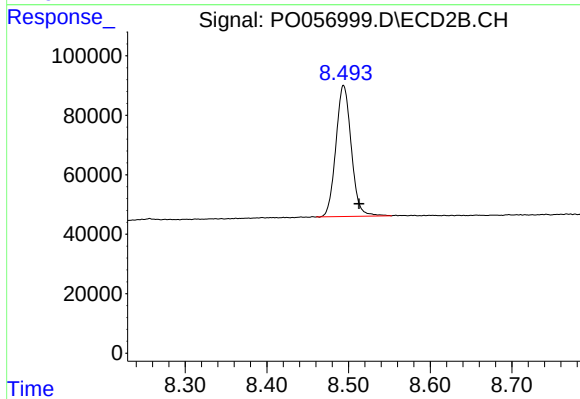

#2 Decachlorobiphenyl

R.T.: 8.494 min  
Delta R.T.: -0.019 min  
Response: 576348  
Conc: 16.16 ng/ml