

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060719\
 Data File : P0056993.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jun 2019 22:28
 Operator : SM/SJ
 Sample : K3242-14
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 Q115-13A

Manual Integrations
 APPROVED

Ankita
 6/10/2019 12:30:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 00:00:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.243	3.563	1135598	991188	29.663	30.056
2)	SA Decachlor...	9.811	8.493	1343672	870205	27.375	24.405m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060719\
Data File : P0056993.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jun 2019 22:28
Operator : SM/SJ
Sample : K3242-14
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
Q115-13A


Manual Integrations
APPROVED

Ankita
6/10/2019 12:30:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 00:00:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

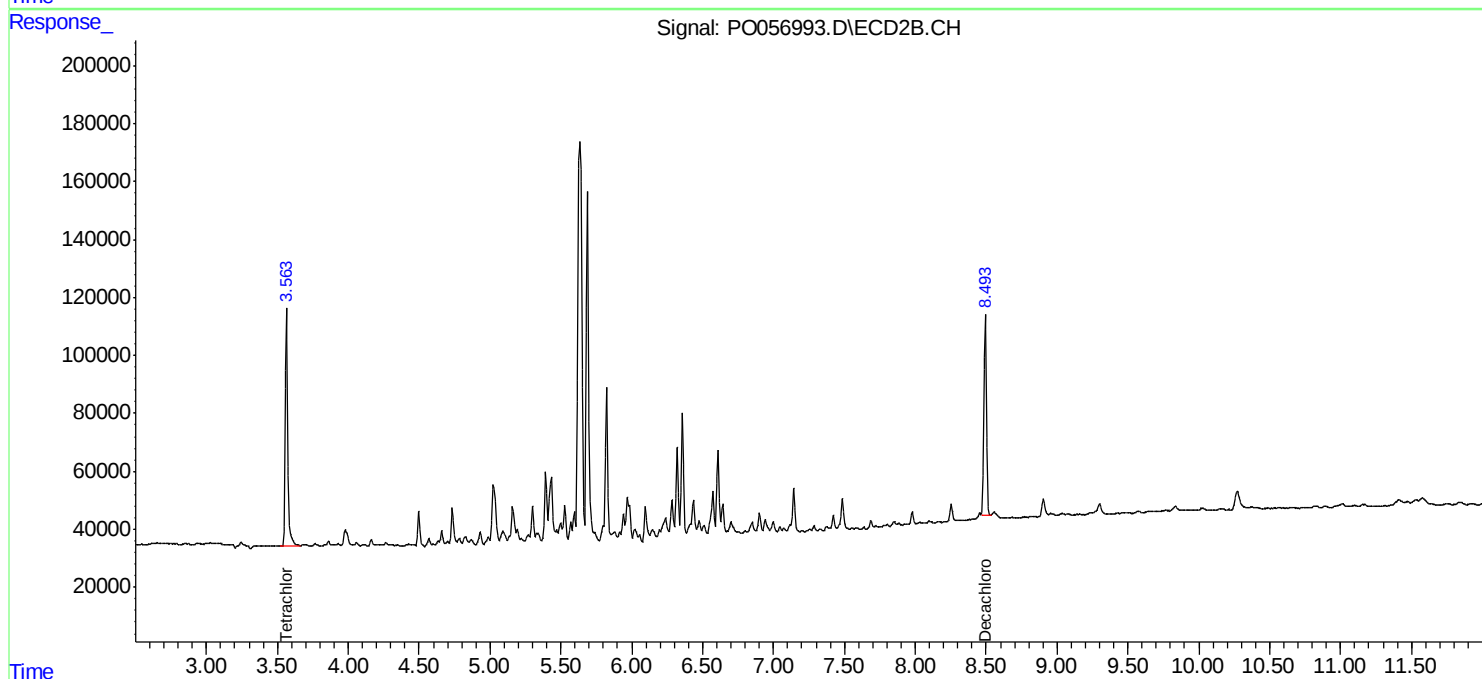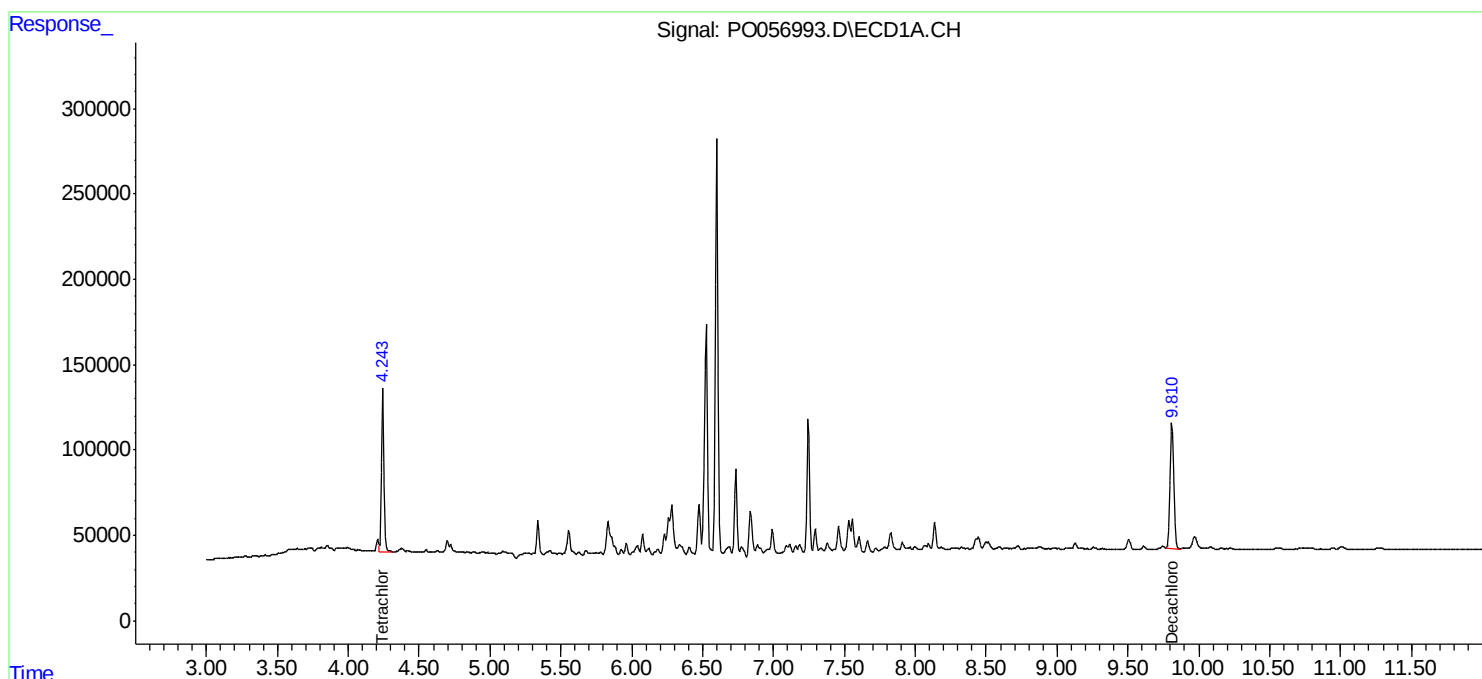

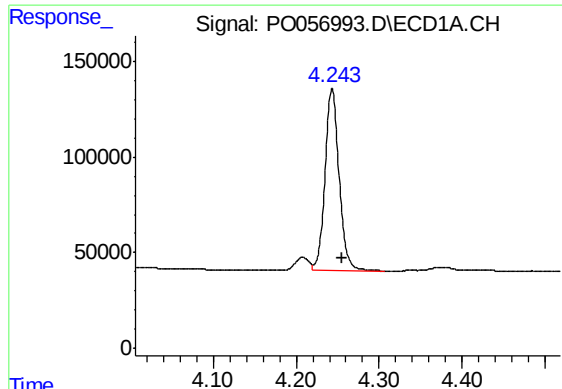


#1 Tetrachloro-m-xylene

R.T.: 4.243 min
Delta R.T.: -0.013 min
Response: 1135598
Conc: 29.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
Q115-13A


Manual Integrations
APPROVED

Ankita
6/10/2019 12:30:16 PM

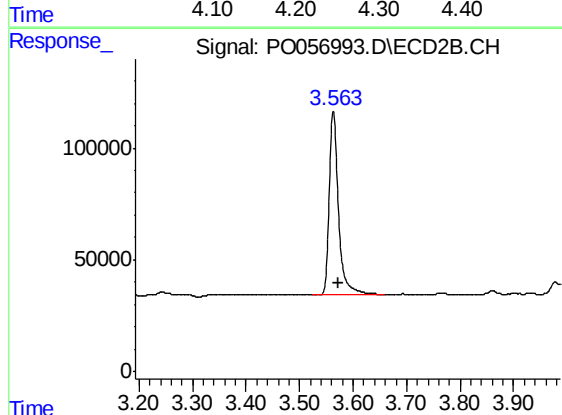


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: -0.010 min
Response: 991188
Conc: 30.06 ng/ml

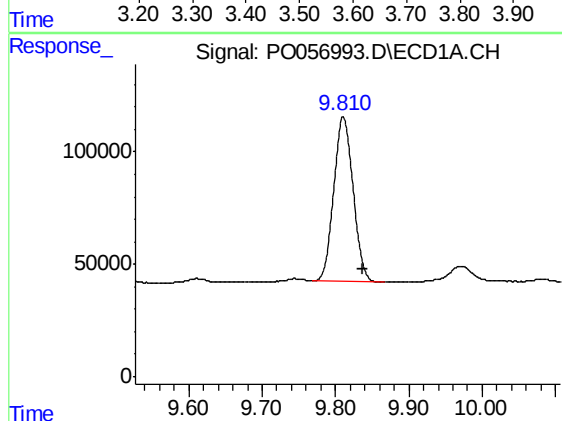

#2 Decachlorobiphenyl

R.T.: 9.811 min
Delta R.T.: -0.026 min
Response: 1343672
Conc: 27.38 ng/ml

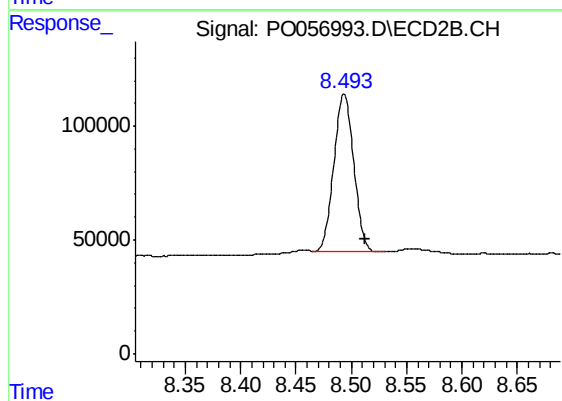

#2 Decachlorobiphenyl

R.T.: 8.493 min
Delta R.T.: -0.020 min
Response: 870205
Conc: 24.41 ng/ml m