

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060719\
 Data File : P0056995.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jun 2019 23:02
 Operator : SM/SJ
 Sample : K3242-20
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 Q115-15B

Manual Integrations
 APPROVED

Ankita
 6/10/2019 12:30:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 00:01:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.243	3.562	1123383	973822	29.344m	29.529m
2)	SA Decachlor...	9.812	8.493	1254007	811987	25.548	22.772

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO060719\
Data File : PO056995.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jun 2019 23:02
Operator : SM/SJ
Sample : K3242-20
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
Q115-15B


Manual Integrations
APPROVED

Ankita
6/10/2019 12:30:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 00:01:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

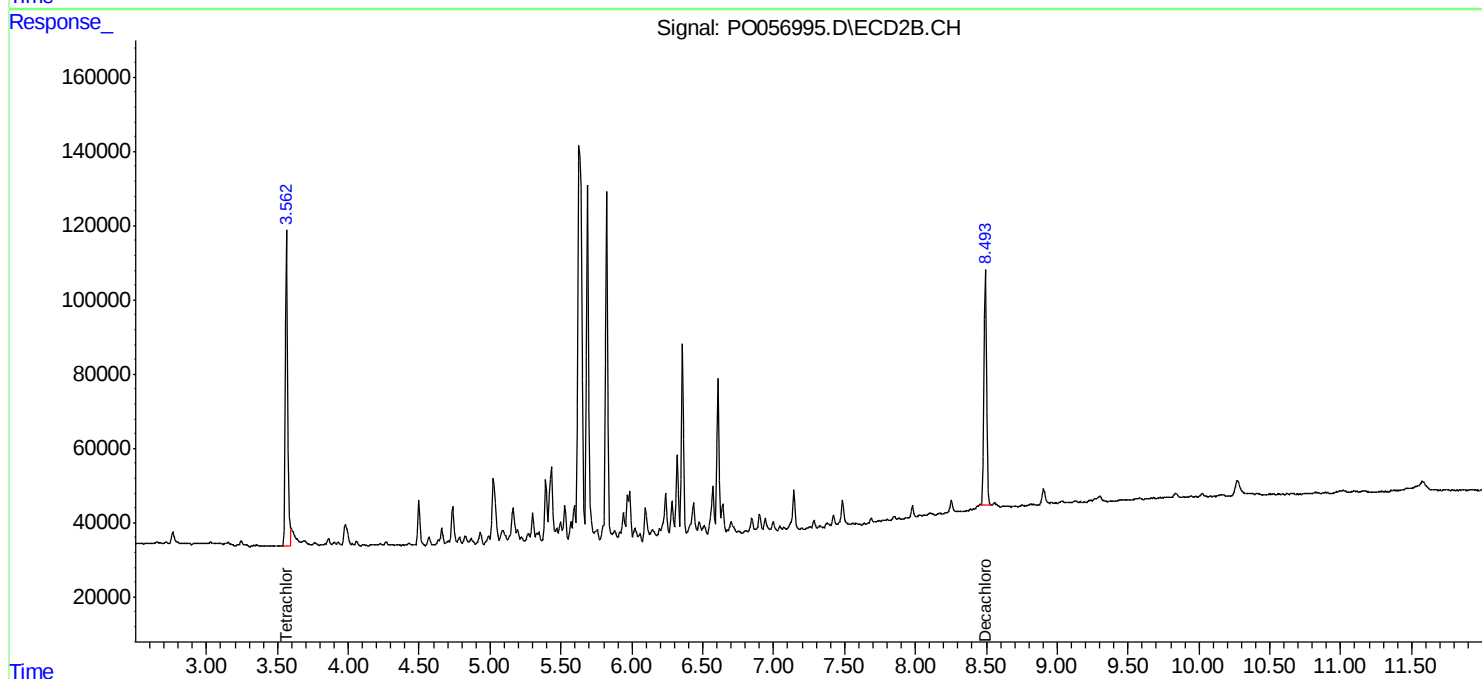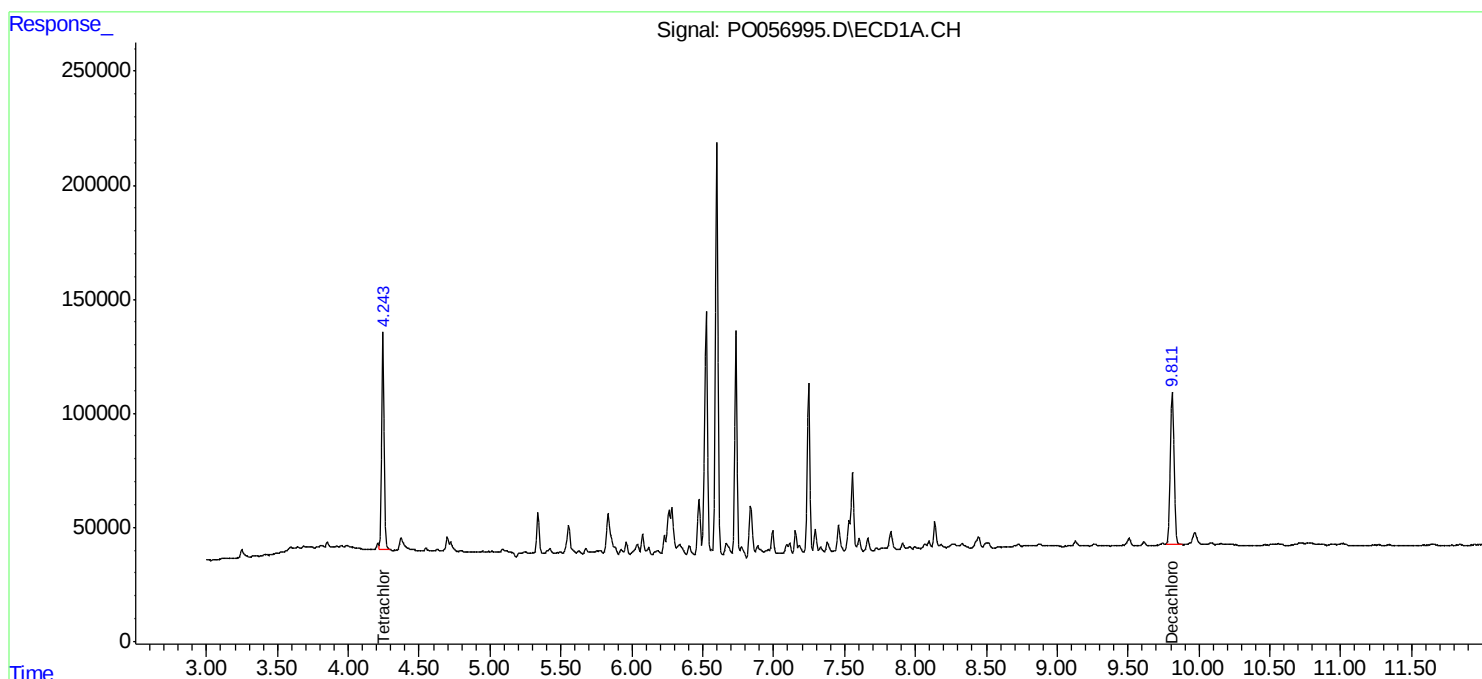

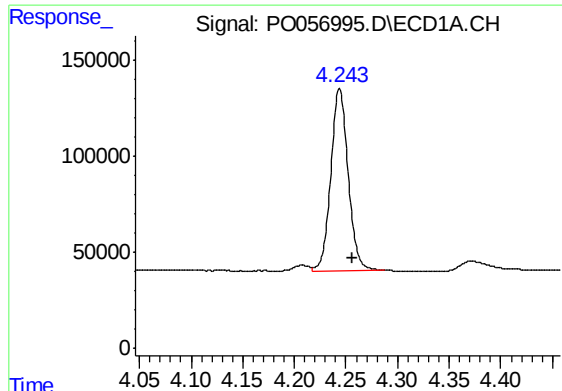


#1 Tetrachloro-m-xylene

R.T.: 4.243 min
Delta R.T.: -0.013 min
Response: 1123383
Conc: 29.34 ng/ml m

Instrument :
ECD_O
ClientSampleId :
Q115-15B


Manual Integrations
APPROVED

Ankita
6/10/2019 12:30:40 PM

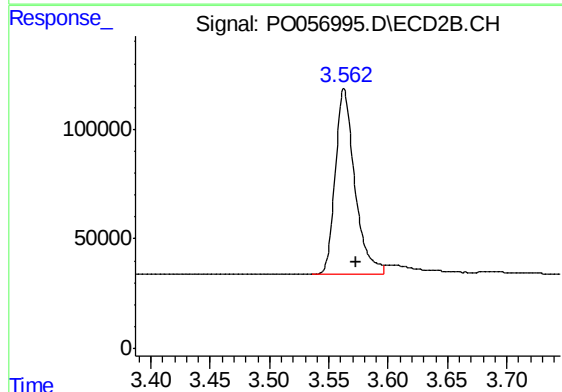


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: -0.011 min
Response: 973822
Conc: 29.53 ng/ml m

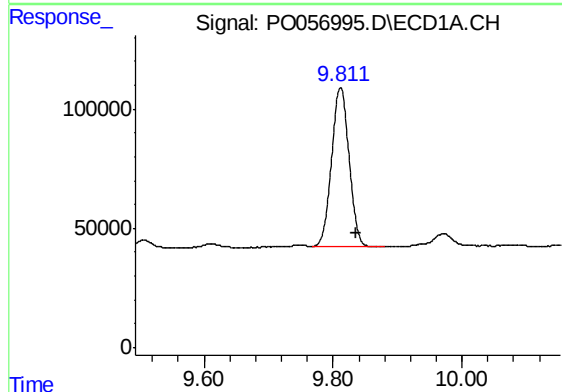

#2 Decachlorobiphenyl

R.T.: 9.812 min
Delta R.T.: -0.024 min
Response: 1254007
Conc: 25.55 ng/ml

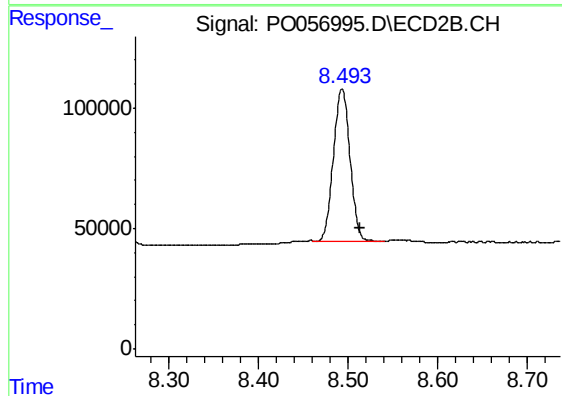

#2 Decachlorobiphenyl

R.T.: 8.493 min
Delta R.T.: -0.020 min
Response: 811987
Conc: 22.77 ng/ml