

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060719\
 Data File : P0057007.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Jun 2019 2:26
 Operator : SM/SJ
 Sample : K3268-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EFFLUENT

Manual Integrations
 APPROVED

Ankita
 6/10/2019 12:30:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 04:10:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.243	3.563	839253	720584	21.922m	21.850
2)	SA Decachlor...	9.810	8.493	1027787	676179	20.939	18.964

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO060719\
Data File : PO057007.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jun 2019 2:26
Operator : SM/SJ
Sample : K3268-02
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
EFFLUENT


Manual Integrations
APPROVED

Ankita
6/10/2019 12:30:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 04:10:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

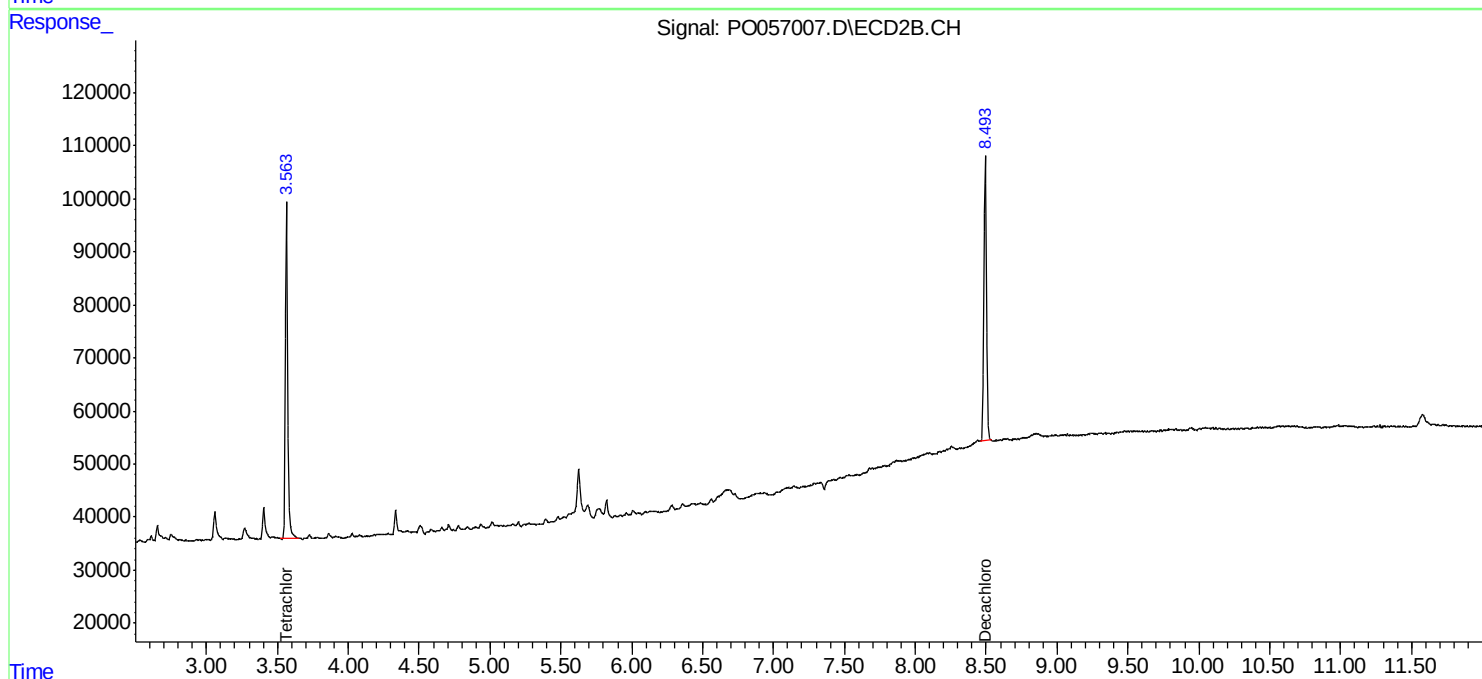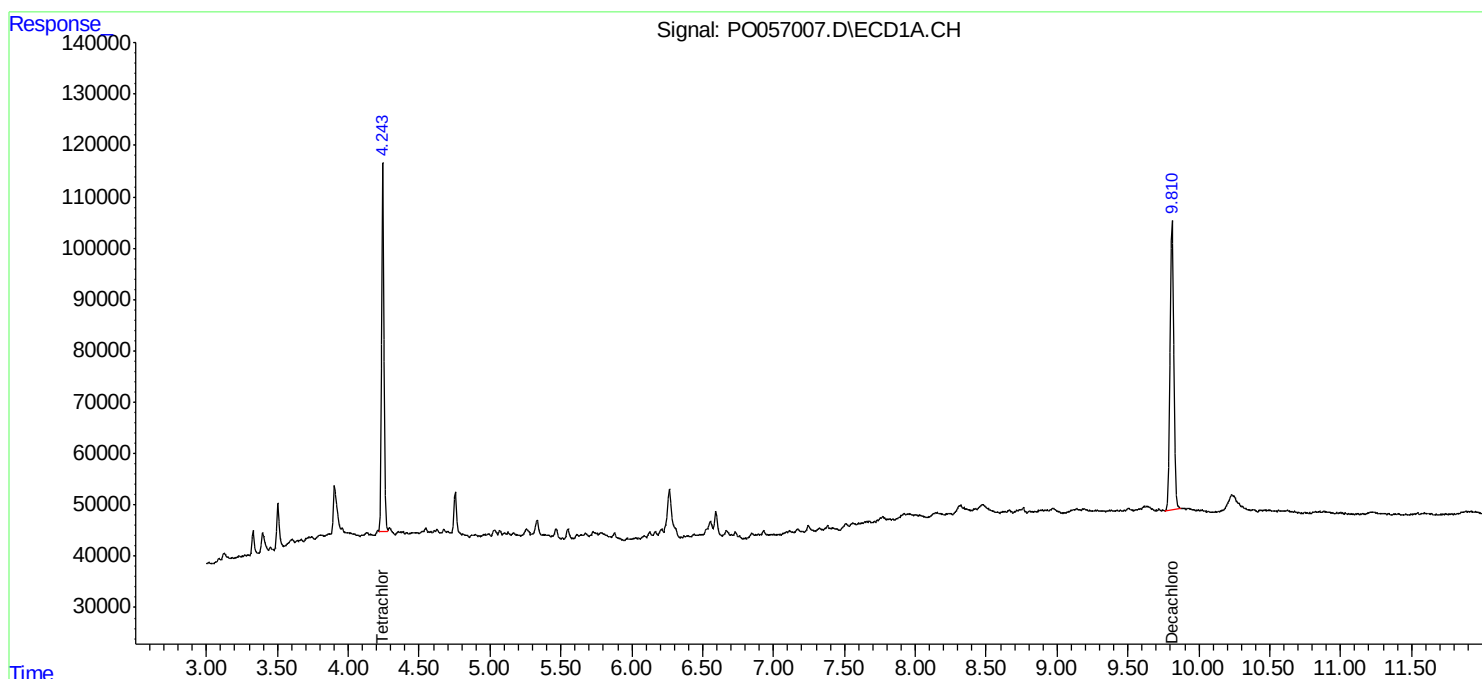

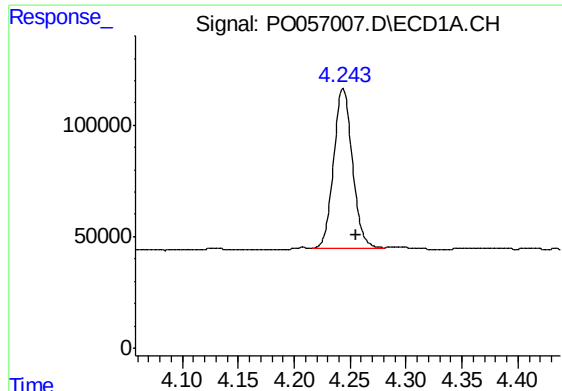


#1 Tetrachloro-m-xylene

R.T.: 4.243 min
Delta R.T.: -0.013 min
Response: 839253
Conc: 21.92 ng/ml m

Instrument :
ECD_O
ClientSampleId :
EFFLUENT


Manual Integrations
APPROVED

Ankita
6/10/2019 12:30:50 PM

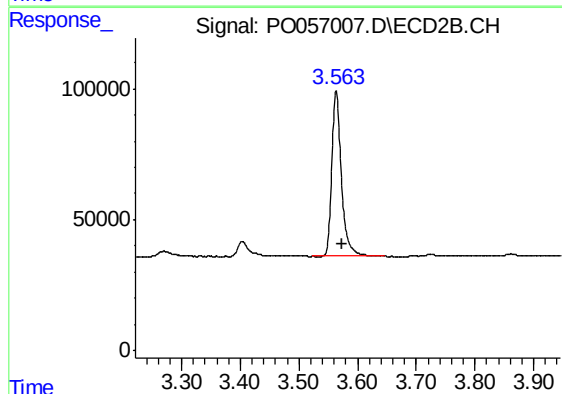


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: -0.010 min
Response: 720584
Conc: 21.85 ng/ml

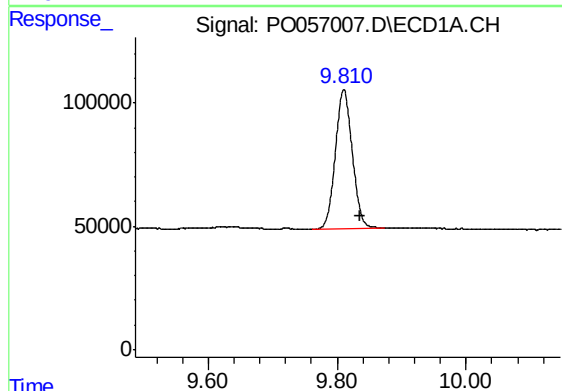

#2 Decachlorobiphenyl

R.T.: 9.810 min
Delta R.T.: -0.026 min
Response: 1027787
Conc: 20.94 ng/ml

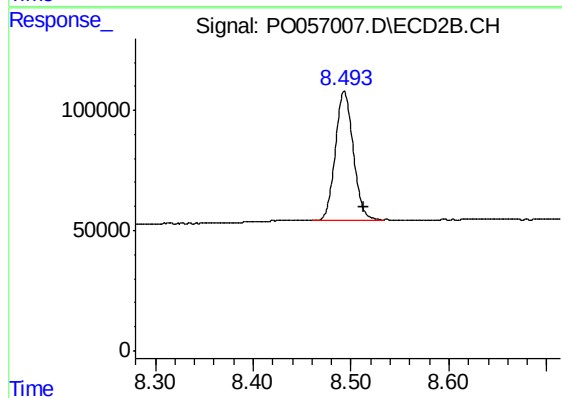

#2 Decachlorobiphenyl

R.T.: 8.493 min
Delta R.T.: -0.020 min
Response: 676179
Conc: 18.96 ng/ml