

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0060818\
Data File : P0045639.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jun 2018 9:18
Operator : SM/UA
Sample : J3304-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FS-CON

Manual Integrations
APPROVED

UGO
6/9/2018 11:35:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 11:41:01 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.989	3.266	4422672	6199424	21.174	22.357
2) SA Decachlor...	9.258	7.983	4796245	5574484	20.883m	19.779

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060818\
Data File : P0045639.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jun 2018 9:18
Operator : SM/UA
Sample : J3304-04
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FS-CON


Manual Integrations
APPROVED

UGO
6/9/2018 11:35:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 11:41:01 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_O\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

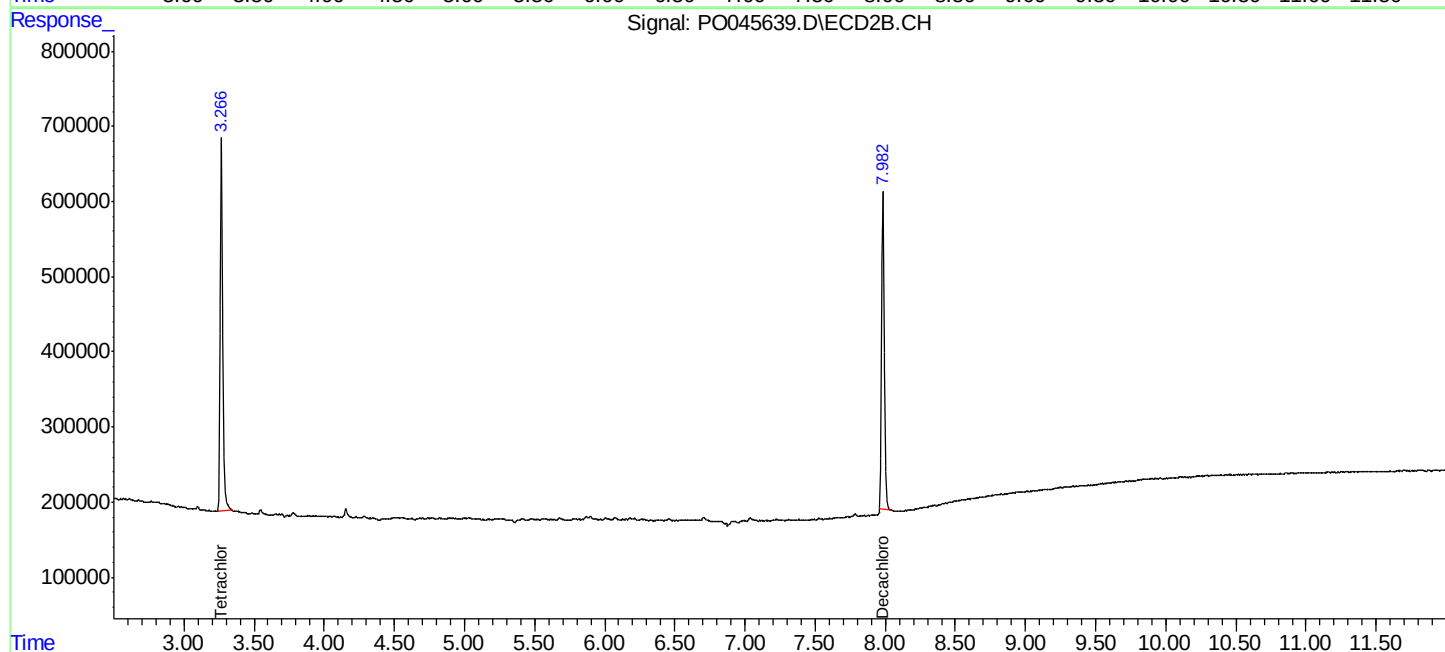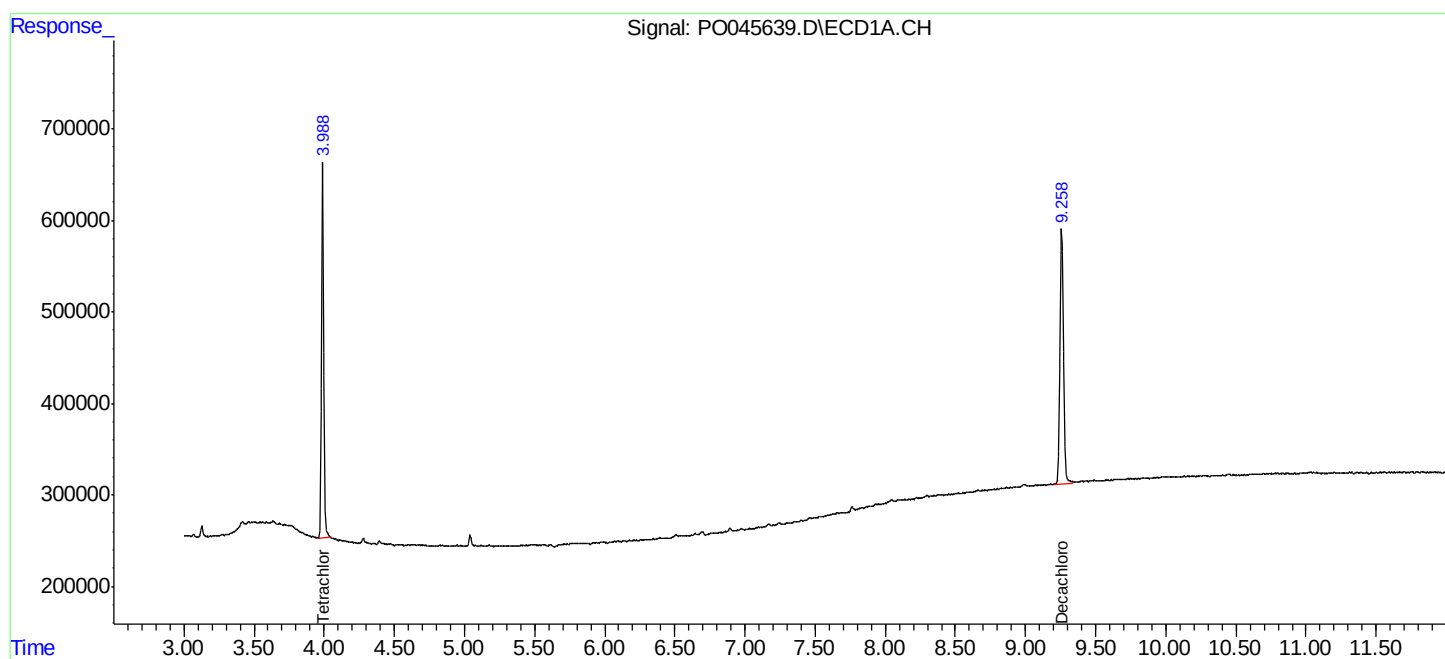

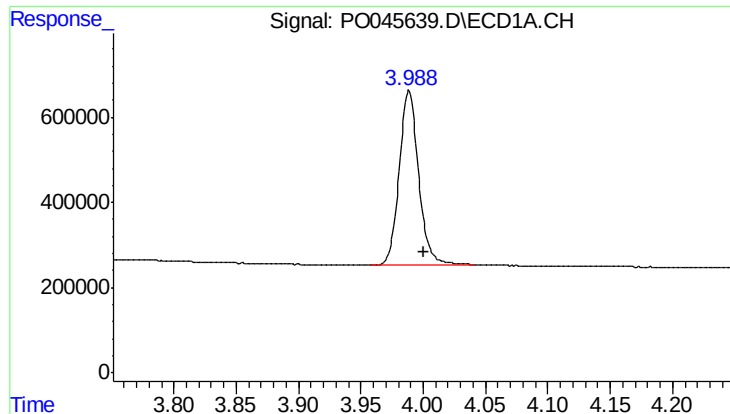


#1 Tetrachloro-m-xylene

R.T.: 3.989 min
Delta R.T.: -0.012 min
Response: 4422672
Conc: 21.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
FS-CON


Manual Integrations
APPROVED

UGO
6/9/2018 11:35:03 AM

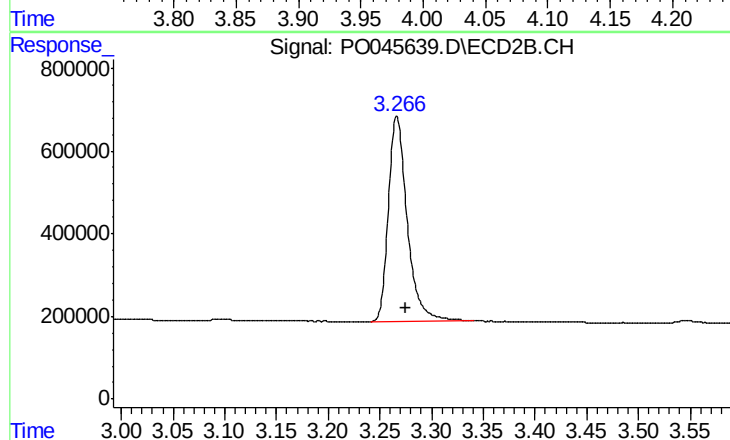


#1 Tetrachloro-m-xylene

R.T.: 3.266 min
Delta R.T.: -0.009 min
Response: 6199424
Conc: 22.36 ng/ml

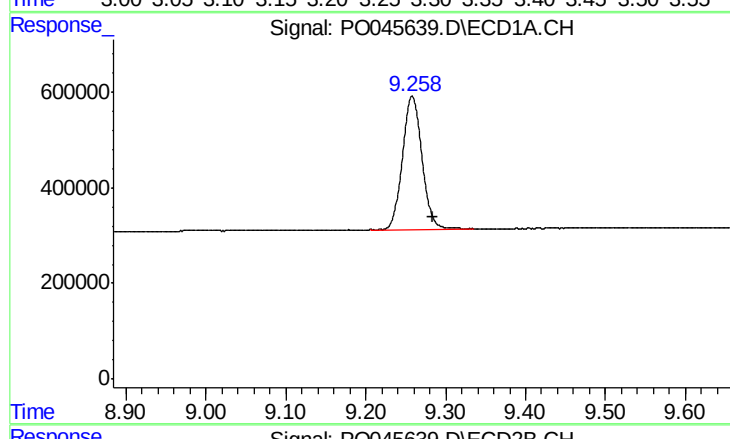

#2 Decachlorobiphenyl

R.T.: 9.258 min
Delta R.T.: -0.026 min
Response: 4796245
Conc: 20.88 ng/ml m

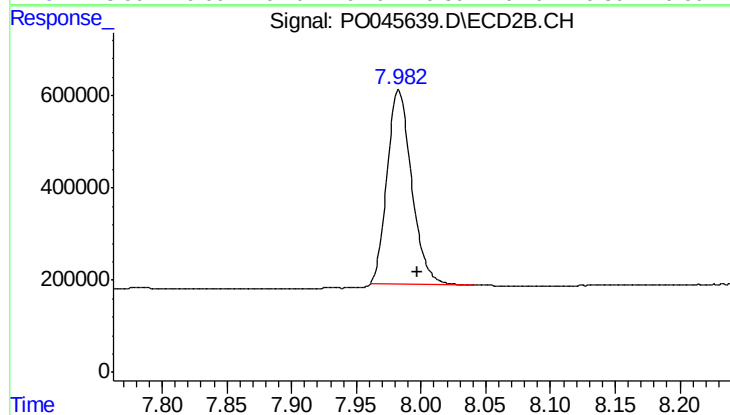

#2 Decachlorobiphenyl

R.T.: 7.983 min
Delta R.T.: -0.015 min
Response: 5574484
Conc: 19.78 ng/ml