

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0060818\
 Data File : P0045650.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jun 2018 12:09
 Operator : SM/UA
 Sample : PB109969BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB109969BL

Manual Integrations
 APPROVED

UGO
 6/9/2018 11:35:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 01:50:30 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_0\methods\P0053018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 31 04:53:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.988	3.267	4319064	5667164	20.678	20.438
2) SA Decachlor...	9.253	7.980	4055134	4859477	17.656m	17.242m

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060818\
Data File : P0045650.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jun 2018 12:09
Operator : SM/UA
Sample : PB109969BL
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB109969BL


Manual Integrations
APPROVED

UGO
6/9/2018 11:35:43 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 01:50:30 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_O\methods\P0053018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 31 04:53:22 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

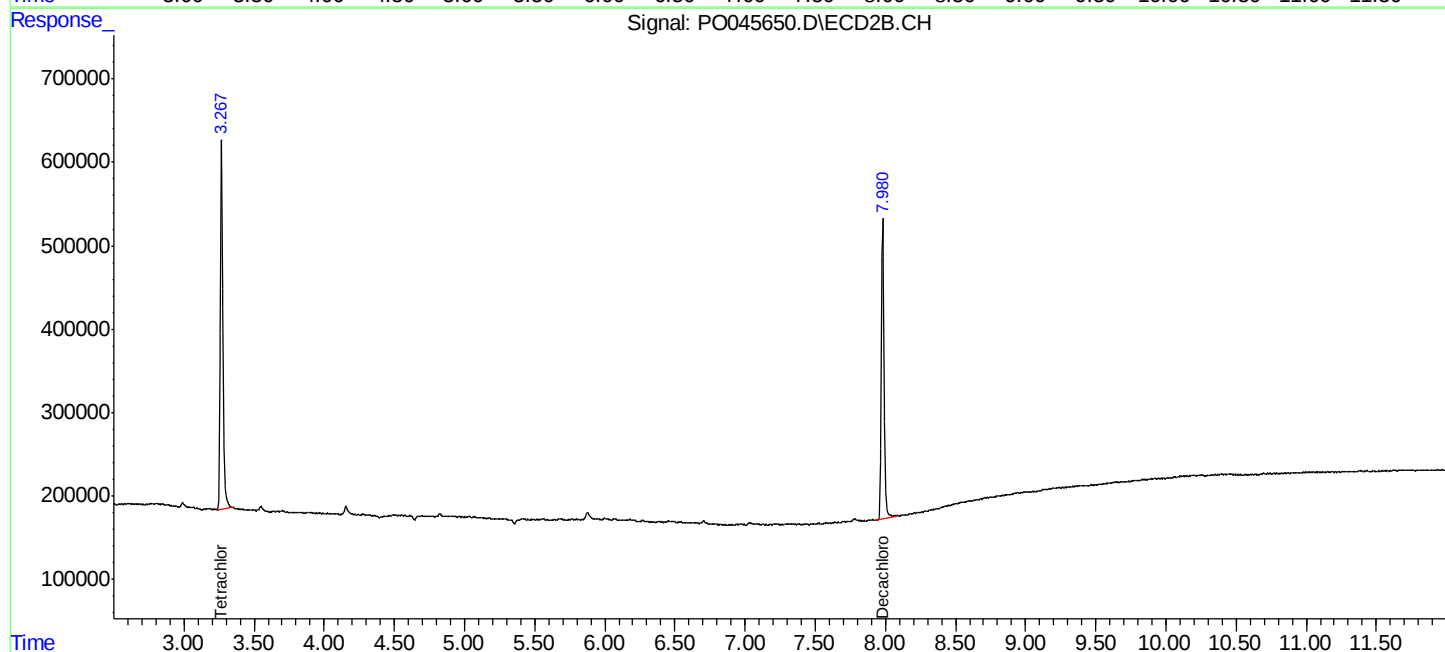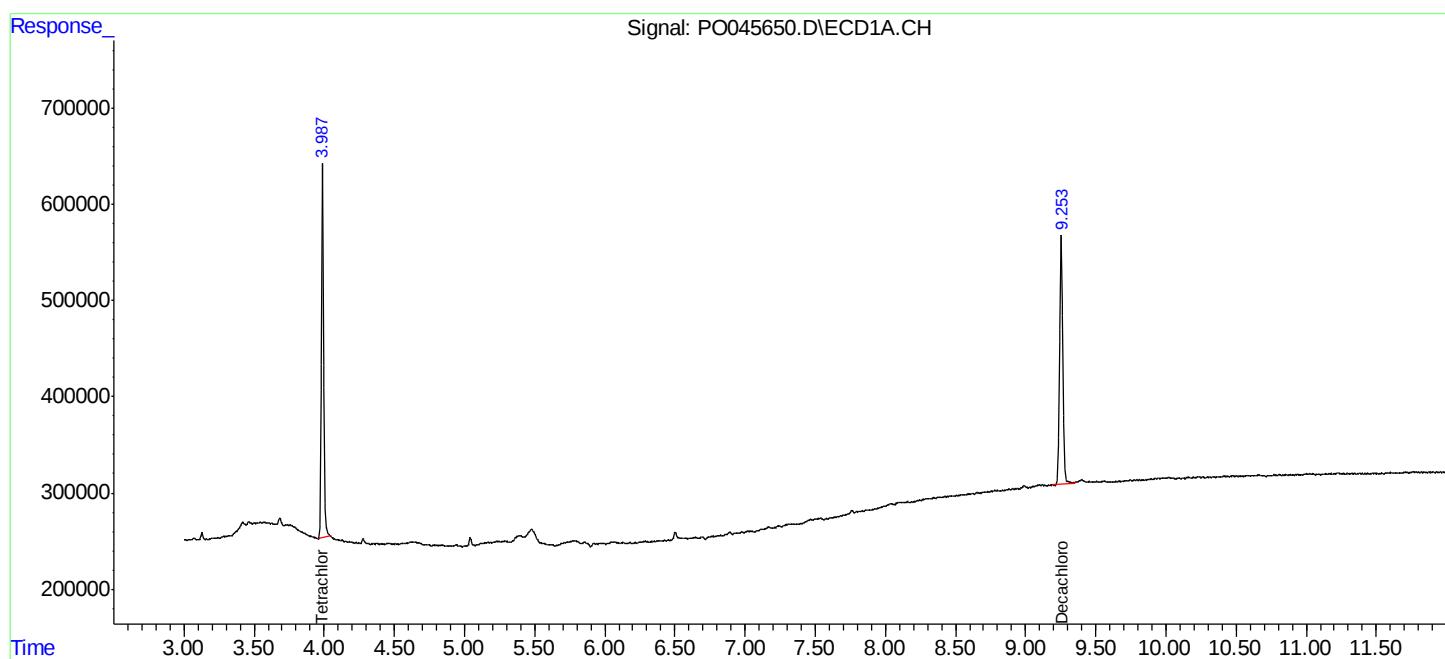

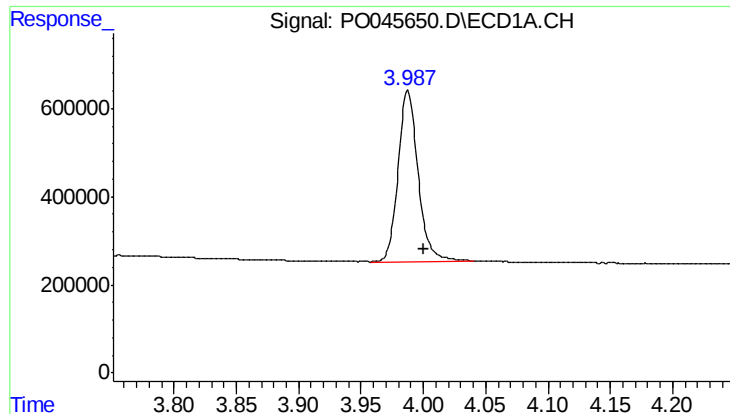


#1 Tetrachloro-m-xylene

R.T.: 3.988 min
Delta R.T.: -0.013 min
Response: 4319064
Conc: 20.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB109969BL


Manual Integrations
APPROVED

UGO
6/9/2018 11:35:43 AM

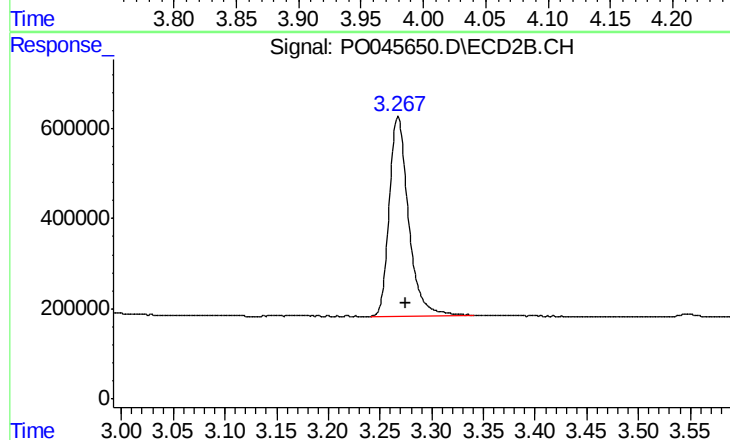


#1 Tetrachloro-m-xylene

R.T.: 3.267 min
Delta R.T.: -0.008 min
Response: 5667164
Conc: 20.44 ng/ml

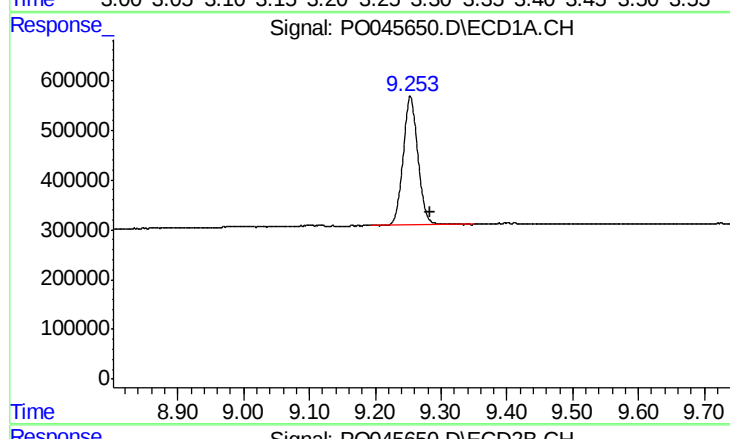

#2 Decachlorobiphenyl

R.T.: 9.253 min
Delta R.T.: -0.031 min
Response: 4055134
Conc: 17.66 ng/ml m

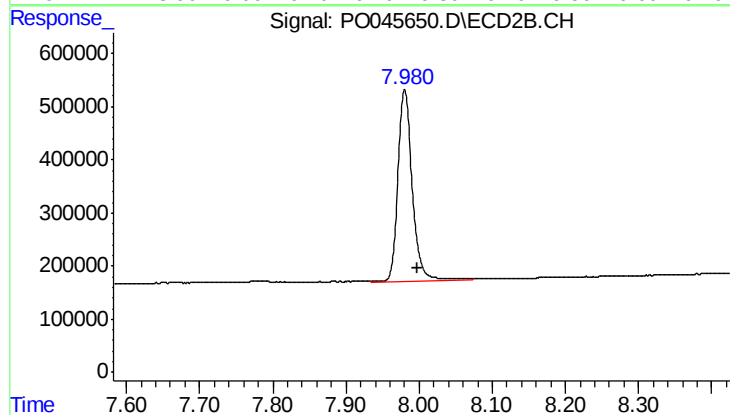

#2 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: -0.018 min
Response: 4859477
Conc: 17.24 ng/ml m