

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0061218\
Data File : P0045731.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jun 2018 20:50
Operator : SM/UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 04:33:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061218.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 13 03:54:48 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.389	3.626	5697872	3231136	29.241	28.427
2) SA Decachlor...	10.043	8.609	4809577	2272364	34.353	32.496

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061218\
Data File : P0045731.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jun 2018 20:50
Operator : SM/UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 04:33:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061218.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 13 03:54:48 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

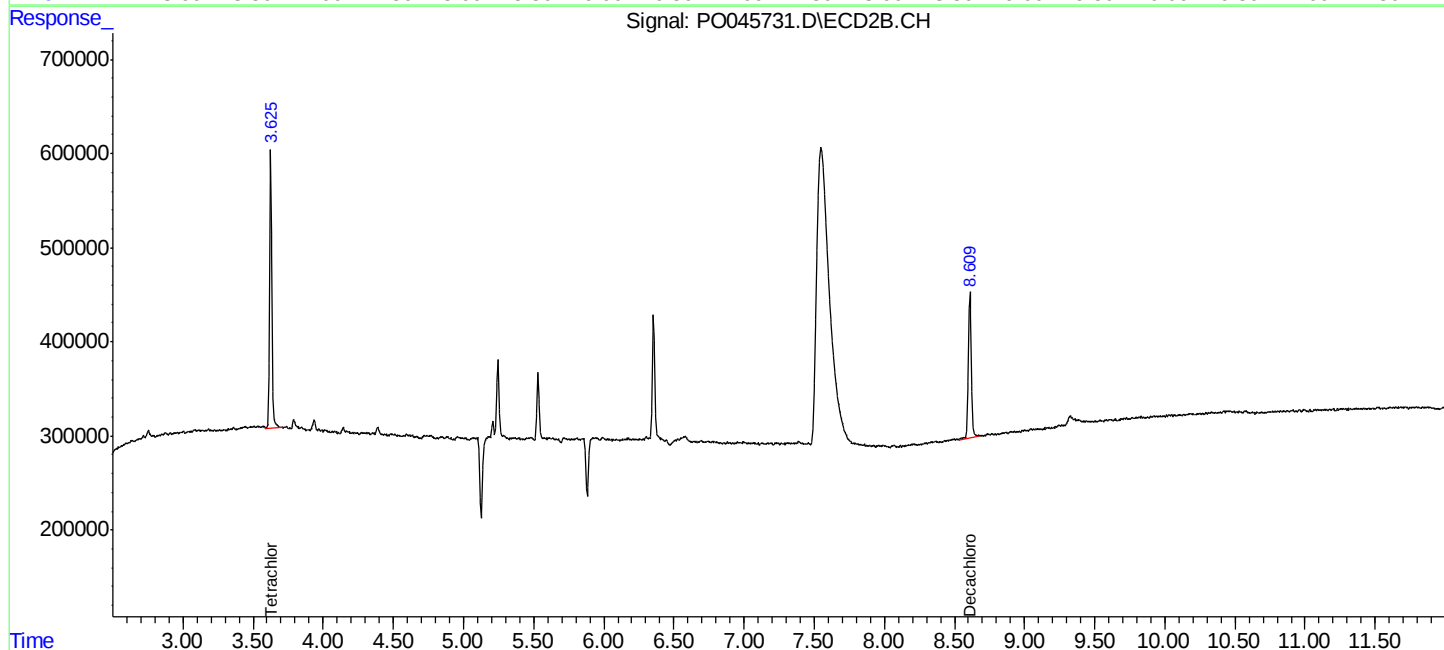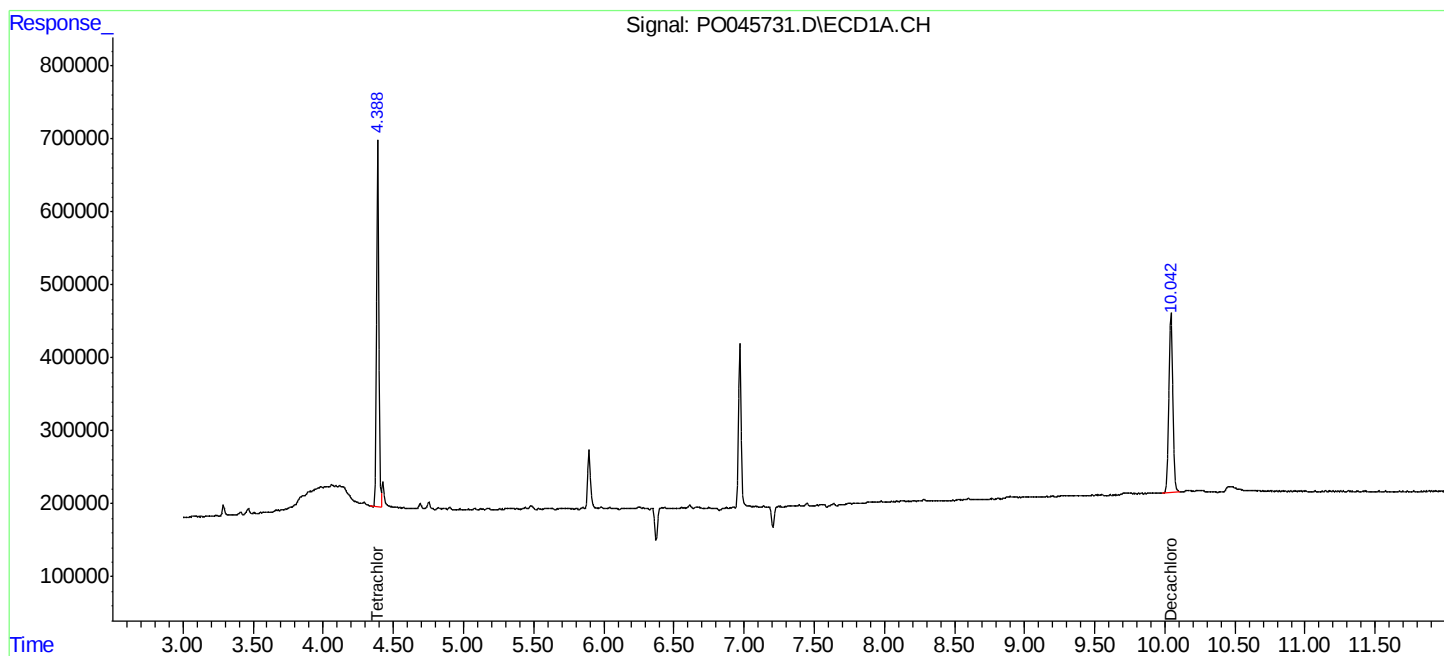


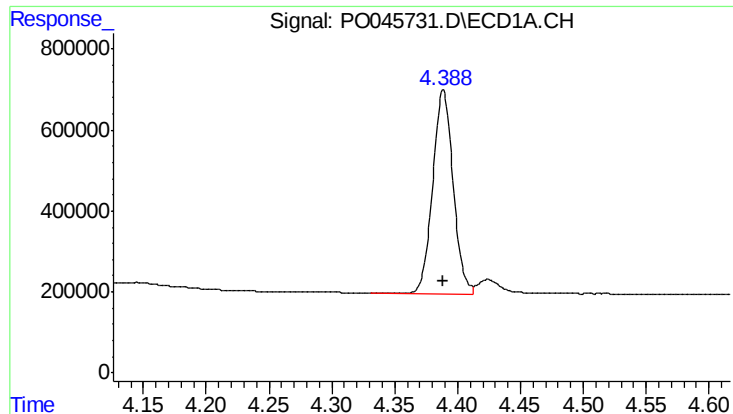

#1 Tetrachloro-m-xylene


R.T.: 4.389 min
Delta R.T.: 0.000 min
Response: 5697872
Conc: 29.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

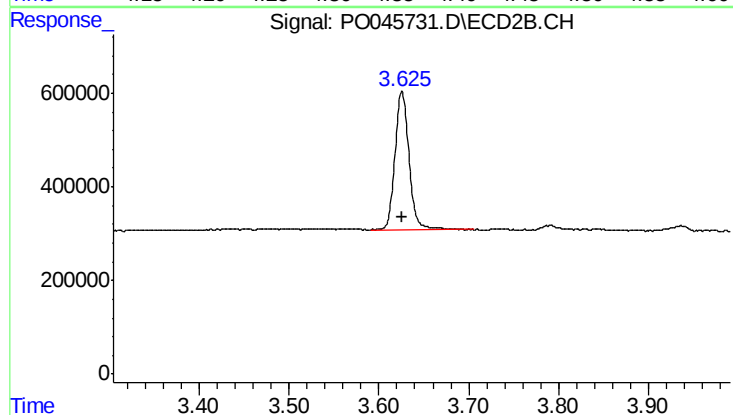


#1 Tetrachloro-m-xylene

R.T.: 3.626 min
Delta R.T.: 0.000 min
Response: 3231136
Conc: 28.43 ng/ml

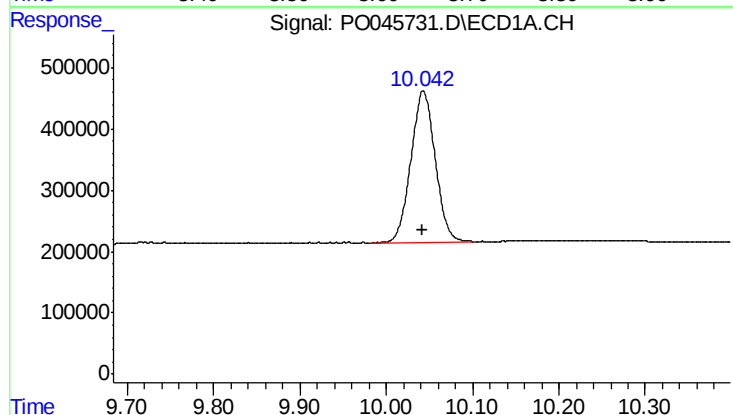

#2 Decachlorobiphenyl

R.T.: 10.043 min
Delta R.T.: 0.001 min
Response: 4809577
Conc: 34.35 ng/ml

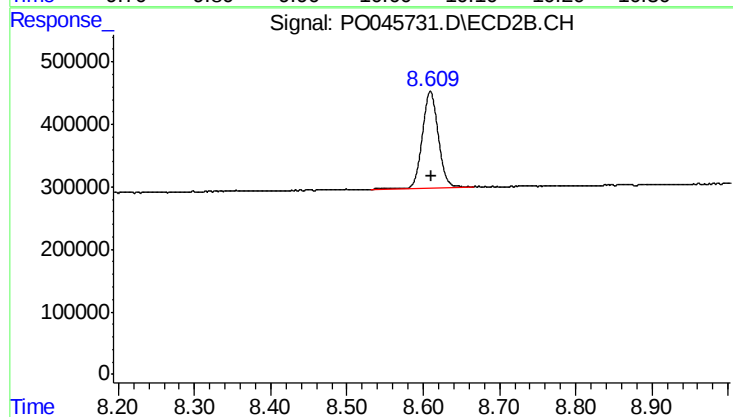

#2 Decachlorobiphenyl

R.T.: 8.609 min
Delta R.T.: -0.002 min
Response: 2272364
Conc: 32.50 ng/ml