

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061219\
 Data File : P0057095.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jun 2019 13:32
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 00:44:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.253	3.561	759445	605311	19.837	18.355
2)	SA Decachlor...	9.824	8.492	977858	640817	19.922	17.972
Target Compounds							
7)	L1 AR-1016-5	0.000	5.047	0	5044	N.D.	4.702 #
15)	L3 AR-1232-5	0.000	5.047	0	5044	N.D.	8.955 #
20)	L4 AR-1242-5	0.000	5.445	0	22653	N.D.	19.160 #
24)	L5 AR-1248-4	0.000	5.047	0	5044	N.D.	3.185 #
25)	L5 AR-1248-5	0.000	5.445	0	22653	N.D.	13.687 #
26)	L6 AR-1254-1	0.000	5.445	0	22653	N.D.	8.565 #
29)	L6 AR-1254-4	0.000	6.278	0	25577	N.D.	11.642 #
32)	L7 AR-1260-2	0.000	6.278	0	25577	N.D.	10.376 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061219\
Data File : PO057095.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jun 2019 13:32
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 00:44:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

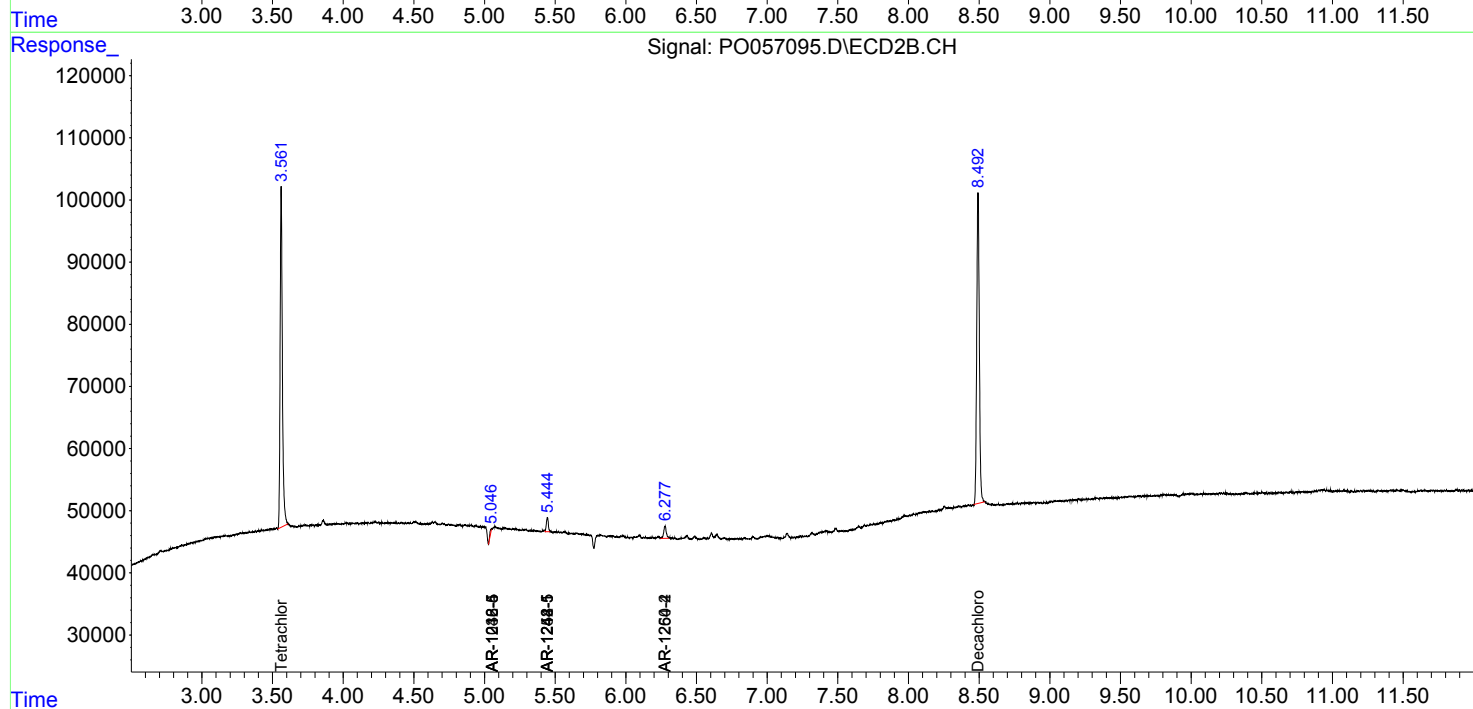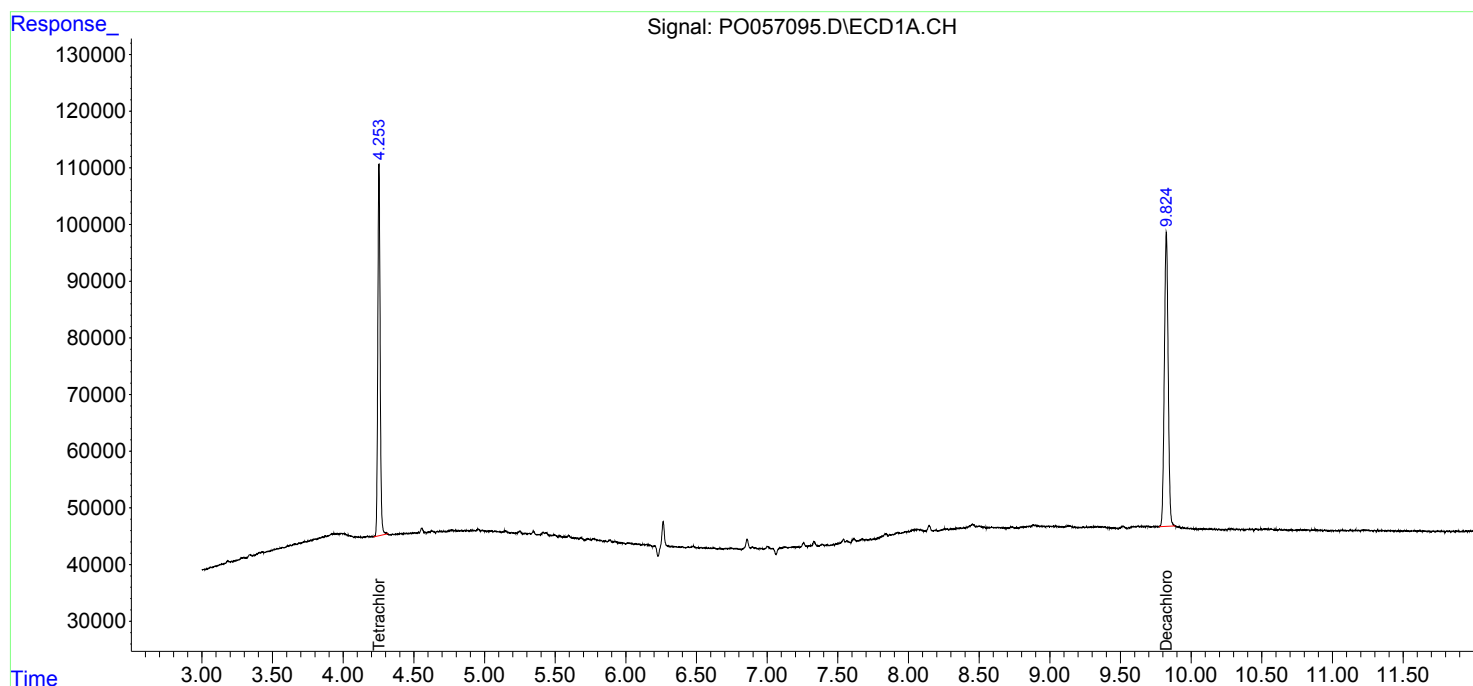


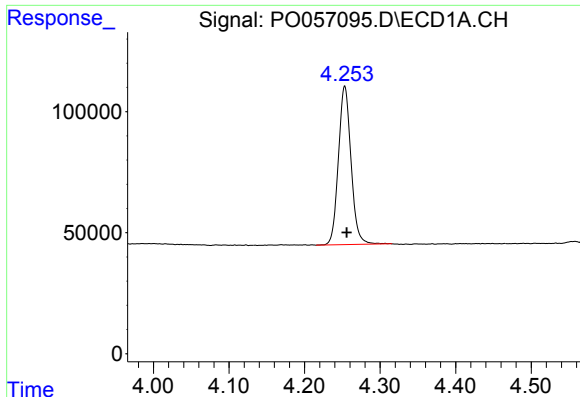

#1 Tetrachloro-m-xylene


R.T.: 4.253 min
Delta R.T.: -0.003 min
Response: 759445
Conc: 19.84 ng/ml

Instrument :
ECD_O
ClientSampleId :

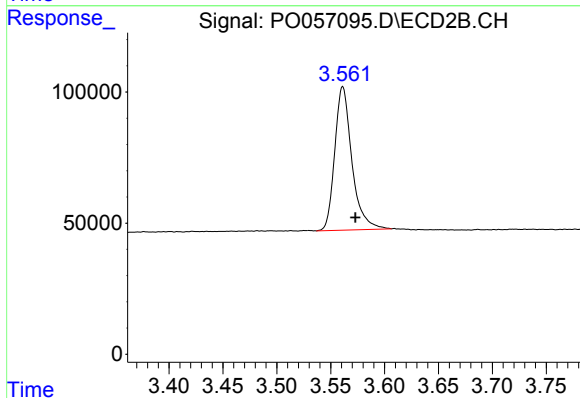


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: -0.012 min
Response: 605311
Conc: 18.35 ng/ml

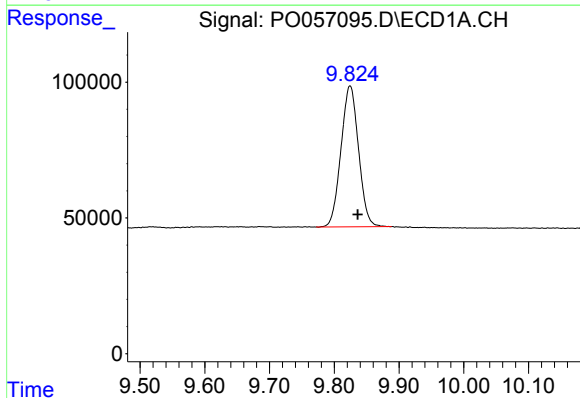


#2 Decachlorobiphenyl

R.T.: 9.824 min
Delta R.T.: -0.012 min
Response: 977858
Conc: 19.92 ng/ml

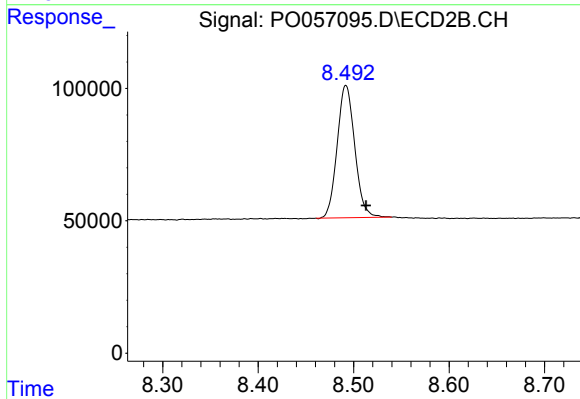

#2 Decachlorobiphenyl


R.T.: 8.492 min
Delta R.T.: -0.021 min
Response: 640817
Conc: 17.97 ng/ml

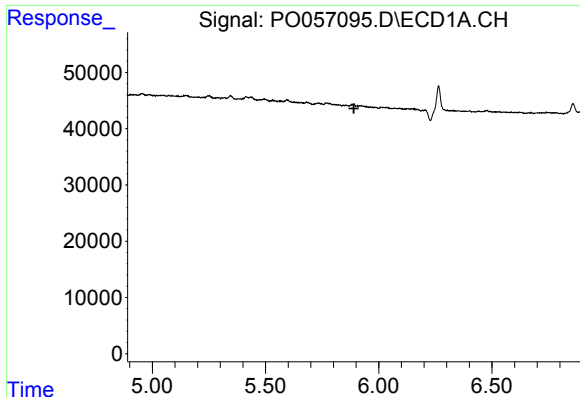

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.890 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

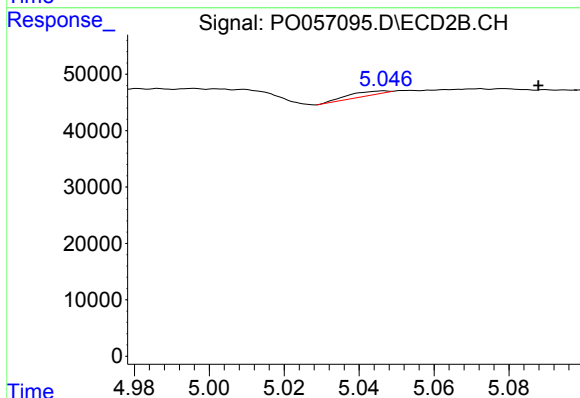


#7 AR-1016-5

R.T.: 5.047 min
Delta R.T.: -0.041 min
Response: 5044
Conc: 4.70 ng/ml

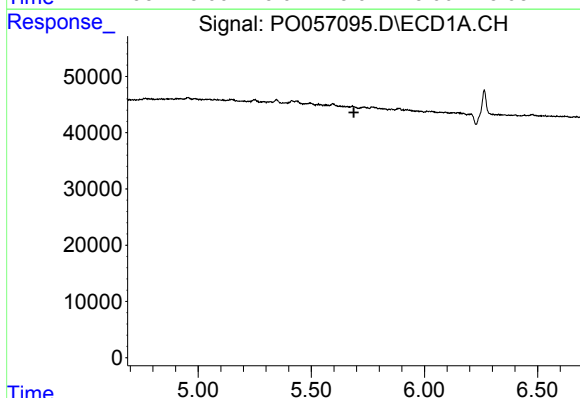


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 5.688 min
Response: 0
Conc: N.D.

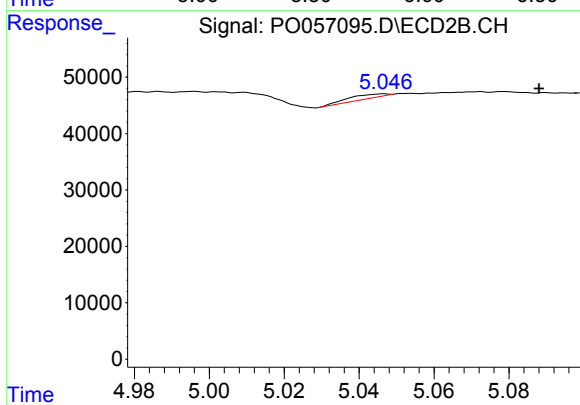

#15 AR-1232-5


R.T.: 5.047 min
Delta R.T.: -0.041 min
Response: 5044
Conc: 8.96 ng/ml

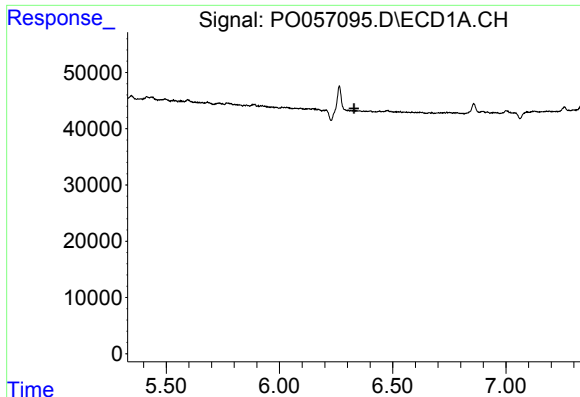

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 6.329 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

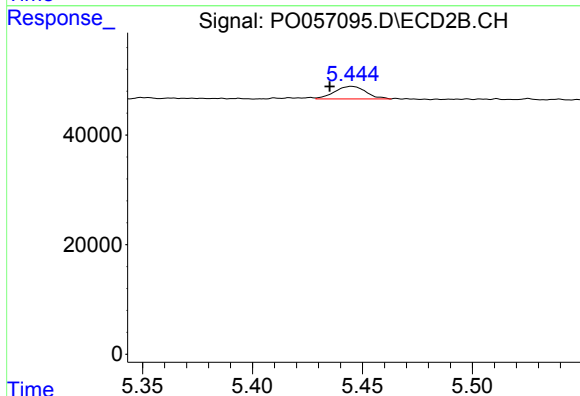


#20 AR-1242-5

R.T.: 5.445 min
Delta R.T.: 0.010 min
Response: 22653
Conc: 19.16 ng/ml

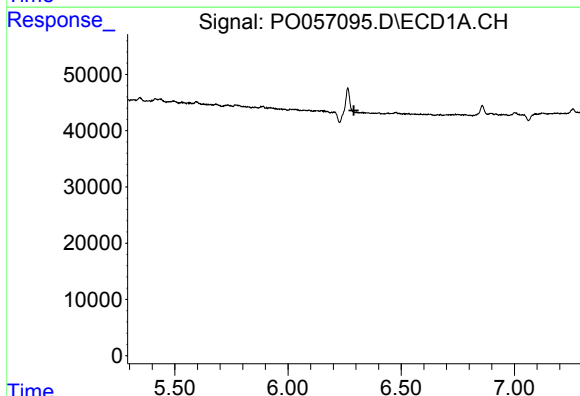


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 6.291 min
Response: 0
Conc: N.D.

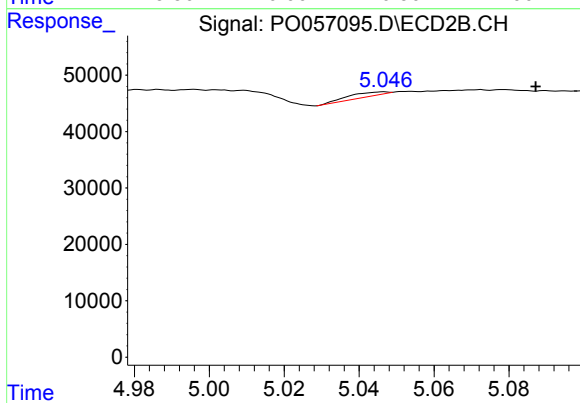

#24 AR-1248-4


R.T.: 5.047 min
Delta R.T.: -0.040 min
Response: 5044
Conc: 3.19 ng/ml

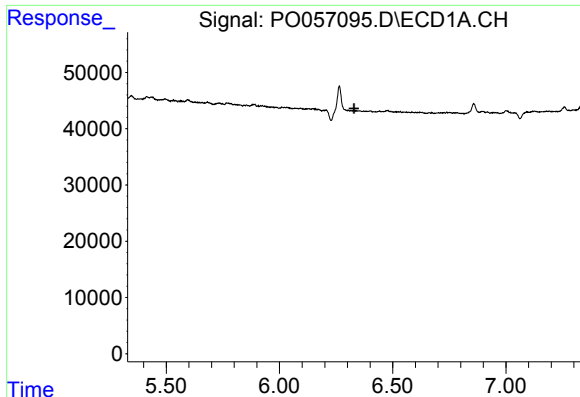

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.329 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

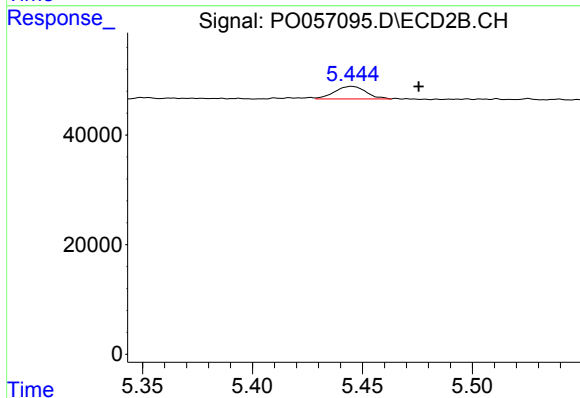


#25 AR-1248-5

R.T.: 5.445 min
Delta R.T.: -0.031 min
Response: 22653
Conc: 13.69 ng/ml

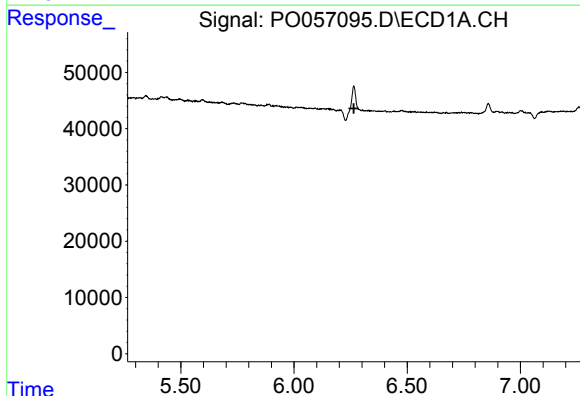


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.264 min
Response: 0
Conc: N.D.

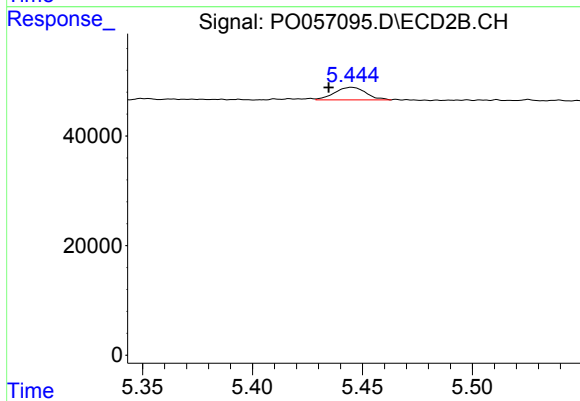

#26 AR-1254-1


R.T.: 5.445 min
Delta R.T.: 0.010 min
Response: 22653
Conc: 8.57 ng/ml

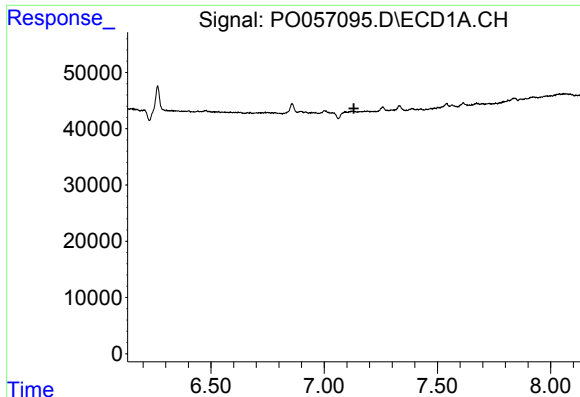

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 7.131 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

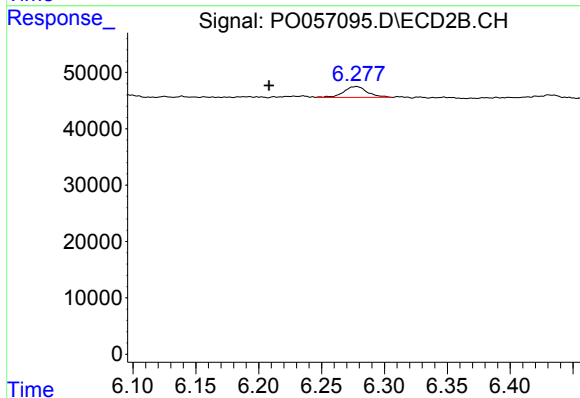


#29 AR-1254-4

R.T.: 6.278 min
Delta R.T.: 0.070 min
Response: 25577
Conc: 11.64 ng/ml

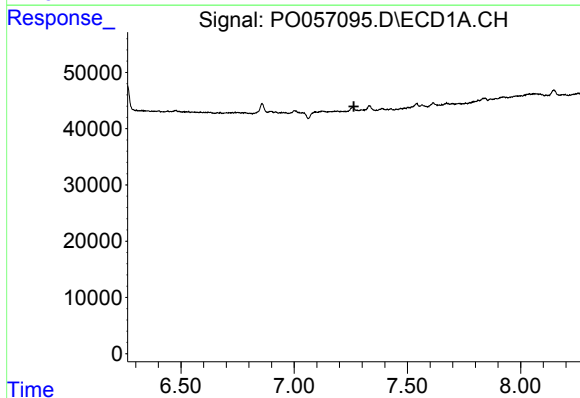

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.264 min
Response: 0
Conc: N.D.

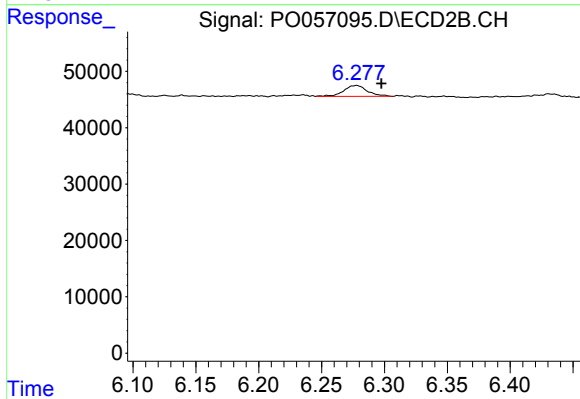

#32 AR-1260-2

R.T.: 6.278 min
Delta R.T.: -0.020 min
Response: 25577
Conc: 10.38 ng/ml