

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061219\
 Data File : P0057100.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jun 2019 15:47
 Operator : SM/SJ
 Sample : K3265-13
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MW-01

Manual Integrations
 APPROVED

Ankita
 6/13/2019 10:20:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 00:46:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.239	3.560	630197	511993	16.461m	15.525
2)	SA Decachlor...	9.803	8.488	910680	590105	18.554	16.550

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061219\
Data File : PO057100.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jun 2019 15:47
Operator : SM/SJ
Sample : K3265-13
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MW-01


Manual Integrations
APPROVED

Ankita
6/13/2019 10:20:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 00:46:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

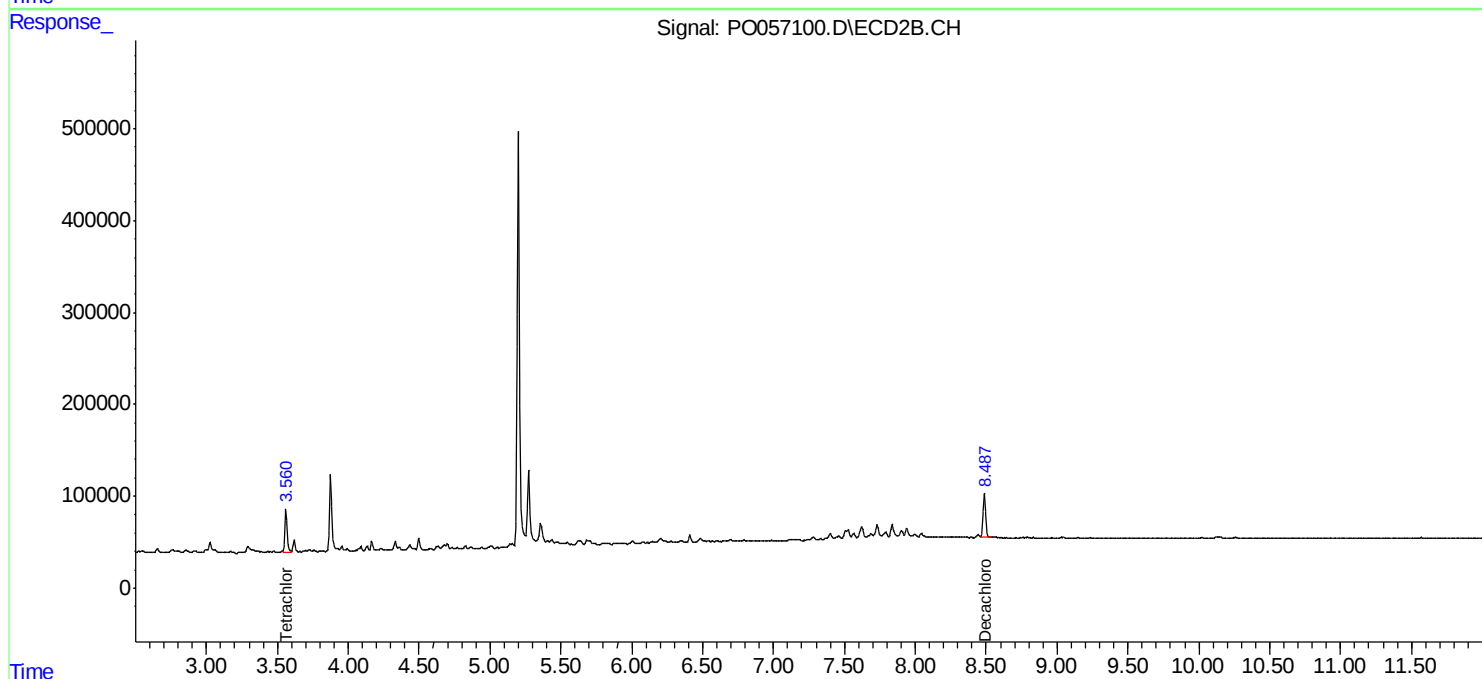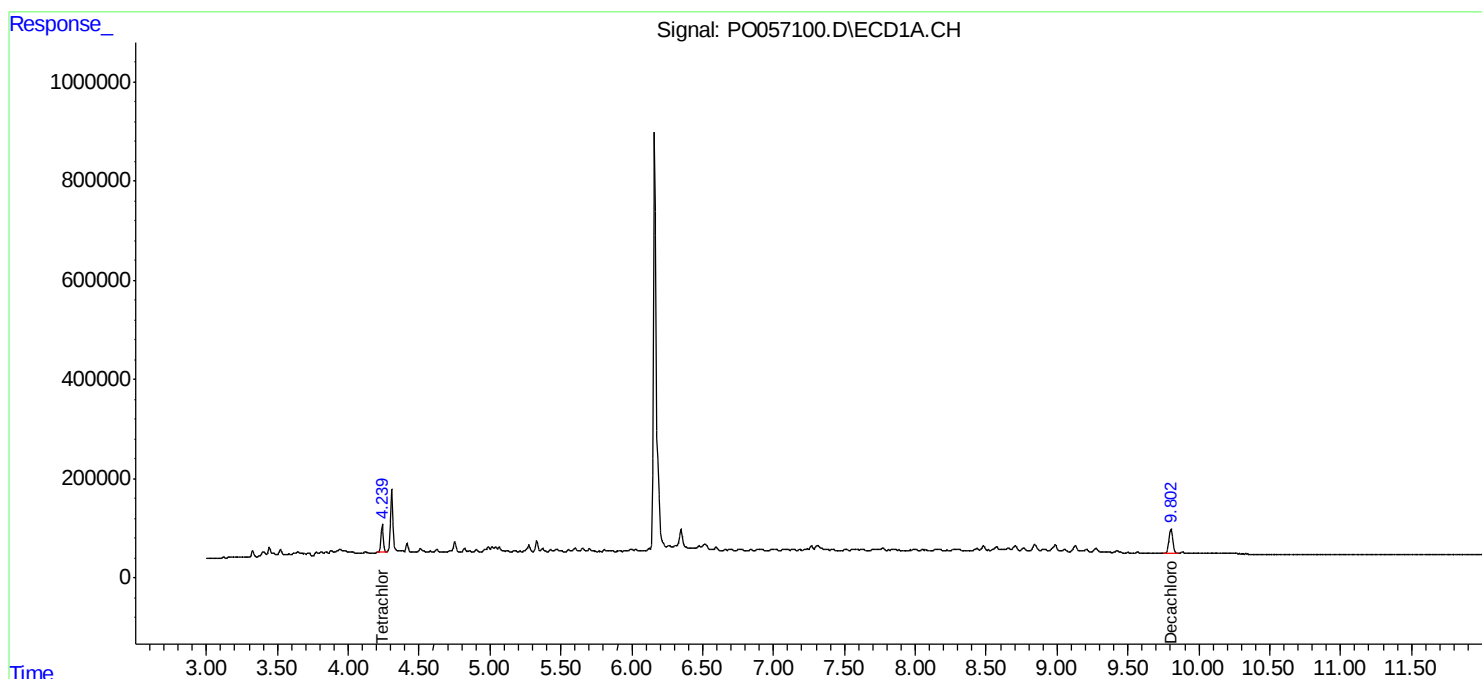

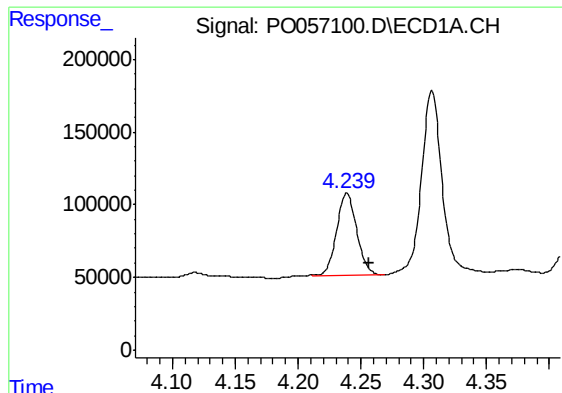


#1 Tetrachloro-m-xylene

R.T.: 4.239 min
Delta R.T.: -0.017 min
Response: 630197
Conc: 16.46 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MW-01


Manual Integrations
APPROVED

Ankita
6/13/2019 10:20:54 AM

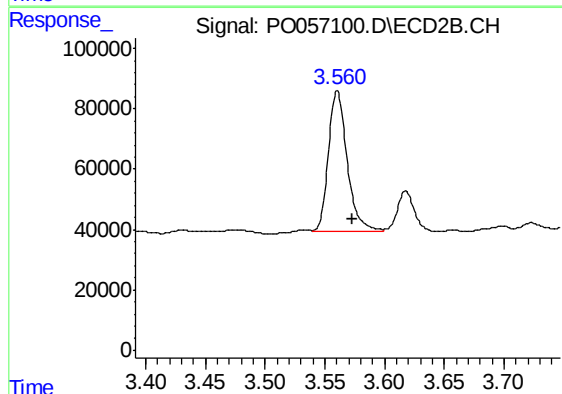


#1 Tetrachloro-m-xylene

R.T.: 3.560 min
Delta R.T.: -0.013 min
Response: 511993
Conc: 15.53 ng/ml

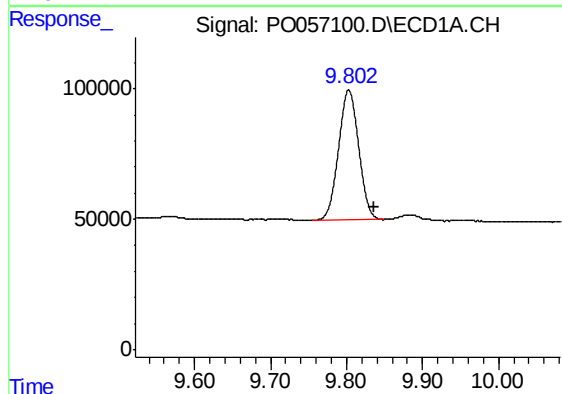

#2 Decachlorobiphenyl

R.T.: 9.803 min
Delta R.T.: -0.033 min
Response: 910680
Conc: 18.55 ng/ml

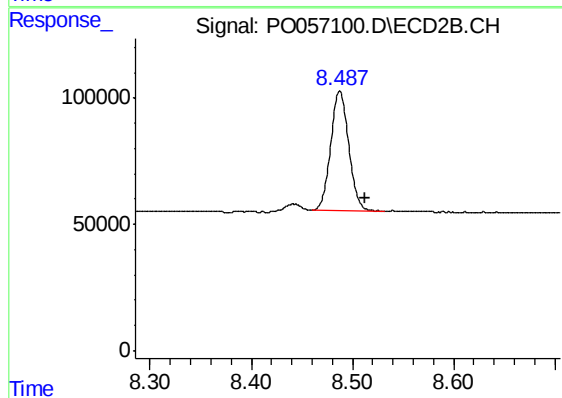

#2 Decachlorobiphenyl

R.T.: 8.488 min
Delta R.T.: -0.025 min
Response: 590105
Conc: 16.55 ng/ml