

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061219\
 Data File : P0057101.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jun 2019 16:08
 Operator : SM/SJ
 Sample : K3299-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TI-658

Manual Integrations
 APPROVED

Ankita
 6/13/2019 10:20:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 00:47:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.247	3.559	549564	511641	14.355m	15.514m
2)	SA Decachlor...	9.810	8.490	284947	171826	5.805m	4.819

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061219\
Data File : P0057101.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jun 2019 16:08
Operator : SM/SJ
Sample : K3299-04
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TI-658


Manual Integrations
APPROVED

Ankita
6/13/2019 10:20:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 00:47:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

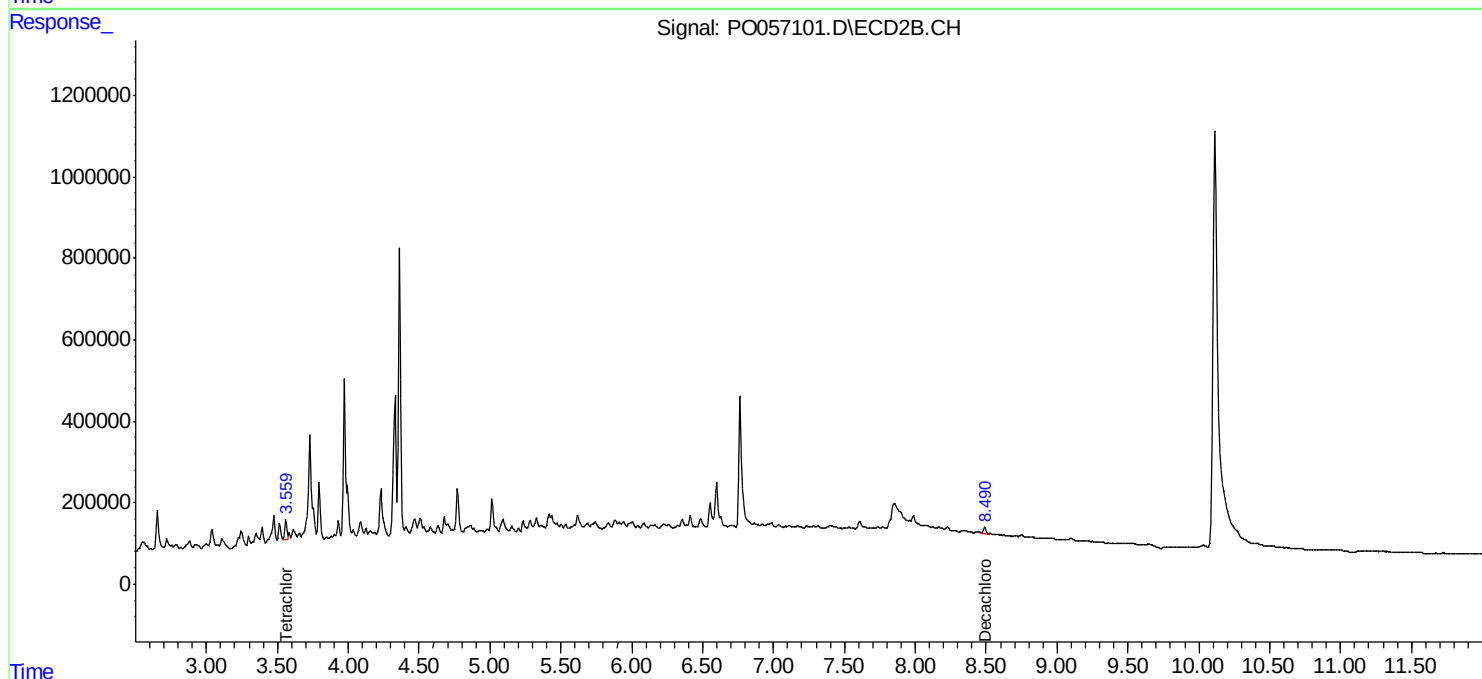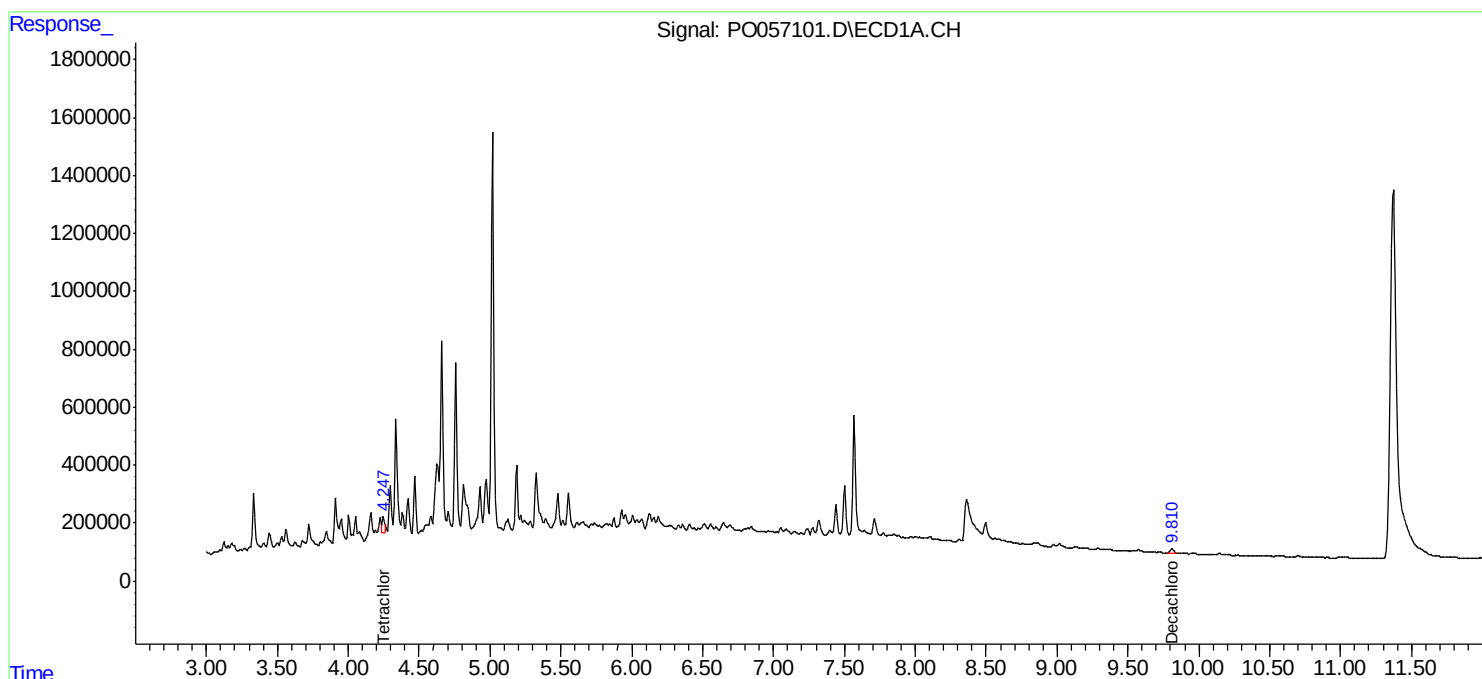

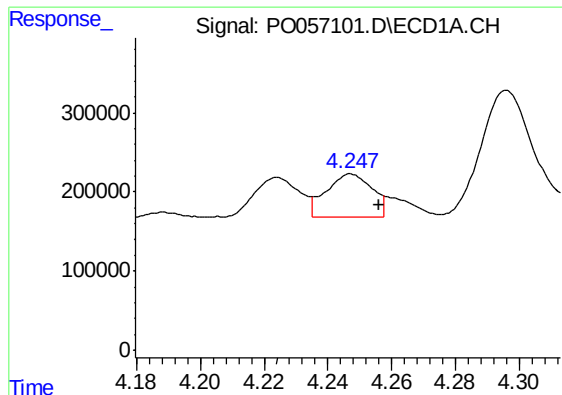


#1 Tetrachloro-m-xylene

R.T.: 4.247 min
Delta R.T.: -0.009 min
Response: 549564
Conc: 14.36 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TI-658


Manual Integrations
APPROVED

Ankita
6/13/2019 10:20:56 AM

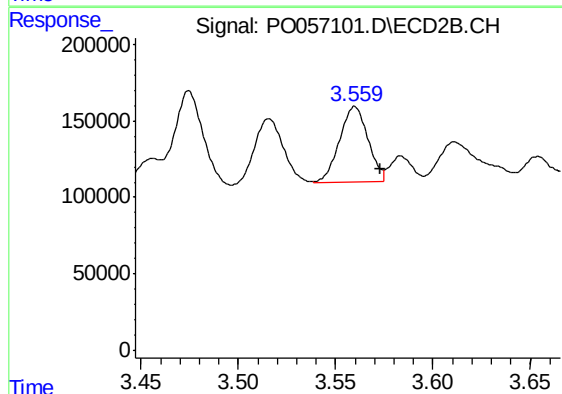


#1 Tetrachloro-m-xylene

R.T.: 3.559 min
Delta R.T.: -0.014 min
Response: 511641
Conc: 15.51 ng/ml m

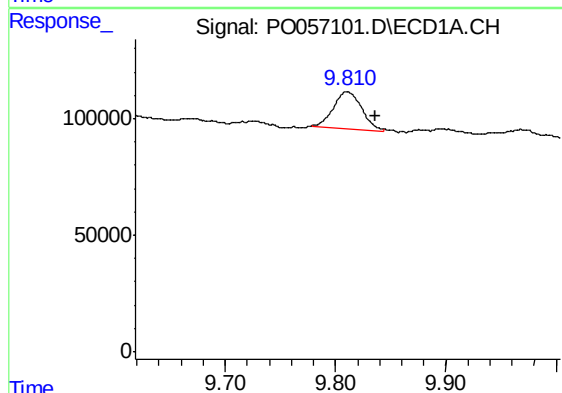

#2 Decachlorobiphenyl

R.T.: 9.810 min
Delta R.T.: -0.026 min
Response: 284947
Conc: 5.81 ng/ml m

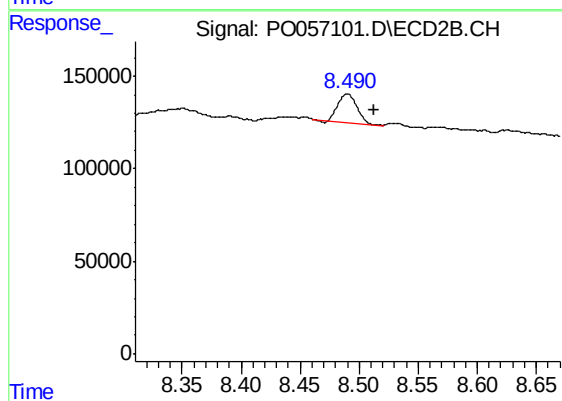

#2 Decachlorobiphenyl

R.T.: 8.490 min
Delta R.T.: -0.023 min
Response: 171826
Conc: 4.82 ng/ml