

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061219\
 Data File : P0057105.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jun 2019 17:27
 Operator : SM/SJ
 Sample : K3304-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 04-A-04-B-04-C

Manual Integrations
 APPROVED

Ankita
 6/13/2019 10:21:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 00:48:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.240	3.561	816114	656229	21.318	19.899
2) SA Decachlor...	9.802	8.488	970036	664058	19.763m	18.624

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061219\
Data File : PO057105.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jun 2019 17:27
Operator : SM/SJ
Sample : K3304-05
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
04-A-04-B-04-C


Manual Integrations
APPROVED

Ankita
6/13/2019 10:21:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 00:48:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

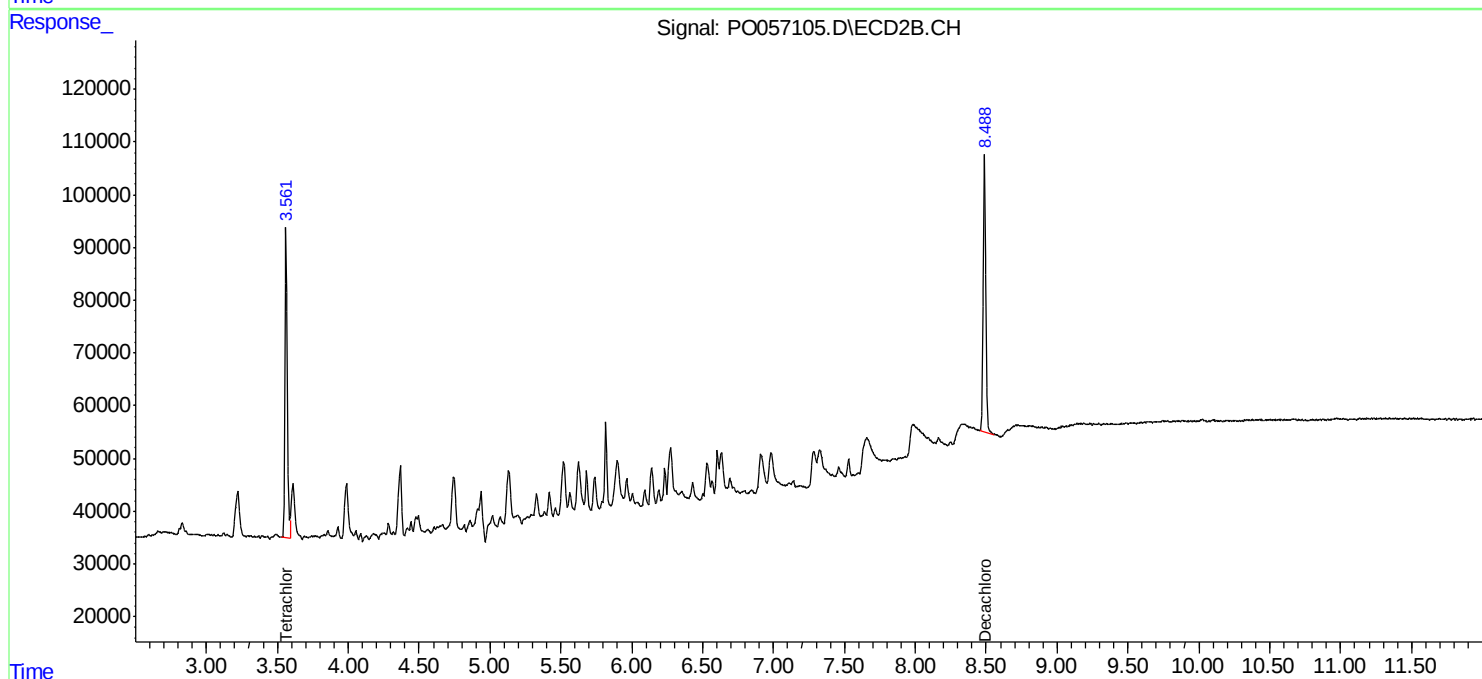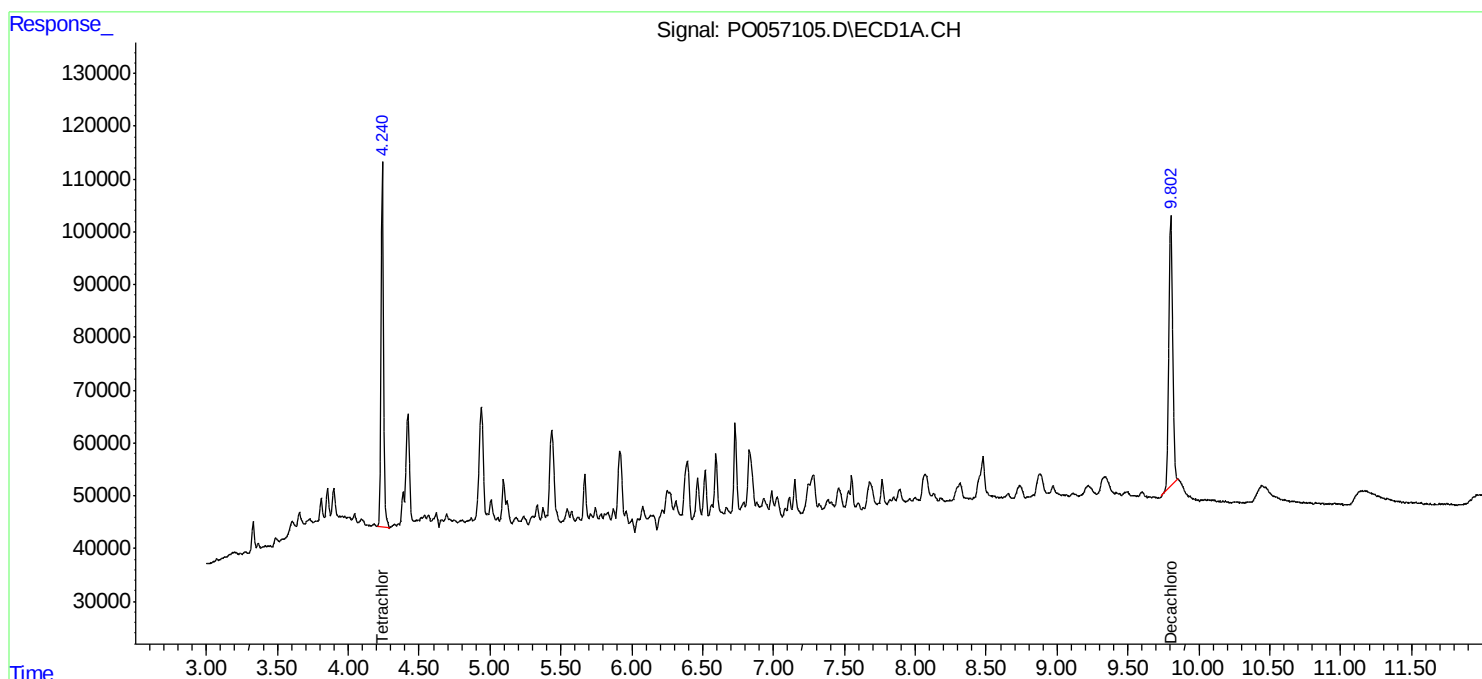

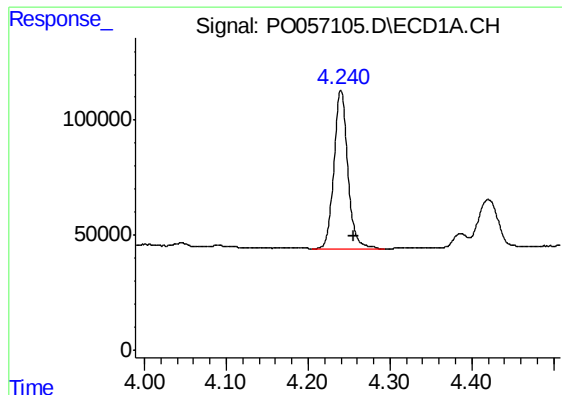


#1 Tetrachloro-m-xylene

R.T.: 4.240 min
Delta R.T.: -0.016 min
Response: 816114
Conc: 21.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
04-A-04-B-04-C


Manual Integrations
APPROVED

Ankita
6/13/2019 10:21:03 AM

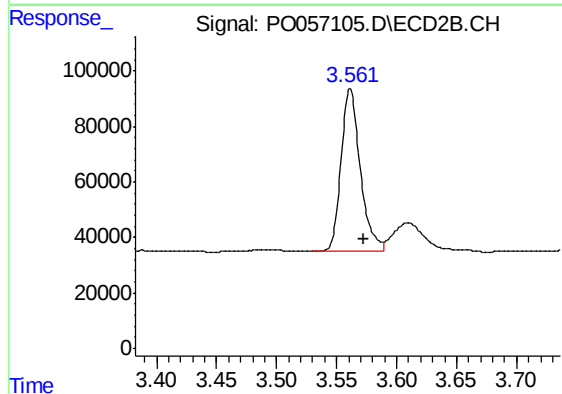


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: -0.012 min
Response: 656229
Conc: 19.90 ng/ml

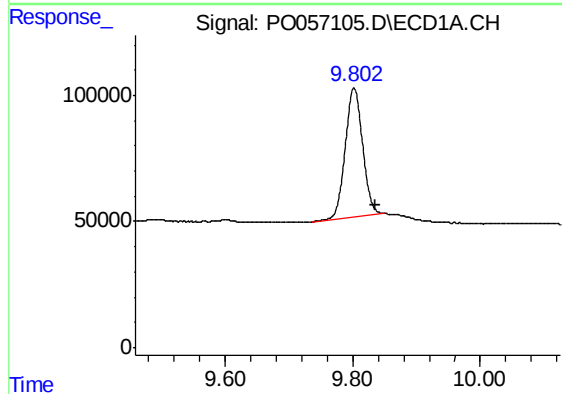

#2 Decachlorobiphenyl

R.T.: 9.802 min
Delta R.T.: -0.034 min
Response: 970036
Conc: 19.76 ng/ml m

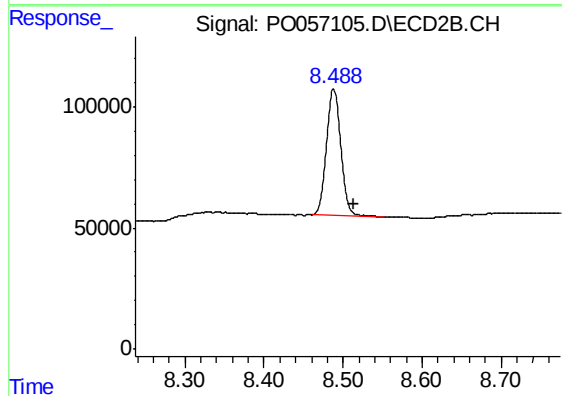

#2 Decachlorobiphenyl

R.T.: 8.488 min
Delta R.T.: -0.025 min
Response: 664058
Conc: 18.62 ng/ml