

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061219\
 Data File : P0057115.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jun 2019 20:17
 Operator : SM/SJ
 Sample : K3304-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 03-A-03-B-03-C

Manual Integrations
 APPROVED

Ankita
 6/13/2019 10:44:30 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 00:52:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.239	3.562	906623	703487	23.682m	21.332m
2) SA Decachlor...	9.801	8.486	1014287	702897	20.664m	19.713m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061219\
Data File : PO057115.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jun 2019 20:17
Operator : SM/SJ
Sample : K3304-03
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
6/13/2019 10:44:30 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 00:52:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

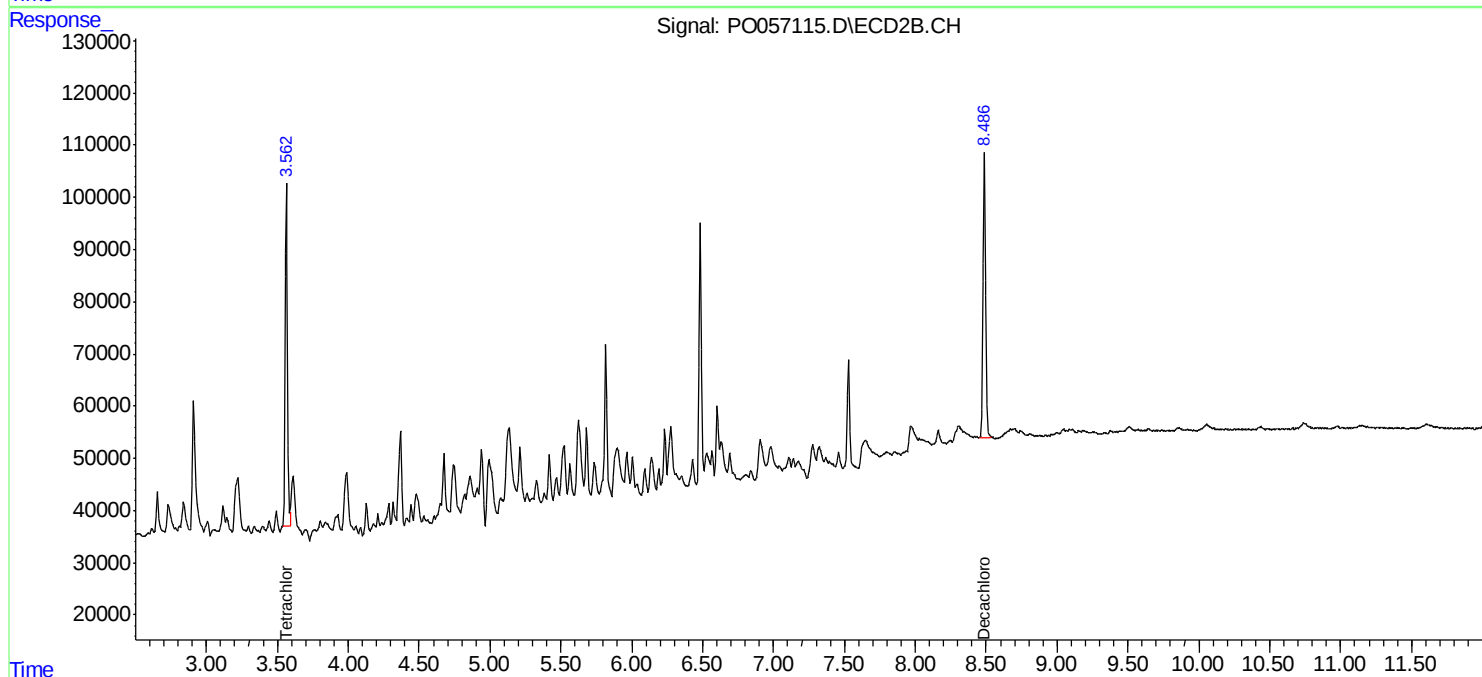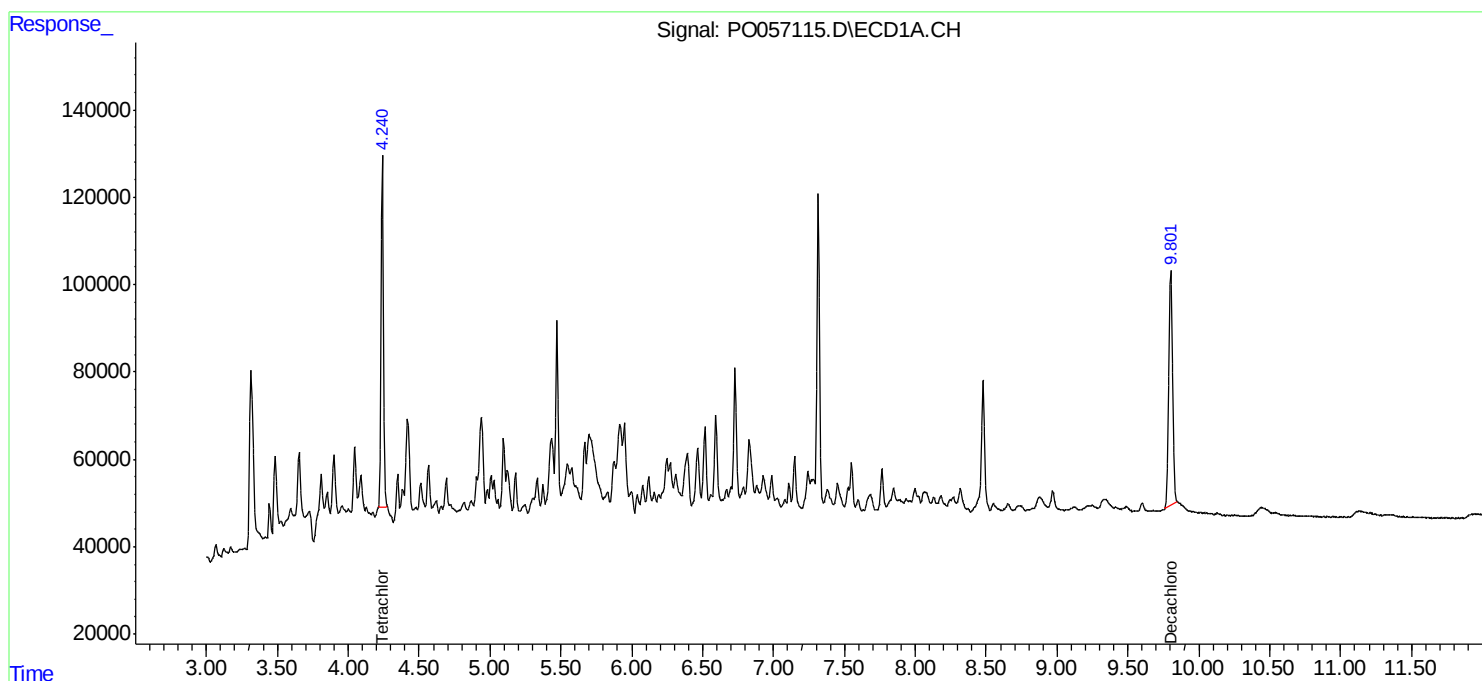

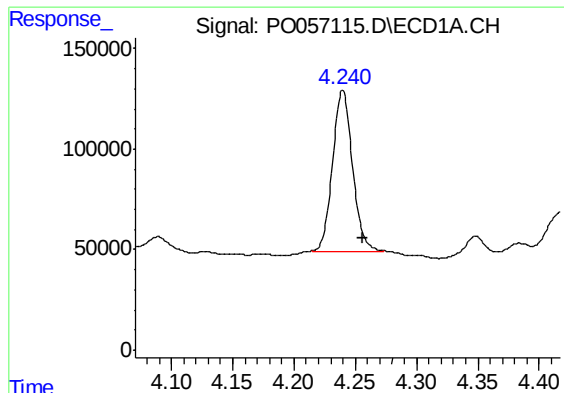


#1 Tetrachloro-m-xylene

R.T.: 4.239 min
Delta R.T.: -0.017 min
Response: 906623
Conc: 23.68 ng/ml m

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
6/13/2019 10:44:30 AM

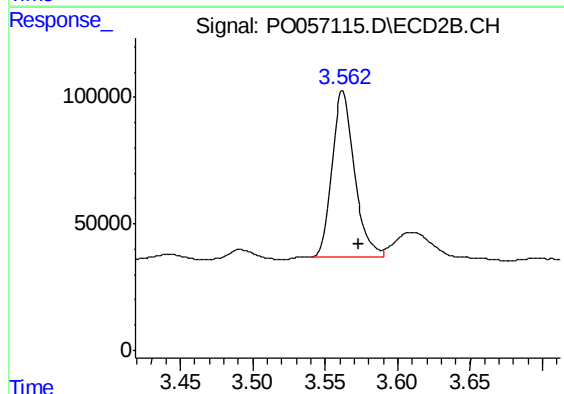


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: -0.011 min
Response: 703487
Conc: 21.33 ng/ml m

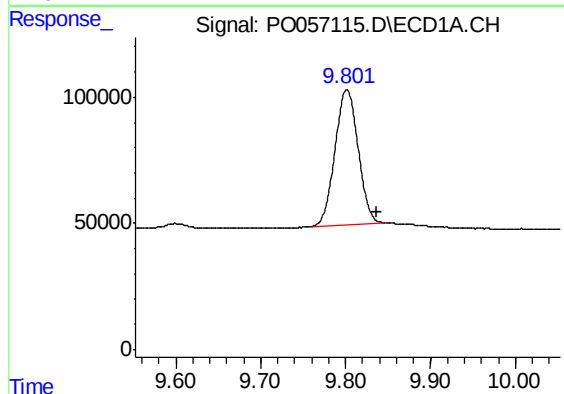

#2 Decachlorobiphenyl

R.T.: 9.801 min
Delta R.T.: -0.036 min
Response: 1014287
Conc: 20.66 ng/ml m

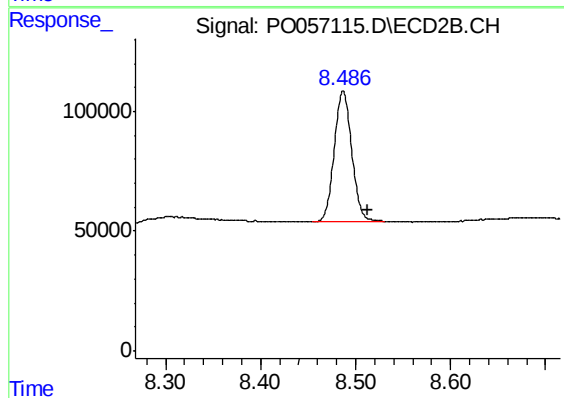

#2 Decachlorobiphenyl

R.T.: 8.486 min
Delta R.T.: -0.027 min
Response: 702897
Conc: 19.71 ng/ml m