

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0061318\
 Data File : P0045739.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jun 2018 18:25
 Operator : SM/UA
 Sample : J3246-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-02-061218

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 02:01:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061218.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 13 03:54:48 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.397	3.631	4589399	2278523	23.552m	20.046m
2) SA Decachlor...	10.061	8.616	3216850	1135716	22.977	16.241m#

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061318\
Data File : P0045739.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jun 2018 18:25
Operator : SM/UA
Sample : J3246-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OK-02-061218

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 02:01:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061218.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 13 03:54:48 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

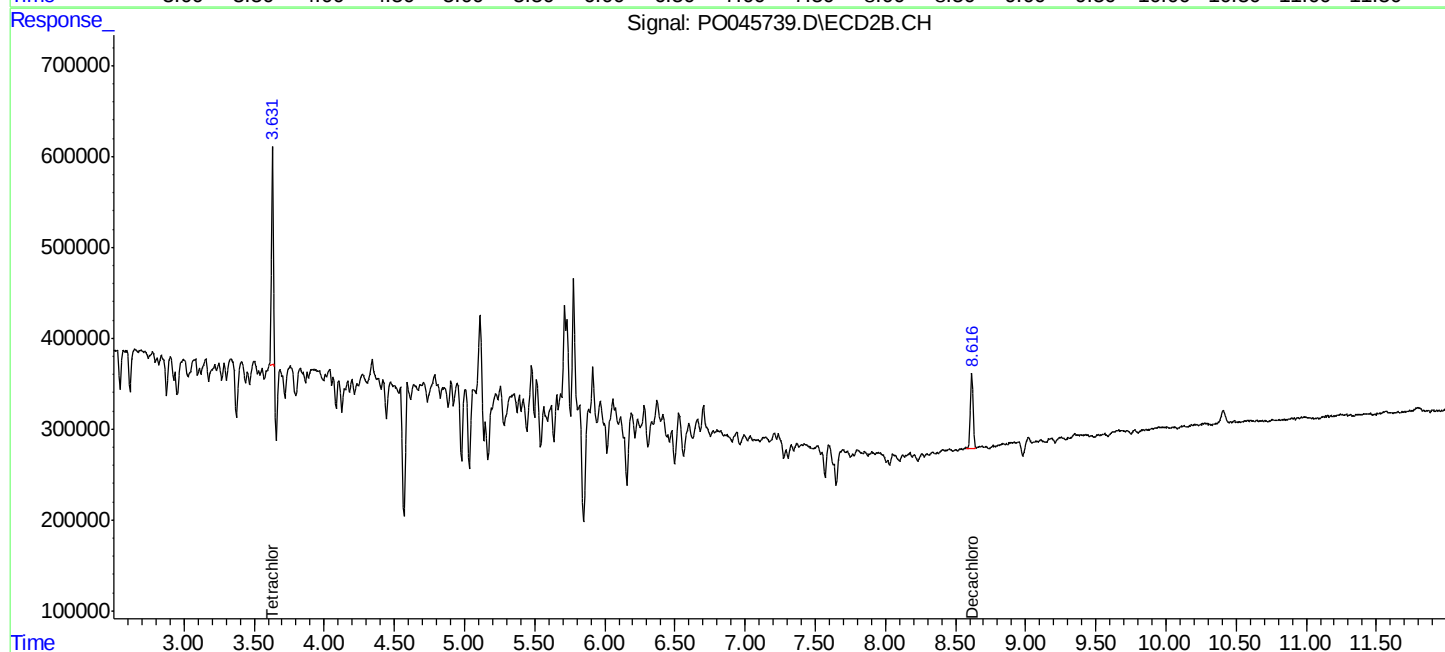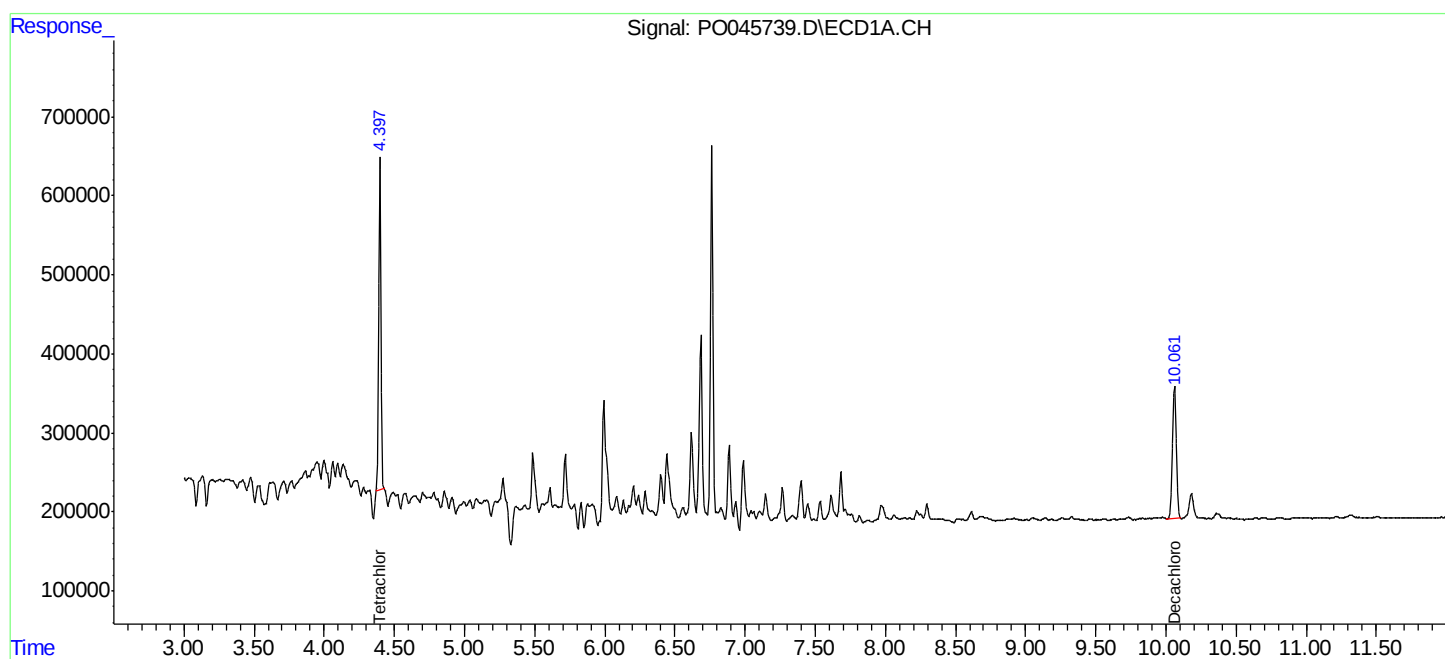


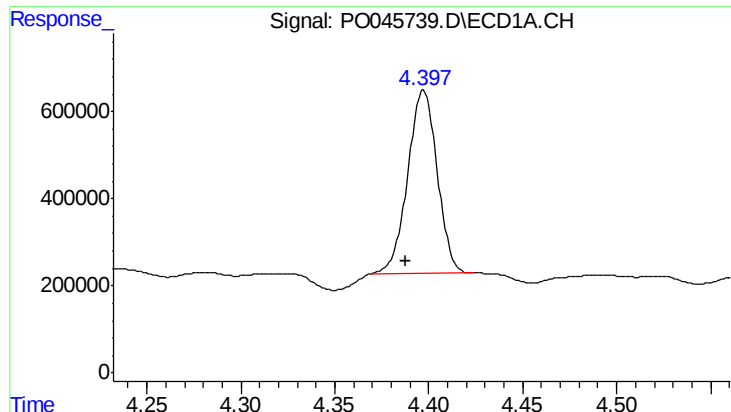

#1 Tetrachloro-m-xylene


R.T.: 4.397 min
Delta R.T.: 0.009 min
Response: 4589399
Conc: 23.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-02-061218

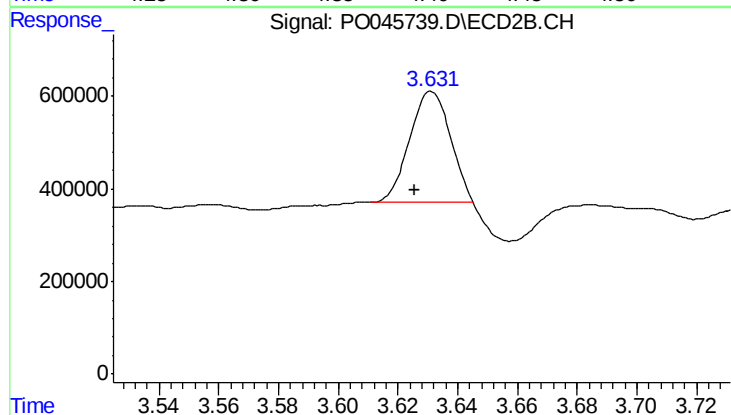


#1 Tetrachloro-m-xylene

R.T.: 3.631 min
Delta R.T.: 0.005 min
Response: 2278523
Conc: 20.05 ng/ml m

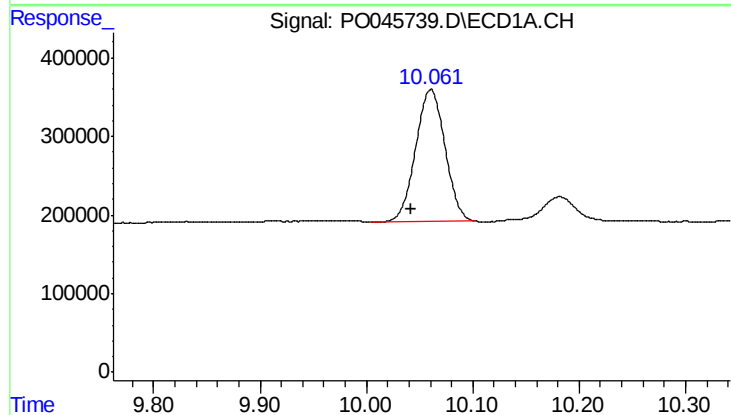

#2 Decachlorobiphenyl

R.T.: 10.061 min
Delta R.T.: 0.019 min
Response: 3216850
Conc: 22.98 ng/ml

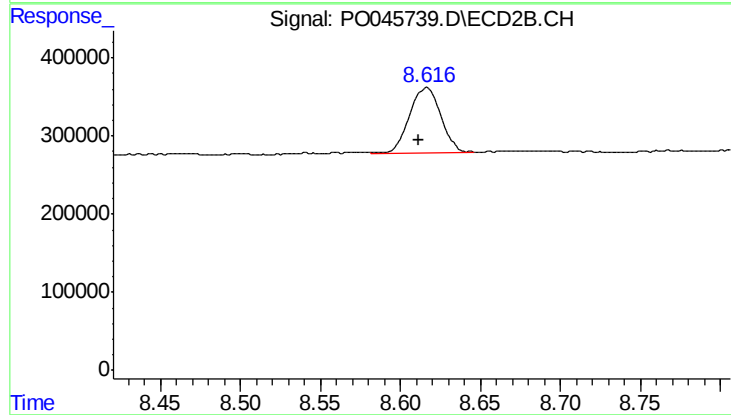

#2 Decachlorobiphenyl

R.T.: 8.616 min
Delta R.T.: 0.005 min
Response: 1135716
Conc: 16.24 ng/ml m