

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061319\
 Data File : P0057149.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jun 2019 22:41
 Operator : SM/SJ
 Sample : K3340-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BUS-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 03:50:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.241	3.563	710964	686596	18.571	20.820
2)	SA Decachlor...	9.806	8.490	1104271	708906	22.498	19.881
Target Compounds							
28)	L6 AR-1254-3	0.000	5.967	0	25137	N.D.	6.866 #
35)	L7 AR-1260-5	0.000	7.199	0	3970	N.D.	0.921 #
37)	L8 AR-1262-2	0.000	7.199	0	3970	N.D.	0.578 #
40)	L8 AR-1262-5	0.000	8.025	0	12180	N.D.	5.245 #
43)	L9 AR-1268-3	0.000	7.773	0	192286	N.D.	32.397 #
44)	L9 AR-1268-4	0.000	8.025	0	12180	N.D.	5.218 #
45)	L9 AR-1268-5	0.000	8.263	0	23455	N.D.	1.355 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061319\
Data File : P0057149.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jun 2019 22:41
Operator : SM/SJ
Sample : K3340-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BUS-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 03:50:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

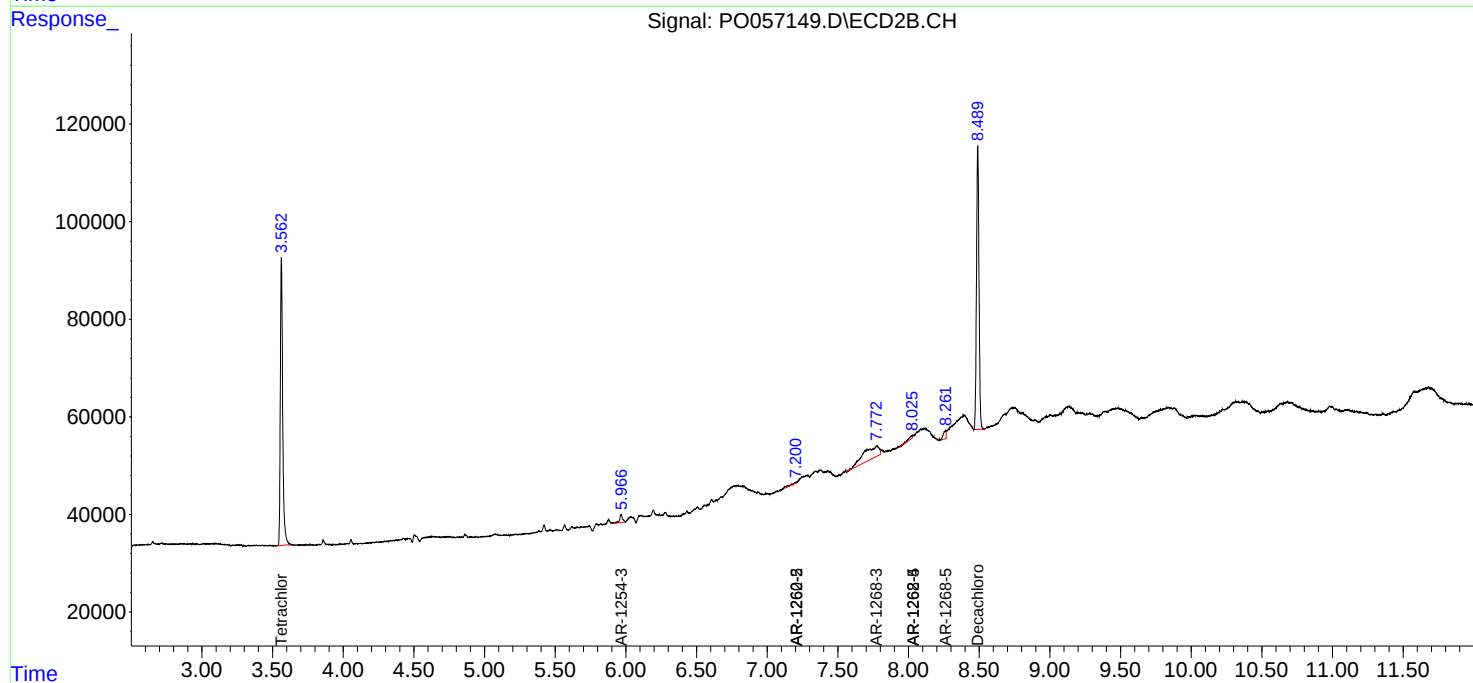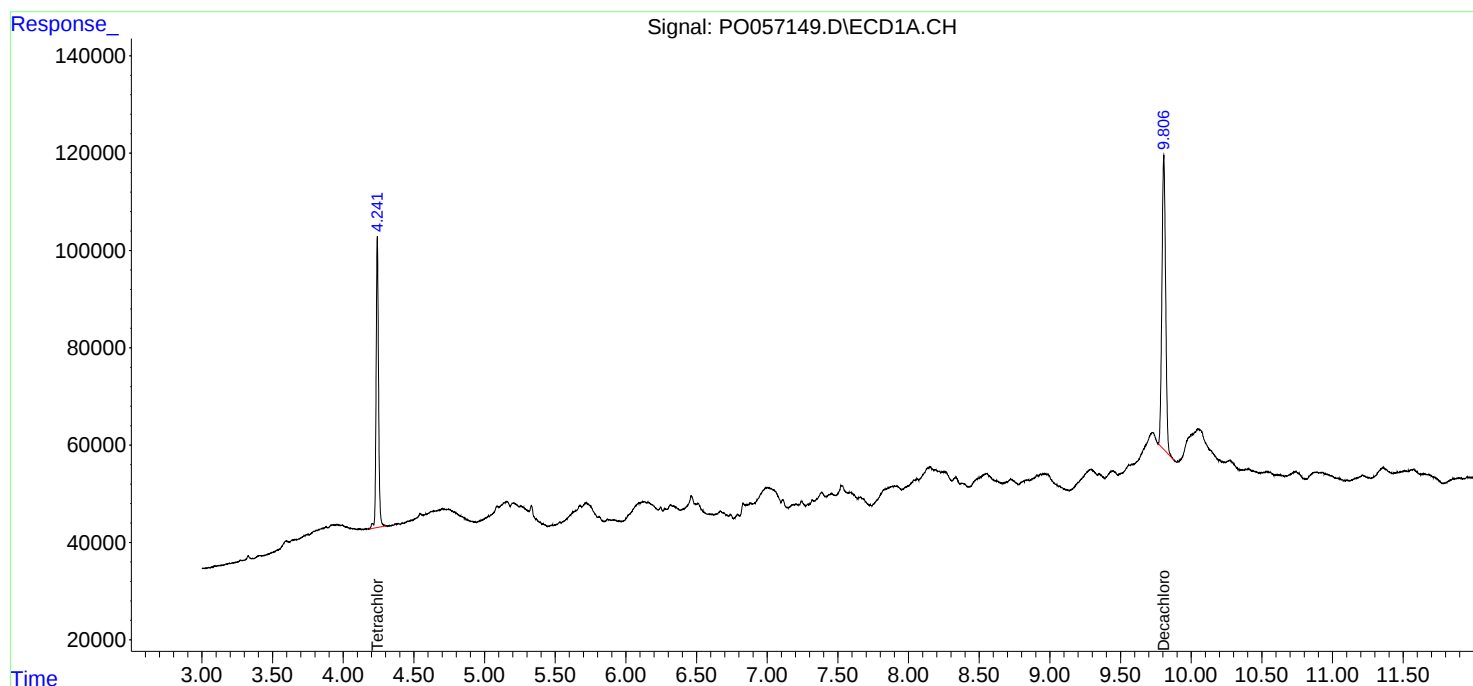


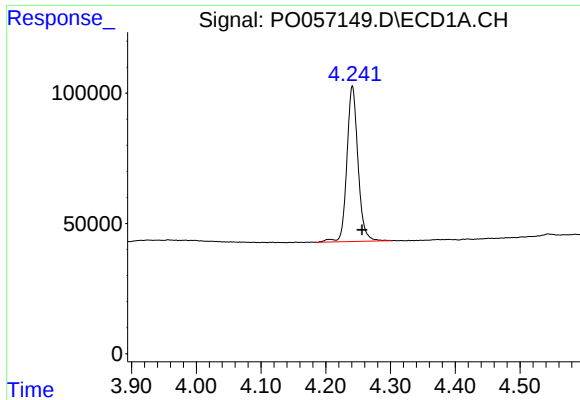

#1 Tetrachloro-m-xylene


R.T.: 4.241 min
Delta R.T.: -0.015 min
Response: 710964
Conc: 18.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
BUS-2

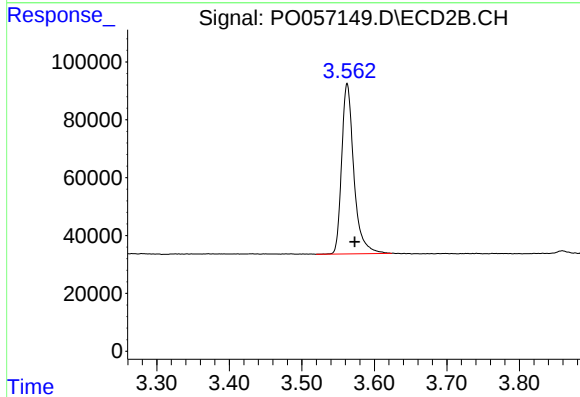


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: -0.011 min
Response: 686596
Conc: 20.82 ng/ml

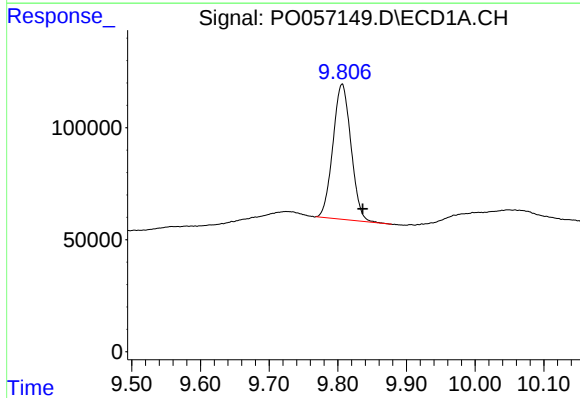


#2 Decachlorobiphenyl

R.T.: 9.806 min
Delta R.T.: -0.030 min
Response: 1104271
Conc: 22.50 ng/ml

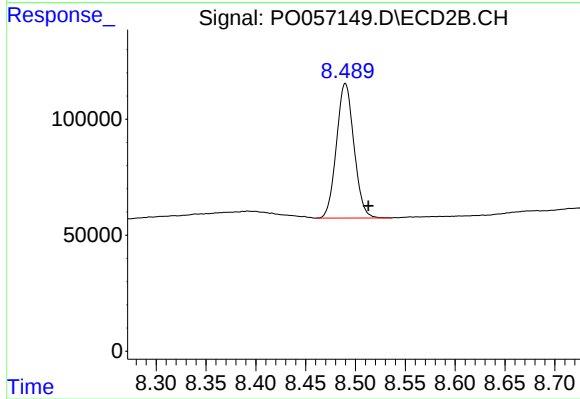

#2 Decachlorobiphenyl


R.T.: 8.490 min
Delta R.T.: -0.023 min
Response: 708906
Conc: 19.88 ng/ml

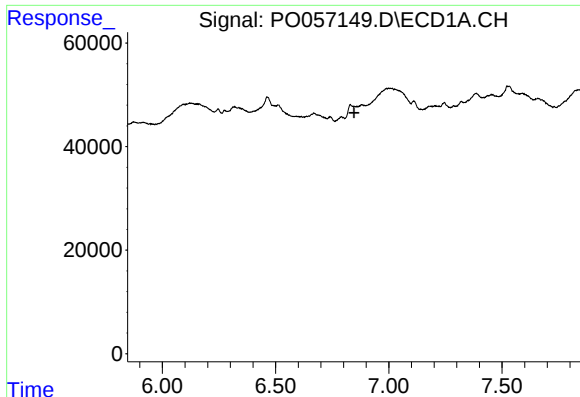

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
BUS-2

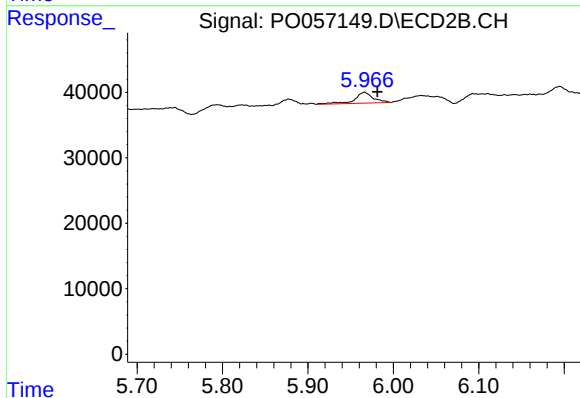


#28 AR-1254-3

R.T.: 5.967 min
Delta R.T.: -0.015 min
Response: 25137
Conc: 6.87 ng/ml

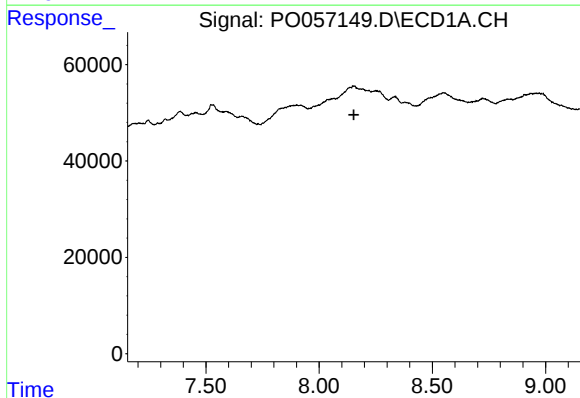


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.153 min
Response: 0
Conc: N.D.

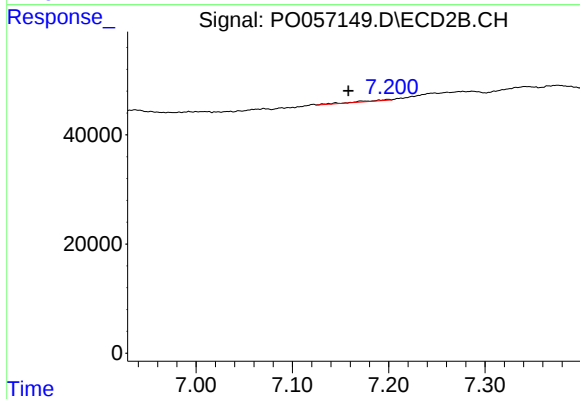

#35 AR-1260-5


R.T.: 7.199 min
Delta R.T.: 0.041 min
Response: 3970
Conc: 0.92 ng/ml

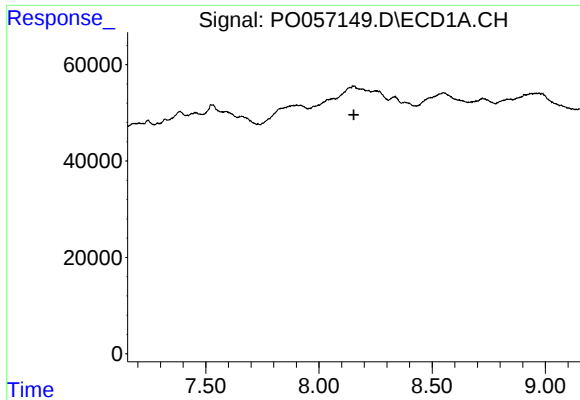

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.154 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
BUS-2

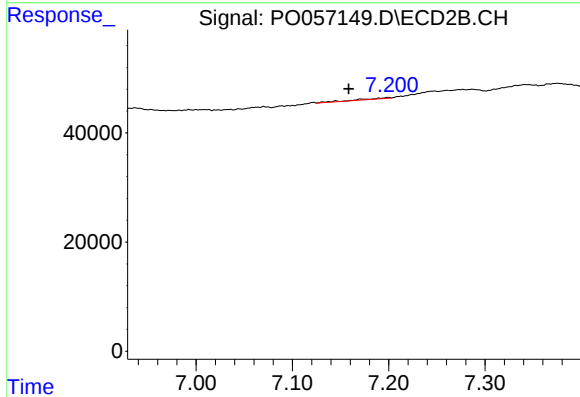


#37 AR-1262-2

R.T.: 7.199 min
Delta R.T.: 0.041 min
Response: 3970
Conc: 0.58 ng/ml

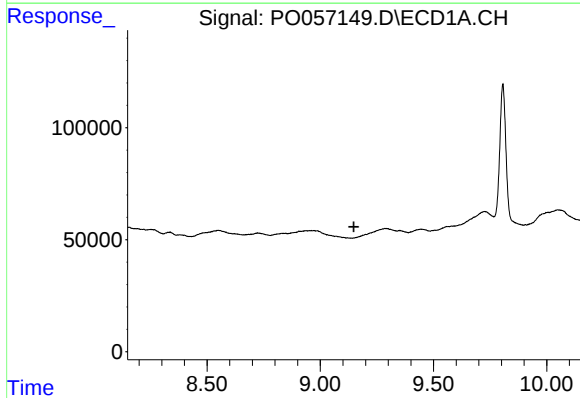


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.148 min
Response: 0
Conc: N.D.

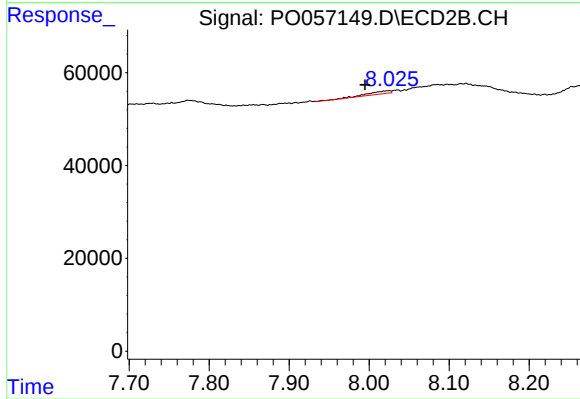

#40 AR-1262-5


R.T.: 8.025 min
Delta R.T.: 0.031 min
Response: 12180
Conc: 5.24 ng/ml

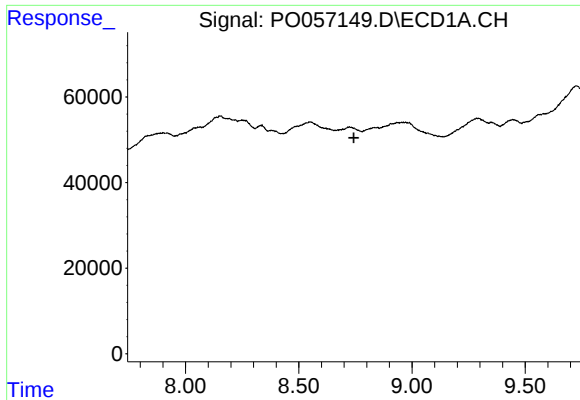

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 8.743 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
BUS-2

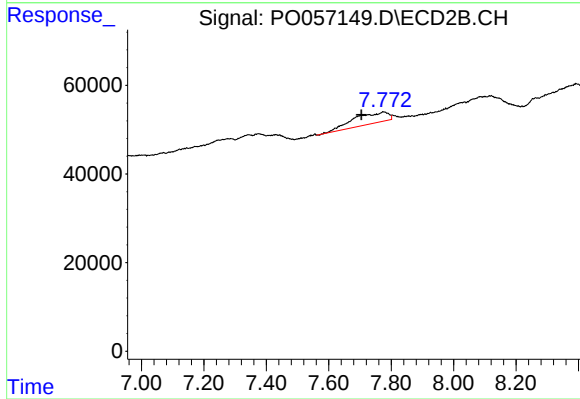


#43 AR-1268-3

R.T.: 7.773 min
Delta R.T.: 0.068 min
Response: 192286
Conc: 32.40 ng/ml

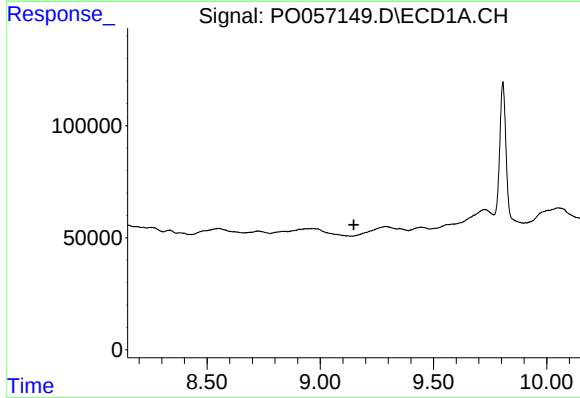


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.148 min
Response: 0
Conc: N.D.

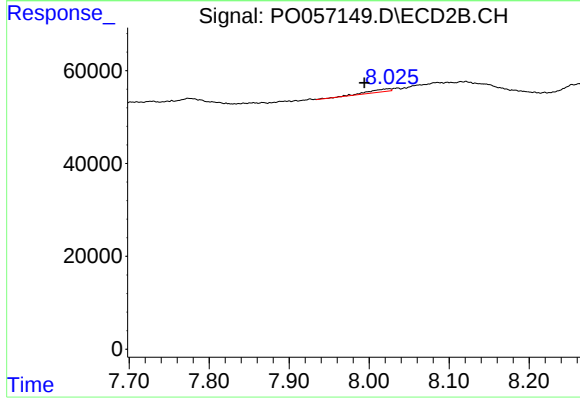

#44 AR-1268-4


R.T.: 8.025 min
Delta R.T.: 0.032 min
Response: 12180
Conc: 5.22 ng/ml

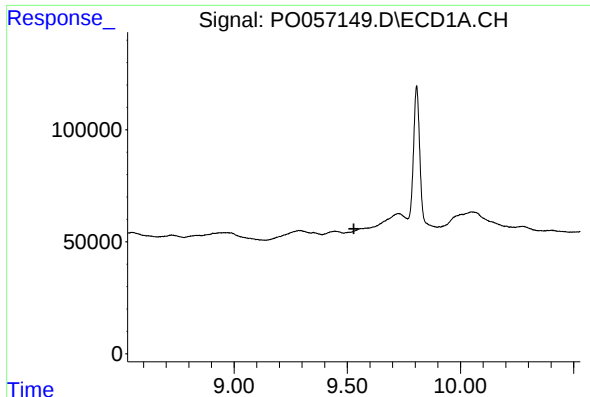

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
BUS-2

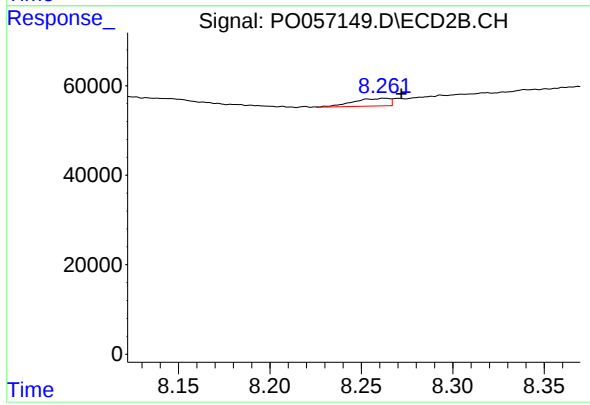

#45 AR-1268-5

R.T.: 8.263 min
Delta R.T.: -0.009 min
Response: 23455
Conc: 1.36 ng/ml